
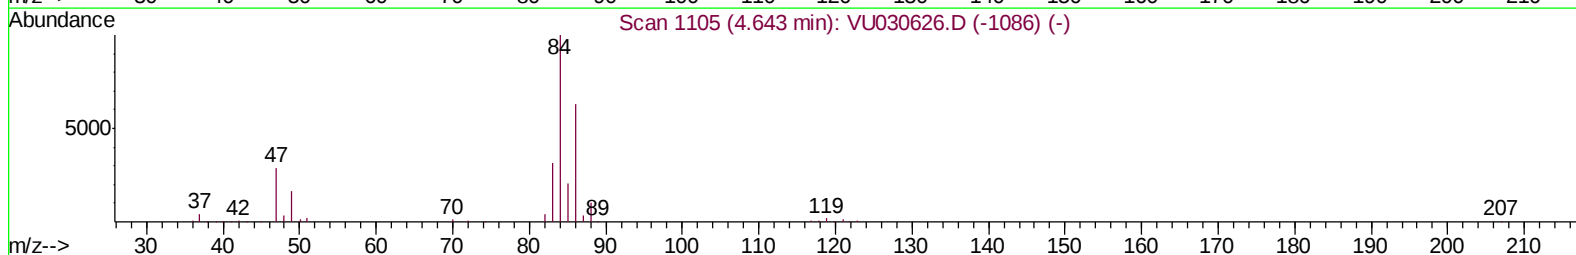
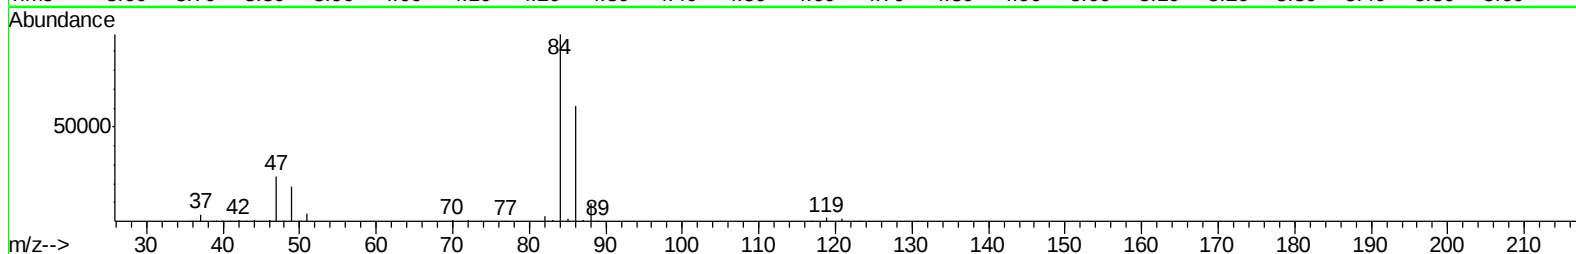


Data File : VU030629.D
Acq On : 03 Apr 2019 16:01
Operator : JC/SP
Sample : K2119-15
Misc : 5.01g/5mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 5 Sample Multiplier: 1

Quant Time: Apr 04 06:55:43 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Apr 04 06:52:42 2019
Response via : Initial Calibration

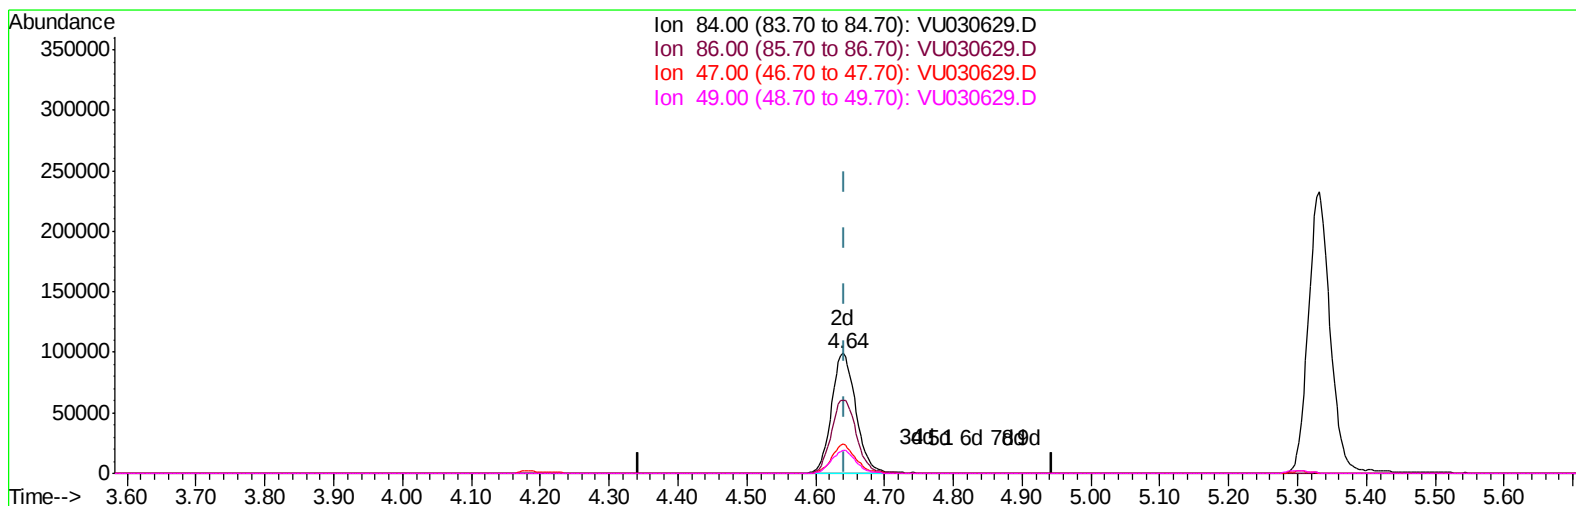

TIC: VU030629.D

(24) Chloroform-d (S)

4.640min (-0.003) 20.46ug/L m

response 242316

Ion	Exp%	Act%
84.00	100	100
86.00	62.50	0.04#
47.00	46.00	0.04#
49.00	27.30	0.02#