
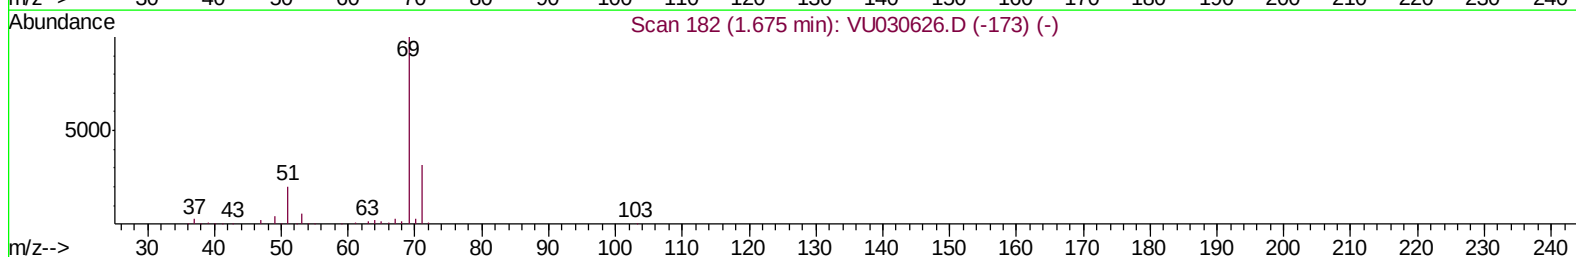
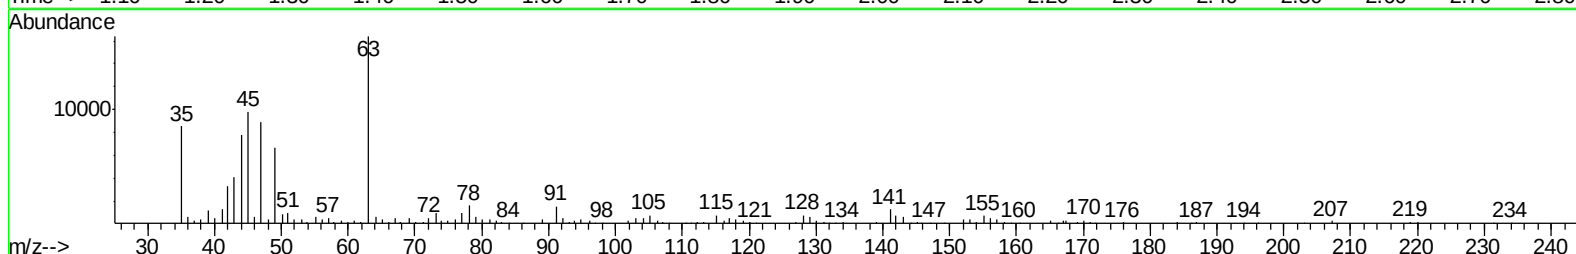


Data File : VU030631.D
Acq On : 03 Apr 2019 16:47
Operator : JC/SP
Sample : K2148-11
Misc : 4.46g/5mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 7 Sample Multiplier: 1

Quant Time: Apr 04 06:56:00 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Apr 04 06:52:42 2019
Response via : Initial Calibration

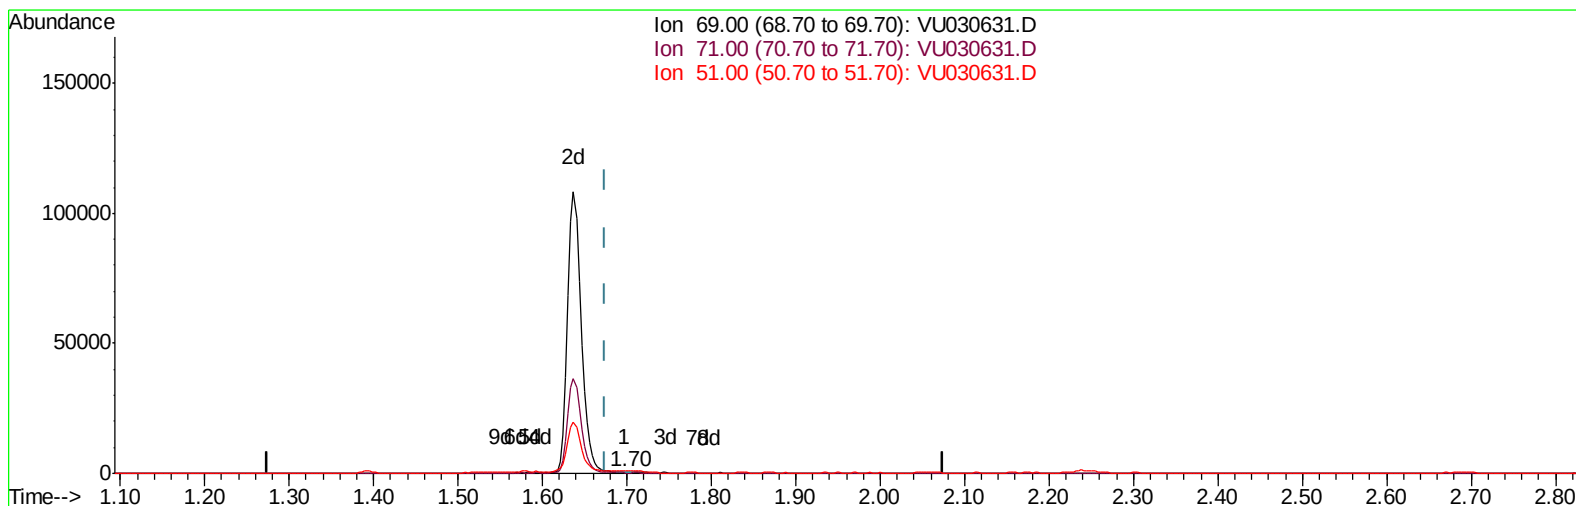

TIC: VU030631.D

(7) Chloroethane-d5 (S)

1.698min (+0.023) 0.03ug/L

response 100

Ion	Exp%	Act%
69.00	100	100
71.00	31.70	402.00#
51.00	28.60	153.00#
0.00	0.00	0.00