
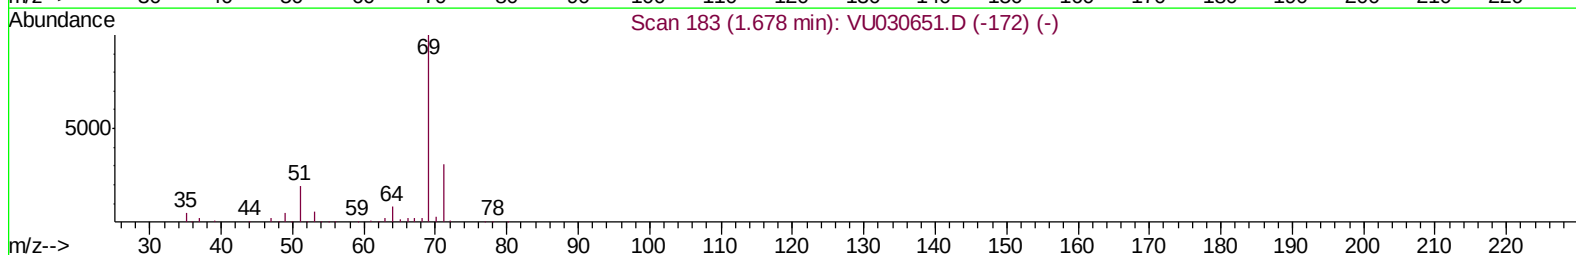
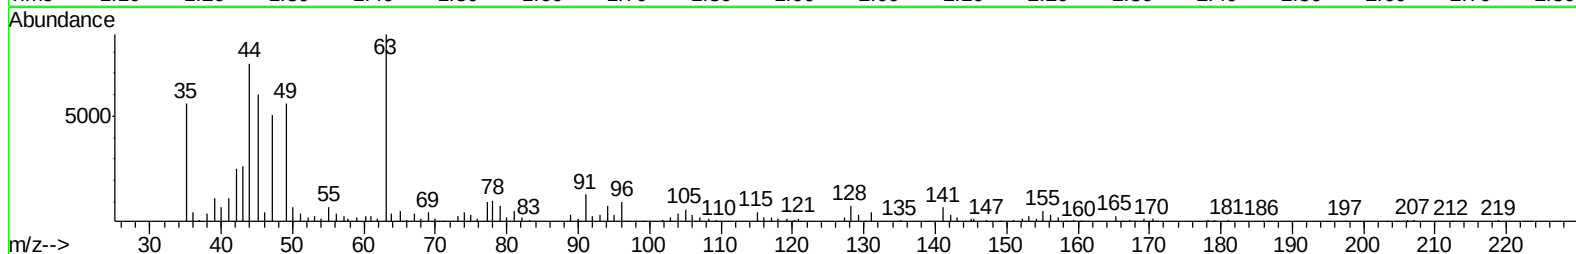


Data File : VU030634.D
Acq On : 03 Apr 2019 17:56
Operator : JC/SP
Sample : K2168-17
Misc : 5.69g/5mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 10 Sample Multiplier: 1

Quant Time: Apr 04 06:56:46 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Apr 04 06:52:42 2019
Response via : Initial Calibration

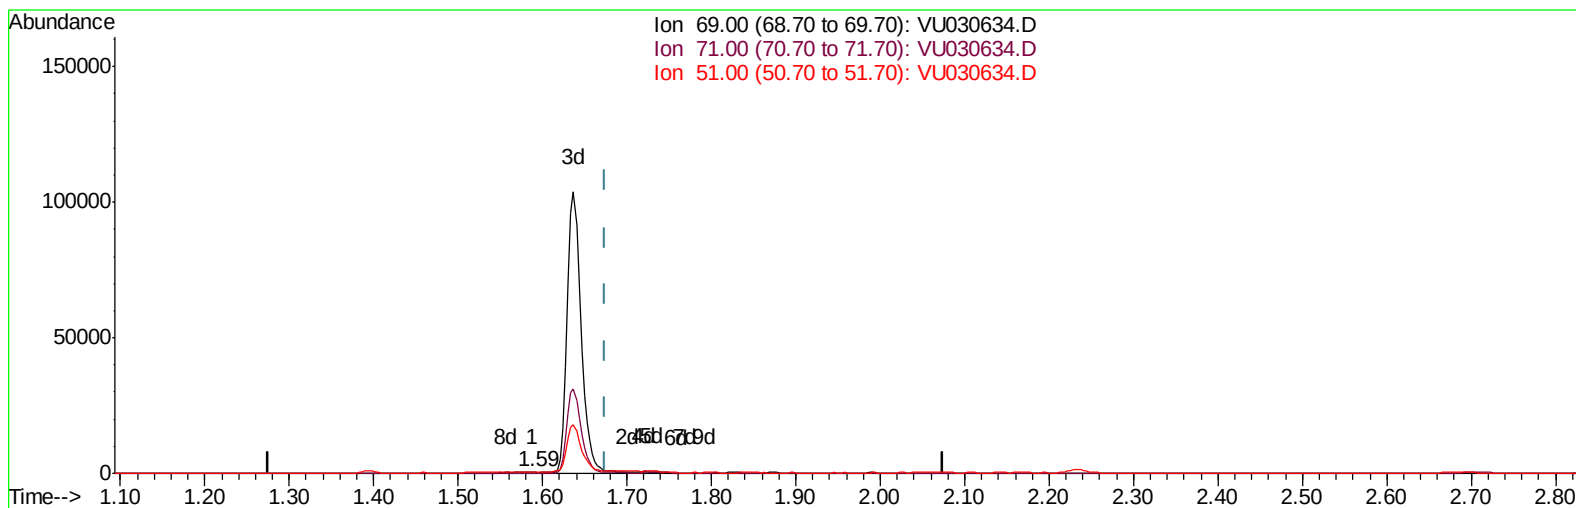

TIC: VU030634.D

(7) Chloroethane-d5 (S)

1.589min (-0.087) 0.19ug/L

response 666

Ion	Exp%	Act%
69.00	100	100
71.00	31.70	28.08
51.00	28.60	27.48
0.00	0.00	0.00