
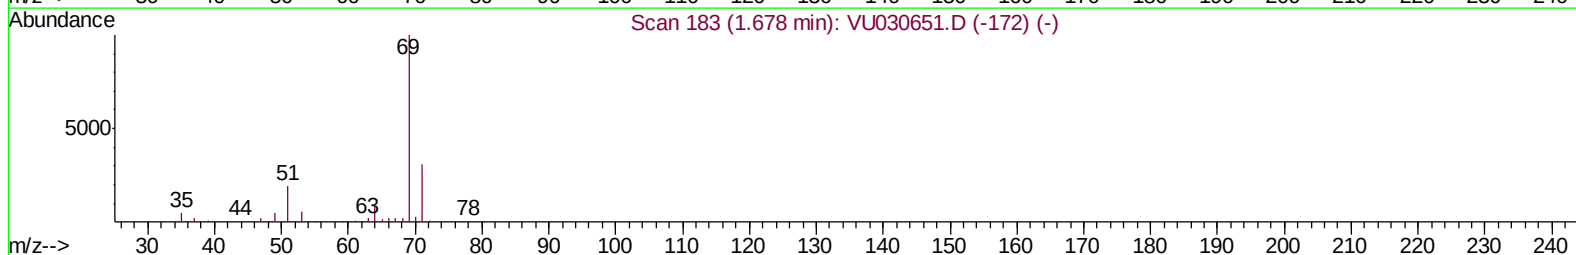
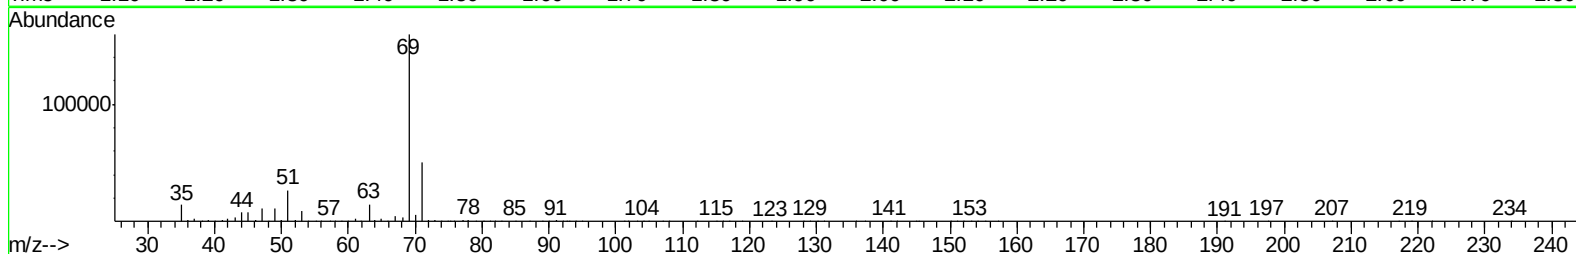


Data File : VU030640.D
Acq On : 03 Apr 2019 20:14
Operator : JC/SP
Sample : K2166-02ME
Misc : 5.96g/5mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 16 Sample Multiplier: 1

Quant Time: Apr 04 06:57:58 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Apr 04 06:52:42 2019
Response via : Initial Calibration

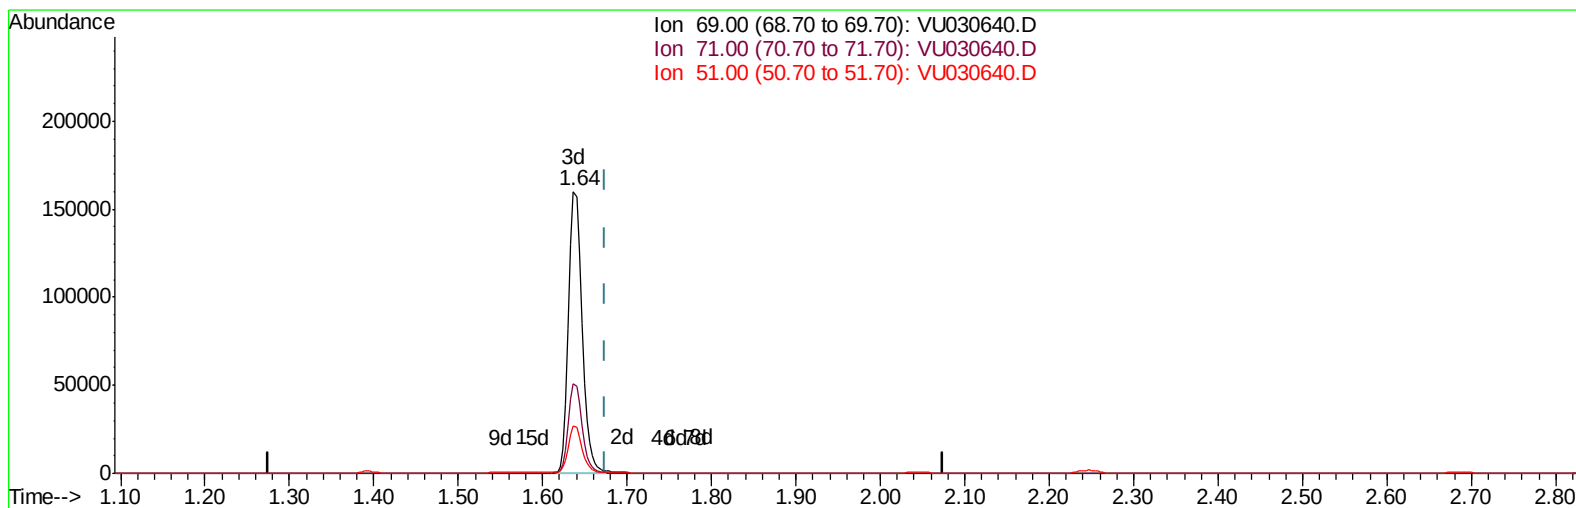

TIC: VU030640.D

(7) Chloroethane-d5 (S)

1.637min (-0.039) 22.47ug/L m

response 177857

Ion	Exp%	Act%
69.00	100	100
71.00	31.70	0.04#
51.00	28.60	0.07#
0.00	0.00	0.00