




Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU040419\
Data File : VU030645.D
Acq On : 03 Apr 2019 22:08
Operator : JC/SP
Sample : K2167-09ME
Misc : 5.90µ/5mL/100µL/5.0mL/MSVOA_U/MEOH
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF110ME

Manual Integrations
APPROVED

MMDadoda
4/4/2019 11:52:39 AM

Quant Time: Apr 04 06:58:46 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Apr 04 06:52:42 2019
Response via : Initial Calibration

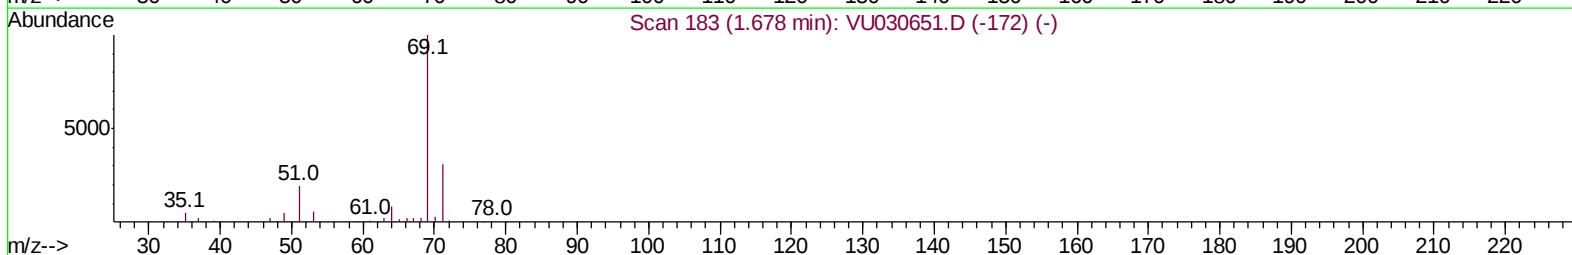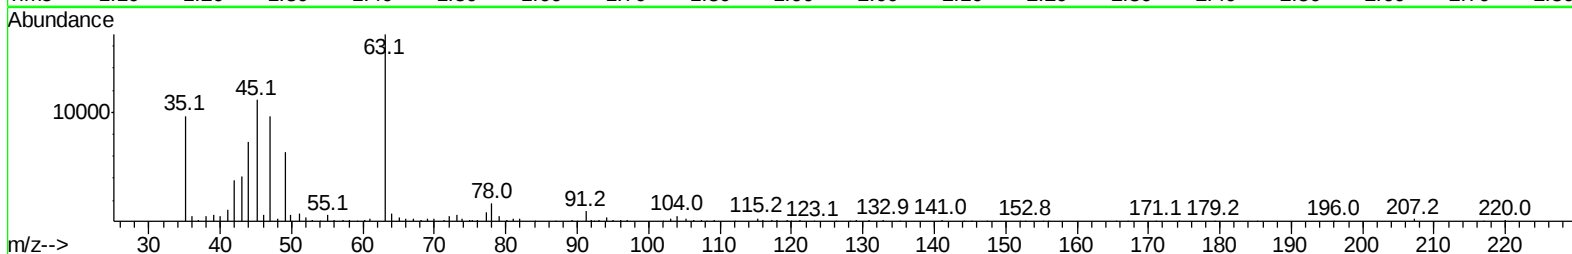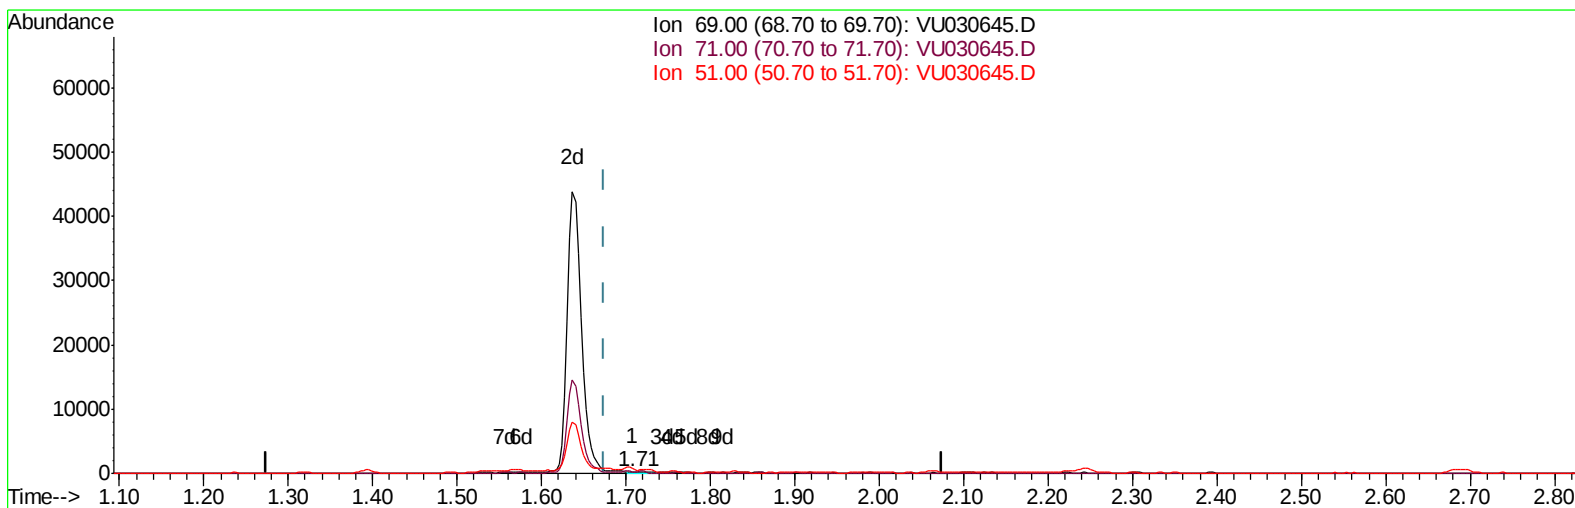

TIC: VU030645.D

(7) Chloroethane-d5 (S)

1.708min (+0.032) 0.10ug/L

response 395

Ion	Exp%	Act%
69.00	100	100
71.00	31.70	69.87#
51.00	28.60	89.37#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU040419\
Data File : VU030645.D
Acq On : 03 Apr 2019 22:08
Operator : JC/SP
Sample : K2167-09ME
Misc : 5.90g/5mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF110ME

Manual Integrations
APPROVED

MMDadoda
4/4/2019 11:52:39 AM

Quant Time: Apr 04 06:58:46 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Apr 04 06:52:42 2019
Response via : Initial Calibration

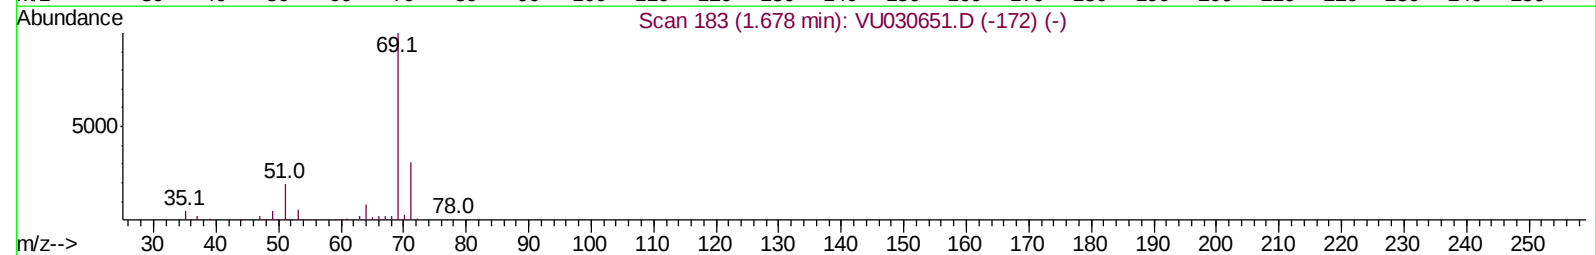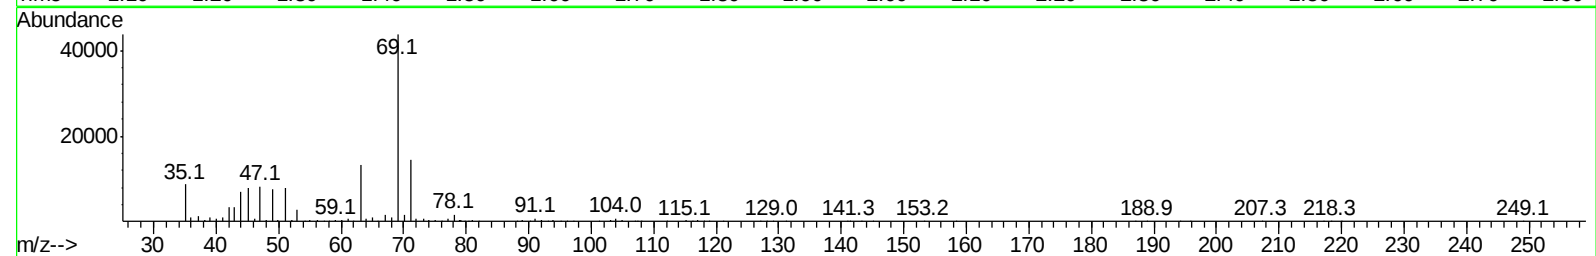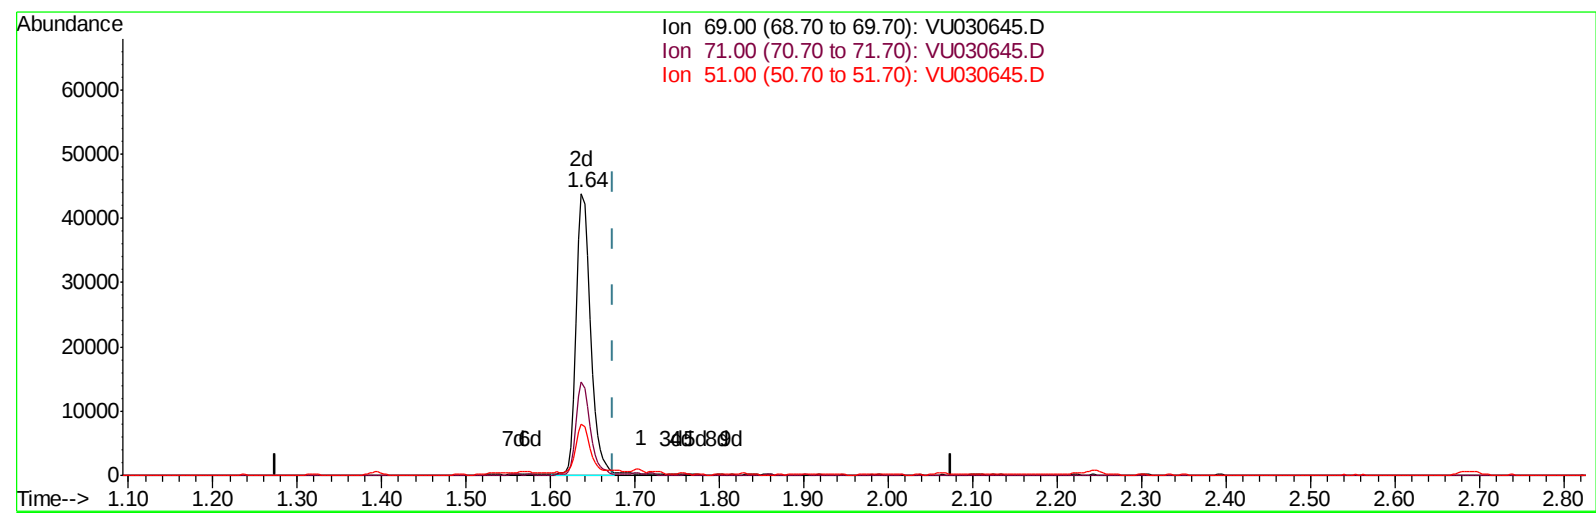

TIC: VU030645.D

(7) Chloroethane-d5 (S)

1.637min (-0.039) 12.88ug/L m

response 51347

Ion	Exp%	Act%
69.00	100	100
71.00	31.70	0.54#
51.00	28.60	0.69#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU040419\
 Data File : VU030645.D
 Acq On : 03 Apr 2019 22:08
 Operator : JC/SP
 Sample : K2167-09ME
 Misc : 5.90g/5mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF110ME

Manual Integrations
 APPROVED

MMDadoda
 4/4/2019 11:52:39 AM

Quant Time: Apr 04 09:12:38 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Apr 04 06:52:42 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	624722	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	603708	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	293254	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.39	65	77978	15.51	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	31.02%#
7) Chloroethane-d5	1.64	69	51347m	12.88	ug/L	-0.04
Spiked Amount	50.000	Range	70 - 130	Recovery	=	25.76%#
11) 1,1-Dichloroethene-d2	2.24	63	117728	12.34	ug/L	-0.03
Spiked Amount	50.000	Range	60 - 125	Recovery	=	24.68%#
21) 2-Butanone-d5	4.19	46	132175	27.97	ug/L	0.02
Spiked Amount	100.000	Range	40 - 130	Recovery	=	27.97%#
24) Chloroform-d	4.64	84	125869	14.53	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	29.06%#
26) 1,2-Dichloroethane-d4	5.30	65	86503	15.26	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	30.52%#
32) Benzene-d6	5.33	84	278645	16.09	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	32.18%#
36) 1,2-Dichloropropane-d6	6.33	67	92918	15.69	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	31.38%#
41) Toluene-d8	7.56	98	243073	15.63	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	31.26%#
43) trans-1,3-Dichloropropene-	7.85	79	39940	14.34	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	28.68%#
47) 2-Hexanone-d5	8.32	63	91893	28.63	ug/L	0.01
Spiked Amount	100.000	Range	45 - 130	Recovery	=	28.63%#
57) 1,1,2,2-Tetrachloroethane-	10.43	84	132157	15.59	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	31.18%#
64) 1,2-Dichlorobenzene-d4	11.86	152	92809	15.79	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	31.58%#

Target Compounds					Ovalue
34) Trichloroethene	6.18	95	41540	8.222 ug/L	98
46) Tetrachloroethene	8.22	164	470354	133.296 ug/L	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU040419\
Data File : VU030645.D
Acq On : 03 Apr 2019 22:08
Operator : JC/SP
Sample : K2167-09ME
Misc : 5.90µ/5mL/100µL/5.0mL/MSVOA_U/MEOH
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF110ME

Manual Integrations
APPROVED

MMDadoda
4/4/2019 11:52:39 AM

Quant Time: Apr 04 09:12:38 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Apr 04 06:52:42 2019
Response via : Initial Calibration

