


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU040419\
 Data File : VU030625.D
 Acq On : 03 Apr 2019 13:41
 Operator : JC/SP
 Sample : BFB49
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB49

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
 Title : VOC Analysis
 Last Update : Thu Apr 04 13:18:40 2019

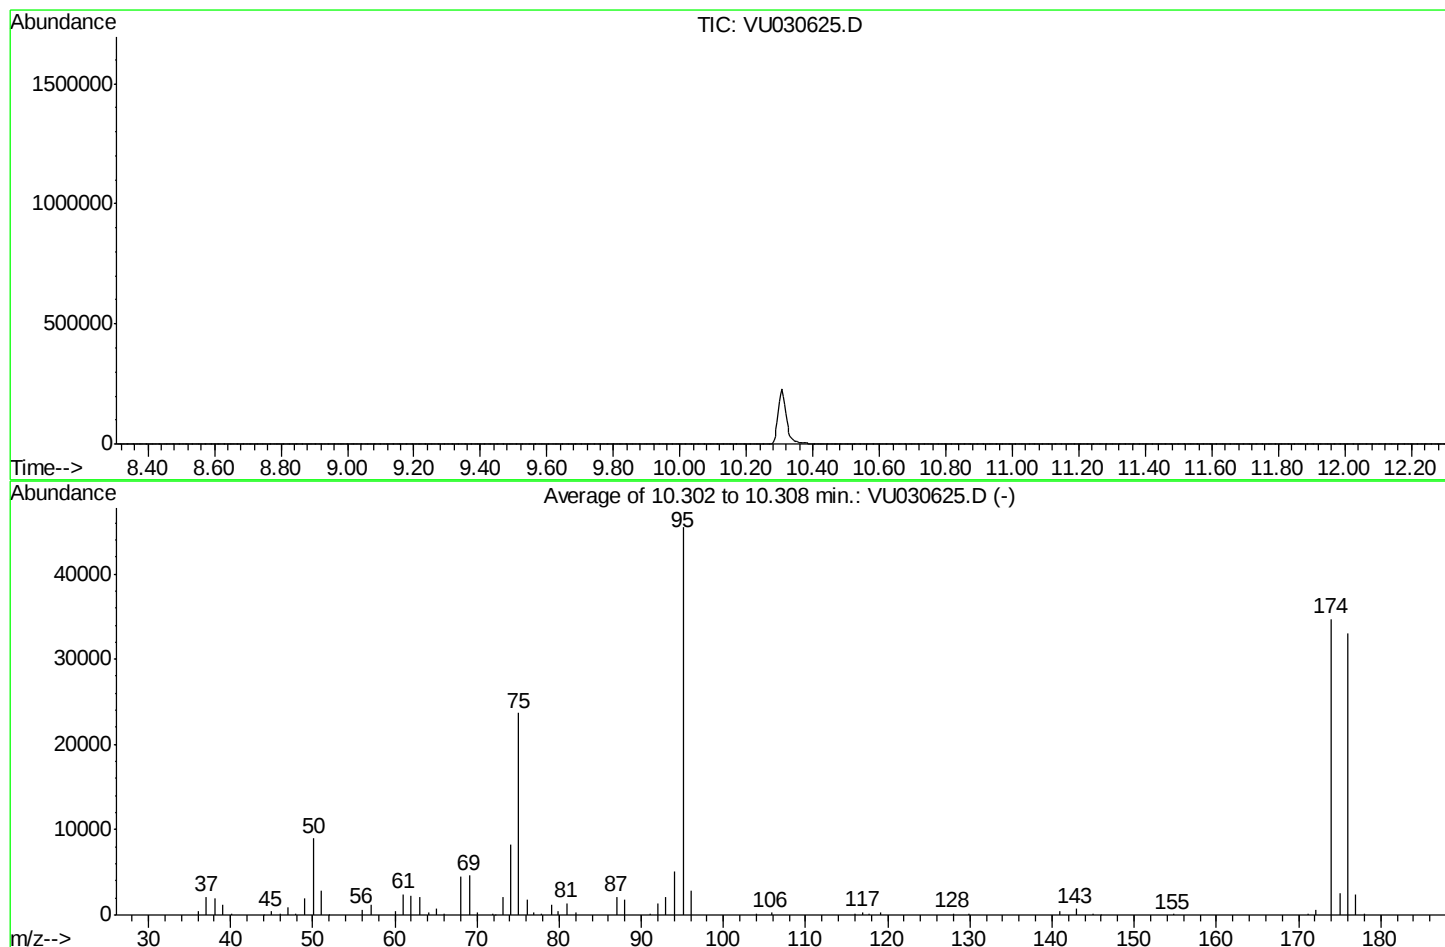

AutoFind: Scans 2865, 2866, 2867; Background Corrected with Scan 2854

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.8	8990	PASS
75	95	30	80	52.1	23693	PASS
95	95	100	100	100.0	45458	PASS
96	95	5	9	6.1	2789	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	76.3	34698	PASS
175	174	5	9	7.4	2567	PASS
176	174	95	101	95.2	33026	PASS
177	176	5	9	7.1	2336	PASS

Scan 2854 (10.267 min): VU030625.D
BFB49

m/z	Abundance
40.00	341.0
43.90	809.0

Instrument :
MSVOA_U
ClientSampleId :
BFB49

m/z	Abundance
36.10	419.0
37.00	2197.0
38.10	1870.0
39.00	1145.0
40.20	343.0
44.00	825.0
44.90	429.0
47.00	963.0
48.00	148.0
49.00	1939.0
50.10	8887.0
51.00	2924.0
56.00	623.0
57.10	1156.0
60.00	514.0
61.00	2186.0
62.00	2420.0
63.10	2021.0
64.10	321.0
65.00	541.0
66.00	109.0
68.10	4185.0
69.10	4546.0
70.10	379.0
71.90	255.0
73.10	2098.0
74.10	8141.0
75.10	22928.0
76.10	1691.0
77.00	223.0
79.00	1192.0
79.90	528.0
80.90	1348.0
82.00	280.0
87.00	2022.0
88.00	1818.0
91.00	144.0
92.10	1240.0
93.00	1923.0
94.10	4990.0
95.10	43600.0
96.10	2844.0
104.00	114.0
105.90	256.0
115.90	143.0
117.00	312.0
117.70	109.0
119.00	248.0
128.00	144.0
129.90	127.0
141.00	576.0
142.90	629.0
145.00	213.0
154.80	125.0
171.10	141.0
172.10	640.0
174.00	32048.0
175.00	2551.0
176.00	30976.0
177.00	2148.0
178.00	137.0

Instrument :
MSVOA_U
ClientSampleId :
BFB49

m/z	Abundance
36.10	503.0
37.10	2203.0
38.10	1995.0
39.00	1174.0
40.20	480.0
44.00	892.0
44.90	444.0
46.10	109.0
47.00	935.0
48.00	132.0
49.00	2045.0
50.10	9278.0
51.00	3013.0
56.00	653.0
57.10	1124.0
60.00	507.0
61.10	2610.0
62.00	2375.0
63.10	2115.0
64.10	322.0
65.00	751.0
66.00	122.0
68.00	4624.0
69.10	4712.0
70.10	325.0
72.00	228.0
73.10	2277.0
74.10	8601.0
75.10	24632.0
76.10	1906.0
76.90	242.0
77.90	189.0
79.00	1261.0
79.90	483.0
80.90	1453.0
82.00	247.0
87.00	2242.0
88.00	1909.0
91.00	185.0
92.00	1394.0
93.00	2188.0
94.10	5201.0
95.10	46840.0
96.10	2857.0
103.90	121.0
105.90	273.0
115.90	187.0
117.00	304.0
117.70	116.0
119.10	281.0
127.90	201.0
129.90	127.0
141.00	528.0
142.90	727.0
144.90	245.0
145.90	108.0
154.80	129.0
171.20	167.0
172.00	670.0
174.00	35744.0
175.00	2637.0
176.00	33960.0
177.00	2412.0
178.00	119.0

Instrument :
MSVOA_U
ClientSampleId :
BFB49

m/z	Abundance
36.10	504.0
37.10	2103.0
38.10	1916.0
39.00	1128.0
40.20	569.0
44.00	885.0
44.90	460.0
46.10	156.0
47.00	722.0
47.90	137.0
49.00	1930.0
50.10	8806.0
51.10	2826.0
51.90	123.0
56.00	633.0
57.00	1153.0
60.00	416.0
61.10	2521.0
62.00	2105.0
63.10	1972.0
64.10	294.0
65.00	838.0
66.10	103.0
68.00	4881.0
69.10	4524.0
70.00	261.0
72.20	183.0
73.10	2127.0
74.10	8094.0
75.10	23520.0
76.10	2012.0
76.90	286.0
77.90	176.0
79.00	1314.0
79.90	391.0
80.90	1375.0
82.00	229.0
87.00	2095.0
87.90	1861.0
91.00	160.0
91.90	1440.0
93.00	2162.0
94.10	4958.0
95.10	45936.0
96.10	2668.0
103.90	124.0
105.80	213.0
116.00	240.0
117.00	300.0
117.70	107.0
119.10	304.0
127.90	203.0
129.80	110.0
141.00	417.0
142.90	720.0
144.90	214.0
145.90	122.0
171.10	142.0
172.00	553.0
174.00	36304.0
175.10	2514.0
176.00	34144.0
177.00	2450.0

Instrument :
MSVOA_U
ClientSampleId :
BFB49