

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040423\
 Data File : VU053572.D
 Acq On : 04 Apr 2023 19:30
 Operator : JC/MD
 Sample : 02158-17DL 20X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 25 Sample Multiplier: 1


Instrument :
 MSVOA_U
 ClientSampleId :
 PMW-2(20230330)DL

Quant Time: Apr 04 23:14:09 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Apr 01 04:51:17 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.243	114	270093	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.414	117	252820	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.806	152	128019	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	67951	32.310	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	64.620%		
7) Chloroethane-d5	1.909	69	60409	37.254	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	74.500%		
11) 1,1-Dichloroethene-d2	2.562	63	92145	28.304	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	56.600%#		
21) 2-Butanone-d5	4.613	46	103224	108.406	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	108.410%		
24) Chloroform-d	5.057	84	134647	38.712	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	77.420%		
26) 1,2-Dichloroethane-d4	5.697	65	89501	43.547	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	87.100%		
32) Benzene-d6	5.723	84	268039	39.277	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	78.560%		
36) 1,2-Dichloropropane-d6	6.687	67	88101	42.237	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	84.480%		
41) Toluene-d8	7.893	98	244776	36.088	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	72.180%#		
43) trans-1,3-Dichloroprop...	8.173	79	41351	38.405	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	76.800%		
47) 2-Hexanone-d5	8.626	63	78364	110.080	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	110.080%		
56) 1,1,2,2-Tetrachloroeth...	10.751	84	130478	44.381	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	88.760%		
66) 1,2-Dichlorobenzene-d4	12.188	152	104300	39.031	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	78.060%#		
Target Compounds						Qvalue
5) Vinyl chloride	1.604	62	3040	1.456	ug/L #	47
10) 1,1,2-Trichloro-1,2,2-...	2.568	101	1559	0.838	ug/L #	64
12) 1,1-Dichloroethene	2.575	96	16603	10.018	ug/L #	1
19) 1,1-Dichloroethane	3.864	63	227796	82.563	ug/L	99
20) cis-1,2-Dichloroethene	4.665	96	26083	13.558	ug/L	93
34) Trichloroethene	6.539	95	39950	20.053	ug/L	95
65) 1,4-Dichlorobenzene	11.835	146	13627	3.381	ug/L	95
70) 1,2,4-trichlorobenzene	13.841	180	5612	2.067	ug/L	96





(#) = qualifier out of range (m) = manual integration (+) = signals summed

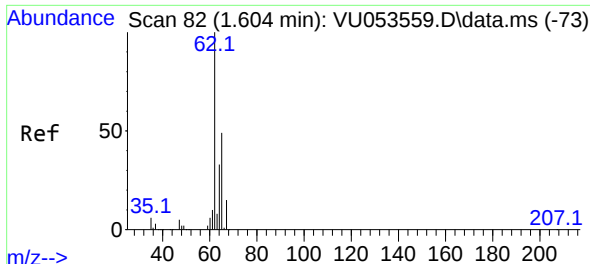

#5
 Vinyl chloride
 Concen: 1.456 ug/L
 RT: 1.604 min Scan# 81
 Delta R.T. 0.000 min
 Lab File: VU053572.D
 Acq: 04 Apr 2023 19:30




Instrument :
 MSVOA_U
 ClientSampleId :
 PMW-2(20230330)DL


Tgt Ion: 62 Resp: 3040
 Ion Ratio Lower Upper
 62 100
 64 62.8 23.2 43.0#

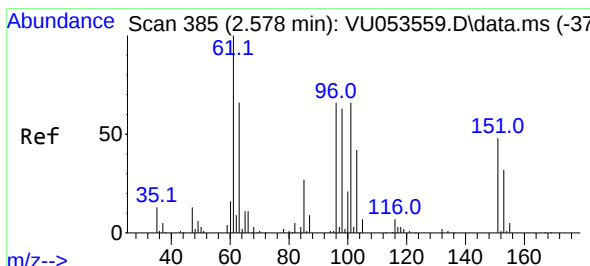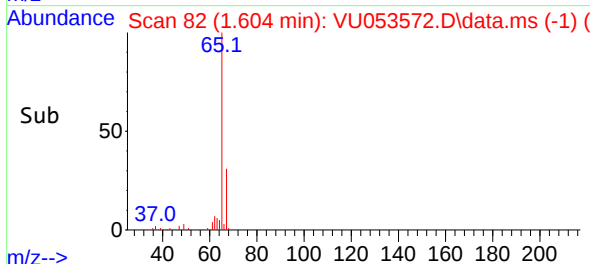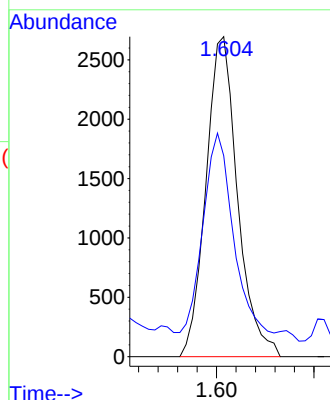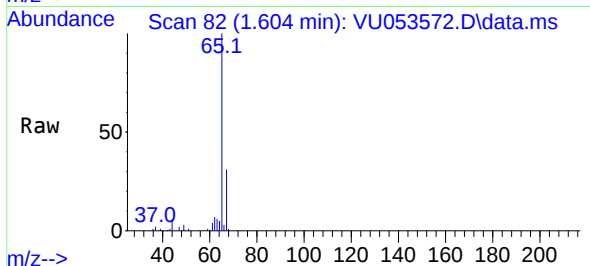

#10
 1,1,2-Trichloro-1,2,2-trifluoroethane
 Concen: 0.838 ug/L
 RT: 2.568 min Scan# 382
 Delta R.T. -0.010 min
 Lab File: VU053572.D
 Acq: 04 Apr 2023 19:30

Tgt Ion: 101 Resp: 1559
 Ion Ratio Lower Upper
 101 100
 85 25.1 32.6 48.8#
 151 45.0 65.8 98.6#

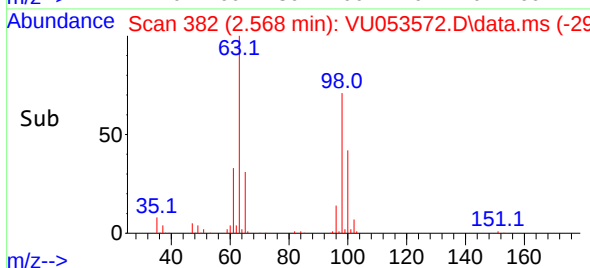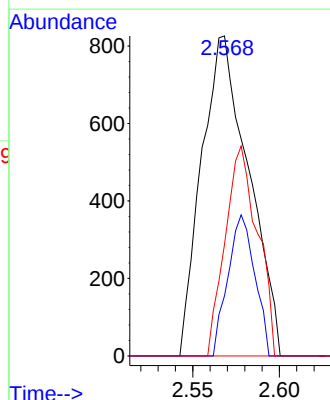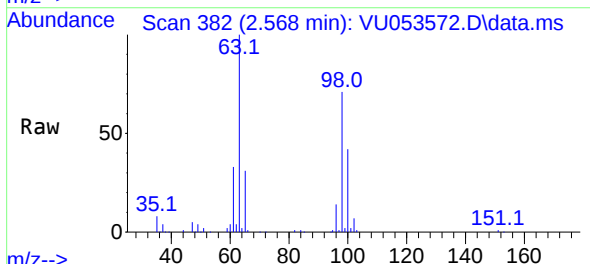

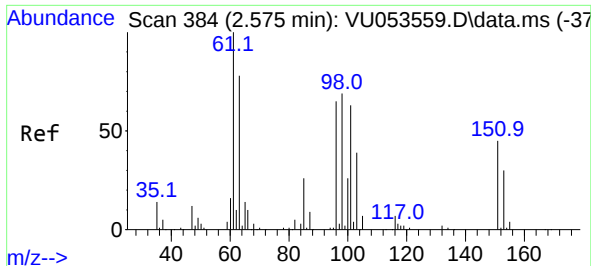

#12

1,1-Dichloroethene

Concen: 10.018 ug/L

RT: 2.575 min Scan# 384

Delta R.T. -0.003 min

Lab File: VU053572.D

Acq: 04 Apr 2023 19:30

Instrument :

MSVOA_U

ClientSampleId :

PMW-2(20230330)DL





Tgt Ion: 96 Resp: 16603

Ion Ratio Lower Upper

96 100

61 182.2 107.9 200.5

63 349.9 79.1 146.9#

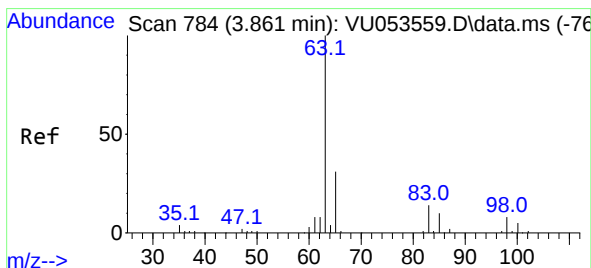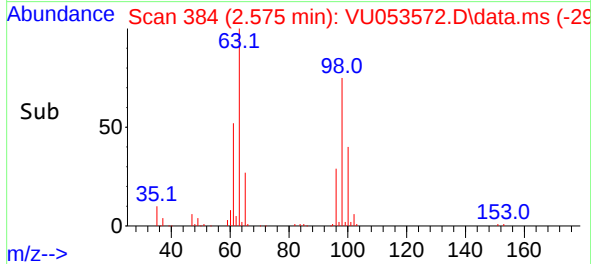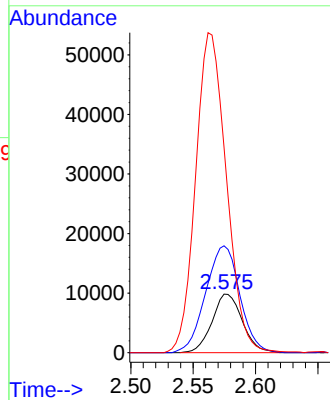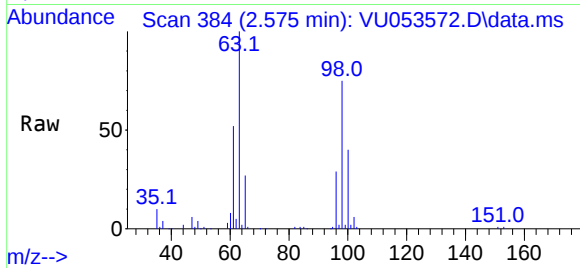

#19

1,1-Dichloroethane

Concen: 82.563 ug/L

RT: 3.864 min Scan# 785

Delta R.T. 0.000 min

Lab File: VU053572.D

Acq: 04 Apr 2023 19:30




Tgt Ion: 63 Resp: 227796


Ion Ratio Lower Upper

63 100

65 31.8 22.0 41.0

83 14.3 10.8 20.0


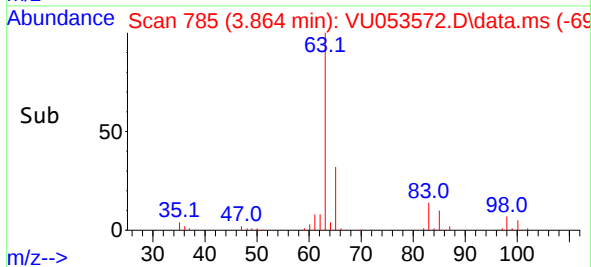
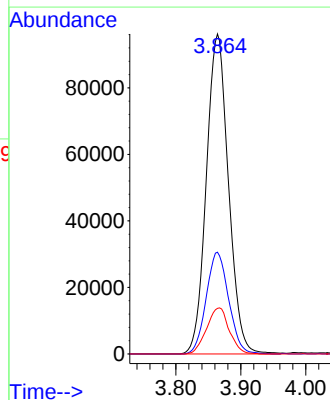
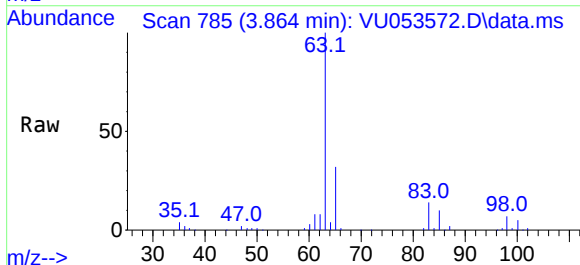


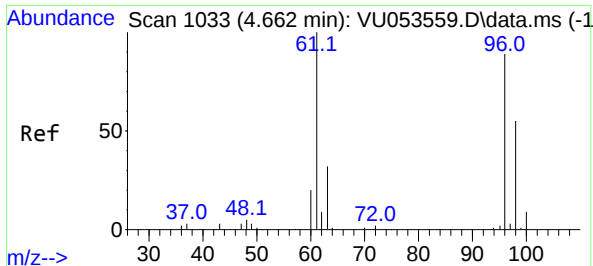

cis-1,2-Dichloroethene
 Concen: 13.558 ug/L
 RT: 4.665 min Scan# 1033
 Delta R.T. 0.003 min
 Lab File: VU053572.D
 Acq: 04 Apr 2023 19:30




Instrument :
 MSVOA_U
 ClientSampleId :
 PMW-2(20230330)DL


Tgt Ion:	96	Resp:	26083
Ion	Ratio	Lower	Upper
96	100		
61	114.2	74.7	138.7
68	0.0	0.0	0.0

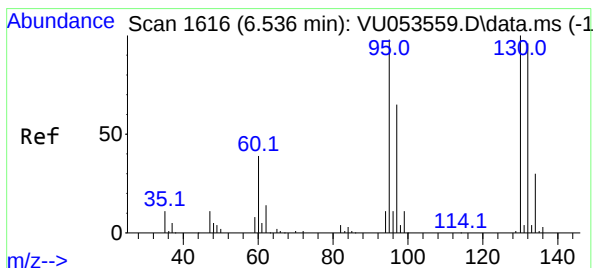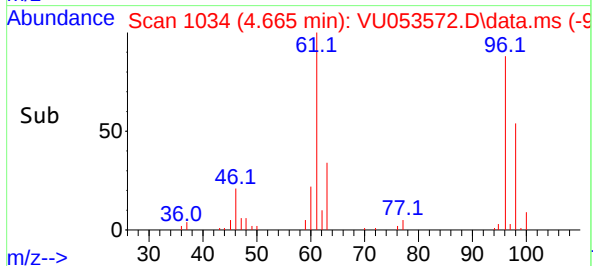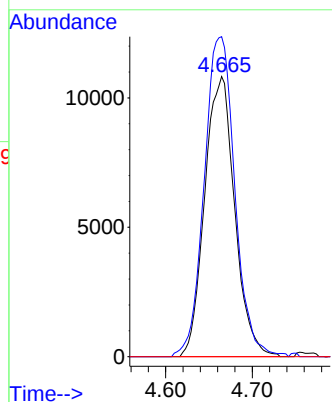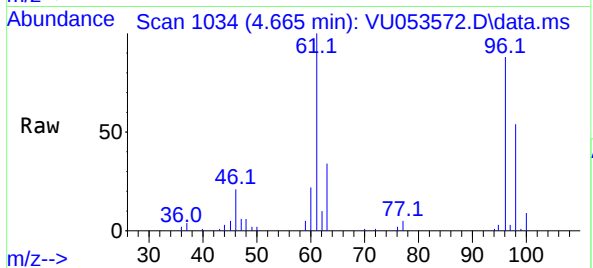

Trichloroethene
 Concen: 20.053 ug/L
 RT: 6.539 min Scan# 1617
 Delta R.T. 0.003 min
 Lab File: VU053572.D
 Acq: 04 Apr 2023 19:30

Tgt Ion:	95	Resp:	39950
Ion	Ratio	Lower	Upper
95	100		
97	64.9	45.1	83.7
132	93.0	74.1	137.5
130	103.8	73.5	136.5

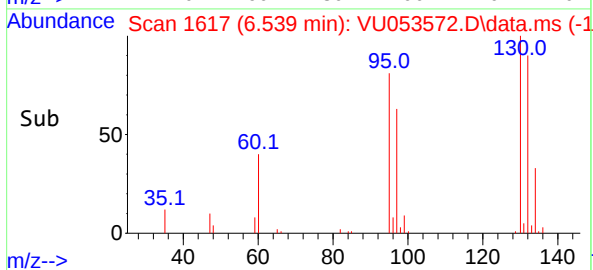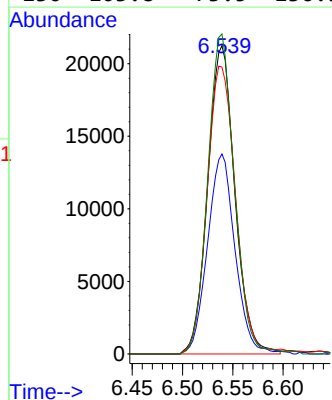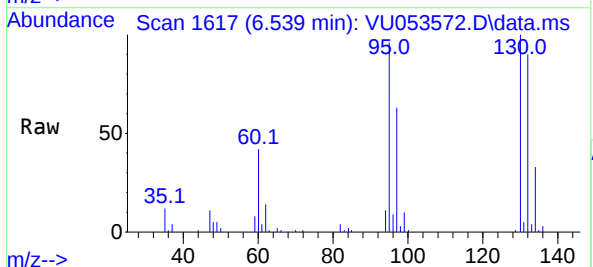




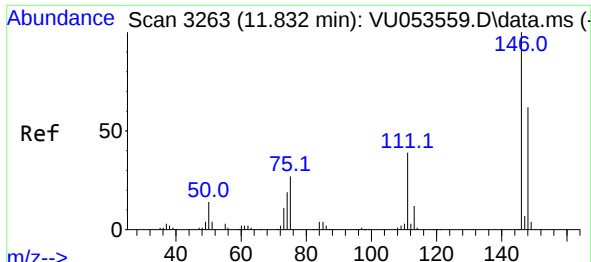


#65
1,4-Dichlorobenzene
Concen: 3.381 ug/L
RT: 11.835 min Scan# 31
Delta R.T. 0.003 min
Lab File: VU053572.D
Acq: 04 Apr 2023 19:30

Instrument :
MSVOA_U
ClientSampleId :
PMW-2(20230330)DL

Tgt Ion:146 Resp: 13627

Ion	Ratio	Lower	Upper
146	100		
111	42.5	25.1	46.5
148	62.8	44.3	82.3

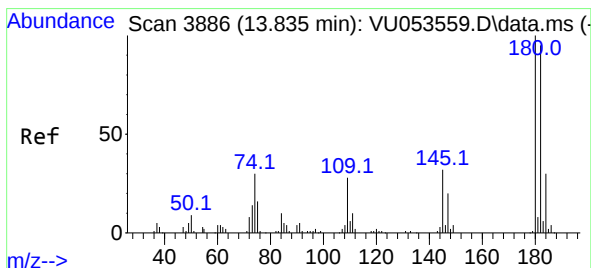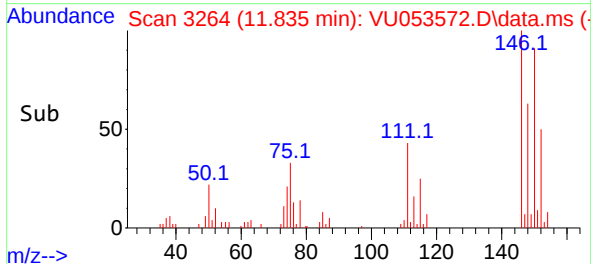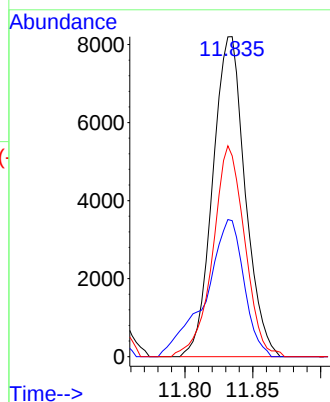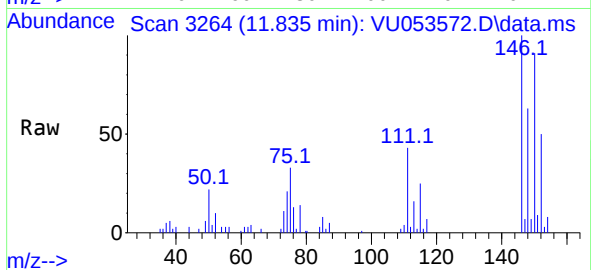

#70
1,2,4-trichlorobenzene
Concen: 2.067 ug/L
RT: 13.841 min Scan# 3888
Delta R.T. 0.006 min
Lab File: VU053572.D
Acq: 04 Apr 2023 19:30

Tgt Ion:180 Resp: 5612

Ion	Ratio	Lower	Upper
180	100		
182	90.5	75.8	113.8
145	28.2	23.4	35.2

