

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040423\
 Data File : VU053552.D
 Acq On : 04 Apr 2023 11:15
 Operator : JC/MD
 Sample : VU0404WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK066

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

Signal : TIC: VU053552.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	97	rVB	119308	135752	15.49%	1.947%
2	1.909	169	177	195	rVB	98210	132057	15.07%	1.894%
3	2.562	368	380	399	rBV	177634	293780	33.52%	4.213%
4	2.777	443	447	448	rBV	745	527	0.06%	0.008%
5	2.919	488	491	496	rBV	334	240	0.03%	0.003%
6	3.038	522	528	538	rVV3	1008	1703	0.19%	0.024%
7	3.083	538	542	546	rVB	294	258	0.03%	0.004%
8	3.247	590	593	597	rBV	284	202	0.02%	0.003%
9	3.356	620	627	636	rBV5	655	1009	0.12%	0.014%
10	3.436	650	652	656	rVV2	202	140	0.02%	0.002%
11	3.485	663	667	672	rBV	260	228	0.03%	0.003%
12	3.539	679	684	689	rBV2	236	242	0.03%	0.003%
13	3.870	785	787	791	rBV	260	150	0.02%	0.002%
14	4.012	826	831	834	rBV	242	222	0.03%	0.003%
15	4.240	899	902	905	rBV2	235	163	0.02%	0.002%
16	4.304	918	922	925	rBV2	251	212	0.02%	0.003%
17	4.481	973	977	981	rBV	340	264	0.03%	0.004%
18	4.616	1006	1019	1049	rBV	75333	183930	20.99%	2.638%
19	4.922	1111	1114	1118	rBV2	216	189	0.02%	0.003%
20	5.057	1140	1156	1177	rBV	159136	359643	41.03%	5.158%
21	5.247	1213	1215	1220	rVB2	372	224	0.03%	0.003%
22	5.317	1233	1237	1240	rBV	262	187	0.02%	0.003%
23	5.401	1258	1263	1266	rVB2	243	223	0.03%	0.003%
24	5.485	1282	1289	1293	rBV	198	234	0.03%	0.003%
25	5.517	1296	1299	1305	rVB	367	252	0.03%	0.004%
26	5.581	1316	1319	1323	rBV2	195	177	0.02%	0.003%
27	5.645	1333	1339	1341	rBV	264	181	0.02%	0.003%
28	5.719	1341	1362	1389	rBV2	320251	876467	100.00%	12.570%
29	5.980	1438	1443	1447	rBV2	280	266	0.03%	0.004%
30	6.009	1447	1452	1454	rVV2	311	209	0.02%	0.003%
31	6.047	1462	1464	1471	rBV	260	194	0.02%	0.003%
32	6.243	1511	1525	1551	rBV	295313	562636	64.19%	8.069%
33	6.472	1593	1596	1602	rVB2	209	148	0.02%	0.002%
34	6.533	1603	1615	1625	rVB6	5608	10827	1.24%	0.155%
35	6.591	1627	1633	1637	rBV2	311	266	0.03%	0.004%
36	6.629	1642	1645	1649	rBV	220	151	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040423\
 Data File : VU053552.D
 Acq On : 04 Apr 2023 11:15
 Operator : JC/MD
 Sample : VU0404WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK066

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

37	6.684	1649	1662	1680	rBV	199733	393526	44.90%	5.644%
38	7.102	1787	1792	1793	rBV	198	144	0.02%	0.002%
39	7.192	1812	1820	1827	rBV3	626	936	0.11%	0.013%
40	7.259	1835	1841	1843	rBV	127	133	0.02%	0.002%
41	7.388	1875	1881	1884	rBV	125	150	0.02%	0.002%
42	7.494	1912	1914	1918	rBV2	255	160	0.02%	0.002%
43	7.562	1923	1935	1953	rBV	115230	201678	23.01%	2.892%
44	7.681	1966	1972	1974	rBV2	341	264	0.03%	0.004%
45	7.697	1974	1977	1983	rVB2	634	501	0.06%	0.007%
46	7.742	1986	1991	1993	rVV	181	200	0.02%	0.003%
47	7.761	1994	1997	2002	rVV2	394	295	0.03%	0.004%
48	7.787	2002	2005	2012	rVV3	385	402	0.05%	0.006%
49	7.893	2024	2038	2057	rBV	408517	710598	81.08%	10.191%
50	8.176	2113	2126	2147	rBV	79577	136217	15.54%	1.954%
51	8.279	2156	2158	2161	rBV2	201	155	0.02%	0.002%
52	8.340	2172	2177	2180	rVB2	283	269	0.03%	0.004%
53	8.369	2183	2186	2189	rBV	302	167	0.02%	0.002%
54	8.410	2195	2199	2201	rBV	268	199	0.02%	0.003%
55	8.465	2213	2216	2221	rVB3	369	296	0.03%	0.004%
56	8.552	2235	2243	2249	rBV4	2765	4349	0.50%	0.062%
57	8.626	2255	2266	2294	rBV	219429	397956	45.40%	5.707%
58	8.928	2355	2360	2362	rBV3	343	273	0.03%	0.004%
59	9.005	2378	2384	2387	rBV2	300	281	0.03%	0.004%
60	9.063	2399	2402	2406	rVV2	161	130	0.01%	0.002%
61	9.127	2418	2422	2427	rVB	279	190	0.02%	0.003%
62	9.153	2427	2430	2432	rBV	241	178	0.02%	0.003%
63	9.324	2480	2483	2486	rBV	239	170	0.02%	0.002%
64	9.414	2497	2511	2532	rBV	400346	663723	75.73%	9.519%
65	9.610	2570	2572	2576	rVB2	379	221	0.03%	0.003%
66	9.693	2591	2598	2606	rVB3	1138	1691	0.19%	0.024%
67	9.896	2657	2661	2664	rBV	287	207	0.02%	0.003%
68	10.008	2693	2696	2700	rVB	172	150	0.02%	0.002%
69	10.111	2717	2728	2729	rBV3	1065	1463	0.17%	0.021%
70	10.192	2750	2753	2756	rVV	301	157	0.02%	0.002%
71	10.211	2756	2759	2762	rVV	192	135	0.02%	0.002%
72	10.385	2808	2813	2815	rBV	150	143	0.02%	0.002%
73	10.484	2836	2844	2852	rVB3	967	1432	0.16%	0.021%
74	10.581	2871	2874	2876	rBV	356	133	0.02%	0.002%
75	10.635	2886	2891	2899	rVB4	860	1148	0.13%	0.016%
76	10.709	2910	2914	2915	rBV	235	161	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040423\
 Data File : VU053552.D
 Acq On : 04 Apr 2023 11:15
 Operator : JC/MD
 Sample : VU0404WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK066

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

77	10.751	2915	2927	2943	rVV	287610	464768	53.03%	6.666%
78	10.870	2960	2964	2967	rVB	231	139	0.02%	0.002%
79	10.944	2984	2987	2991	rBV2	256	207	0.02%	0.003%
80	11.005	3003	3006	3010	rBV2	219	216	0.02%	0.003%
81	11.024	3010	3012	3018	rVV	221	147	0.02%	0.002%
82	11.317	3100	3103	3106	rVB2	272	173	0.02%	0.002%
83	11.468	3143	3150	3159	rBV5	1130	1687	0.19%	0.024%
84	11.658	3207	3209	3213	rVB2	333	229	0.03%	0.003%
85	11.748	3229	3237	3244	rBV3	3593	5020	0.57%	0.072%
86	11.806	3244	3255	3275	rBV	420768	682288	77.85%	9.785%
87	11.992	3310	3313	3317	rBV2	274	256	0.03%	0.004%
88	12.188	3361	3374	3390	rBV	420537	678804	77.45%	9.735%
89	12.311	3409	3412	3416	rVB4	438	324	0.04%	0.005%
90	12.410	3440	3443	3446	rBV	375	181	0.02%	0.003%
91	12.526	3475	3479	3482	rBV2	509	409	0.05%	0.006%
92	13.034	3634	3637	3639	rBV2	289	213	0.02%	0.003%
93	13.114	3658	3662	3668	rVB2	312	355	0.04%	0.005%
94	13.166	3675	3678	3684	rBV2	307	365	0.04%	0.005%
95	13.221	3689	3695	3706	rVV4	2415	3436	0.39%	0.049%
96	13.381	3742	3745	3747	rBV	268	148	0.02%	0.002%
97	13.690	3838	3841	3842	rBV	294	198	0.02%	0.003%
98	13.841	3878	3888	3899	rBV2	16850	26107	2.98%	0.374%
99	14.092	3958	3966	3977	rVB2	7814	12372	1.41%	0.177%
100	14.330	4032	4040	4051	rVB4	6637	10379	1.18%	0.149%




Sum of corrected areas: 6972555

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040423\
Data File : VU053552.D
Acq On : 04 Apr 2023 11:15
Operator : JC/MD
Sample : VU0404WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK066

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

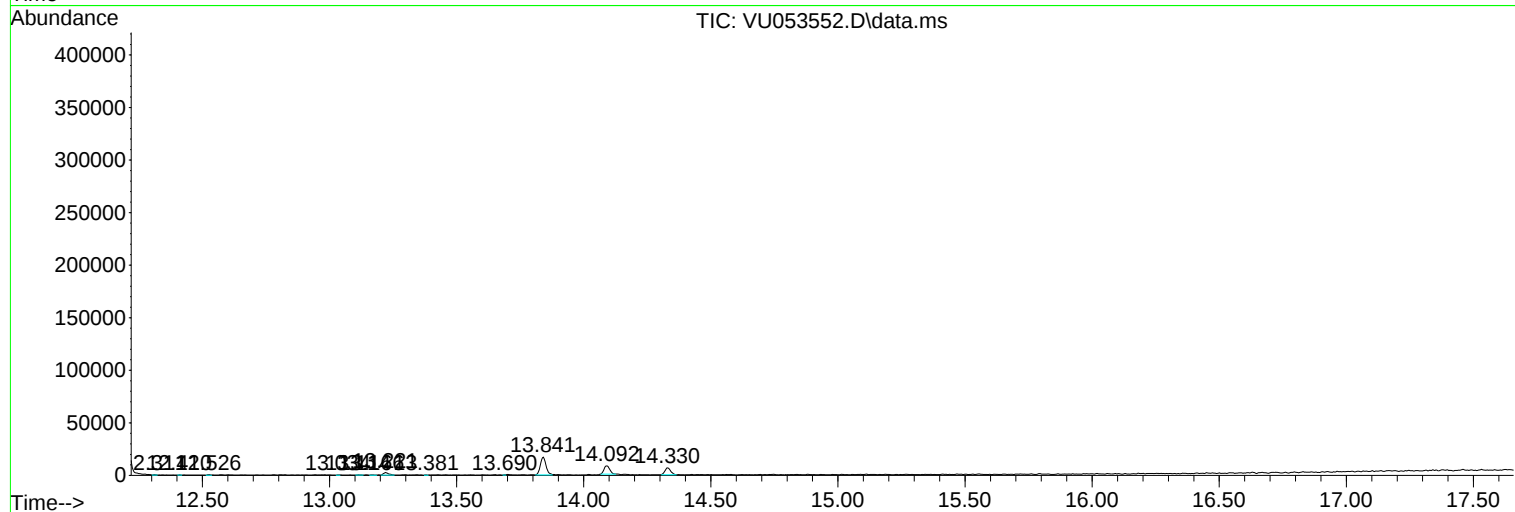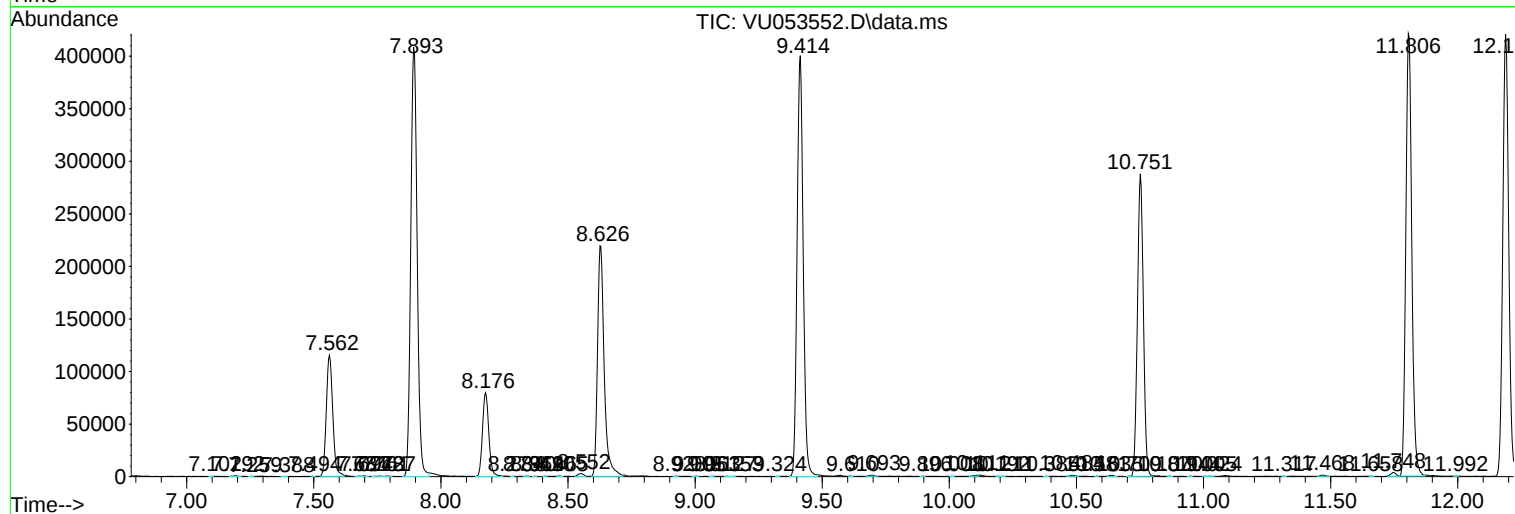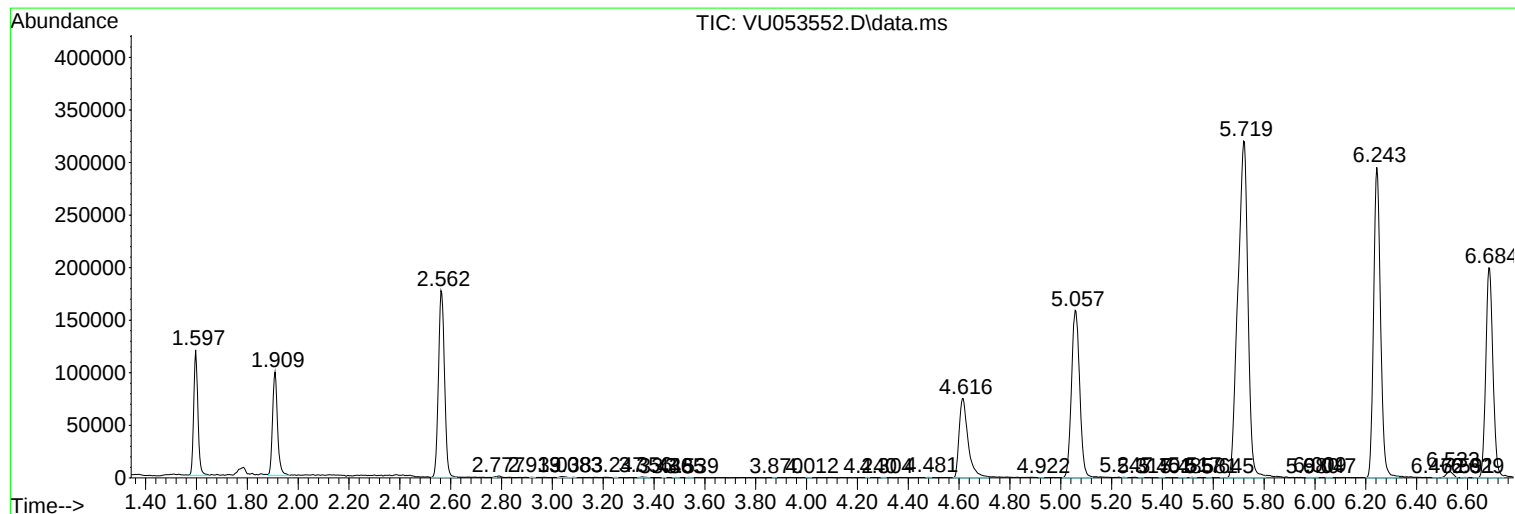

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040423\
Data File : VU053552.D
Acq On : 04 Apr 2023 11:15
Operator : JC/MD
Sample : VU0404WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK066

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040423\
Data File : VU053552.D
Acq On : 04 Apr 2023 11:15
Operator : JC/MD
Sample : VU0404WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK066

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------