

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040423\
 Data File : VU053553.D
 Acq On : 04 Apr 2023 11:46
 Operator : JC/MD
 Sample : 02158-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 PMW-10(20230329)

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

Signal : TIC: VU053553.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	96	rVB	112277	126526	15.20%	1.880%
2	1.912	170	178	194	rVB	91450	126115	15.16%	1.874%
3	2.565	369	381	396	rBV	172543	278562	33.47%	4.140%
4	3.173	563	570	582	rVB4	1911	3481	0.42%	0.052%
5	3.301	608	610	612	rBV	217	71	0.01%	0.001%
6	3.565	689	692	696	rBV2	190	163	0.02%	0.002%
7	3.864	771	785	802	rBV3	13991	32827	3.94%	0.488%
8	3.986	811	823	835	rBV5	2375	5262	0.63%	0.078%
9	4.063	844	847	850	rBV2	275	212	0.03%	0.003%
10	4.237	898	901	903	rVB	236	121	0.01%	0.002%
11	4.330	928	930	934	rBV	163	108	0.01%	0.002%
12	4.382	943	946	947	rBV	132	54	0.01%	0.001%
13	4.481	973	977	981	rBV	218	231	0.03%	0.003%
14	4.613	1006	1018	1048	rBV	71372	169361	20.35%	2.517%
15	5.060	1141	1157	1176	rBV	158821	351007	42.18%	5.216%
16	5.276	1222	1224	1226	rBV	159	86	0.01%	0.001%
17	5.314	1233	1236	1242	rBV2	188	230	0.03%	0.003%
18	5.504	1293	1295	1297	rBV	193	116	0.01%	0.002%
19	5.723	1341	1363	1386	rBV3	303679	832150	100.00%	12.367%
20	5.906	1418	1420	1423	rVV	339	141	0.02%	0.002%
21	5.941	1427	1431	1434	rBV2	279	265	0.03%	0.004%
22	5.999	1447	1449	1450	rBV2	264	107	0.01%	0.002%
23	6.044	1461	1463	1466	rVB2	167	96	0.01%	0.001%
24	6.089	1476	1477	1479	rBV2	108	43	0.01%	0.001%
25	6.118	1483	1486	1488	rBV	295	195	0.02%	0.003%
26	6.247	1511	1526	1544	rBV	278536	530686	63.77%	7.887%
27	6.530	1605	1614	1628	rVB10	4406	8244	0.99%	0.123%
28	6.620	1639	1642	1643	rBV	250	137	0.02%	0.002%
29	6.687	1650	1663	1687	rBV	192070	373194	44.85%	5.546%
30	6.964	1740	1749	1762	rVB2	6078	11717	1.41%	0.174%
31	7.015	1763	1765	1766	rVV2	167	56	0.01%	0.001%
32	7.028	1767	1769	1778	rVB2	365	282	0.03%	0.004%
33	7.124	1795	1799	1802	rVB2	226	196	0.02%	0.003%
34	7.343	1864	1867	1870	rVB	192	108	0.01%	0.002%
35	7.562	1923	1935	1961	rBV	108060	192347	23.11%	2.859%
36	7.777	1999	2002	2005	rBV	337	256	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040423\
 Data File : VU053553.D
 Acq On : 04 Apr 2023 11:46
 Operator : JC/MD
 Sample : 02158-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 PMW-10(20230329)

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

37	7.803	2005	2010	2014	rVV	398	407	0.05%	0.006%
38	7.896	2025	2039	2059	rBV	391265	687718	82.64%	10.220%
39	8.176	2114	2126	2149	rBV	78720	130038	15.63%	1.933%
40	8.349	2179	2180	2181	rBV	155	32	0.00%	0.000%
41	8.362	2181	2184	2187	rBV	229	174	0.02%	0.003%
42	8.423	2200	2203	2205	rBV	180	119	0.01%	0.002%
43	8.449	2209	2211	2213	rVV	157	51	0.01%	0.001%
44	8.549	2237	2242	2254	rVB6	1444	2187	0.26%	0.033%
45	8.591	2254	2255	2256	rBV	181	41	0.00%	0.001%
46	8.629	2256	2267	2301	rBV	205205	381043	45.79%	5.663%
47	8.864	2337	2340	2341	rBV	158	74	0.01%	0.001%
48	9.099	2411	2413	2415	rBV	179	105	0.01%	0.002%
49	9.362	2492	2495	2498	rBV	223	157	0.02%	0.002%
50	9.414	2498	2511	2532	rBV	380901	633144	76.09%	9.409%
51	9.571	2554	2560	2563	rBV2	600	637	0.08%	0.009%
52	9.600	2567	2569	2572	rBV	191	106	0.01%	0.002%
53	10.433	2825	2828	2831	rBV2	285	188	0.02%	0.003%
54	10.645	2887	2894	2898	rBV3	412	385	0.05%	0.006%
55	10.751	2915	2927	2946	rBV	283253	450656	54.16%	6.697%
56	10.967	2992	2994	2995	rBV	174	57	0.01%	0.001%
57	11.230	3073	3076	3079	rBV	291	173	0.02%	0.003%
58	11.404	3128	3130	3131	rBV	240	69	0.01%	0.001%
59	11.446	3138	3143	3145	rBV	279	223	0.03%	0.003%
60	11.468	3145	3150	3155	rBV3	763	859	0.10%	0.013%
61	11.526	3165	3168	3170	rBV	266	155	0.02%	0.002%
62	11.745	3230	3236	3244	rBV5	2550	3626	0.44%	0.054%
63	11.809	3244	3256	3277	rBV	406391	663460	79.73%	9.860%
64	12.008	3316	3318	3321	rBV	253	156	0.02%	0.002%
65	12.060	3331	3334	3335	rBV	206	106	0.01%	0.002%
66	12.188	3362	3374	3395	rBV	412320	663719	79.76%	9.864%
67	12.359	3423	3427	3430	rVB2	312	216	0.03%	0.003%
68	12.912	3597	3599	3601	rBV	155	60	0.01%	0.001%
69	13.018	3630	3632	3636	rBV	297	233	0.03%	0.003%
70	13.227	3691	3697	3705	rVB3	1162	1571	0.19%	0.023%
71	13.645	3825	3827	3828	rBV	302	125	0.02%	0.002%
72	13.764	3862	3864	3865	rVB	434	110	0.01%	0.002%
73	13.780	3865	3869	3873	rBV2	452	361	0.04%	0.005%
74	13.841	3878	3888	3901	rBV3	26868	44486	5.35%	0.661%
75	14.041	3946	3950	3951	rBV3	1452	1049	0.13%	0.016%
76	14.092	3959	3966	3975	rBV6	5354	8179	0.98%	0.122%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040423\
Data File : VU053553.D
Acq On : 04 Apr 2023 11:46
Operator : JC/MD
Sample : 02158-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PMW-10(20230329)

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Title : VOC Analysis

77	14.327	4034	4039	4048	rVB6	5347	7320	0.88%	0.109%
78	14.520	4096	4099	4101	rBV4	859	539	0.06%	0.008%




Sum of corrected areas: 6728867

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040423\
Data File : VU053553.D
Acq On : 04 Apr 2023 11:46
Operator : JC/MD
Sample : 02158-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PMW-10(20230329)

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

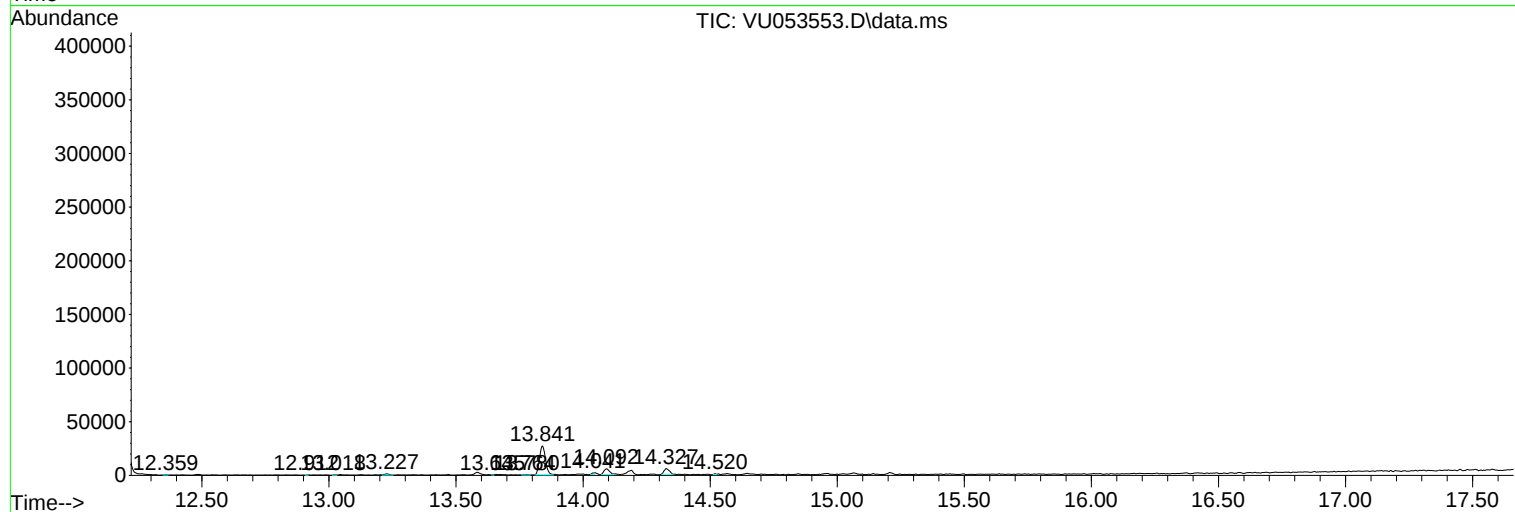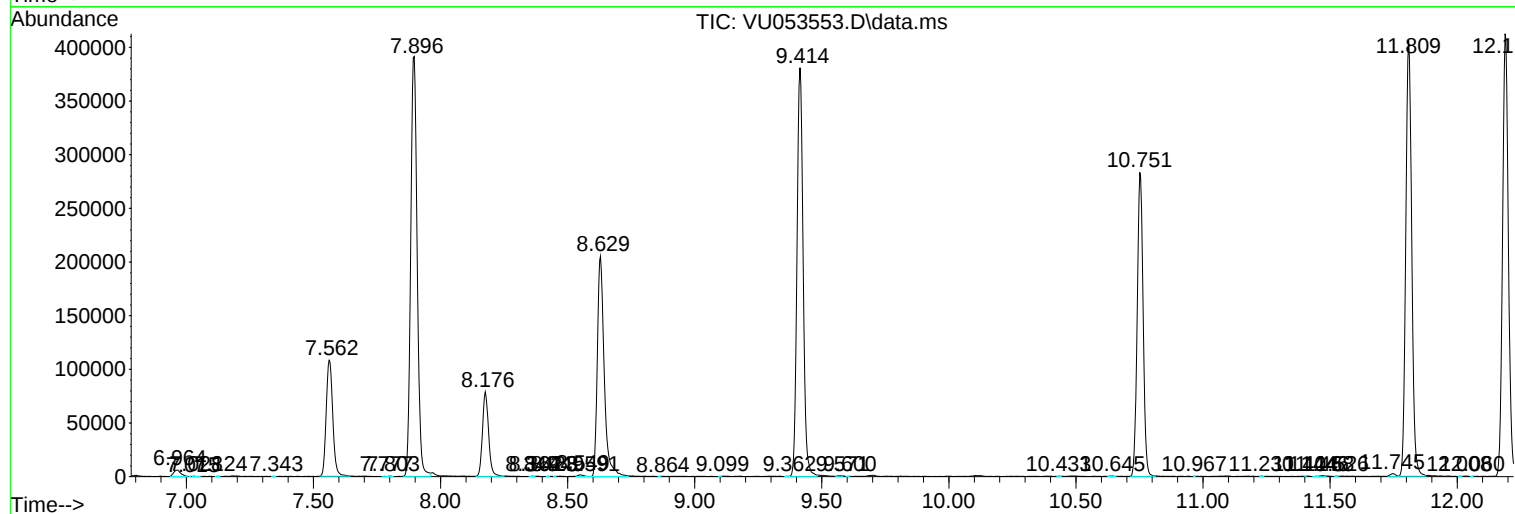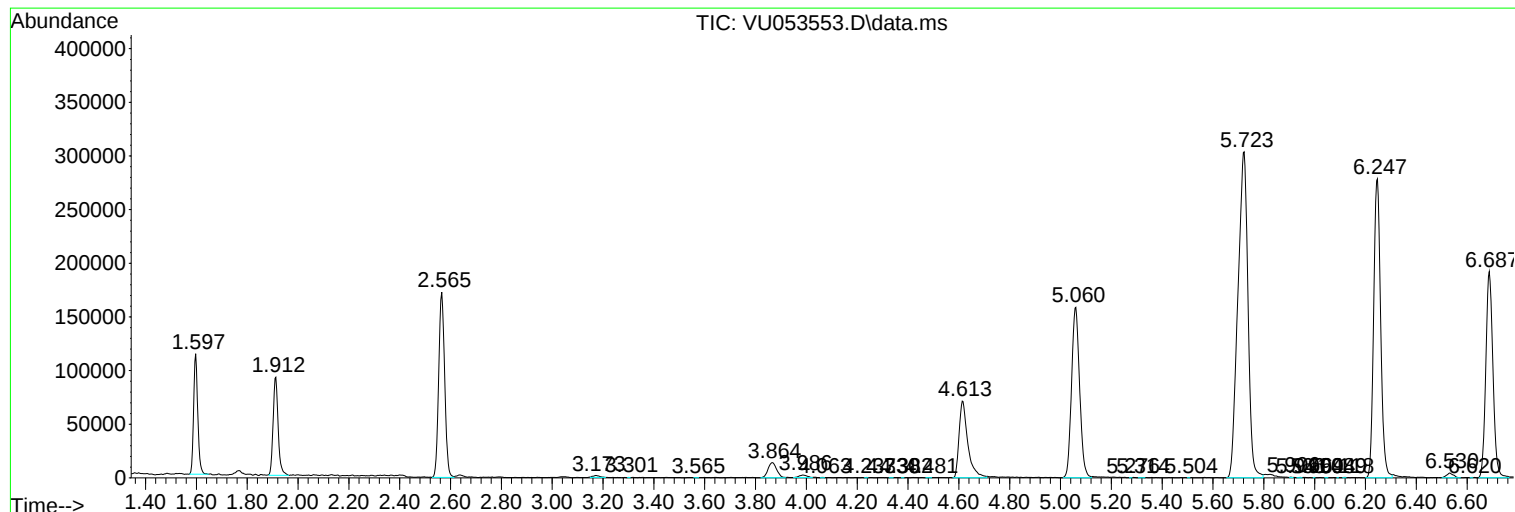

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040423\
Data File : VU053553.D
Acq On : 04 Apr 2023 11:46
Operator : JC/MD
Sample : 02158-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PMW-10(20230329)

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040423\
Data File : VU053553.D
Acq On : 04 Apr 2023 11:46
Operator : JC/MD
Sample : 02158-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PMW-10(20230329)

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------