

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040423\
 Data File : VU053554.D
 Acq On : 04 Apr 2023 12:10
 Operator : JC/MD
 Sample : 02158-01RE
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 PMW-7S(20230329)RE

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M

Title : VOC Analysis

Signal : TIC: VU053554.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	95	rVB	126658	144753	4.82%	1.430%
2	1.912	170	178	194	rVB	94153	129449	4.31%	1.279%
3	2.565	369	381	395	rBV	180040	295534	9.85%	2.920%
4	2.723	427	430	432	rBV2	306	270	0.01%	0.003%
5	2.742	432	436	438	rBV	614	543	0.02%	0.005%
6	2.890	479	482	484	rBV2	251	153	0.01%	0.002%
7	2.973	506	508	513	rVB2	347	234	0.01%	0.002%
8	3.044	520	530	537	rBV4	1383	2563	0.09%	0.025%
9	3.157	563	565	566	rBV	439	174	0.01%	0.002%
10	3.350	614	625	644	rBV2	19129	37937	1.26%	0.375%
11	3.581	694	697	699	rVB	279	168	0.01%	0.002%
12	3.626	703	711	713	rBV2	240	366	0.01%	0.004%
13	3.800	763	765	769	rBV2	243	227	0.01%	0.002%
14	3.867	771	786	803	rVB	22986	52572	1.75%	0.519%
15	3.967	811	817	818	rBV2	599	538	0.02%	0.005%
16	4.067	844	848	854	rBV2	311	305	0.01%	0.003%
17	4.182	880	884	888	rBV2	296	341	0.01%	0.003%
18	4.240	899	902	908	rVB2	205	210	0.01%	0.002%
19	4.375	941	944	948	rVB2	242	167	0.01%	0.002%
20	4.398	948	951	957	rBV	349	298	0.01%	0.003%
21	4.523	986	990	995	rVB2	365	249	0.01%	0.002%
22	4.613	1006	1018	1024	rBV	77340	153218	5.10%	1.514%
23	4.931	1115	1117	1119	rBV	334	165	0.01%	0.002%
24	5.060	1138	1157	1179	rBV	162838	363111	12.10%	3.588%
25	5.282	1224	1226	1233	rVB2	377	329	0.01%	0.003%
26	5.382	1251	1257	1258	rBV	327	255	0.01%	0.003%
27	5.719	1340	1362	1399	rBV2	329826	922471	30.73%	9.116%
28	6.243	1508	1525	1545	rBV	250631	475994	15.86%	4.704%
29	6.533	1602	1615	1626	rVB9	4685	9712	0.32%	0.096%
30	6.687	1649	1663	1682	rBV	204841	400156	13.33%	3.954%
31	6.957	1741	1747	1748	rBV2	1222	941	0.03%	0.009%
32	7.012	1760	1764	1767	rVB2	373	232	0.01%	0.002%
33	7.041	1772	1773	1779	rVB	252	145	0.00%	0.001%
34	7.070	1779	1782	1786	rBV2	250	166	0.01%	0.002%
35	7.144	1800	1805	1807	rBV2	296	299	0.01%	0.003%
36	7.189	1813	1819	1820	rBV2	380	332	0.01%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040423\
 Data File : VU053554.D
 Acq On : 04 Apr 2023 12:10
 Operator : JC/MD
 Sample : 02158-01RE
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 PMW-7S(20230329)RE

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

37	7.285	1846	1849	1857	rBV	158	223	0.01%	0.002%
38	7.330	1861	1863	1867	rVV	186	171	0.01%	0.002%
39	7.349	1867	1869	1875	rVB2	288	194	0.01%	0.002%
40	7.513	1915	1920	1923	rBV	151	154	0.01%	0.002%
41	7.562	1923	1935	1960	rBV	116197	207153	6.90%	2.047%
42	7.764	1993	1998	2001	rBV2	218	151	0.01%	0.001%
43	7.848	2020	2024	2025	rBV2	234	141	0.00%	0.001%
44	7.893	2025	2038	2057	rBV	431767	741152	24.69%	7.324%
45	8.124	2104	2110	2113	rBV	172	190	0.01%	0.002%
46	8.176	2113	2126	2147	rBV2	81560	142189	4.74%	1.405%
47	8.365	2182	2185	2191	rVB	246	201	0.01%	0.002%
48	8.394	2191	2194	2196	rVB	233	145	0.00%	0.001%
49	8.420	2196	2202	2205	rBV	271	225	0.01%	0.002%
50	8.462	2211	2215	2218	rBV2	395	300	0.01%	0.003%
51	8.552	2236	2243	2249	rVB3	1797	2359	0.08%	0.023%
52	8.626	2255	2266	2297	rBV	218776	408114	13.60%	4.033%
53	8.957	2366	2369	2372	rVB	204	142	0.00%	0.001%
54	8.992	2372	2380	2383	rBV	306	254	0.01%	0.003%
55	9.131	2420	2423	2427	rBV	232	182	0.01%	0.002%
56	9.301	2473	2476	2481	rVB	355	241	0.01%	0.002%
57	9.414	2498	2511	2539	rBV2	351396	826309	27.53%	8.165%
58	9.565	2554	2558	2560	rBV3	910	825	0.03%	0.008%
59	9.671	2588	2591	2594	rBV2	451	330	0.01%	0.003%
60	9.687	2594	2596	2602	rVV3	658	620	0.02%	0.006%
61	9.725	2607	2608	2611	rVV	273	139	0.00%	0.001%
62	9.738	2611	2612	2616	rVB	278	144	0.00%	0.001%
63	10.105	2720	2726	2727	rBV2	615	547	0.02%	0.005%
64	10.304	2783	2788	2790	rBV	242	189	0.01%	0.002%
65	10.324	2791	2794	2796	rVB2	250	149	0.00%	0.001%
66	10.349	2796	2802	2808	rVB2	299	379	0.01%	0.004%
67	10.417	2820	2823	2825	rBV2	204	154	0.01%	0.002%
68	10.481	2838	2843	2845	rBV	540	547	0.02%	0.005%
69	10.639	2888	2892	2895	rBV3	265	216	0.01%	0.002%
70	10.664	2896	2900	2903	rVB2	341	244	0.01%	0.002%
71	10.751	2912	2927	2946	rBV	298496	479757	15.98%	4.741%
72	10.838	2953	2954	2958	rVB	292	165	0.01%	0.002%
73	11.089	3027	3032	3037	rBV2	428	511	0.02%	0.005%
74	11.185	3059	3062	3067	rVB2	256	195	0.01%	0.002%
75	11.298	3095	3097	3100	rVB2	331	173	0.01%	0.002%
76	11.414	3123	3133	3147	rBV2	42271	67482	2.25%	0.667%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040423\
 Data File : VU053554.D
 Acq On : 04 Apr 2023 12:10
 Operator : JC/MD
 Sample : 02158-01RE
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 PMW-7S(20230329)RE

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

77	11.552	3173	3176	3182	rVB	278	282	0.01%	0.003%
78	11.584	3182	3186	3190	rBV	272	196	0.01%	0.002%
79	11.684	3215	3217	3221	rBV	214	143	0.00%	0.001%
80	11.741	3223	3235	3245	rBV	276074	432967	14.42%	4.278%
81	11.832	3246	3263	3285	rVB2	1539546	3001702	100.00%	29.662%
82	12.092	3340	3344	3349	rBV2	328	349	0.01%	0.003%
83	12.188	3361	3374	3397	rBV	460895	771335	25.70%	7.622%
84	12.320	3413	3415	3417	rBV2	475	214	0.01%	0.002%
85	12.449	3452	3455	3460	rVB2	333	286	0.01%	0.003%
86	12.500	3466	3471	3474	rBV	233	261	0.01%	0.003%
87	12.706	3532	3535	3538	rBV	254	183	0.01%	0.002%
88	12.967	3613	3616	3621	rBB	236	176	0.01%	0.002%
89	13.111	3658	3661	3663	rBV2	323	165	0.01%	0.002%
90	13.221	3691	3695	3705	rVB2	729	1023	0.03%	0.010%
91	13.391	3743	3748	3753	rBV	426	374	0.01%	0.004%
92	13.417	3753	3756	3760	rVB	535	322	0.01%	0.003%
93	13.442	3760	3764	3768	rBV2	428	375	0.01%	0.004%
94	13.465	3768	3771	3773	rBV2	233	145	0.00%	0.001%
95	13.558	3796	3800	3802	rBV	414	324	0.01%	0.003%
96	13.658	3827	3831	3834	rBV2	298	270	0.01%	0.003%
97	13.841	3879	3888	3902	rVB4	14074	22280	0.74%	0.220%
98	14.092	3957	3966	3973	rBV4	2927	4472	0.15%	0.044%
99	14.182	3992	3994	4000	rVB2	673	391	0.01%	0.004%
100	14.333	4034	4041	4049	rBV5	2818	3973	0.13%	0.039%




Sum of corrected areas: 10119741

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040423\
Data File : VU053554.D
Acq On : 04 Apr 2023 12:10
Operator : JC/MD
Sample : 02158-01RE
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PMW-7S(20230329)RE

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

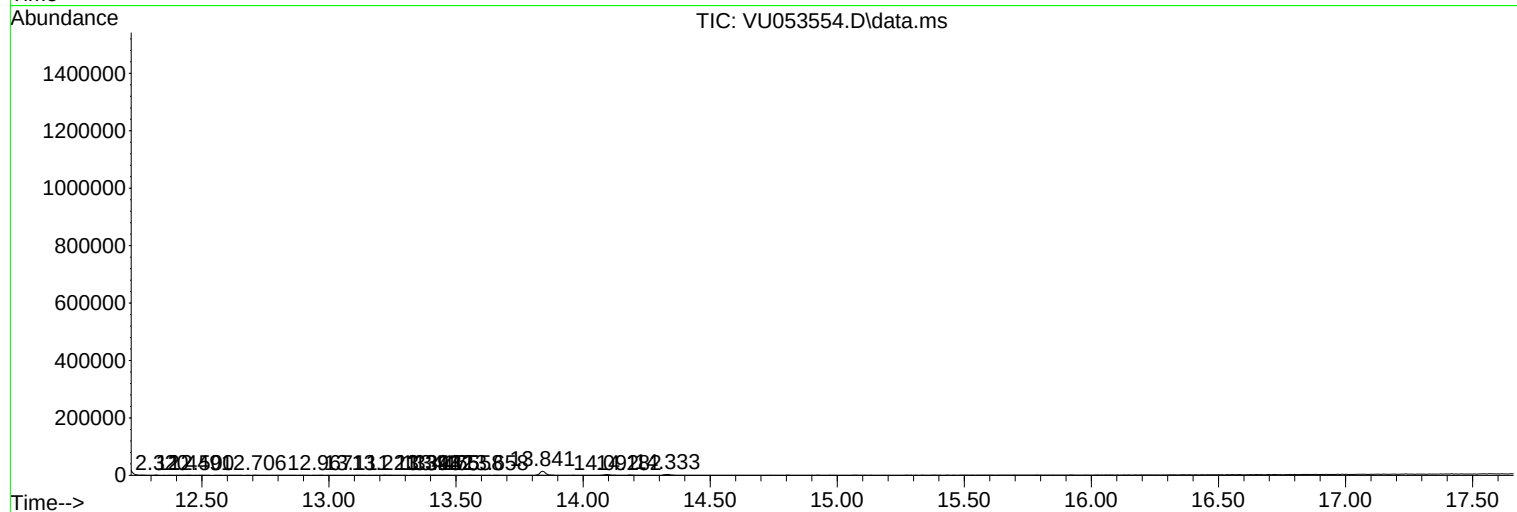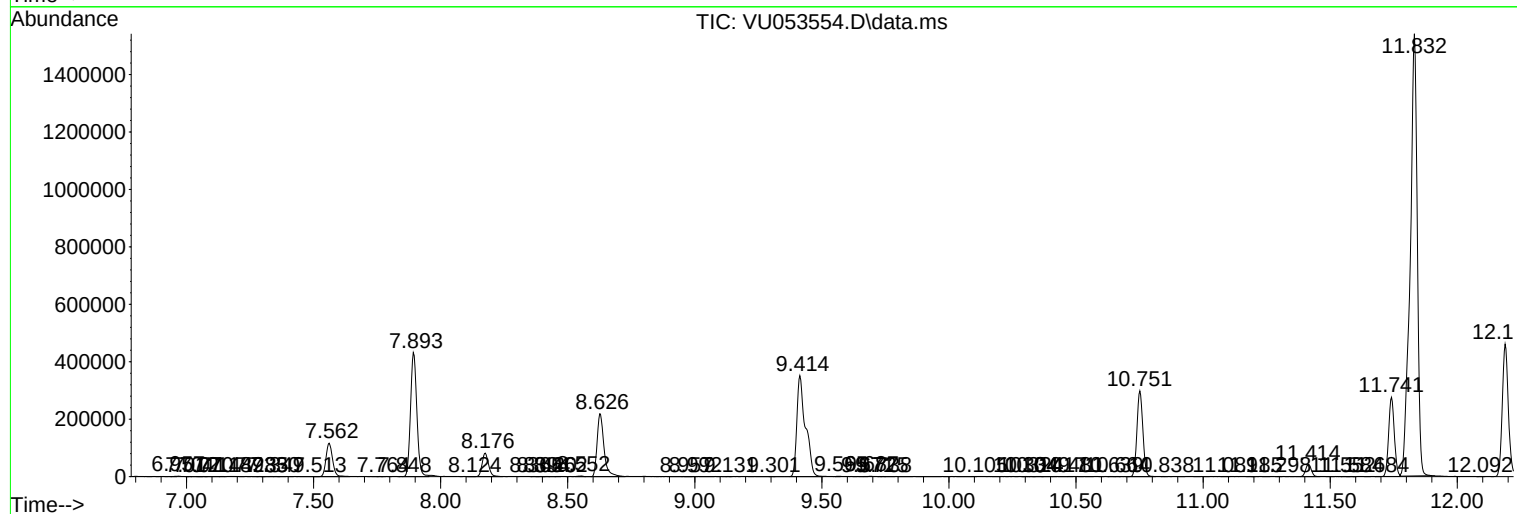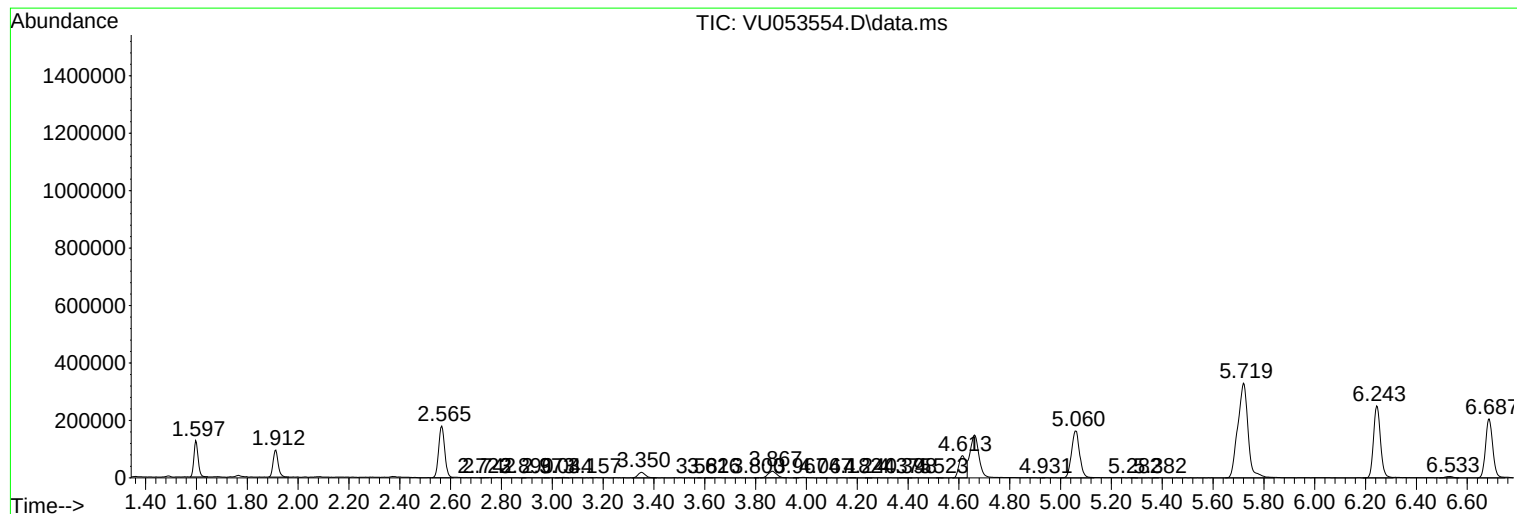

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040423\
Data File : VU053554.D
Acq On : 04 Apr 2023 12:10
Operator : JC/MD
Sample : 02158-01RE
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PMW-7S(20230329)RE

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040423\
Data File : VU053554.D
Acq On : 04 Apr 2023 12:10
Operator : JC/MD
Sample : 02158-01RE
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PMW-7S(20230329)RE

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------