

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040423\
 Data File : VU053555.D
 Acq On : 04 Apr 2023 12:32
 Operator : JC/MD
 Sample : 02158-08
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 PMW-4(20230329)

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

Signal : TIC: VU053555.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	89	rVB	114475	125665	12.46%	1.651%
2	1.909	169	177	197	rVB	93365	130255	12.92%	1.712%
3	2.562	369	380	392	rBV	174515	282491	28.01%	3.712%
4	2.684	415	418	419	rBV	552	277	0.03%	0.004%
5	2.742	433	436	439	rBV2	562	487	0.05%	0.006%
6	2.922	489	492	496	rVB	411	285	0.03%	0.004%
7	2.970	505	507	512	rBV2	285	258	0.03%	0.003%
8	3.041	524	529	536	rVB3	1038	1478	0.15%	0.019%
9	3.231	585	588	594	rBV2	317	362	0.04%	0.005%
10	3.289	603	606	608	rBV2	234	163	0.02%	0.002%
11	3.324	614	617	619	rBV	267	150	0.01%	0.002%
12	3.353	619	626	632	rVV4	1075	1405	0.14%	0.018%
13	3.539	680	684	686	rBV2	302	207	0.02%	0.003%
14	3.694	729	732	738	rBV2	225	236	0.02%	0.003%
15	4.022	831	834	836	rBV2	286	200	0.02%	0.003%
16	4.089	853	855	858	rBV	260	135	0.01%	0.002%
17	4.266	907	910	913	rBV	294	199	0.02%	0.003%
18	4.324	925	928	933	rVB2	275	218	0.02%	0.003%
19	4.456	966	969	972	rBV2	204	180	0.02%	0.002%
20	4.498	977	982	984	rBV	318	257	0.03%	0.003%
21	4.613	1006	1018	1046	rBV	70827	191395	18.98%	2.515%
22	5.057	1140	1156	1174	rBV	163063	355758	35.28%	4.675%
23	5.363	1246	1251	1255	rVV2	241	264	0.03%	0.003%
24	5.391	1259	1260	1267	rVB	267	230	0.02%	0.003%
25	5.424	1267	1270	1275	rVB	379	273	0.03%	0.004%
26	5.453	1275	1279	1281	rBV2	448	289	0.03%	0.004%
27	5.472	1281	1285	1290	rBV	246	268	0.03%	0.004%
28	5.510	1295	1297	1302	rVB2	257	195	0.02%	0.003%
29	5.591	1318	1322	1330	rVB2	559	531	0.05%	0.007%
30	5.719	1340	1362	1390	rBV2	309277	855610	84.85%	11.243%
31	6.035	1457	1460	1461	rBV	259	135	0.01%	0.002%
32	6.080	1468	1474	1478	rBV2	220	235	0.02%	0.003%
33	6.166	1492	1501	1505	rBV2	390	584	0.06%	0.008%
34	6.244	1511	1525	1551	rBV	304148	578347	57.36%	7.600%
35	6.462	1588	1593	1597	rBV2	362	409	0.04%	0.005%
36	6.536	1603	1616	1630	rVB8	7788	16515	1.64%	0.217%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040423\
 Data File : VU053555.D
 Acq On : 04 Apr 2023 12:32
 Operator : JC/MD
 Sample : 02158-08
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 PMW-4(20230329)

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

37	6.620	1638	1642	1646	rBV	227	185	0.02%	0.002%
38	6.684	1649	1662	1680	rBV	193524	378829	37.57%	4.978%
39	6.825	1704	1706	1710	rVV2	353	250	0.02%	0.003%
40	6.935	1737	1740	1745	rVB	225	156	0.02%	0.002%
41	7.047	1771	1775	1779	rBV	238	239	0.02%	0.003%
42	7.301	1851	1854	1858	rBV	197	161	0.02%	0.002%
43	7.465	1899	1905	1908	rBV2	247	299	0.03%	0.004%
44	7.562	1922	1935	1948	rBV	115139	198847	19.72%	2.613%
45	7.681	1969	1972	1973	rBV	491	211	0.02%	0.003%
46	7.710	1979	1981	1986	rBV2	200	143	0.01%	0.002%
47	7.803	2007	2010	2013	rVB2	459	242	0.02%	0.003%
48	7.893	2025	2038	2056	rBV	405461	707192	70.13%	9.293%
49	8.176	2115	2126	2145	rBV	80762	134381	13.33%	1.766%
50	8.459	2210	2214	2216	rBV	233	187	0.02%	0.002%
51	8.549	2236	2242	2249	rVB5	1889	2345	0.23%	0.031%
52	8.626	2255	2266	2292	rBV	218481	397784	39.45%	5.227%
53	8.755	2304	2306	2307	rBV	322	138	0.01%	0.002%
54	8.967	2370	2372	2375	rVB	227	133	0.01%	0.002%
55	9.034	2390	2393	2399	rVB	226	260	0.03%	0.003%
56	9.166	2431	2434	2440	rBV2	221	181	0.02%	0.002%
57	9.211	2444	2448	2453	rVB2	364	307	0.03%	0.004%
58	9.253	2458	2461	2464	rBV	207	175	0.02%	0.002%
59	9.308	2476	2478	2484	rVB2	290	188	0.02%	0.002%
60	9.414	2496	2511	2515	rBV	432314	716353	71.04%	9.413%
61	9.565	2554	2558	2567	rVB4	1282	1462	0.14%	0.019%
62	9.620	2572	2575	2581	rBV3	250	224	0.02%	0.003%
63	9.694	2592	2598	2600	rBV3	654	729	0.07%	0.010%
64	9.819	2633	2637	2638	rBV3	353	234	0.02%	0.003%
65	9.877	2652	2655	2659	rBV2	204	161	0.02%	0.002%
66	9.925	2667	2670	2675	rBV2	246	192	0.02%	0.003%
67	10.038	2701	2705	2707	rVB	210	149	0.01%	0.002%
68	10.092	2715	2722	2723	rBV2	561	505	0.05%	0.007%
69	10.266	2773	2776	2782	rVB	327	305	0.03%	0.004%
70	10.639	2889	2892	2895	rVB2	283	207	0.02%	0.003%
71	10.751	2914	2927	2947	rBV	294475	469025	46.51%	6.163%
72	10.893	2966	2971	2976	rBV	289	359	0.04%	0.005%
73	10.967	2990	2994	2998	rVB	293	172	0.02%	0.002%
74	10.989	2998	3001	3003	rBV2	220	169	0.02%	0.002%
75	11.041	3011	3017	3025	rBV2	296	542	0.05%	0.007%
76	11.124	3038	3043	3046	rBV	231	229	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040423\
 Data File : VU053555.D
 Acq On : 04 Apr 2023 12:32
 Operator : JC/MD
 Sample : 02158-08
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 PMW-4(20230329)

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

77	11.214	3068	3071	3073	rVV	265	145	0.01%	0.002%
78	11.420	3129	3135	3140	rBV2	477	558	0.06%	0.007%
79	11.443	3140	3142	3145	rVV2	266	160	0.02%	0.002%
80	11.465	3145	3149	3156	rVV3	716	709	0.07%	0.009%
81	11.513	3161	3164	3168	rBV	294	202	0.02%	0.003%
82	11.549	3172	3175	3179	rBV	306	258	0.03%	0.003%
83	11.665	3208	3211	3215	rBV	276	191	0.02%	0.003%
84	11.742	3224	3235	3244	rBV	85860	134411	13.33%	1.766%
85	11.809	3244	3256	3279	rVB2	479570	1008361	100.00%	13.250%
86	12.021	3319	3322	3325	rVB2	231	134	0.01%	0.002%
87	12.108	3344	3349	3351	rBV	305	211	0.02%	0.003%
88	12.121	3351	3353	3356	rVB	292	144	0.01%	0.002%
89	12.189	3360	3374	3398	rBV	442944	729510	72.35%	9.586%
90	12.803	3560	3565	3570	rBV2	318	346	0.03%	0.005%
91	12.938	3605	3607	3613	rBV2	310	248	0.02%	0.003%
92	13.214	3690	3693	3705	rVB7	2391	3449	0.34%	0.045%
93	13.320	3724	3726	3731	rBV	251	223	0.02%	0.003%
94	13.616	3815	3818	3823	rVB2	384	338	0.03%	0.004%
95	13.658	3825	3831	3836	rBV2	470	512	0.05%	0.007%
96	13.751	3856	3860	3863	rBV2	422	365	0.04%	0.005%
97	13.838	3876	3887	3904	rBV2	100267	158017	15.67%	2.076%
98	14.089	3961	3965	3971	rVB3	1970	2262	0.22%	0.030%
99	14.163	3985	3988	3991	rBV3	282	274	0.03%	0.004%
100	14.330	4031	4040	4049	rBV5	6216	9180	0.91%	0.121%




Sum of corrected areas: 7610004

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040423\
Data File : VU053555.D
Acq On : 04 Apr 2023 12:32
Operator : JC/MD
Sample : 02158-08
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PMW-4(20230329)

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

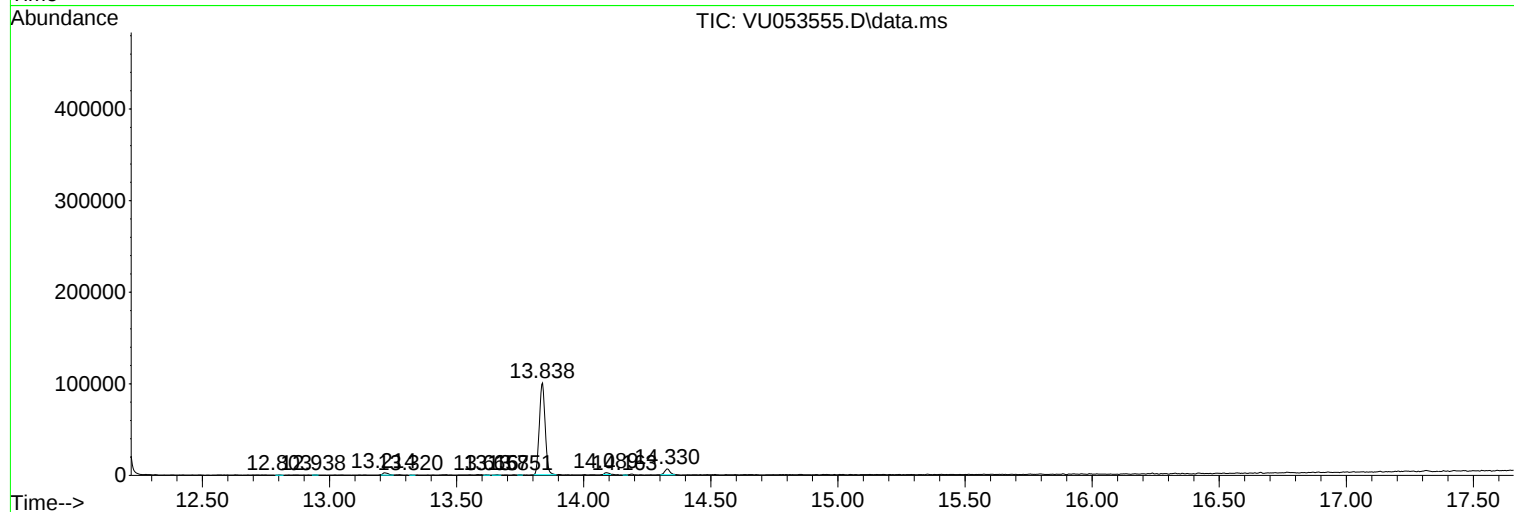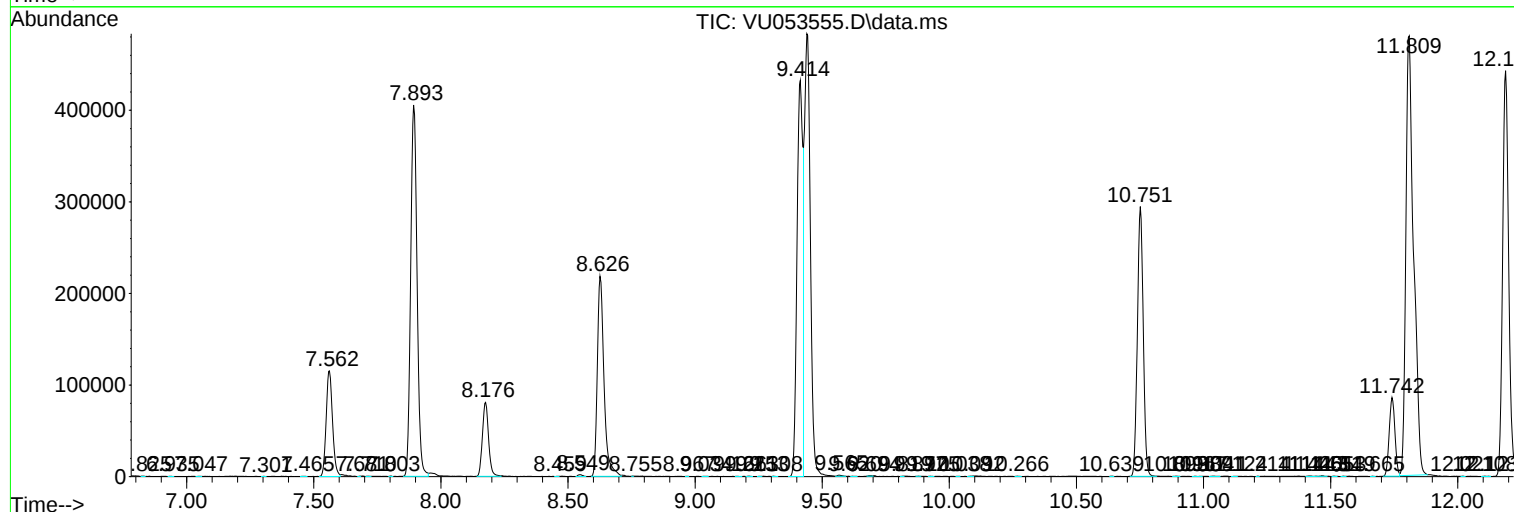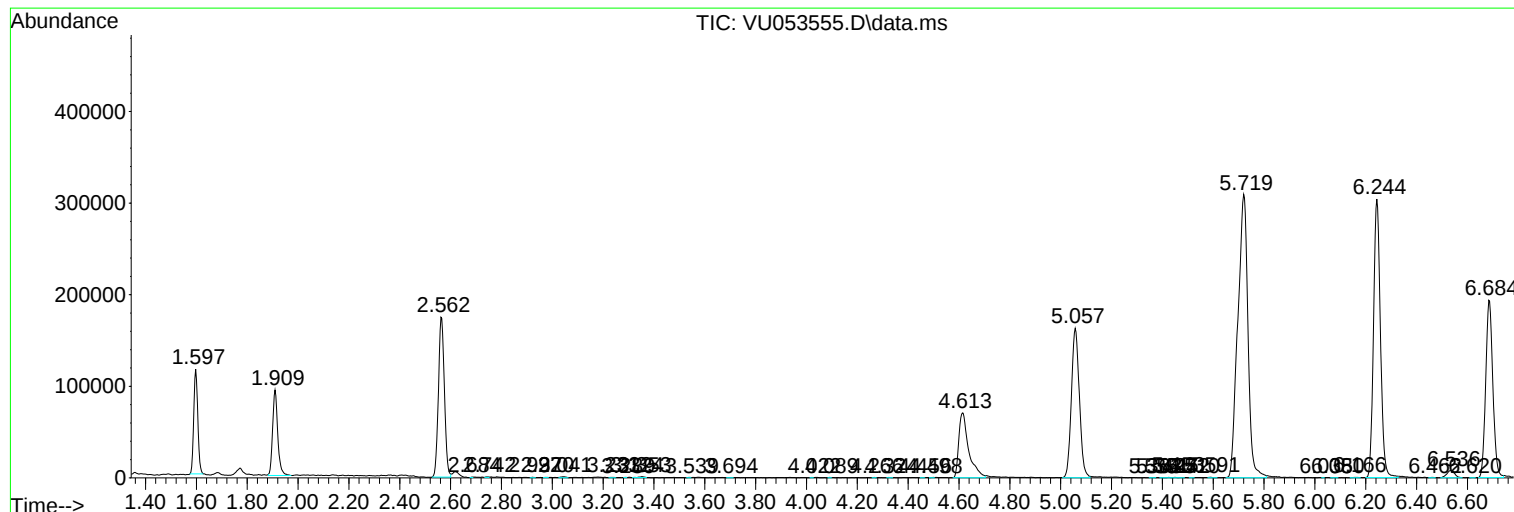

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040423\
Data File : VU053555.D
Acq On : 04 Apr 2023 12:32
Operator : JC/MD
Sample : 02158-08
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PMW-4(20230329)

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040423\
Data File : VU053555.D
Acq On : 04 Apr 2023 12:32
Operator : JC/MD
Sample : 02158-08
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PMW-4(20230329)

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------