

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040423\
 Data File : VU053557.D
 Acq On : 04 Apr 2023 13:18
 Operator : JC/MD
 Sample : 02158-15
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 PMW-8D(20230330)

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

Signal : TIC: VU053557.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.491	42	47	56	rVB	24698	24722	2.69%	0.344%
2	1.597	73	80	93	rVB2	121730	143754	15.66%	2.002%
3	1.909	170	177	192	rVB	86245	118273	12.89%	1.647%
4	2.565	368	381	396	rBV	163700	275851	30.06%	3.842%
5	3.041	521	529	538	rBV4	1223	2148	0.23%	0.030%
6	3.170	560	569	581	rBV6	2237	4837	0.53%	0.067%
7	3.353	613	626	643	rBV3	20109	40313	4.39%	0.561%
8	3.494	666	670	678	rVB2	363	443	0.05%	0.006%
9	3.690	729	731	734	rBV2	525	364	0.04%	0.005%
10	3.864	769	785	803	rBV	45463	106372	11.59%	1.481%
11	3.961	811	815	816	rBV3	530	393	0.04%	0.005%
12	4.105	855	860	864	rBV2	237	244	0.03%	0.003%
13	4.372	940	943	946	rVB	223	175	0.02%	0.002%
14	4.424	953	959	964	rBV	149	220	0.02%	0.003%
15	4.504	982	984	987	rVB2	215	152	0.02%	0.002%
16	4.549	995	998	1003	rBV	201	197	0.02%	0.003%
17	4.613	1003	1018	1021	rBV	71997	113554	12.37%	1.581%
18	4.993	1133	1136	1140	rBV2	321	273	0.03%	0.004%
19	5.057	1140	1156	1182	rBV	153212	343919	37.48%	4.789%
20	5.288	1225	1228	1231	rBV	297	175	0.02%	0.002%
21	5.324	1231	1239	1243	rBV	193	186	0.02%	0.003%
22	5.468	1281	1284	1289	rVV	284	250	0.03%	0.003%
23	5.719	1341	1362	1376	rBV2	299056	828300	90.26%	11.535%
24	5.935	1426	1429	1434	rVB2	236	248	0.03%	0.003%
25	5.983	1440	1444	1448	rVV2	216	188	0.02%	0.003%
26	6.028	1454	1458	1462	rVB3	425	288	0.03%	0.004%
27	6.140	1489	1493	1496	rBV2	372	296	0.03%	0.004%
28	6.243	1511	1525	1544	rBV	294495	563511	61.40%	7.848%
29	6.533	1602	1615	1626	rVB8	5594	11211	1.22%	0.156%
30	6.594	1629	1634	1638	rBV2	271	284	0.03%	0.004%
31	6.684	1649	1662	1682	rBV	189364	369521	40.27%	5.146%
32	6.877	1718	1722	1726	rVB2	258	231	0.03%	0.003%
33	6.960	1738	1748	1760	rBV2	3366	6584	0.72%	0.092%
34	7.189	1810	1819	1821	rBV3	464	579	0.06%	0.008%
35	7.314	1851	1858	1865	rVB2	305	390	0.04%	0.005%
36	7.562	1923	1935	1964	rBV	108645	192064	20.93%	2.675%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040423\
 Data File : VU053557.D
 Acq On : 04 Apr 2023 13:18
 Operator : JC/MD
 Sample : 02158-15
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 PMW-8D(20230330)

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

37	7.829	2011	2018	2021	rBV	294	309	0.03%	0.004%
38	7.893	2025	2038	2056	rBV	387081	677061	73.78%	9.429%
39	8.176	2114	2126	2142	rBV2	73632	128456	14.00%	1.789%
40	8.311	2164	2168	2171	rBV	183	154	0.02%	0.002%
41	8.398	2192	2195	2198	rBV	200	178	0.02%	0.002%
42	8.452	2208	2212	2213	rBV	431	303	0.03%	0.004%
43	8.549	2238	2242	2249	rVB4	1686	2302	0.25%	0.032%
44	8.626	2254	2266	2293	rBV	209678	384516	41.90%	5.355%
45	8.800	2314	2320	2331	rVB4	1925	3487	0.38%	0.049%
46	8.951	2363	2367	2371	rVB	232	162	0.02%	0.002%
47	9.134	2420	2424	2428	rVB2	296	278	0.03%	0.004%
48	9.192	2439	2442	2445	rVB2	219	155	0.02%	0.002%
49	9.221	2448	2451	2454	rBV2	275	223	0.02%	0.003%
50	9.333	2482	2486	2489	rBV2	321	248	0.03%	0.003%
51	9.414	2497	2511	2533	rBV	414299	718980	78.34%	10.013%
52	9.549	2550	2553	2554	rBV2	291	160	0.02%	0.002%
53	9.600	2567	2569	2572	rBV	275	176	0.02%	0.002%
54	9.671	2584	2591	2594	rBV3	1056	1134	0.12%	0.016%
55	9.697	2594	2599	2604	rVB3	552	583	0.06%	0.008%
56	10.066	2711	2714	2717	rVB	321	229	0.02%	0.003%
57	10.092	2717	2722	2724	rBV2	259	217	0.02%	0.003%
58	10.172	2745	2747	2751	rBV	234	178	0.02%	0.002%
59	10.266	2772	2776	2779	rBV	213	179	0.02%	0.002%
60	10.401	2814	2818	2822	rVB2	314	230	0.03%	0.003%
61	10.430	2822	2827	2828	rBV2	319	217	0.02%	0.003%
62	10.481	2841	2843	2849	rBV2	504	393	0.04%	0.005%
63	10.648	2891	2895	2897	rBV2	364	186	0.02%	0.003%
64	10.684	2901	2906	2910	rBV	217	221	0.02%	0.003%
65	10.751	2915	2927	2949	rVB	281966	449431	48.97%	6.259%
66	10.854	2956	2959	2966	rVB	346	399	0.04%	0.006%
67	10.886	2966	2969	2970	rBV	379	249	0.03%	0.003%
68	10.951	2984	2989	2992	rBV	202	180	0.02%	0.003%
69	11.092	3029	3033	3036	rVB2	322	248	0.03%	0.003%
70	11.163	3051	3055	3058	rVV2	224	185	0.02%	0.003%
71	11.227	3072	3075	3078	rBV2	207	168	0.02%	0.002%
72	11.307	3097	3100	3104	rVB	246	168	0.02%	0.002%
73	11.330	3104	3107	3110	rVB	281	158	0.02%	0.002%
74	11.349	3110	3113	3115	rBV	264	203	0.02%	0.003%
75	11.420	3122	3135	3140	rBV4	1330	2007	0.22%	0.028%
76	11.459	3144	3147	3149	rBV	235	152	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040423\
 Data File : VU053557.D
 Acq On : 04 Apr 2023 13:18
 Operator : JC/MD
 Sample : 02158-15
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 PMW-8D(20230330)

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

77	11.475	3149	3152	3158	rVB2	539	361	0.04%	0.005%
78	11.623	3193	3198	3201	rBV2	343	298	0.03%	0.004%
79	11.742	3224	3235	3244	rBV2	22107	33146	3.61%	0.462%
80	11.809	3244	3256	3283	rVB2	453810	917719	100.00%	12.780%
81	12.037	3325	3327	3329	rBV	217	156	0.02%	0.002%
82	12.188	3361	3374	3392	rBV	419245	677059	73.78%	9.429%
83	12.324	3414	3416	3419	rVB	588	254	0.03%	0.004%
84	12.417	3442	3445	3450	rVV	217	180	0.02%	0.003%
85	12.938	3600	3607	3611	rBV2	378	541	0.06%	0.008%
86	12.970	3614	3617	3623	rVV	267	250	0.03%	0.003%
87	13.098	3655	3657	3660	rVB	252	169	0.02%	0.002%
88	13.224	3693	3696	3699	rVV2	535	370	0.04%	0.005%
89	13.282	3710	3714	3717	rBV2	372	269	0.03%	0.004%
90	13.333	3726	3730	3731	rBV	324	280	0.03%	0.004%
91	13.394	3747	3749	3752	rBV	284	184	0.02%	0.003%
92	13.455	3766	3768	3770	rBV	329	178	0.02%	0.002%
93	13.471	3770	3773	3776	rVB	390	252	0.03%	0.004%
94	13.487	3776	3778	3783	rBV	319	253	0.03%	0.004%
95	13.594	3806	3811	3813	rBV	332	315	0.03%	0.004%
96	13.610	3813	3816	3819	rBV	333	234	0.03%	0.003%
97	13.735	3853	3855	3860	rVB	336	216	0.02%	0.003%
98	13.758	3860	3862	3865	rBV2	345	217	0.02%	0.003%
99	13.838	3879	3887	3901	rBV3	13259	20388	2.22%	0.284%
100	14.327	4035	4039	4049	rVB6	2079	2464	0.27%	0.034%


Sum of corrected areas: 7180726

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040423\
Data File : VU053557.D
Acq On : 04 Apr 2023 13:18
Operator : JC/MD
Sample : 02158-15
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PMW-8D(20230330)

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

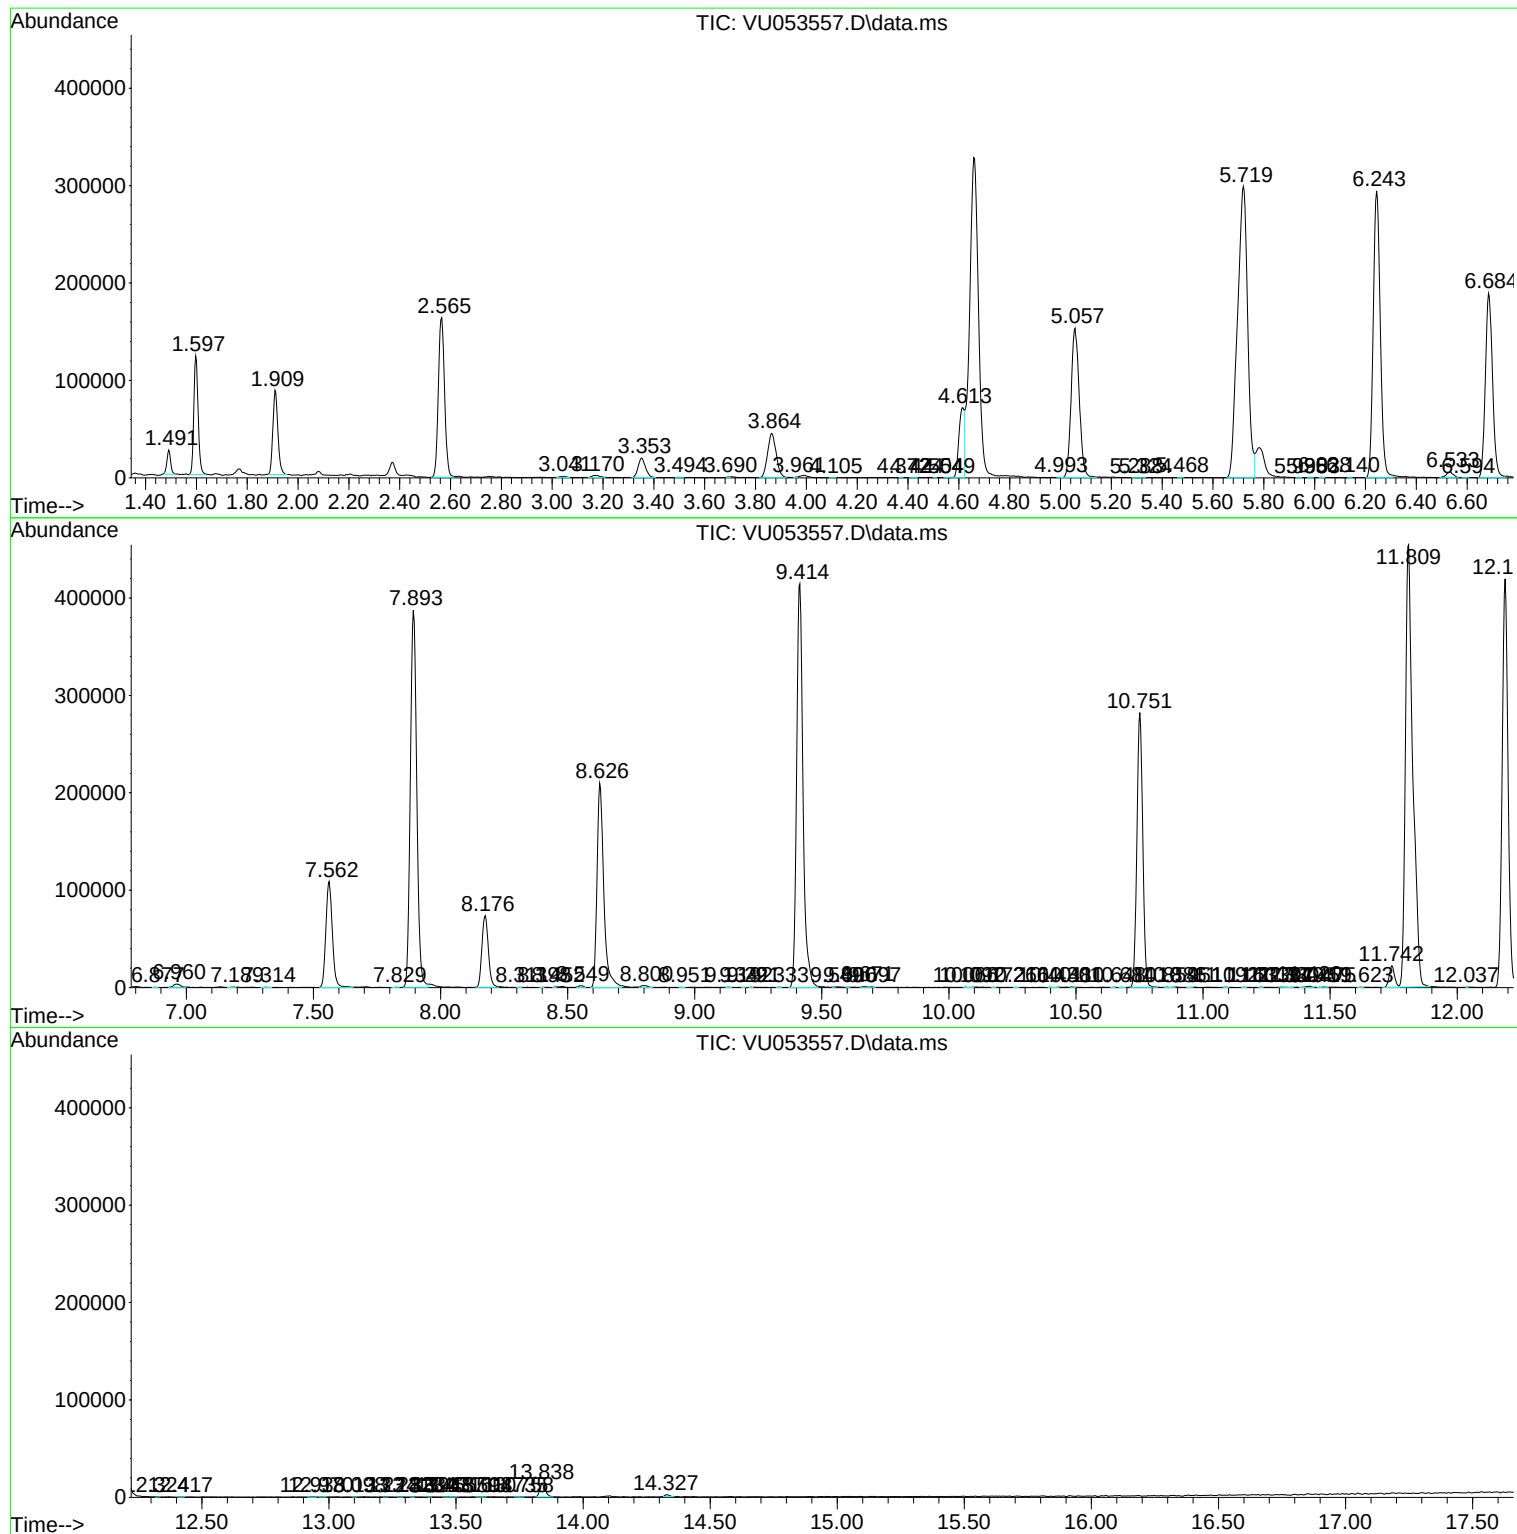

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040423\
Data File : VU053557.D
Acq On : 04 Apr 2023 13:18
Operator : JC/MD
Sample : 02158-15
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PMW-8D(20230330)

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040423\
Data File : VU053557.D
Acq On : 04 Apr 2023 13:18
Operator : JC/MD
Sample : 02158-15
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PMW-8D(20230330)

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------