

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040423\
 Data File : VU053570.D
 Acq On : 04 Apr 2023 18:42
 Operator : JC/MD
 Sample : 02158-13DL 20X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 PMW-9D(20230330)DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

Signal : TIC: VU053570.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	92	rVB	96427	108092	11.46%	1.398%
2	1.909	169	177	197	rVB	81058	111999	11.87%	1.449%
3	2.562	369	380	395	rBV	151205	245204	26.00%	3.172%
4	2.732	430	433	435	rBV	254	177	0.02%	0.002%
5	2.845	466	468	469	rVB	281	65	0.01%	0.001%
6	3.041	520	529	540	rVB2	5073	9118	0.97%	0.118%
7	3.166	566	568	571	rBV2	439	177	0.02%	0.002%
8	3.266	595	599	600	rBV	251	193	0.02%	0.002%
9	3.485	664	667	668	rBV	316	150	0.02%	0.002%
10	3.716	737	739	741	rVB	195	77	0.01%	0.001%
11	3.906	795	798	800	rBV	223	119	0.01%	0.002%
12	4.128	865	867	869	rBV2	171	125	0.01%	0.002%
13	4.250	902	905	909	rBV	204	177	0.02%	0.002%
14	4.301	919	921	924	rBV	190	76	0.01%	0.001%
15	4.375	942	944	947	rVB2	179	89	0.01%	0.001%
16	4.449	964	967	971	rVB	388	189	0.02%	0.002%
17	4.546	994	997	999	rVB	240	141	0.01%	0.002%
18	4.568	999	1004	1006	rBV2	215	197	0.02%	0.003%
19	4.610	1006	1017	1045	rBV	72760	174470	18.50%	2.257%
20	5.057	1139	1156	1178	rBV2	148940	327598	34.73%	4.238%
21	5.260	1216	1219	1223	rBV2	350	253	0.03%	0.003%
22	5.462	1279	1282	1284	rBV2	232	169	0.02%	0.002%
23	5.559	1308	1312	1315	rVB2	206	124	0.01%	0.002%
24	5.604	1325	1326	1327	rBV2	153	53	0.01%	0.001%
25	5.629	1331	1334	1336	rBV	235	183	0.02%	0.002%
26	5.719	1341	1362	1381	rBV2	280090	775910	82.26%	10.037%
27	6.095	1478	1479	1480	rBV2	120	28	0.00%	0.000%
28	6.182	1504	1506	1508	rBV	240	111	0.01%	0.001%
29	6.243	1511	1525	1550	rBV	310777	593526	62.93%	7.678%
30	6.523	1603	1612	1623	rBV8	4115	7622	0.81%	0.099%
31	6.684	1649	1662	1679	rBV	181331	354375	37.57%	4.584%
32	6.841	1708	1711	1715	rVB2	247	189	0.02%	0.002%
33	6.896	1726	1728	1734	rVB2	267	201	0.02%	0.003%
34	7.012	1761	1764	1767	rBV2	228	168	0.02%	0.002%
35	7.121	1795	1798	1801	rBV	349	268	0.03%	0.003%
36	7.224	1826	1830	1833	rBV2	252	191	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040423\
 Data File : VU053570.D
 Acq On : 04 Apr 2023 18:42
 Operator : JC/MD
 Sample : 02158-13DL 20X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 PMW-9D(20230330)DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

37	7.279	1846	1847	1848	rBV2	256	91	0.01%	0.001%
38	7.340	1864	1866	1870	rBV	175	91	0.01%	0.001%
39	7.366	1873	1874	1875	rBV	124	34	0.00%	0.000%
40	7.478	1906	1909	1910	rBV	127	71	0.01%	0.001%
41	7.562	1923	1935	1950	rBV	101972	180181	19.10%	2.331%
42	7.700	1977	1978	1983	rVB2	537	334	0.04%	0.004%
43	7.755	1993	1995	1998	rVB2	231	128	0.01%	0.002%
44	7.774	1998	2001	2004	rVB2	330	212	0.02%	0.003%
45	7.800	2004	2009	2015	rBV	310	334	0.04%	0.004%
46	7.822	2015	2016	2018	rBV	124	52	0.01%	0.001%
47	7.893	2023	2038	2058	rBV	363640	635796	67.41%	8.225%
48	8.176	2114	2126	2153	rVV2	74251	123360	13.08%	1.596%
49	8.272	2154	2156	2161	rVB	333	179	0.02%	0.002%
50	8.340	2174	2177	2181	rBV	183	100	0.01%	0.001%
51	8.404	2193	2197	2199	rBV	186	133	0.01%	0.002%
52	8.478	2217	2220	2225	rVB2	473	392	0.04%	0.005%
53	8.549	2236	2242	2247	rVB4	1325	1485	0.16%	0.019%
54	8.574	2248	2250	2252	rBV	163	47	0.00%	0.001%
55	8.626	2255	2266	2292	rBV2	209962	392747	41.64%	5.081%
56	8.809	2321	2323	2326	rVB	343	112	0.01%	0.001%
57	8.947	2363	2366	2369	rBV	245	176	0.02%	0.002%
58	9.005	2382	2384	2385	rBV	206	91	0.01%	0.001%
59	9.111	2415	2417	2424	rBV	216	150	0.02%	0.002%
60	9.304	2472	2477	2481	rVB2	291	312	0.03%	0.004%
61	9.353	2490	2492	2495	rVB	266	75	0.01%	0.001%
62	9.414	2497	2511	2533	rBV	426038	744779	78.96%	9.635%
63	10.060	2708	2712	2716	rBV	218	197	0.02%	0.003%
64	10.108	2724	2727	2730	rBV	169	117	0.01%	0.002%
65	10.147	2735	2739	2741	rBV2	222	136	0.01%	0.002%
66	10.407	2818	2820	2822	rBV	179	70	0.01%	0.001%
67	10.600	2878	2880	2884	rBV2	275	185	0.02%	0.002%
68	10.751	2914	2927	2946	rBV	284359	446653	47.35%	5.778%
69	11.095	3032	3034	3037	rBV	268	133	0.01%	0.002%
70	11.394	3125	3127	3130	rBV	196	91	0.01%	0.001%
71	11.465	3148	3149	3157	rVB	333	275	0.03%	0.004%
72	11.742	3226	3235	3244	rBV	43003	66365	7.04%	0.859%
73	11.809	3244	3256	3278	rVB2	494232	943206	100.00%	12.201%
74	12.121	3350	3353	3358	rBV	274	180	0.02%	0.002%
75	12.188	3361	3374	3397	rBV	413785	680671	72.17%	8.805%
76	12.819	3567	3570	3571	rBV	257	126	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040423\
 Data File : VU053570.D
 Acq On : 04 Apr 2023 18:42
 Operator : JC/MD
 Sample : 02158-13DL 20X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 PMW-9D(20230330)DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M

Title : VOC Analysis

77	12.841	3575	3577	3581	rVB2	472	252	0.03%	0.003%
78	13.301	3717	3720	3726	rBV2	294	343	0.04%	0.004%
79	13.391	3747	3748	3749	rBV	241	72	0.01%	0.001%
80	13.487	3775	3778	3781	rBV2	371	263	0.03%	0.003%
81	13.835	3874	3886	3906	rBV	475666	755392	80.09%	9.772%
82	14.327	4029	4039	4056	rBV	27612	42311	4.49%	0.547%


Sum of corrected areas: 7730304

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040423\
Data File : VU053570.D
Acq On : 04 Apr 2023 18:42
Operator : JC/MD
Sample : 02158-13DL 20X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PMW-9D(20230330)DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

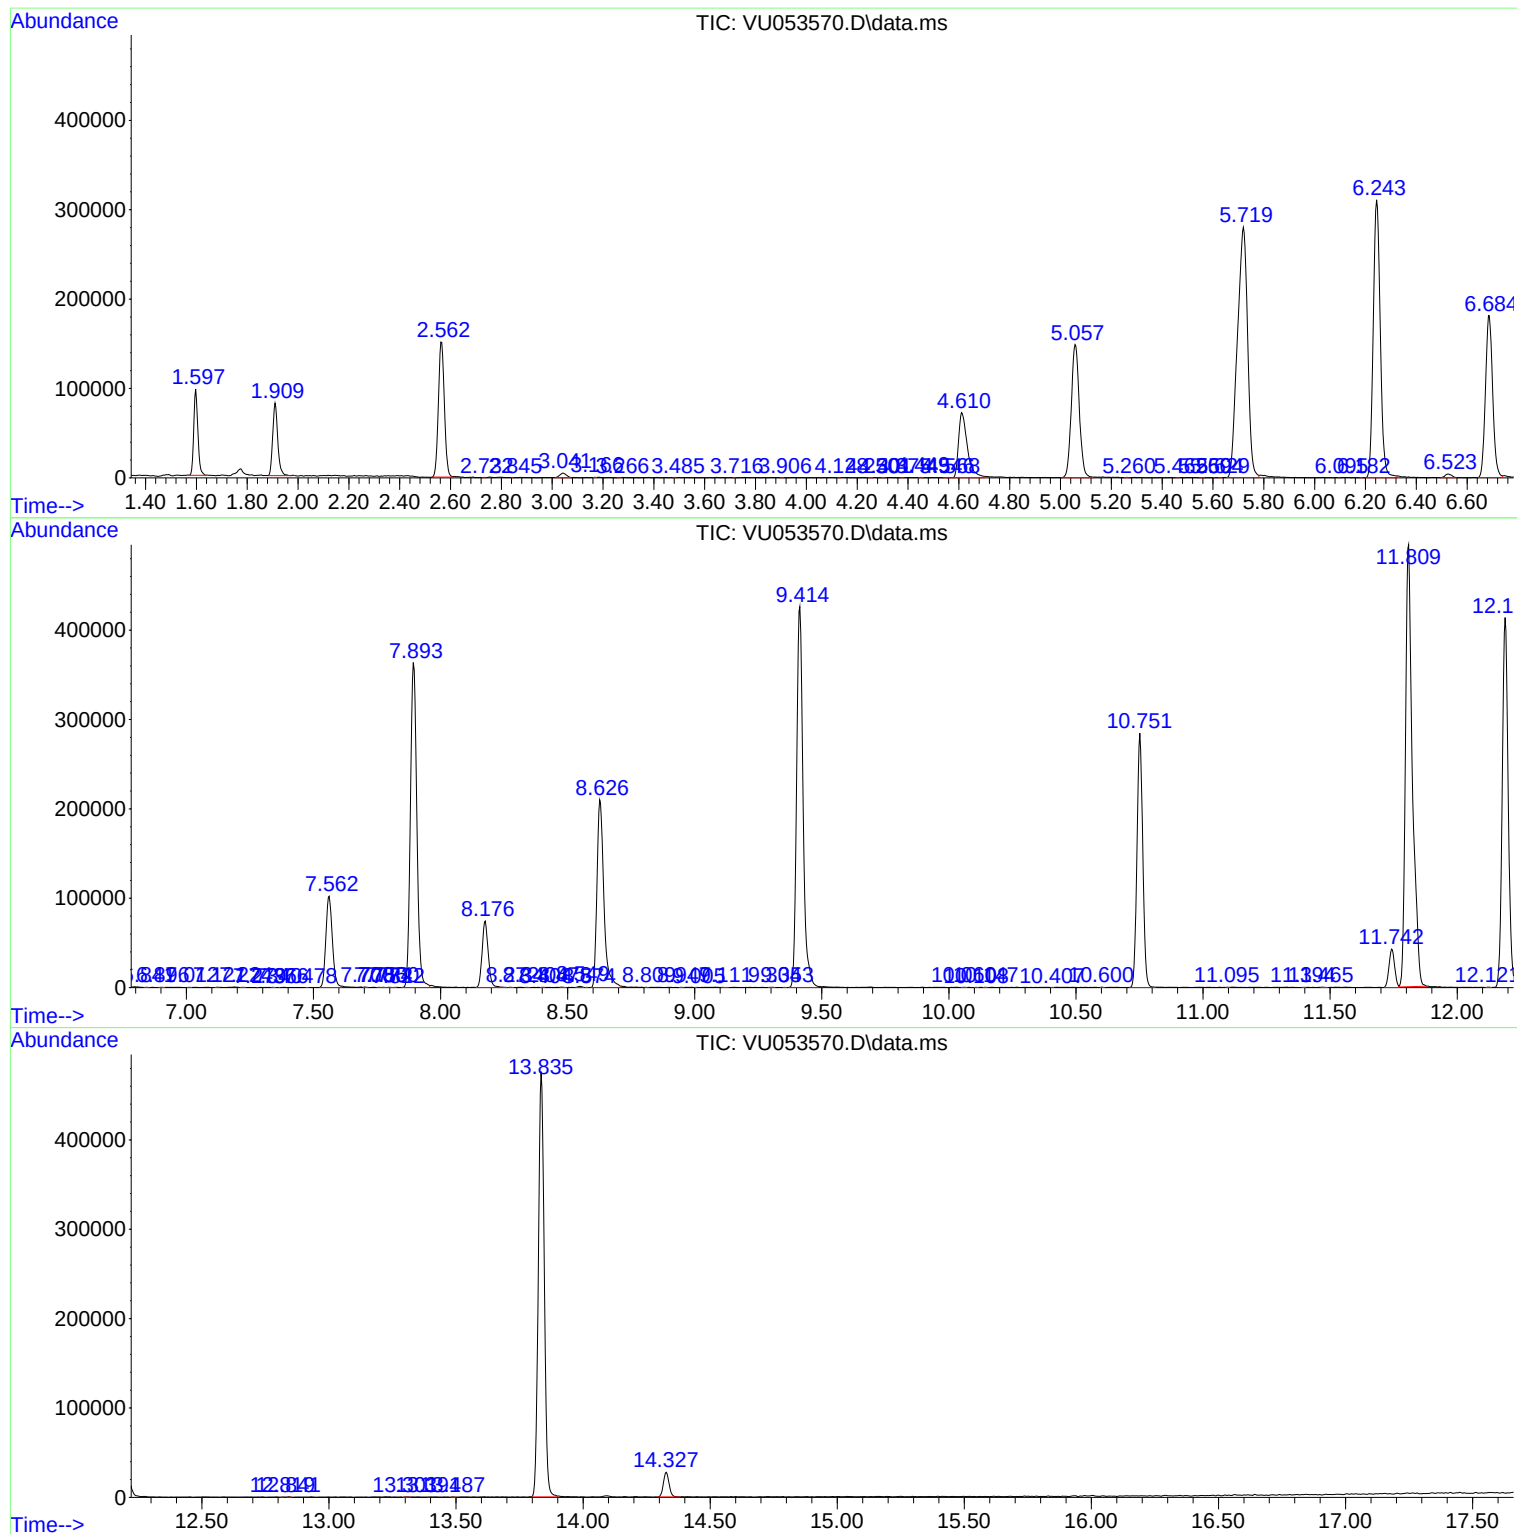

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040423\
Data File : VU053570.D
Acq On : 04 Apr 2023 18:42
Operator : JC/MD
Sample : 02158-13DL 20X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PMW-9D(20230330)DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040423\
Data File : VU053570.D
Acq On : 04 Apr 2023 18:42
Operator : JC/MD
Sample : 02158-13DL 20X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PMW-9D(20230330)DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------