

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040423\
 Data File : VU053573.D
 Acq On : 04 Apr 2023 19:53
 Operator : JC/MD
 Sample : 02158-07DL 5X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 PMW-6(20230329)DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M

Title : VOC Analysis

Signal : TIC: VU053573.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	96	rVB	93639	108776	9.46%	1.455%
2	1.909	170	177	192	rVB	83637	110994	9.66%	1.485%
3	2.565	369	381	395	rBV	147406	239370	20.83%	3.202%
4	2.745	434	437	441	rBV3	470	329	0.03%	0.004%
5	2.861	471	473	474	rBV	294	71	0.01%	0.001%
6	2.928	492	494	500	rVB	415	240	0.02%	0.003%
7	3.044	519	530	545	rBV2	7587	14984	1.30%	0.200%
8	3.253	592	595	597	rBV	243	139	0.01%	0.002%
9	3.340	620	622	627	rBV	222	181	0.02%	0.002%
10	3.752	748	750	752	rVB	276	105	0.01%	0.001%
11	3.989	821	824	826	rBV	255	130	0.01%	0.002%
12	4.054	841	844	846	rBV	240	128	0.01%	0.002%
13	4.218	893	895	897	rBV	168	69	0.01%	0.001%
14	4.253	904	906	907	rBV	150	68	0.01%	0.001%
15	4.613	1007	1018	1049	rBV2	72436	181785	15.82%	2.432%
16	4.938	1117	1119	1121	rBV	148	66	0.01%	0.001%
17	4.957	1124	1125	1127	rVB	257	58	0.01%	0.001%
18	5.057	1140	1156	1174	rBV	150394	322708	28.08%	4.317%
19	5.475	1284	1286	1289	rBV2	175	96	0.01%	0.001%
20	5.559	1308	1312	1315	rBV	276	198	0.02%	0.003%
21	5.719	1342	1362	1393	rBV2	284221	788538	68.61%	10.549%
22	5.925	1423	1426	1427	rBV	188	106	0.01%	0.001%
23	5.960	1435	1437	1439	rBV	222	118	0.01%	0.002%
24	5.999	1447	1449	1452	rVB2	233	126	0.01%	0.002%
25	6.115	1483	1485	1488	rVB2	279	134	0.01%	0.002%
26	6.195	1508	1510	1511	rBV	142	77	0.01%	0.001%
27	6.243	1511	1525	1548	rBV	304586	577910	50.28%	7.732%
28	6.533	1603	1615	1627	rVB9	5019	10707	0.93%	0.143%
29	6.687	1648	1663	1681	rBV	179703	354601	30.85%	4.744%
30	7.005	1756	1762	1765	rBV	279	324	0.03%	0.004%
31	7.021	1765	1767	1768	rBV	117	36	0.00%	0.000%
32	7.282	1844	1848	1851	rBV2	389	354	0.03%	0.005%
33	7.321	1857	1860	1863	rBV	275	171	0.01%	0.002%
34	7.356	1868	1871	1873	rBV	184	125	0.01%	0.002%
35	7.391	1879	1882	1883	rBV	250	139	0.01%	0.002%
36	7.484	1908	1911	1914	rBV2	166	125	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040423\
 Data File : VU053573.D
 Acq On : 04 Apr 2023 19:53
 Operator : JC/MD
 Sample : 02158-07DL 5X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 PMW-6(20230329)DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

37	7.520	1919	1922	1923	rBV2	201	112	0.01%	0.001%
38	7.562	1923	1935	1957	rBV	102199	179247	15.60%	2.398%
39	7.787	2002	2005	2012	rVB2	384	393	0.03%	0.005%
40	7.822	2014	2016	2017	rBV	162	41	0.00%	0.001%
41	7.835	2017	2020	2023	rBV2	248	162	0.01%	0.002%
42	7.893	2025	2038	2058	rBV	364362	629344	54.76%	8.420%
43	8.176	2115	2126	2144	rBV	73587	121532	10.57%	1.626%
44	8.433	2204	2206	2207	rBV	147	41	0.00%	0.001%
45	8.555	2236	2244	2247	rVB6	970	1134	0.10%	0.015%
46	8.574	2247	2250	2252	rBV	255	190	0.02%	0.003%
47	8.629	2256	2267	2295	rBV	217890	399625	34.77%	5.346%
48	8.806	2320	2322	2327	rVB	199	80	0.01%	0.001%
49	8.886	2343	2347	2350	rBV	269	228	0.02%	0.003%
50	8.992	2378	2380	2384	rBV	174	110	0.01%	0.001%
51	9.414	2498	2511	2516	rBV	427627	728008	63.34%	9.740%
52	9.591	2563	2566	2568	rBV2	351	175	0.02%	0.002%
53	9.639	2579	2581	2585	rVB2	470	212	0.02%	0.003%
54	9.774	2619	2623	2626	rBV2	199	155	0.01%	0.002%
55	9.928	2668	2671	2674	rVB	308	169	0.01%	0.002%
56	9.992	2688	2691	2692	rBV	183	93	0.01%	0.001%
57	10.002	2692	2694	2697	rVB2	232	128	0.01%	0.002%
58	10.031	2700	2703	2704	rBV2	196	89	0.01%	0.001%
59	10.076	2714	2717	2718	rBV2	193	97	0.01%	0.001%
60	10.147	2736	2739	2743	rBV2	227	219	0.02%	0.003%
61	10.288	2781	2783	2785	rBV	188	68	0.01%	0.001%
62	10.304	2785	2788	2790	rBV	213	105	0.01%	0.001%
63	10.375	2808	2810	2811	rBV	216	69	0.01%	0.001%
64	10.751	2914	2927	2945	rBV	283078	449989	39.15%	6.020%
65	10.928	2980	2982	2988	rVB	319	210	0.02%	0.003%
66	11.086	3027	3031	3032	rBV	321	210	0.02%	0.003%
67	11.166	3053	3056	3058	rBV	251	189	0.02%	0.003%
68	11.304	3096	3099	3100	rBV	184	99	0.01%	0.001%
69	11.742	3224	3235	3245	rBV2	102285	163268	14.21%	2.184%
70	11.809	3245	3256	3280	rVB2	503727	1149286	100.00%	15.376%
71	11.973	3305	3307	3309	rBV2	245	103	0.01%	0.001%
72	12.188	3361	3374	3397	rBV	411820	706009	61.43%	9.445%
73	13.455	3766	3768	3772	rBV	281	200	0.02%	0.003%
74	13.838	3875	3887	3905	rBV2	137255	221297	19.26%	2.961%
75	14.330	4029	4040	4051	rBV5	4793	7900	0.69%	0.106%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040423\
Data File : VU053573.D
Acq On : 04 Apr 2023 19:53
Operator : JC/MD
Sample : 02158-07DL 5X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PMW-6(20230329)DL

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Title : VOC Analysis


Sum of corrected areas: 7474672

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040423\
Data File : VU053573.D
Acq On : 04 Apr 2023 19:53
Operator : JC/MD
Sample : 02158-07DL 5X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PMW-6(20230329)DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

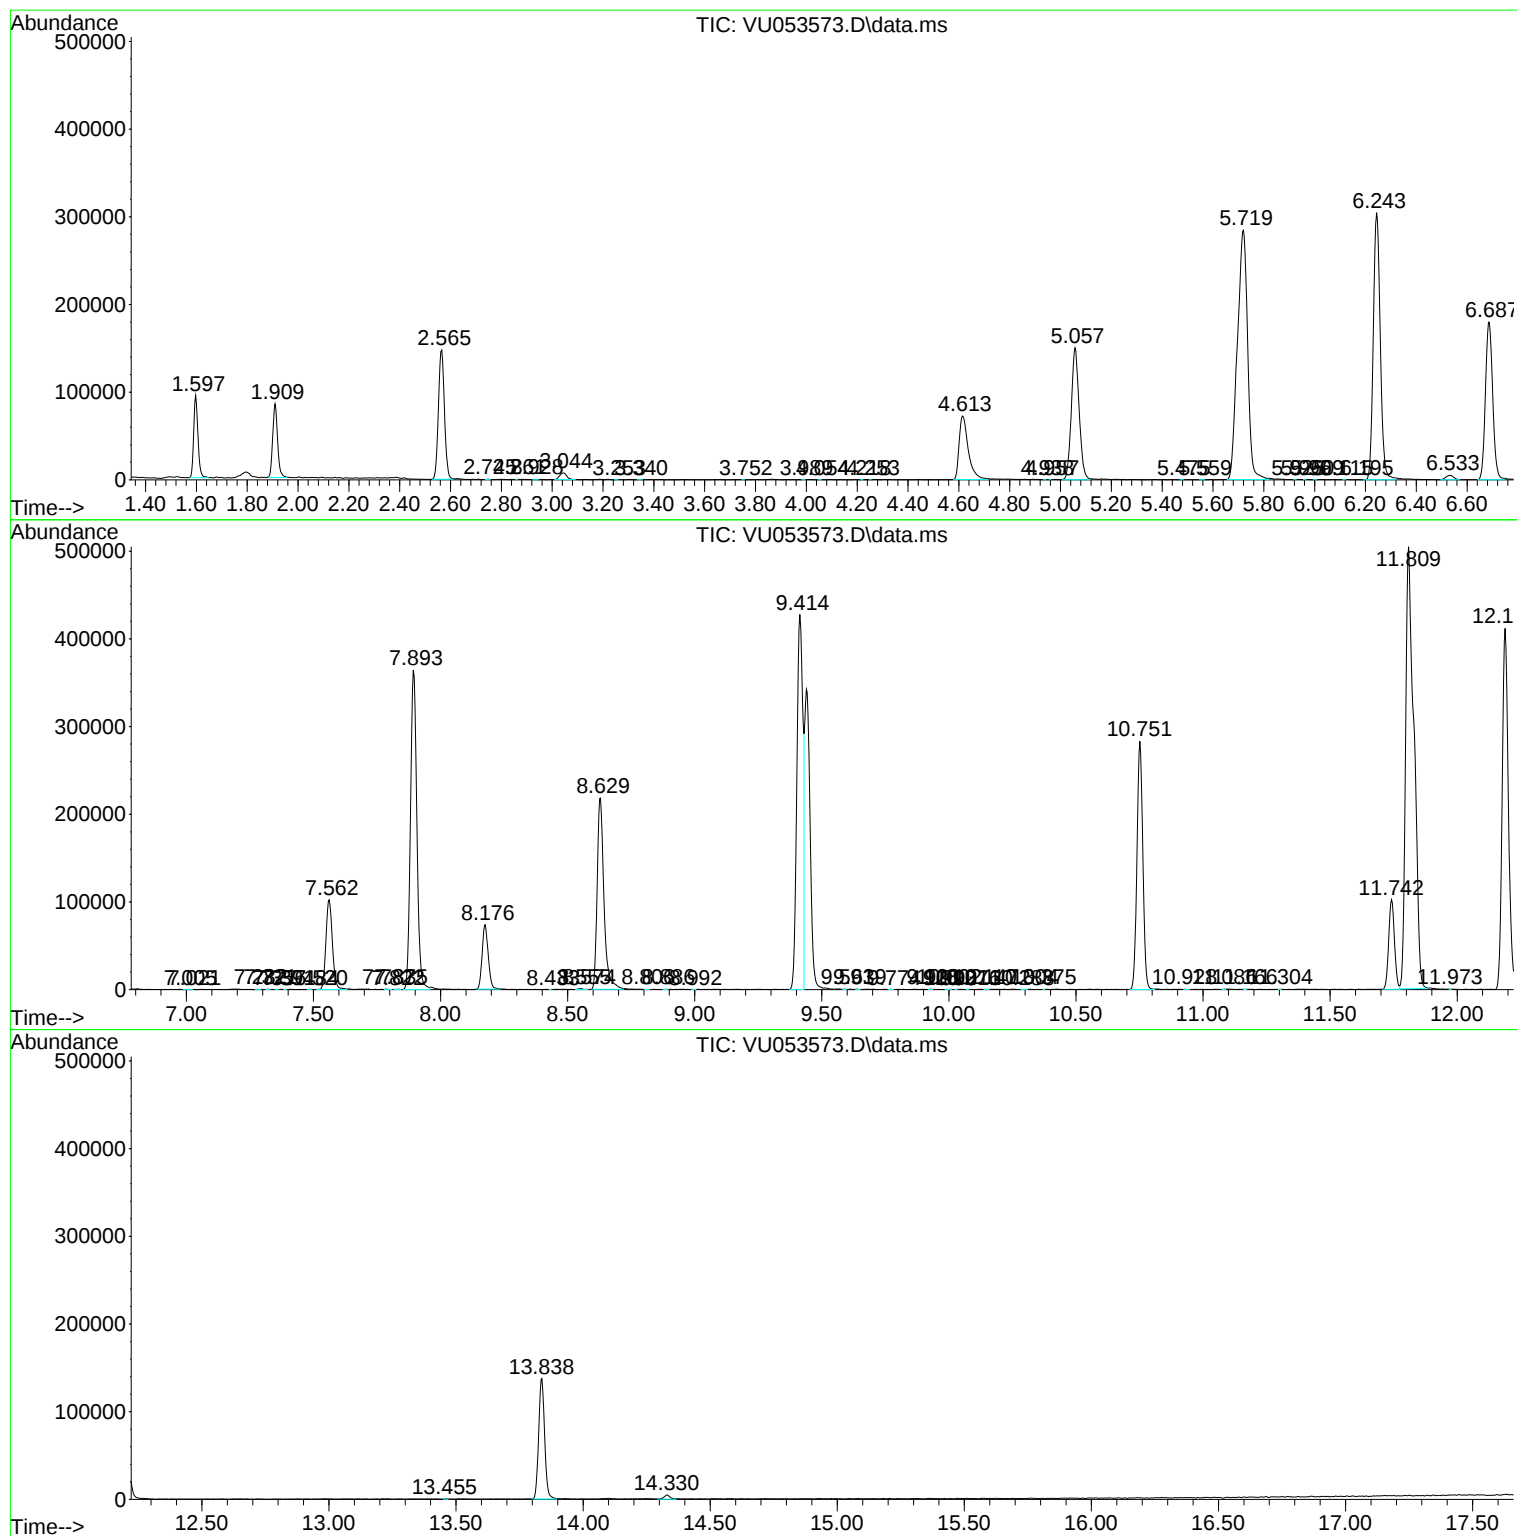

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040423\
Data File : VU053573.D
Acq On : 04 Apr 2023 19:53
Operator : JC/MD
Sample : 02158-07DL 5X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PMW-6(20230329)DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040423\
Data File : VU053573.D
Acq On : 04 Apr 2023 19:53
Operator : JC/MD
Sample : 02158-07DL 5X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PMW-6(20230329)DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------