

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040423\
 Data File : VU053574.D
 Acq On : 04 Apr 2023 20:17
 Operator : JC/MD
 Sample : 02158-06DL 400X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 PMW-5(20230329)DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M

Title : VOC Analysis

Signal : TIC: VU053574.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.598	73	80	91	rVB	93435	105631	12.18%	1.339%
2	1.910	169	177	191	rVB	83365	112290	12.95%	1.424%
3	2.562	369	380	400	rVB	147171	239898	27.66%	3.042%
4	3.045	519	530	543	rBV3	10413	19015	2.19%	0.241%
5	3.382	633	635	637	rBV	192	89	0.01%	0.001%
6	3.527	678	680	683	rBV	198	93	0.01%	0.001%
7	4.077	849	851	853	rBV	164	52	0.01%	0.001%
8	4.395	947	950	952	rBV2	219	156	0.02%	0.002%
9	4.508	984	985	987	rVB	250	54	0.01%	0.001%
10	4.617	1007	1019	1025	rBV2	71704	147768	17.04%	1.874%
11	4.906	1106	1109	1110	rBV2	157	89	0.01%	0.001%
12	4.948	1119	1122	1124	rBV2	274	158	0.02%	0.002%
13	5.057	1140	1156	1177	rBV	145179	320192	36.92%	4.060%
14	5.241	1210	1213	1215	rBV2	335	269	0.03%	0.003%
15	5.620	1330	1331	1334	rVB	124	33	0.00%	0.000%
16	5.720	1341	1362	1387	rBV2	282890	768391	88.61%	9.743%
17	5.958	1429	1436	1440	rBV	499	651	0.08%	0.008%
18	6.022	1452	1456	1457	rBV	145	107	0.01%	0.001%
19	6.112	1482	1484	1485	rBV	190	78	0.01%	0.001%
20	6.244	1512	1525	1544	rBV	307925	582212	67.14%	7.382%
21	6.482	1597	1599	1602	rVB	210	98	0.01%	0.001%
22	6.536	1604	1616	1632	rVB5	20378	42562	4.91%	0.540%
23	6.684	1648	1662	1680	rBV2	178177	346145	39.92%	4.389%
24	6.851	1711	1714	1715	rBV	178	97	0.01%	0.001%
25	7.035	1768	1771	1773	rBV2	190	127	0.01%	0.002%
26	7.051	1773	1776	1779	rVB2	227	130	0.01%	0.002%
27	7.138	1800	1803	1807	rBV	270	233	0.03%	0.003%
28	7.186	1814	1818	1828	rVV2	506	692	0.08%	0.009%
29	7.231	1830	1832	1836	rVB	212	98	0.01%	0.001%
30	7.263	1840	1842	1845	rBV	151	72	0.01%	0.001%
31	7.366	1872	1874	1876	rBV	152	88	0.01%	0.001%
32	7.562	1923	1935	1956	rBV2	98891	173256	19.98%	2.197%
33	7.739	1986	1990	1991	rBV	218	135	0.02%	0.002%
34	7.765	1995	1998	2002	rVB2	370	230	0.03%	0.003%
35	7.832	2017	2019	2022	rBV	287	113	0.01%	0.001%
36	7.893	2025	2038	2051	rBV	356323	613281	70.72%	7.776%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040423\
 Data File : VU053574.D
 Acq On : 04 Apr 2023 20:17
 Operator : JC/MD
 Sample : 02158-06DL 400X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 PMW-5(20230329)DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

37	7.964	2051	2060	2081	rVB	177637	306590	35.35%	3.888%
38	8.105	2100	2104	2106	rBV	208	116	0.01%	0.001%
39	8.176	2113	2126	2146	rBV	70471	120441	13.89%	1.527%
40	8.392	2191	2193	2195	rBV	185	73	0.01%	0.001%
41	8.507	2226	2229	2230	rBV	226	101	0.01%	0.001%
42	8.549	2230	2242	2256	rVV	107077	180152	20.77%	2.284%
43	8.630	2256	2267	2292	rBV2	210551	388145	44.76%	4.922%
44	8.877	2340	2344	2348	rBB	258	193	0.02%	0.002%
45	8.896	2348	2350	2355	rVB	284	184	0.02%	0.002%
46	8.919	2355	2357	2364	rBV	345	288	0.03%	0.004%
47	9.179	2437	2438	2439	rBV	201	47	0.01%	0.001%
48	9.308	2475	2478	2480	rBV	239	200	0.02%	0.003%
49	9.337	2485	2487	2488	rBV	218	73	0.01%	0.001%
50	9.414	2498	2511	2536	rBV	418191	723695	83.45%	9.176%
51	9.568	2550	2559	2567	rBV2	8262	12604	1.45%	0.160%
52	9.691	2586	2597	2610	rBV2	29750	47412	5.47%	0.601%
53	9.906	2662	2664	2668	rVB	223	110	0.01%	0.001%
54	10.099	2715	2724	2735	rVB2	9762	15409	1.78%	0.195%
55	10.186	2747	2751	2754	rBV	279	225	0.03%	0.003%
56	10.221	2759	2762	2768	rVB	313	254	0.03%	0.003%
57	10.353	2800	2803	2807	rBV	322	226	0.03%	0.003%
58	10.388	2812	2814	2816	rBV	165	91	0.01%	0.001%
59	10.440	2828	2830	2831	rBV	228	89	0.01%	0.001%
60	10.478	2840	2842	2851	rVB3	1116	1209	0.14%	0.015%
61	10.752	2914	2927	2942	rBV	274412	436304	50.31%	5.532%
62	10.996	2995	3003	3009	rBV3	3563	4919	0.57%	0.062%
63	11.086	3022	3031	3043	rBV4	1560	2557	0.29%	0.032%
64	11.150	3048	3051	3054	rVB	269	168	0.02%	0.002%
65	11.224	3071	3074	3078	rBV	297	235	0.03%	0.003%
66	11.256	3082	3084	3085	rVB	265	105	0.01%	0.001%
67	11.285	3090	3093	3094	rBV	896	509	0.06%	0.006%
68	11.465	3143	3149	3162	rVB2	5922	7729	0.89%	0.098%
69	11.745	3227	3236	3244	rBV4	14961	23709	2.73%	0.301%
70	11.809	3244	3256	3278	rVV2	467779	867189	100.00%	10.996%
71	11.925	3290	3292	3293	rBV	417	156	0.02%	0.002%
72	12.189	3362	3374	3398	rBV	405081	672644	77.57%	8.529%
73	12.321	3412	3415	3417	rBV2	202	128	0.01%	0.002%
74	12.613	3503	3506	3508	rBV2	272	171	0.02%	0.002%
75	12.880	3586	3589	3590	rBV	282	145	0.02%	0.002%
76	13.752	3857	3860	3863	rBV2	483	410	0.05%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040423\
Data File : VU053574.D
Acq On : 04 Apr 2023 20:17
Operator : JC/MD
Sample : 02158-06DL 400X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PMW-5(20230329)DL

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Title : VOC Analysis

77	13.835	3874	3886	3905	rBV	314250	498202	57.45%	6.317%
78	14.089	3958	3965	3979	rVB3	2910	4467	0.52%	0.057%
79	14.327	4028	4039	4051	rBV	58307	93936	10.83%	1.191%
80	15.690	4461	4463	4467	rBV3	626	291	0.03%	0.004%




Sum of corrected areas: 7886484

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040423\
Data File : VU053574.D
Acq On : 04 Apr 2023 20:17
Operator : JC/MD
Sample : 02158-06DL 400X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PMW-5(20230329)DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

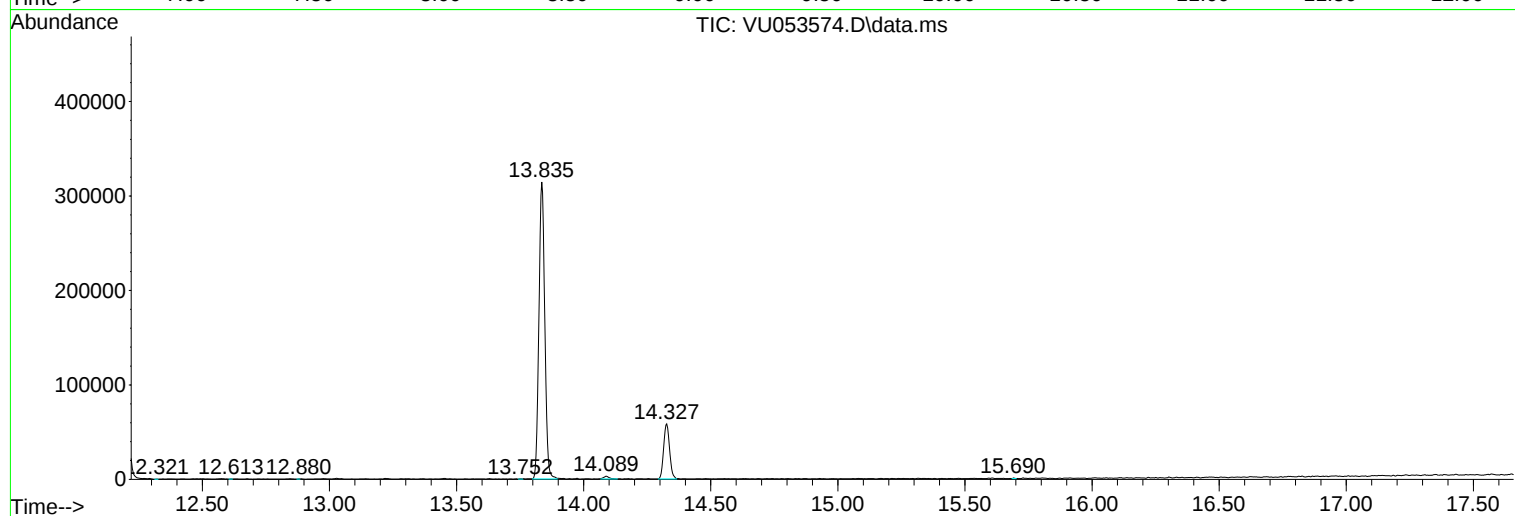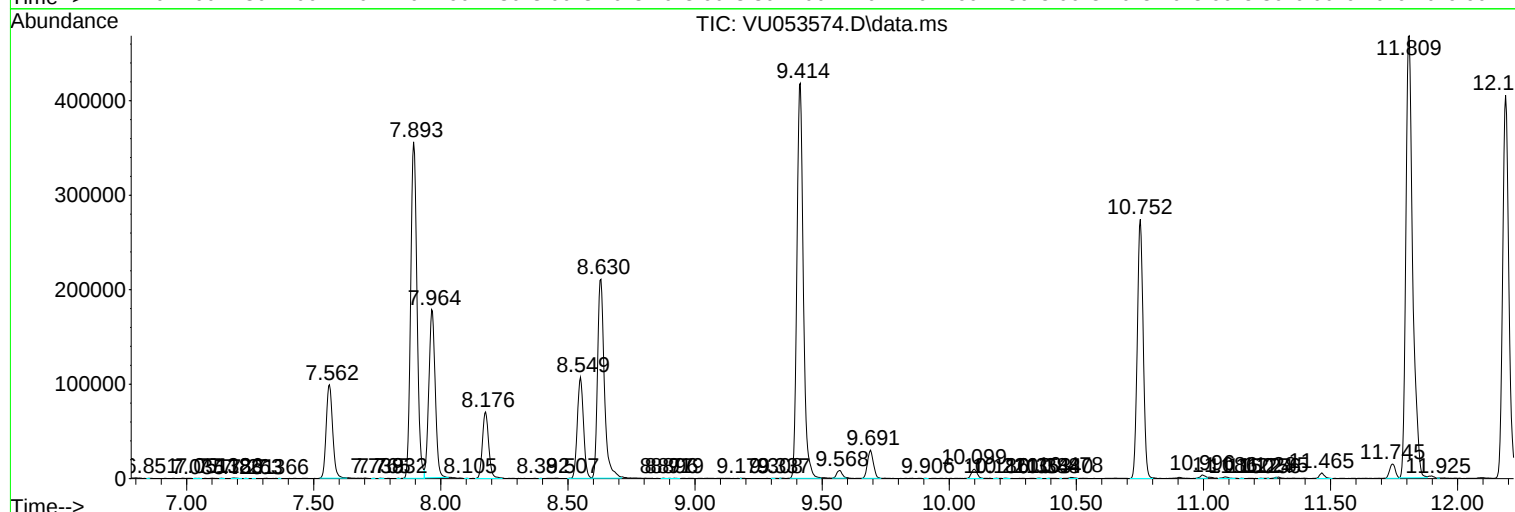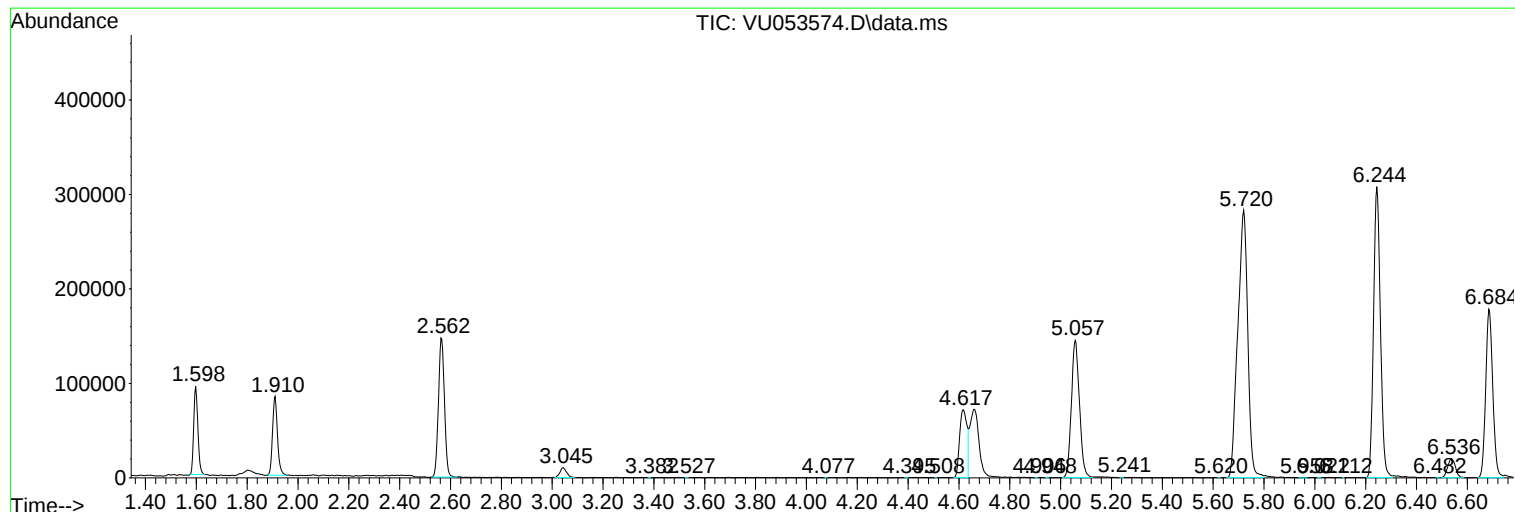

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040423\
Data File : VU053574.D
Acq On : 04 Apr 2023 20:17
Operator : JC/MD
Sample : 02158-06DL 400X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PMW-5(20230329)DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040423\
Data File : VU053574.D
Acq On : 04 Apr 2023 20:17
Operator : JC/MD
Sample : 02158-06DL 400X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PMW-5(20230329)DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------