

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU040519\
 Data File : VU030703.D
 Acq On : 04 Apr 2019 23:14
 Operator : JC/SP
 Sample : K2168-13DL 5X
 Misc : 6.26g/5mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF638DL

Quant Time: Apr 05 02:22:51 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Apr 05 02:15:56 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	532576	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	511336	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	242011	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.39	65	206168	43.37	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	86.74%
7) Chloroethane-d5	1.65	69	157971	43.78	ug/L	-0.02
Spiked Amount	50.000	Range	70 - 130	Recovery	=	87.56%
11) 1,1-Dichloroethene-d2	2.35	63	212	0.02	ug/L	0.08
Spiked Amount	50.000	Range	60 - 125	Recovery	=	0.04%#
21) 2-Butanone-d5	4.17	46	369551	98.08	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	98.08%
24) Chloroform-d	4.64	84	317391	43.70	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	87.40%
26) 1,2-Dichloroethane-d4	5.30	65	225274	45.46	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	90.92%
32) Benzene-d6	5.33	84	692488	46.39	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	92.78%
36) 1,2-Dichloropropane-d6	6.32	67	243229	47.55	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	95.10%
41) Toluene-d8	7.56	98	622492	47.05	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	94.10%
43) trans-1,3-Dichloropropene-	7.85	79	106399	45.61	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	91.22%
47) 2-Hexanone-d5	8.31	63	238400	101.96	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	101.96%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	320385	46.43	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	92.86%
64) 1,2-Dichlorobenzene-d4	11.85	152	224956	47.26	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	94.52%

Target Compounds

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
10) 1,1,2-Trichloro-1,2,2-trif	2.25	101	2217	0.581	ug/L #	25
13) Acetone	2.29	43	5458	1.416	ug/L	45
25) Chloroform	4.67	83	16808	2.073	ug/L	99
29) Cyclohexane	4.98	56	222957	30.593	ug/L	87
33) Benzene	5.39	78	35867	2.143	ug/L	100
35) Methylcyclohexane	6.41	83	334500	52.812	ug/L	96
37) 1,2-Dichloropropane	6.41	63	4151	0.876	ug/L	99
39) cis-1,3-Dichloropropene	7.23	75	6714	0.996	ug/L #	53
42) Toluene	7.64	91	24541	1.437	ug/L	99
45) 1,1,2-Trichloroethane	8.04	97	32005	7.965	ug/L #	17
48) 2-Hexanone	8.32	43	109447	18.411	ug/L #	39
52) Ethylbenzene	9.25	91	247856	13.312	ug/L	98
53) m,p-Xylene	9.37	106	173237	26.679	ug/L	99
54) o-xylene	9.77	106	22706	3.515	ug/L	94
56) Isopropylbenzene	10.16	105	49184	2.892	ug/L	98
59) 1,2,3-Trichloropropane	11.48	75	31936	5.628	ug/L	90
69) Naphthalene	13.74	128	101538	6.590	ug/L	100

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU040519\
Data File : VU030703.D
Acq On : 04 Apr 2019 23:14
Operator : JC/SP
Sample : K2168-13DL 5X
Misc : 6.26g/5mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF638DL

Quant Time: Apr 05 02:22:51 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Apr 05 02:15:56 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
--------------------	------	------	----------	------	-------	----------


-----	-----	-----	-----	-----	-----	-----
-----	-----	-----	-----	-----	-----	-----


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU040519\
Data File : VU030703.D
Acq On : 04 Apr 2019 23:14
Operator : JC/SP
Sample : K2168-13DL 5X
Misc : 6.26g/5mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF638DL

Quant Time: Apr 05 02:22:51 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Apr 05 02:15:56 2019
Response via : Initial Calibration

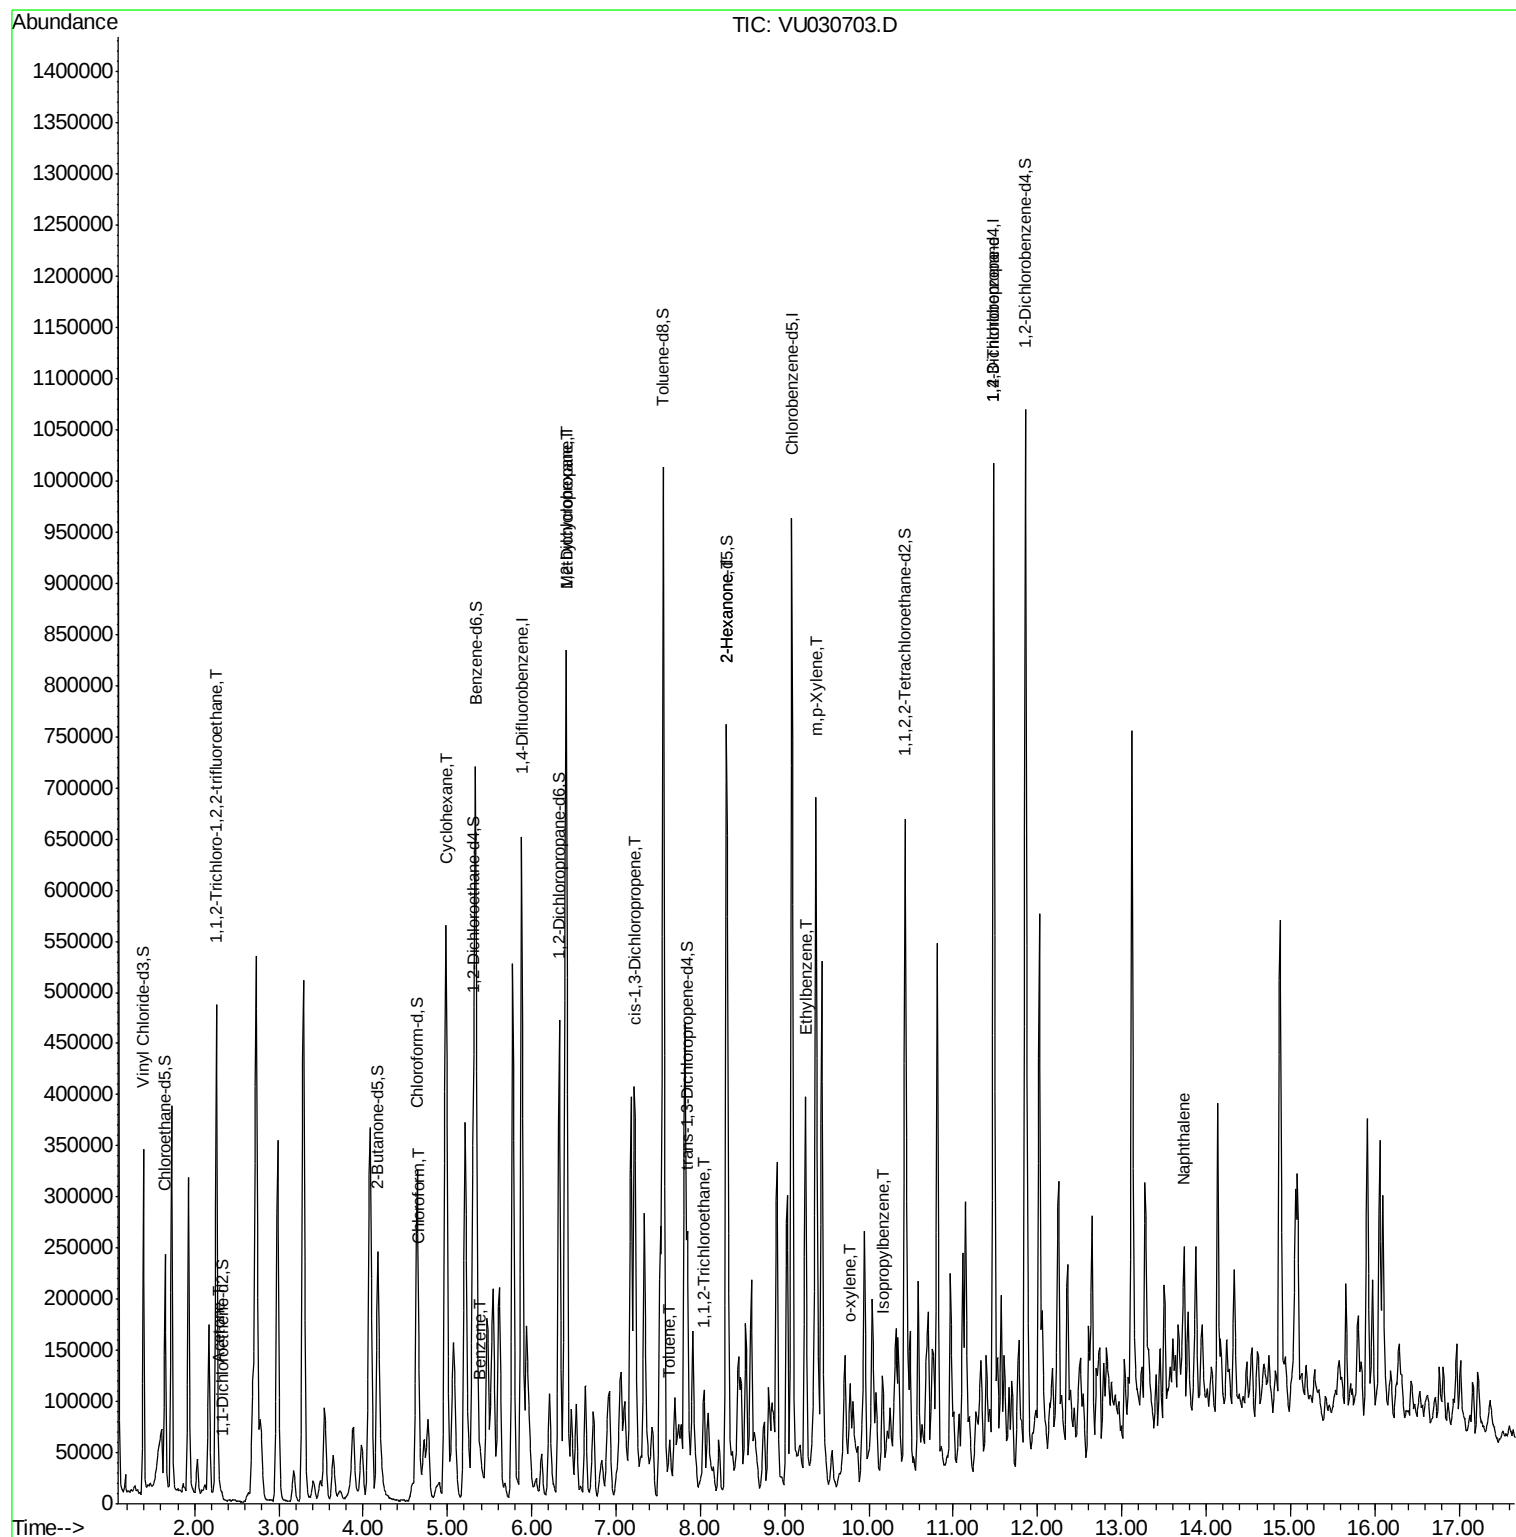

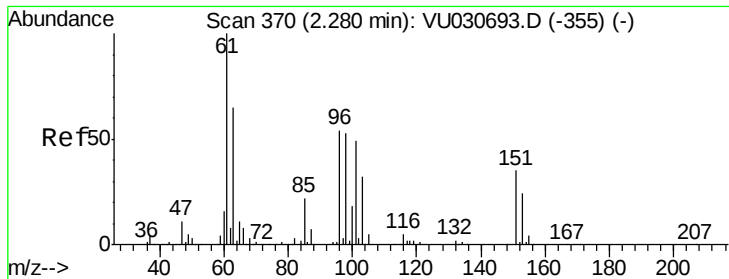

#10

1,1,2-Trichloro-1,2,2-trifluoroethane

Concen: 0.581 ug/L

RT: 2.25 min Scan# 362

Delta R.T. -0.03 min

Lab File: VU030703.D

Acq: 04 Apr 2019 23:14

Instrument :

MSVOA_U

ClientSampleId :

BF638DL


Tot Ion:101 Resp: 2217

Ion Ratio Lower Upper

101 100

85 0.0 36.8 55.2#




151 5.8 57.4 86.0#

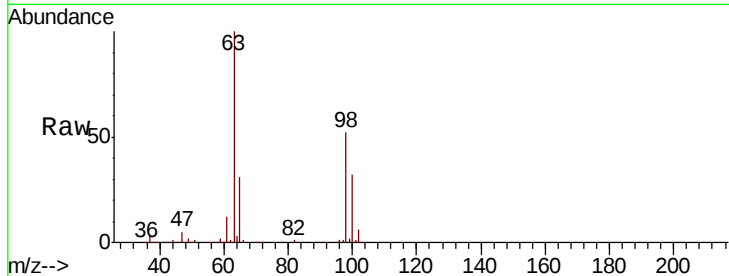

Abundance Ion 101.00 (100.70 to 101.70): V

Ion 85.00 (84.70 to 85.70): VU0

Ion 151.00 (150.70 to 151.70): V

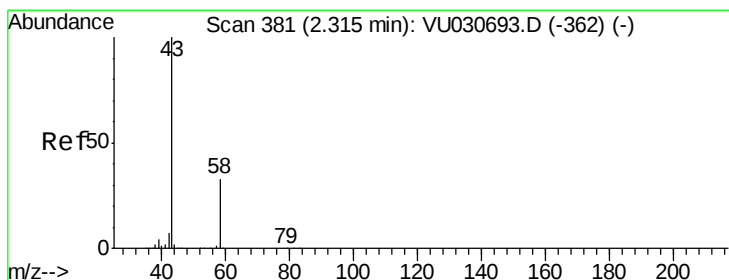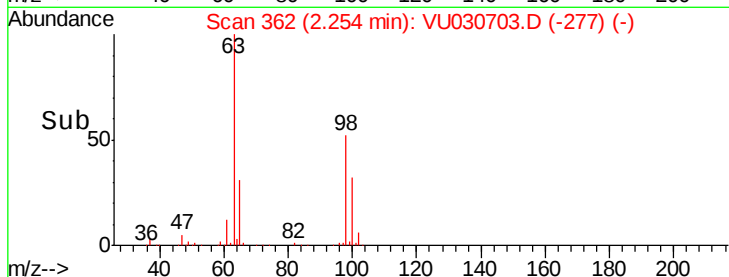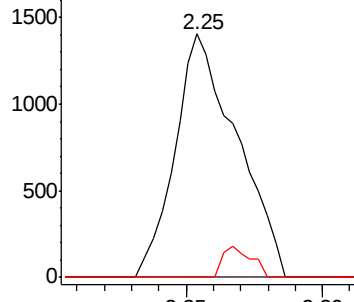

#13

Acetone

Concen: 1.416 ug/L

RT: 2.29 min Scan# 373

Delta R.T. -0.03 min

Lab File: VU030703.D


Acq: 04 Apr 2019 23:14

Tgt Ion: 43 Resp: 5458

Ion Ratio Lower Upper



43 100


58 1.3 0.0 64.0

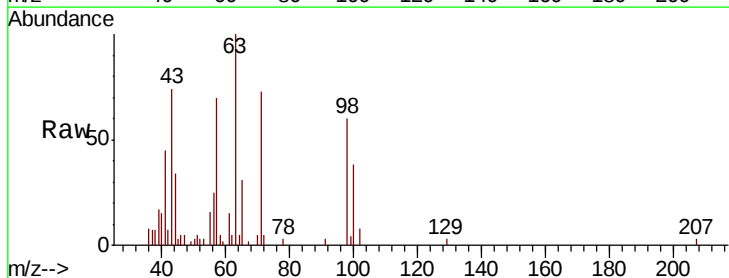

Abundance Ion 43.00 (42.70 to 43.70): VU0

Ion 58.00 (57.70 to 58.70): VU0



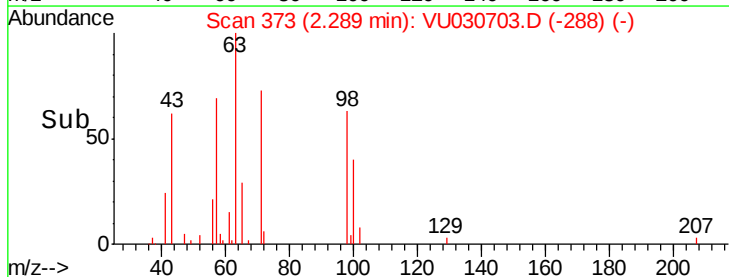
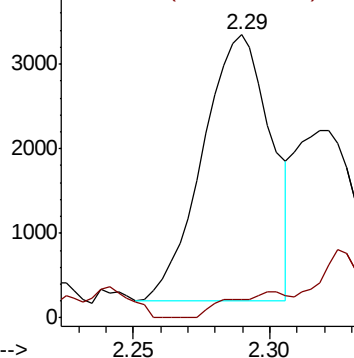


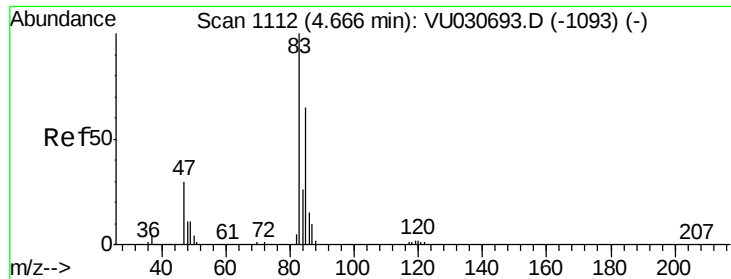

#25
Chloroform
Concen: 2.073 ug/L
RT: 4.67 min Scan# 1112
Delta R.T. -0.00 min
Lab File: VU030703.D
Acq: 04 Apr 2019 23:14




Instrument :
MSVOA_U
ClientSampled :
BF638DL


Tot Ion: 83 Resp: 16808
Ion Ratio Lower Upper
83 100
85 66.2 45.8 85.0

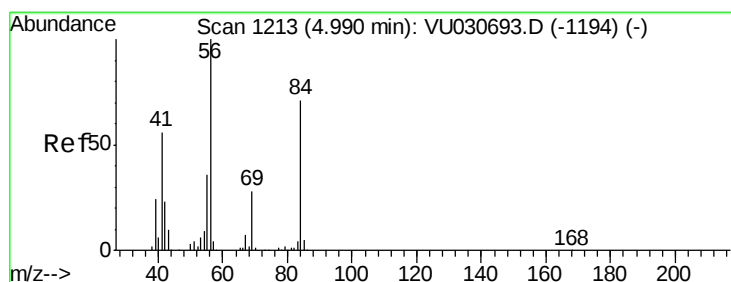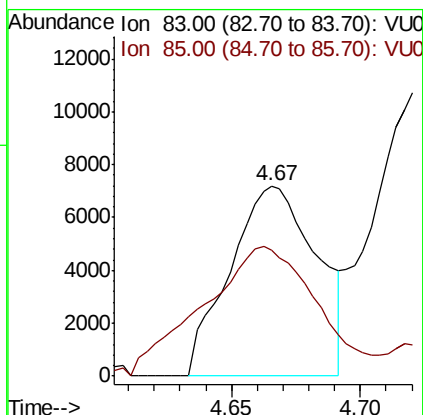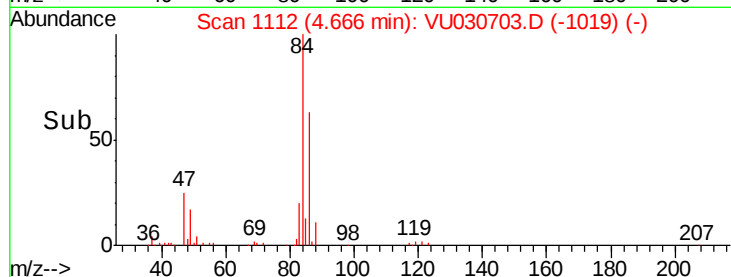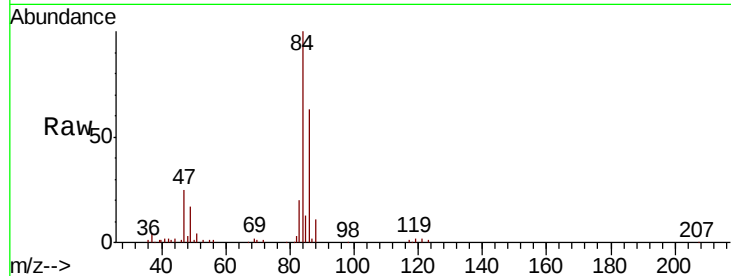

#29
Cyclohexane
Concen: 30.593 ug/L
RT: 4.98 min Scan# 1211
Delta R.T. -0.01 min
Lab File: VU030703.D
Acq: 04 Apr 2019 23:14

Tgt Ion: 56 Resp: 222957
Ion Ratio Lower Upper
56 100
69 22.7 22.0 33.0
84 60.8 58.2 87.2

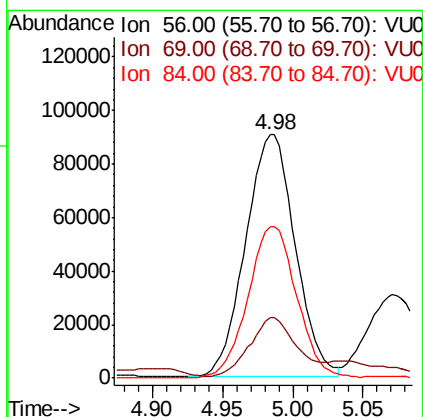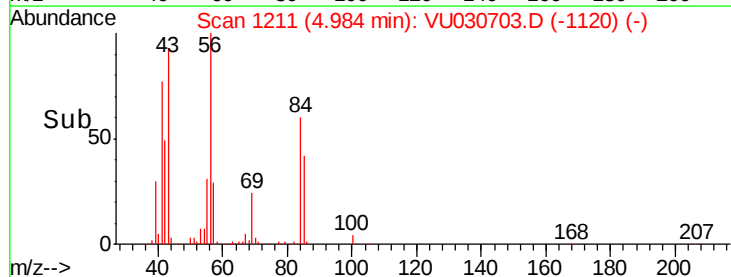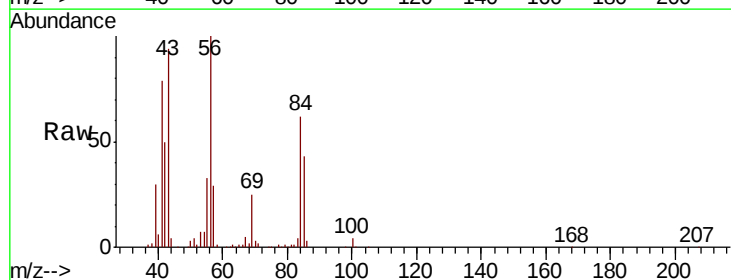


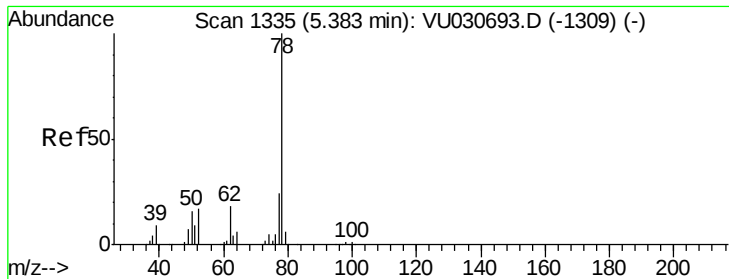




#33
Benzene
Concen: 2.143 ug/L
RT: 5.39 min Scan# 1336
Delta R.T. 0.00 min
Lab File: VU030703.D
Acq: 04 Apr 2019 23:14

Instrument :
MSVOA_U
ClientSampleId :
BF638DL

Tgt Ion: 78 Resp: 35867

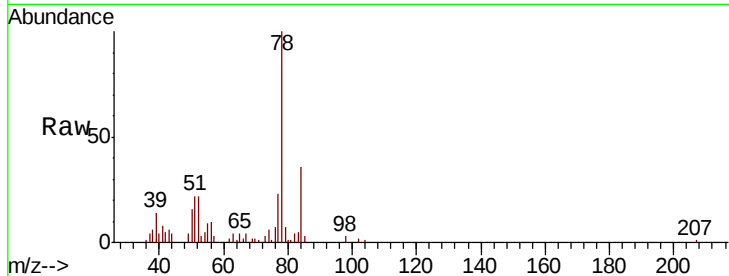


Abundance Ion 78.00 (77.70 to 78.70): VU0

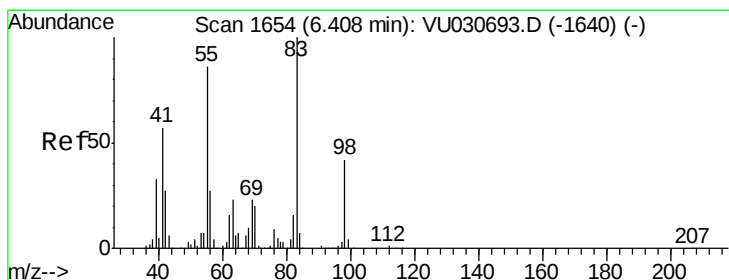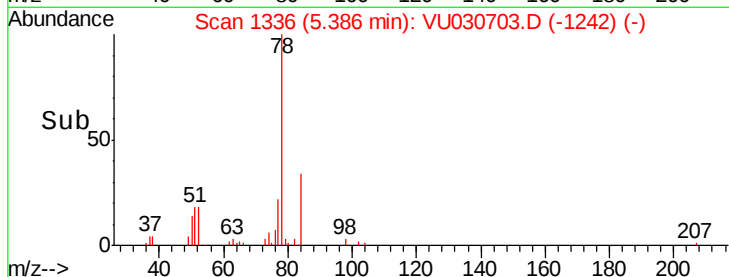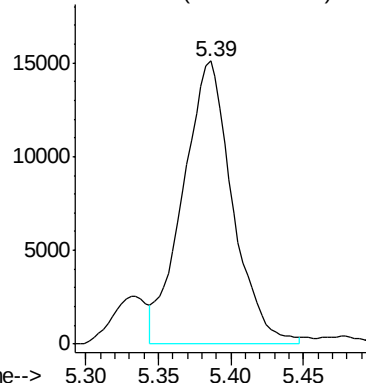



#35
Methylcyclohexane
Concen: 52.812 ug/L
RT: 6.41 min Scan# 1654
Delta R.T. -0.00 min
Lab File: VU030703.D
Acq: 04 Apr 2019 23:14


Tgt Ion: 83 Resp: 334500
Ion Ratio Lower Upper
83 100
55 94.5 71.6 107.4
98 43.7 35.4 53.0

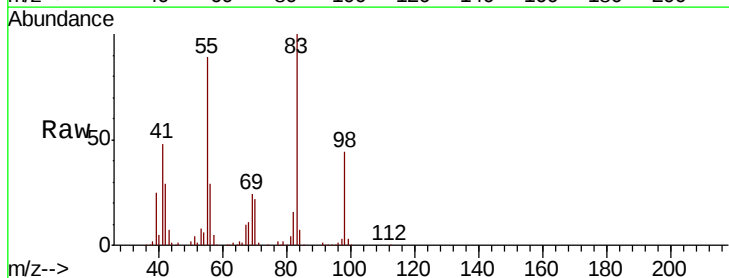

Abundance Ion 83.00 (82.70 to 83.70): VU0

Ion 55.00 (54.70 to 55.70): VU0
Ion 98.00 (97.70 to 98.70): VU0



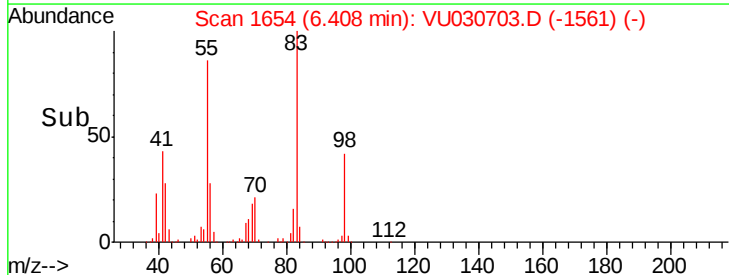
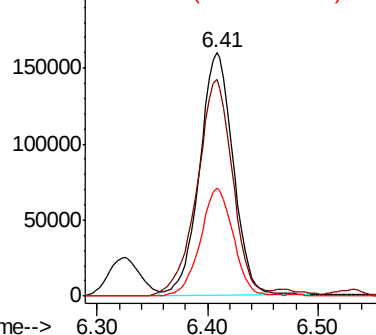


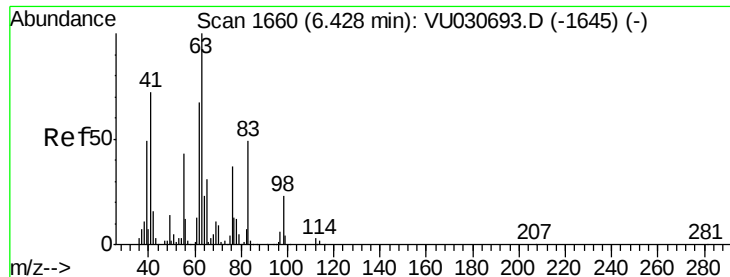

#37
 1,2-Dichloropropane
 Concen: 0.876 ug/L
 RT: 6.41 min Scan# 1653
 Delta R.T. -0.02 min
 Lab File: VU030703.D
 Acq: 04 Apr 2019 23:14




Instrument :
 MSVOA_U
 ClientSampleId :
 BF638DL


Tot Ion: 63 Resp: 4151
 Ion Ratio Lower Upper
 63 100
 112 3.4 3.0 4.4

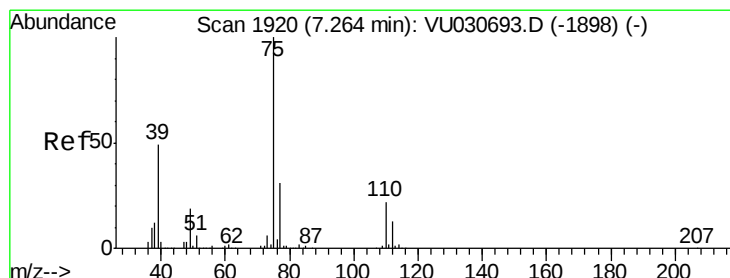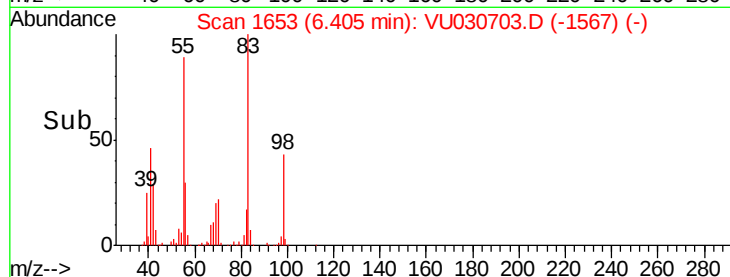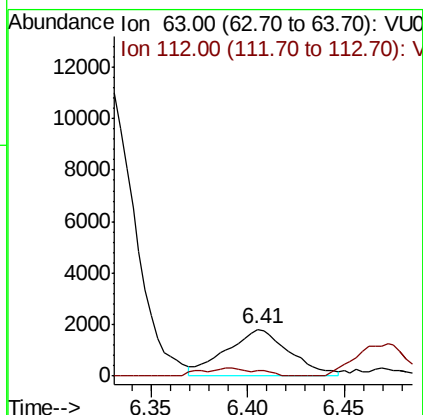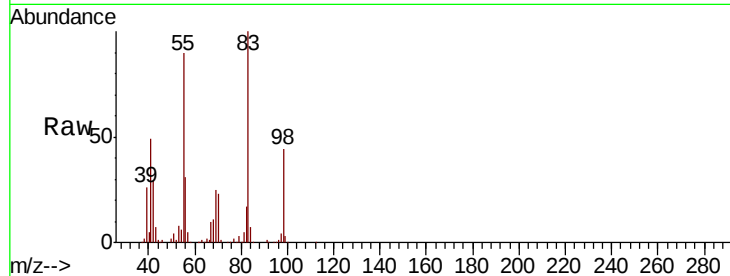

#39
 cis-1,3-Dichloropropene
 Concen: 0.996 ug/L
 RT: 7.23 min Scan# 1909
 Delta R.T. -0.04 min
 Lab File: VU030703.D
 Acq: 04 Apr 2019 23:14

Tgt Ion: 75 Resp: 6714
 Ion Ratio Lower Upper
 75 100
 77 59.7 23.1 42.9#

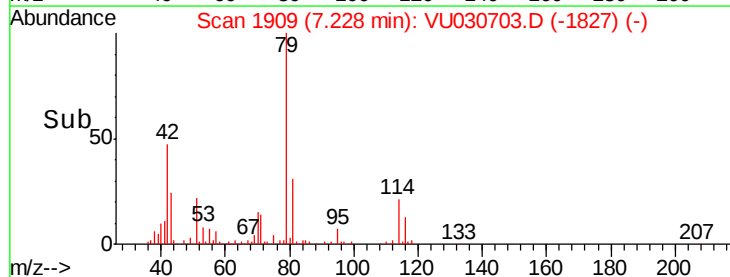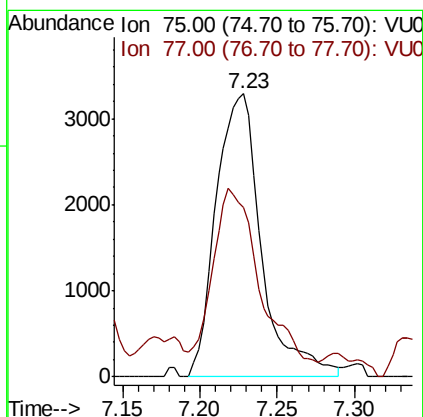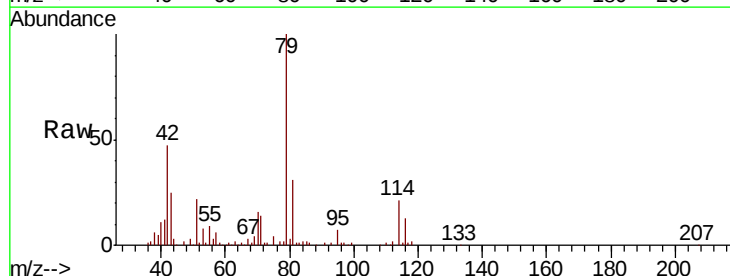

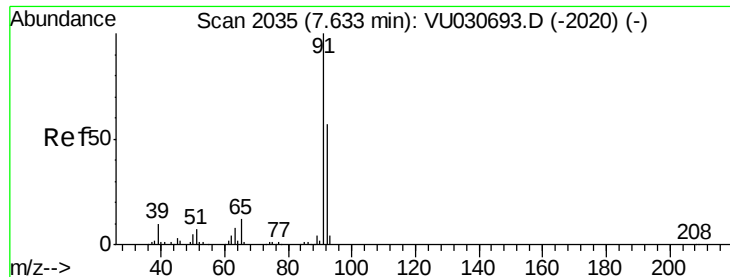

#42

Toluene

Concen: 1.437 ug/L

RT: 7.64 min Scan# 2036

Delta R.T. 0.00 min

Lab File: VU030703.D

Acq: 04 Apr 2019 23:14

Instrument :

MSVOA_U

ClientSampleId :


BF638DL

Tot Ion: 91 Resp: 24541




Ion Ratio Lower Upper

91 100

92 56.6 40.0 74.4

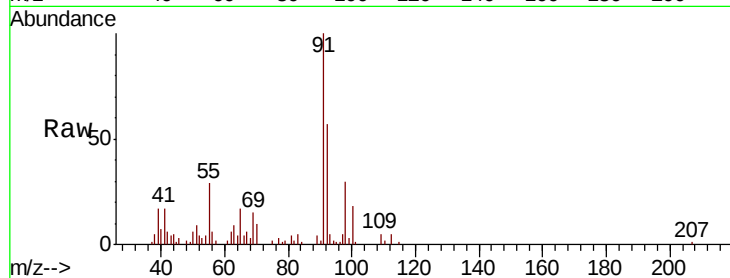

Abundance Ion 91.00 (90.70 to 91.70): VU030703.D (-1942) (-)

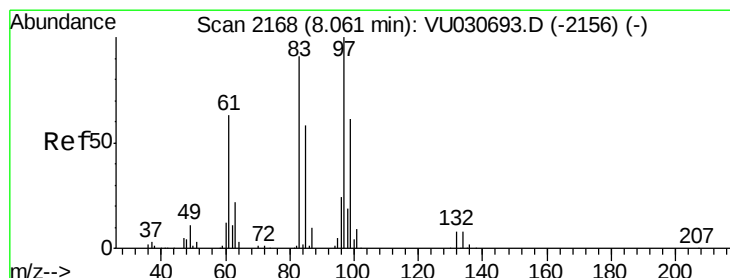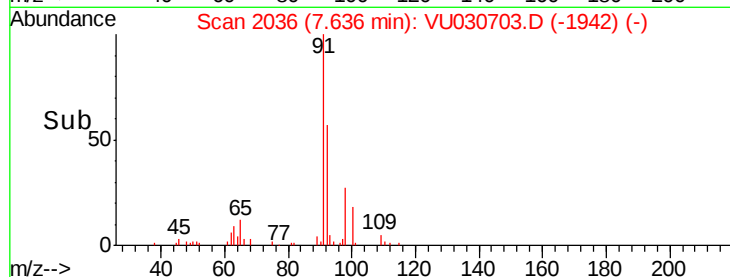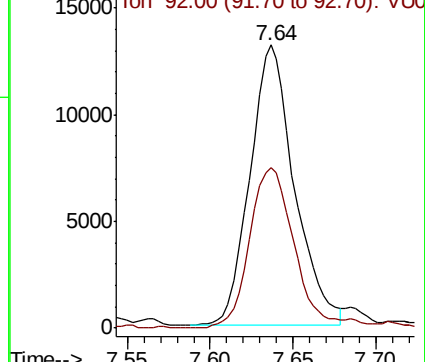

#45

1,1,2-Trichloroethane

Concen: 7.965 ug/L

RT: 8.04 min Scan# 2162

Delta R.T. -0.02 min

Lab File: VU030703.D

Acq: 04 Apr 2019 23:14

Tgt Ion: 97 Resp: 32005


Ion Ratio Lower Upper

97 100



99 0.0 44.0 81.8#


83 10.4 65.3 121.3#

85 0.6 42.5 78.9#

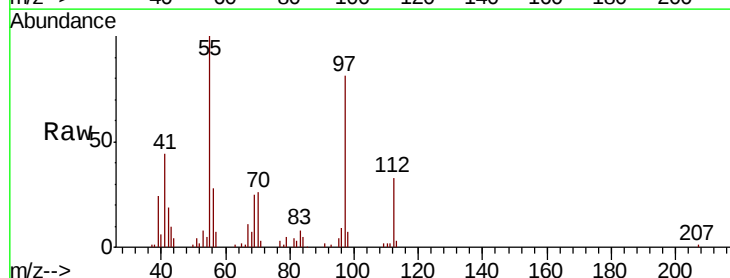

Abundance Ion 97.00 (96.70 to 97.70): VU030703.D (-2075) (-)



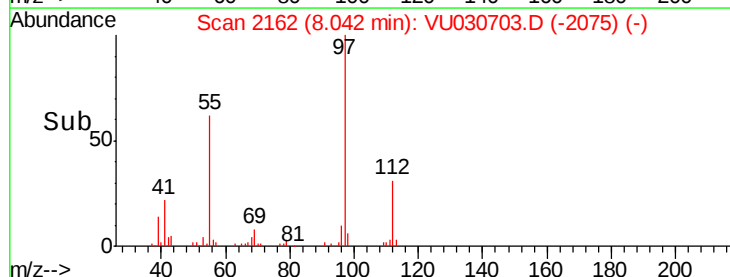
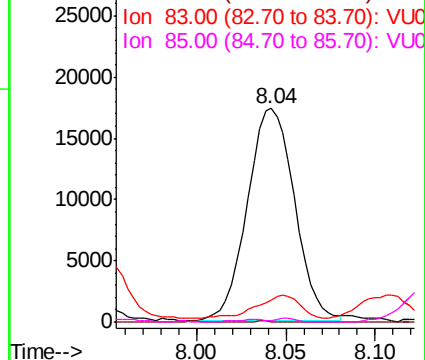


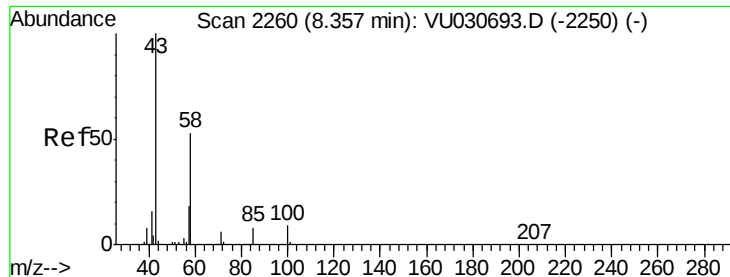

#48
2-Hexanone
Concen: 18.411 ug/L
RT: 8.32 min Scan# 2249
Delta R.T. -0.04 min
Lab File: VU030703.D
Acq: 04 Apr 2019 23:14




Instrument :
MSVOA_U
ClientSampleId :
BF638DL


Tot Ion	Ratio	Lower	Upper
43	100		
58	10.5	41.9	62.9#
57	54.7	14.3	21.5#
100	0.1	7.1	10.7#

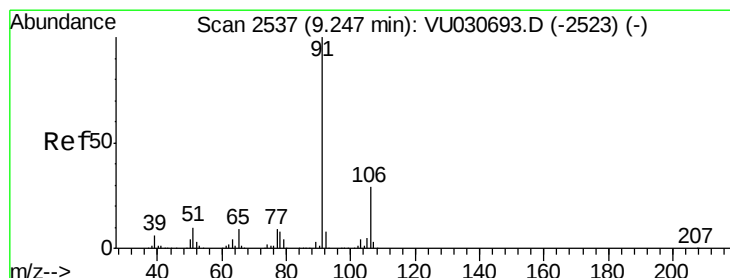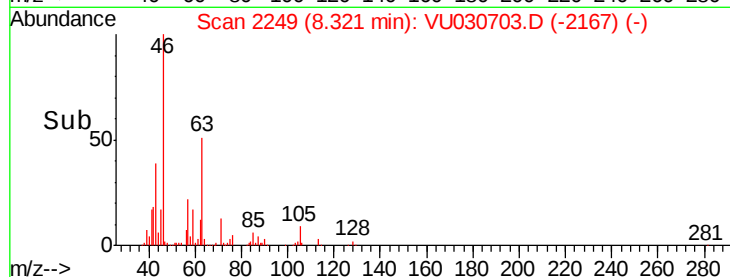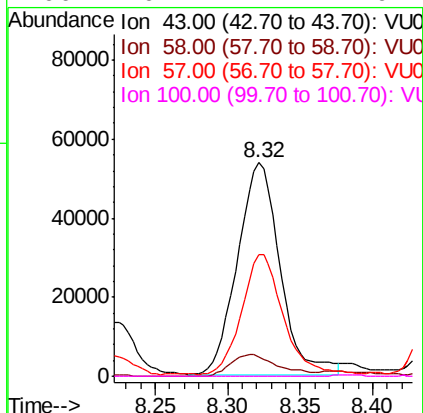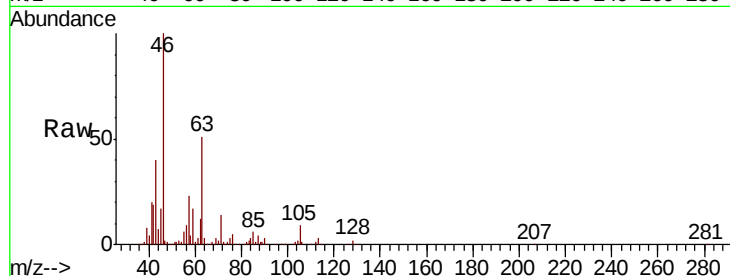

#52
Ethylbenzene
Concen: 13.312 ug/L
RT: 9.25 min Scan# 2537
Delta R.T. -0.00 min
Lab File: VU030703.D
Acq: 04 Apr 2019 23:14

Tgt Ion	Ratio	Lower	Upper
91	100		
106	29.9	20.4	37.8

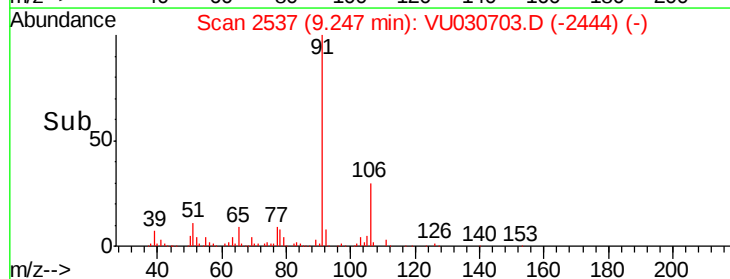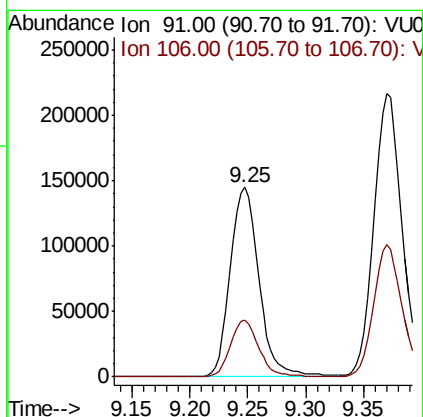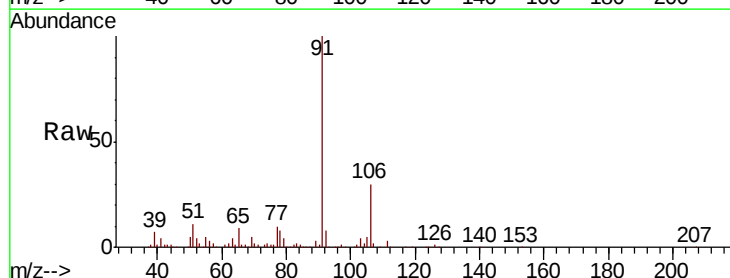

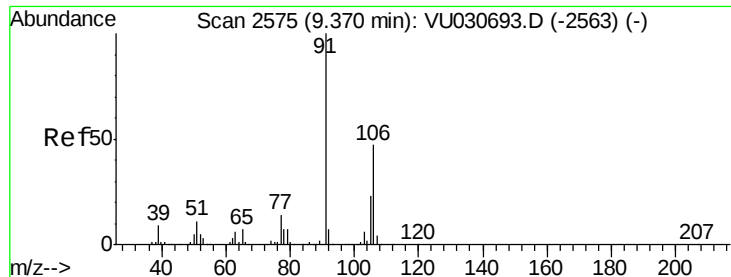

#53

m,p-Xylene

Concen: 26.679 ug/L

RT: 9.37 min Scan# 2575

Delta R.T. -0.00 min

Lab File: VU030703.D

Acq: 04 Apr 2019 23:14

Instrument :

MSVOA_U

ClientSampled :


BF638DL

Tot Ion:106 Resp: 173237

Ion Ratio Lower Upper




106 100

91 213.2 148.0 274.8

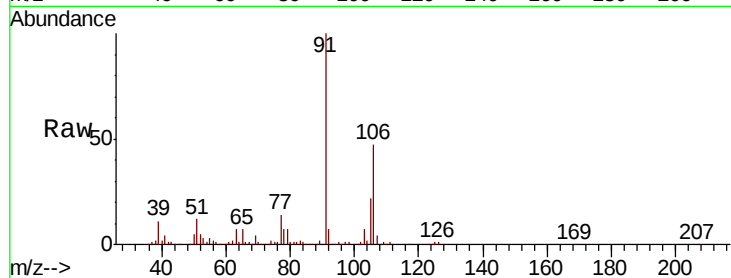

Abundance Ion 106.00 (105.70 to 106.70): V

Ion 91.00 (90.70 to 91.70): VU0

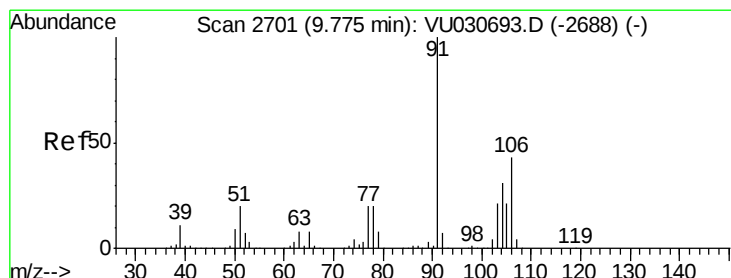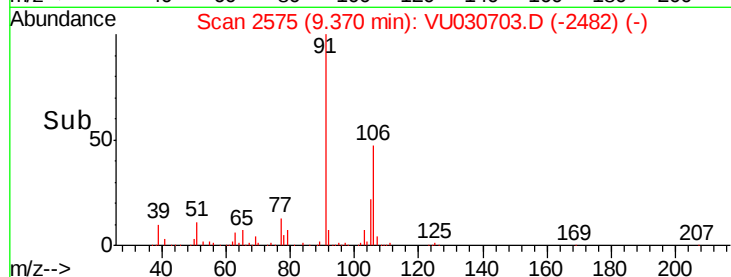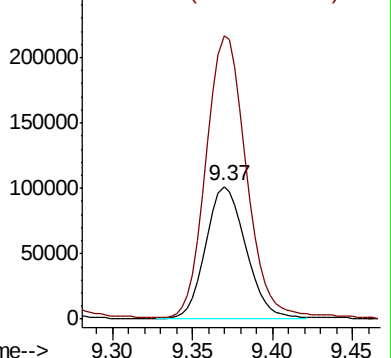

#54

o-xylene

Concen: 3.515 ug/L

RT: 9.77 min Scan# 2701

Delta R.T. -0.00 min

Lab File: VU030703.D


Acq: 04 Apr 2019 23:14

Tgt Ion:106 Resp: 22706

Ion Ratio Lower Upper



106 100


91 234.0 156.7 290.9

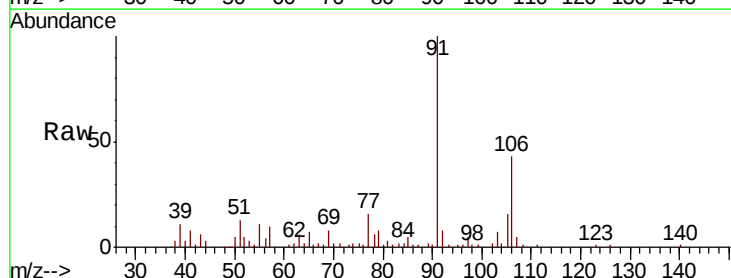

Abundance Ion 106.00 (105.70 to 106.70): V

Ion 91.00 (90.70 to 91.70): VU0

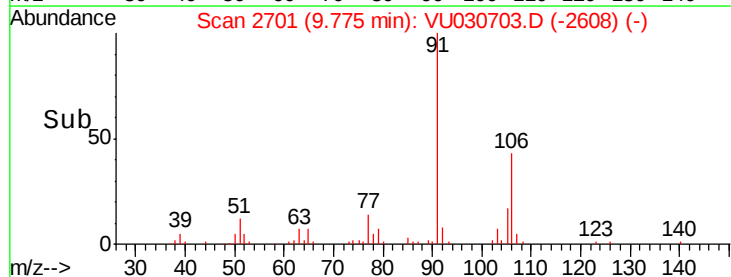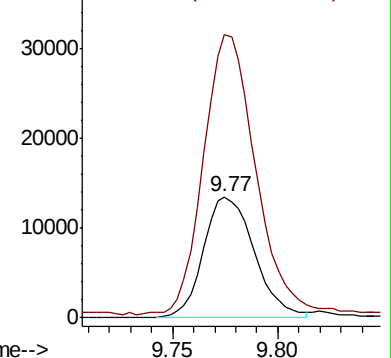

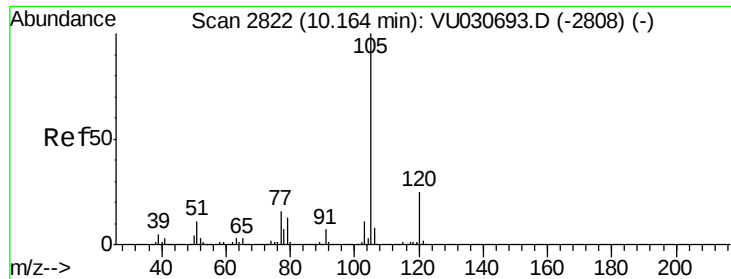

#56

Isopropylbenzene

Concen: 2.892 ug/L

RT: 10.16 min Scan# 2822

Delta R.T. -0.00 min

Lab File: VU030703.D

Acq: 04 Apr 2019 23:14

Instrument :

MSVOA_U

ClientSampleId :

BF638DL


Tot Ion:105 Resp: 49184

Ion Ratio Lower Upper

105 100

120 24.4 20.4 30.6




77 17.3 13.4 20.2

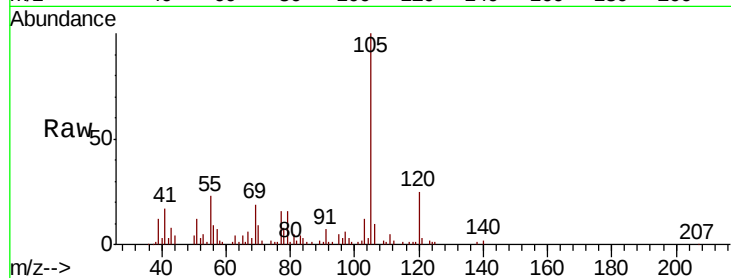

Abundance Ion 105.00 (104.70 to 105.70): V

Ion 120.00 (119.70 to 120.70): V

Ion 77.00 (76.70 to 77.70): VU

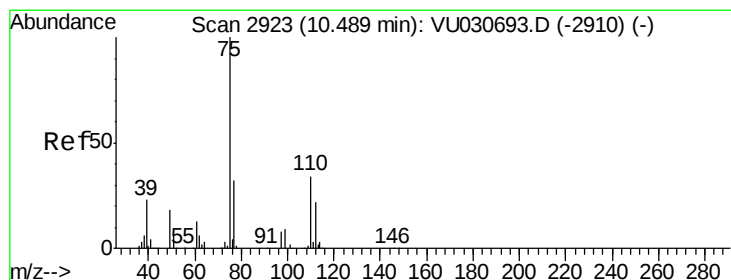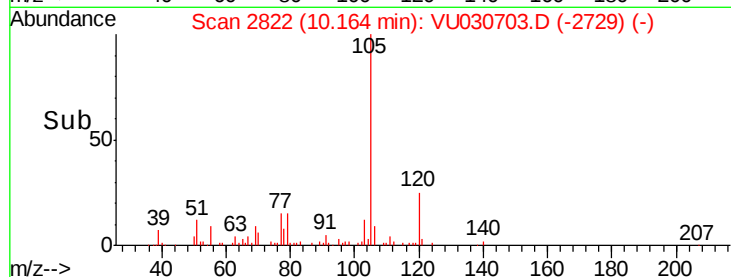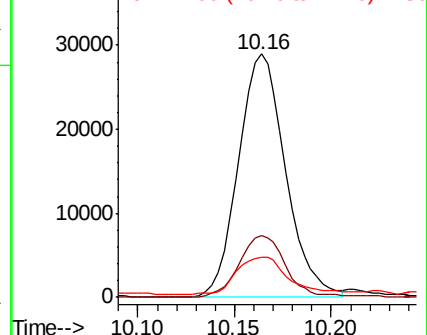

#59

1,2,3-Trichloropropane

Concen: 5.628 ug/L

RT: 11.48 min Scan# 3231

Delta R.T. 0.99 min

Lab File: VU030703.D


Acq: 04 Apr 2019 23:14

Tgt Ion: 75 Resp: 31936

Ion Ratio Lower Upper



75 100


77 38.0 26.1 39.1

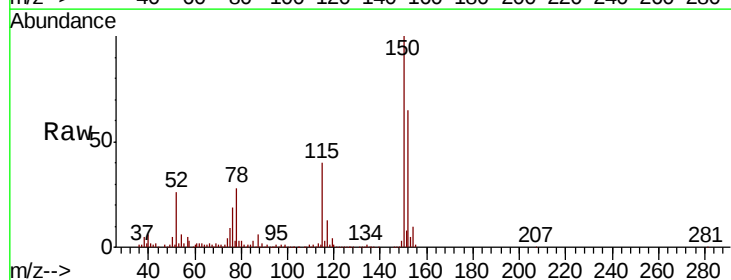

Abundance Ion 75.00 (74.70 to 75.70): VU

Ion 77.00 (76.70 to 77.70): VU

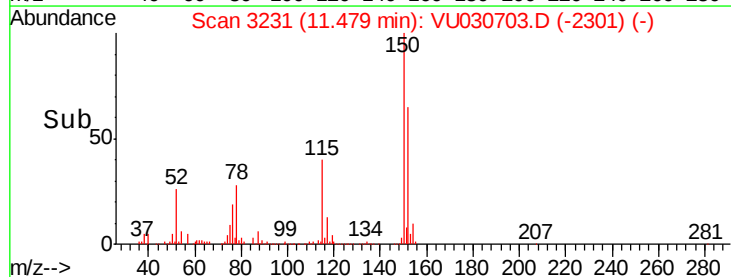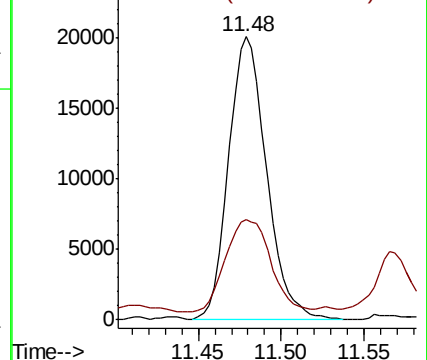

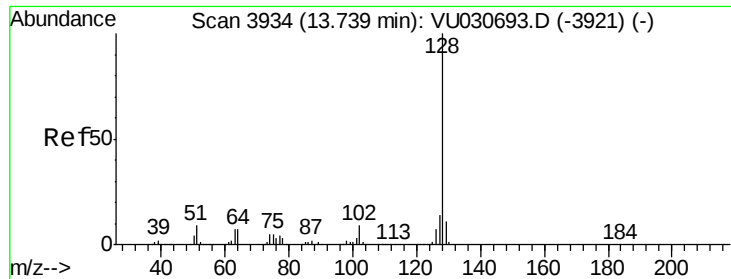

#69

Naphthalene

Concen: 6.590 ug/L

RT: 13.74 min Scan# 3935

Delta R.T. 0.00 min

Lab File: VU030703.D

Acq: 04 Apr 2019 23:14

Instrument :

MSVOA_U

ClientSampleId :

BF638DL


Tot Ion:128 Resp: 101538

Ion Ratio Lower Upper

128 100

127 13.1 10.4 15.6

129 10.5 8.6 12.8

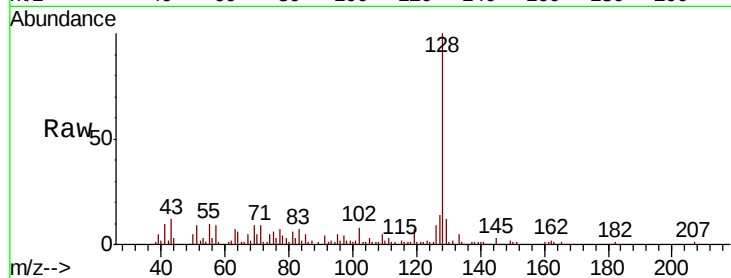

Abundance

Ion 128.00 (127.70 to 128.70): V

Ion 127.00 (126.70 to 127.70): V

Ion 129.00 (128.70 to 129.70): V

