


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU040519\
Data File : VU030696.D
Acq On : 04 Apr 2019 20:33
Operator : JC/SP
Sample : K2166-16ME
Misc : 5.64µ/5mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF0M6ME

Manual Integrations
APPROVED

MMDadoda
4/5/2019 10:01:44 AM

Quant Time: Apr 05 02:37:13 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Apr 05 02:15:56 2019
Response via : Initial Calibration

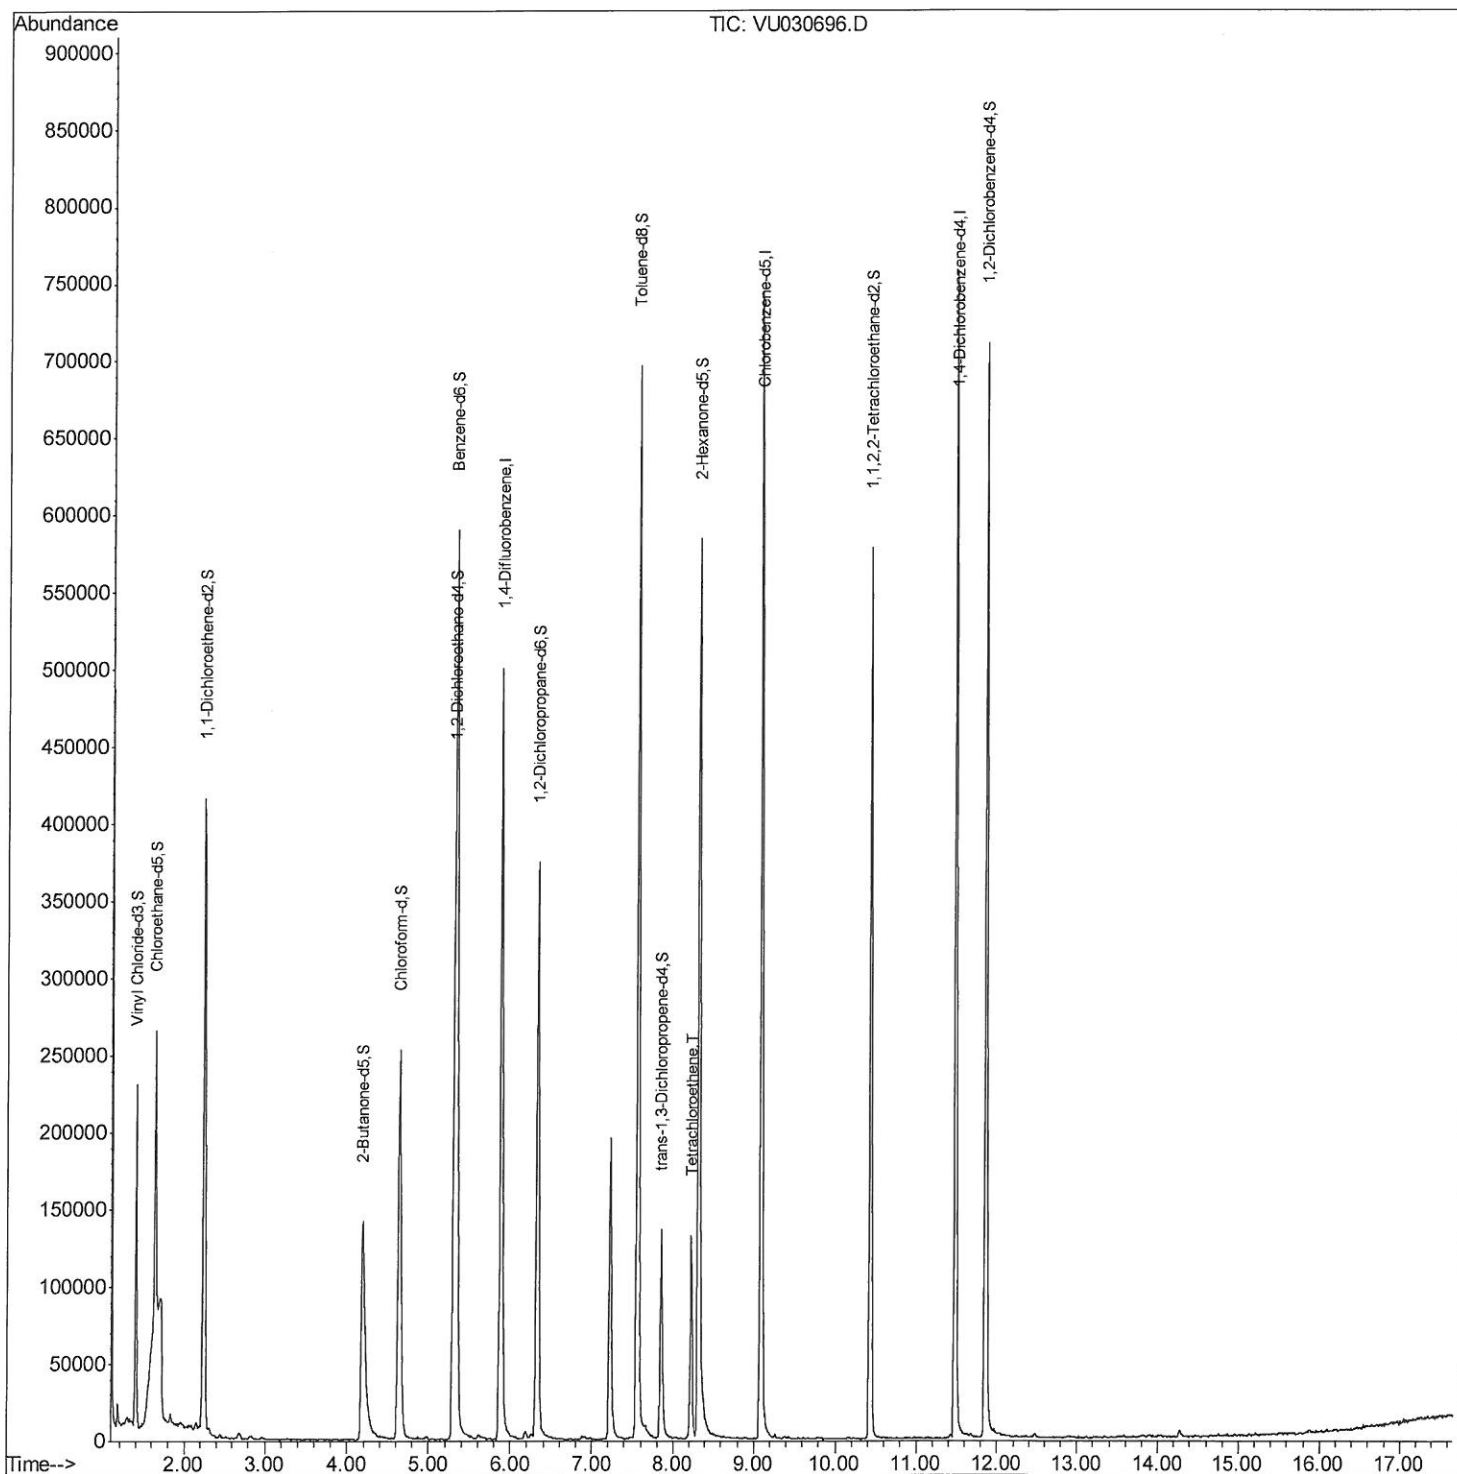

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU040519\
Data File : VU030696.D
Acq On : 04 Apr 2019 20:33
Operator : JC/SP
Sample : K2166-16ME
Misc : 5.64µ/5mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF0M6ME

Manual Integrations
APPROVED

MMDadoda
4/5/2019 10:01:44 AM

Quant Time: Apr 05 02:21:51 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Apr 05 02:15:56 2019
Response via : Initial Calibration

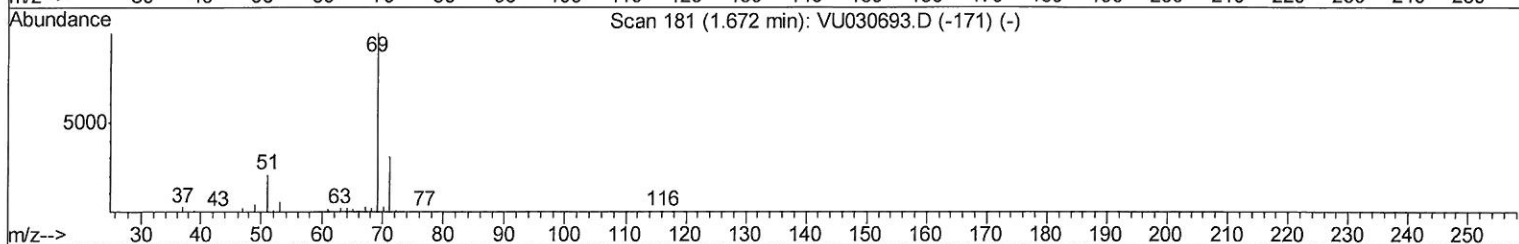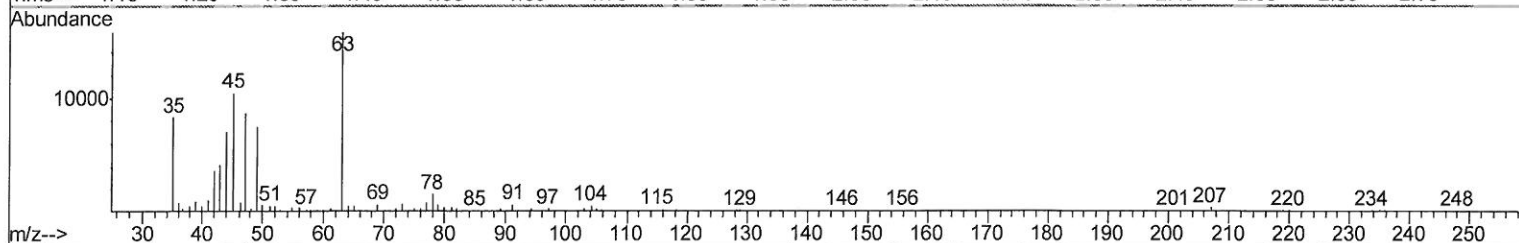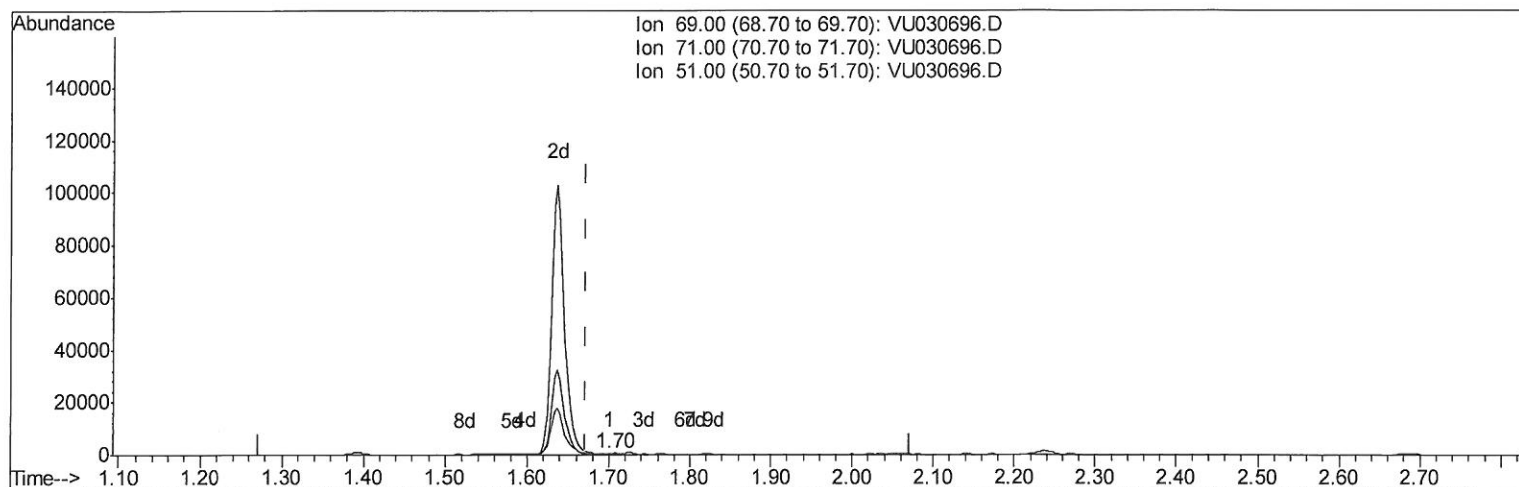

TIC: VU030696.D

(7) Chloroethane-d5 (S)

1.701min (+0.029) 0.24ug/L

response 679

Ion	Exp%	Act%
69.00	100	100
71.00	31.60	28.28
51.00	27.70	33.73
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU040519\
Data File : VU030696.D
Acq On : 04 Apr 2019 20:33
Operator : JC/SP
Sample : K2166-16ME
Misc : 5.64g/5mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF0M6ME

Manual Integrations
APPROVED

MMDadoda
4/5/2019 10:01:44 AM

Quant Time: Apr 05 02:21:51 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Apr 05 02:15:56 2019
Response via : Initial Calibration

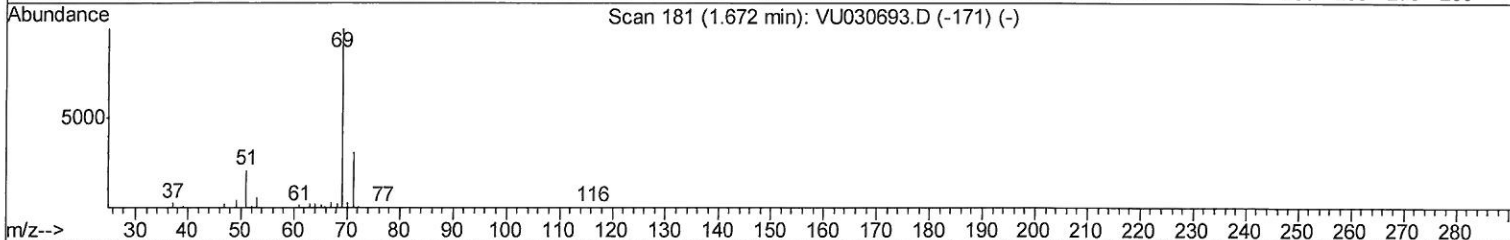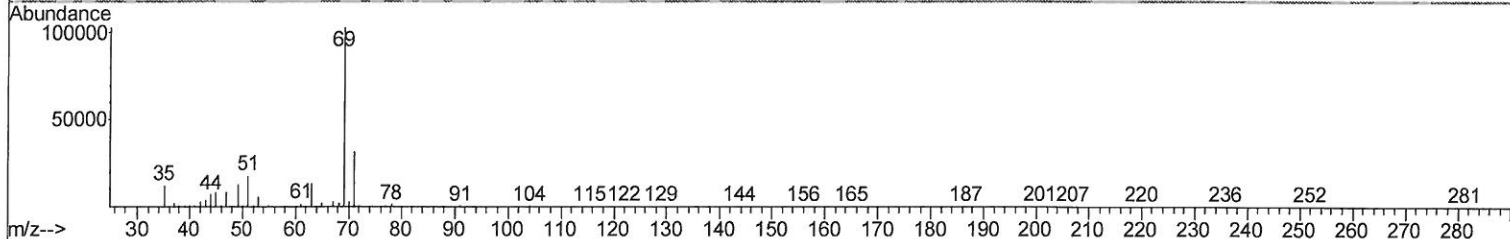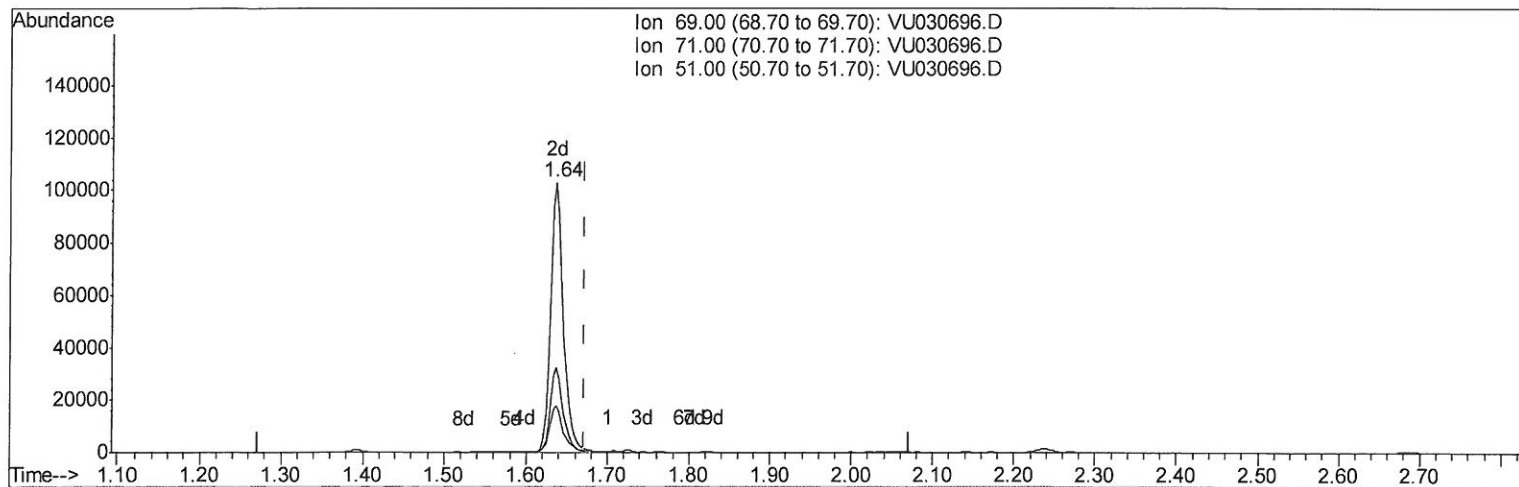

TIC: VU030696.D

(7) Chloroethane-d5 (S)

1.637min (-0.036) 40.37ug/L m

response 115063

Ion	Exp%	Act%
69.00	100	100
71.00	31.60	0.17#
51.00	27.70	0.20#
0.00	0.00	0.00

7MO
4/6/19

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\UU040519\
 Data File : VU030696.D
 Acq On : 04 Apr 2019 20:33
 Operator : JC/SP
 Sample : K2166-16ME
 Misc : 5.64g/5mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF0M6ME

Manual Integrations
 APPROVED

MMDadoda
 4/5/2019 10:01:44 AM

Quant Time: Apr 05 02:37:13 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Apr 05 02:15:56 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	420712	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	412170	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	192215	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.39	65	162321	43.22	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	86.44%		
7) Chloroethane-d5	1.64	69	115063m	40.37	ug/L	-0.04
Spiked Amount 50.000	Range 70 - 130		Recovery =	80.74%		
11) 1,1-Dichloroethene-d2	2.24	63	242647	35.72	ug/L	-0.03
Spiked Amount 50.000	Range 60 - 125		Recovery =	71.44%		
21) 2-Butanone-d5	4.18	46	308358	103.60	ug/L	0.01
Spiked Amount 100.000	Range 40 - 130		Recovery =	103.60%		
24) Chloroform-d	4.64	84	254593	44.38	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	88.76%		
26) 1,2-Dichloroethane-d4	5.30	65	187892	48.00	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	96.00%		
32) Benzene-d6	5.33	84	562631	46.76	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	93.52%		
36) 1,2-Dichloropropane-d6	6.32	67	197825	47.97	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	95.94%		
41) Toluene-d8	7.56	98	476692	44.70	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	89.40%		
43) trans-1,3-Dichloropropene-	7.85	79	86394	45.95	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	91.90%		
47) 2-Hexanone-d5	8.32	63	214059	113.58	ug/L	0.01
Spiked Amount 100.000	Range 45 - 130		Recovery =	113.58%		
57) 1,1,2,2-Tetrachloroethane-	10.43	84	295404	53.11	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	106.22%		
64) 1,2-Dichlorobenzene-d4	11.86	152	185916	49.18	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	98.36%		

7 MD
 4/6/19

Target Compounds					Ovalue
46) Tetrachloroethene	8.22	164	30019	12.481 ug/L	93

(#) = qualifier out of range (m) = manual integration (+) = signals summed