


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU040519\
Data File : VU030703.D
Acq On : 04 Apr 2019 23:14
Operator : JC/SP
Sample : K2168-13DL 5X
Misc : 6.26µ/5mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleID :
BF638DL

Manual Integrations
APPROVED

MMDadoda
4/5/2019 10:21:13 AM

Quant Time: Apr 05 03:50:49 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Apr 05 02:15:56 2019
Response via : Initial Calibration

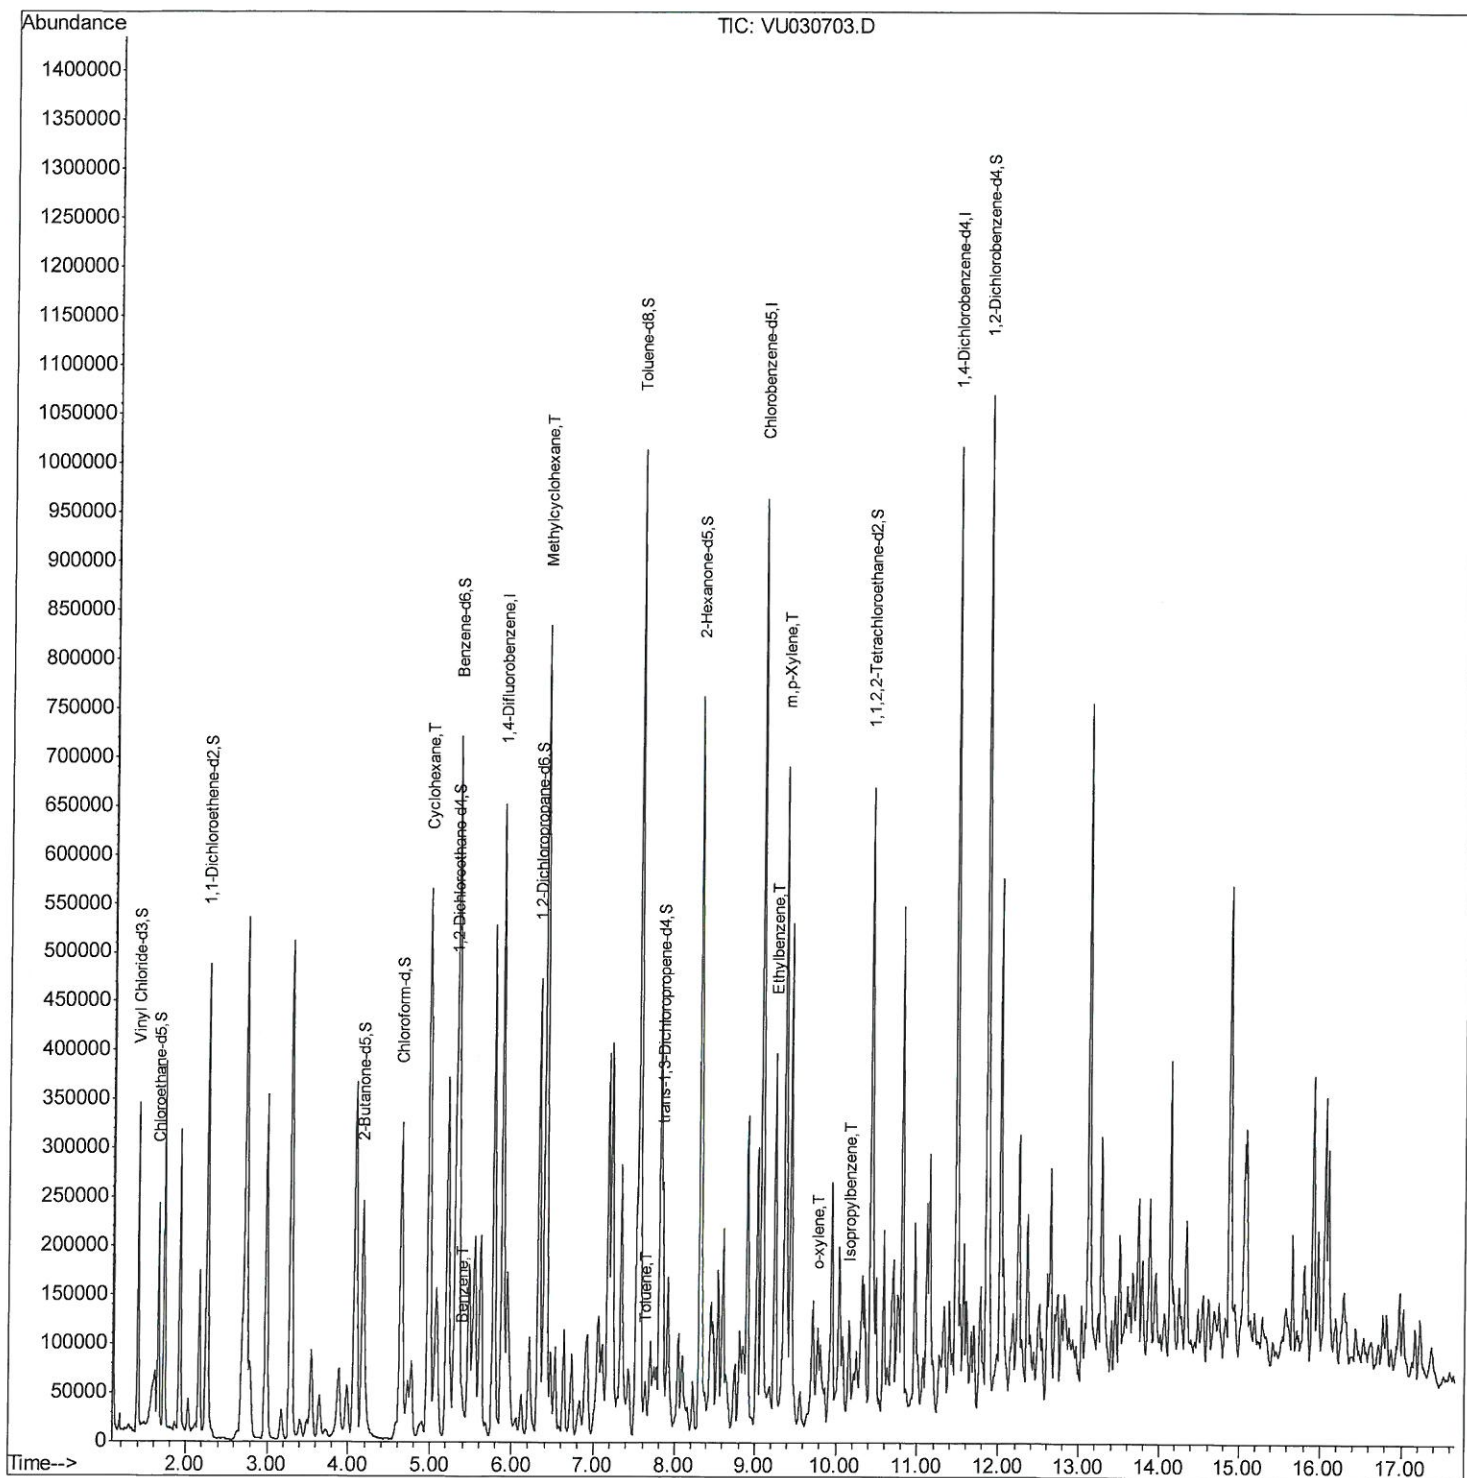

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU040519\
 Data File : VU030703.D
 Acq On : 04 Apr 2019 23:14
 Operator : JC/SP
 Sample : K2168-13DL 5X
 Misc : 6.26g/5mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
ClientSampleId :
 BF638DL

Manual Integrations
APPROVED

MMDadoda
 4/5/2019 10:21:13 AM

Quant Time: Apr 05 02:22:51 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Apr 05 02:15:56 2019
 Response via : Initial Calibration

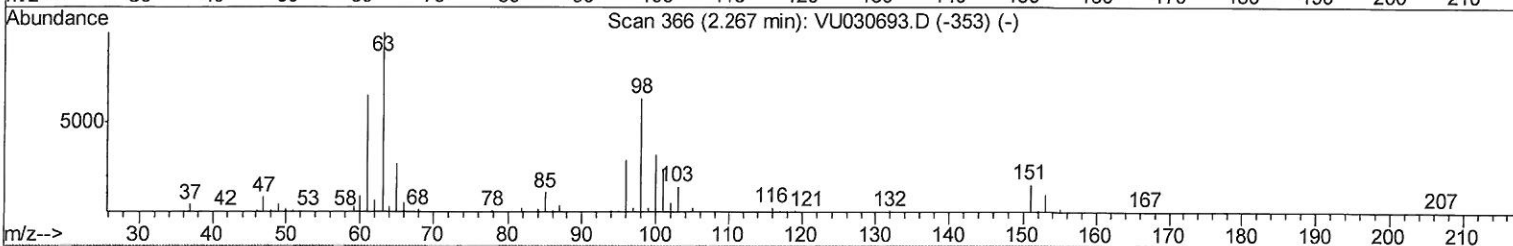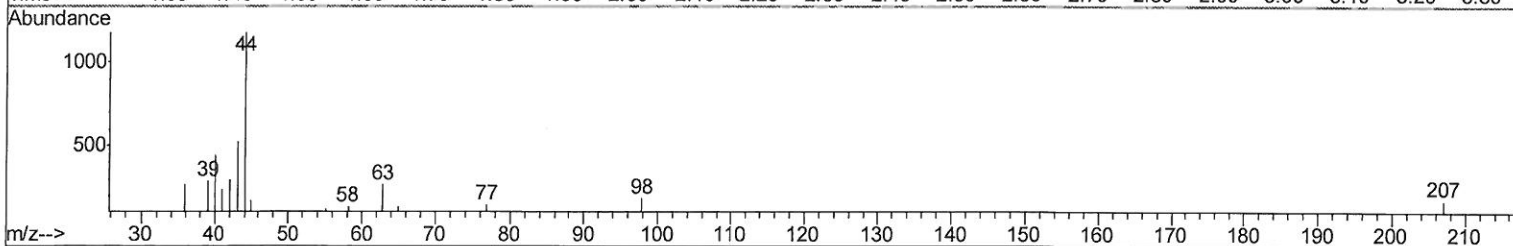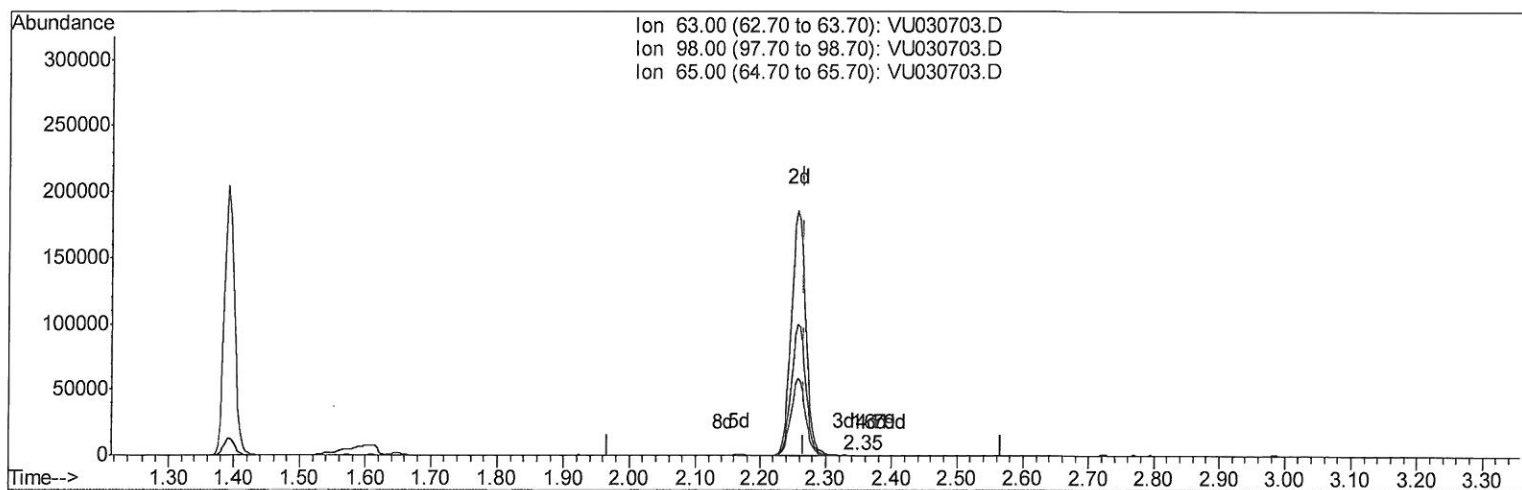

TIC: VU030703.D

(11) 1,1-Dichloroethene-d2 (S)

2.347min (+0.080) 0.02ug/L

response 212

Ion	Exp%	Act%
63.00	100	100
98.00	67.20	55.66
65.00	24.00	23.58
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU040519\
Data File : VU030703.D
Acq On : 04 Apr 2019 23:14
Operator : JC/SP
Sample : K2168-13DL 5X
Misc : 6.26µ/5mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF638DL

Manual Integrations
APPROVED

MMDadoda
4/5/2019 10:21:13 AM

Quant Time: Apr 05 02:22:51 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Apr 05 02:15:56 2019
Response via : Initial Calibration

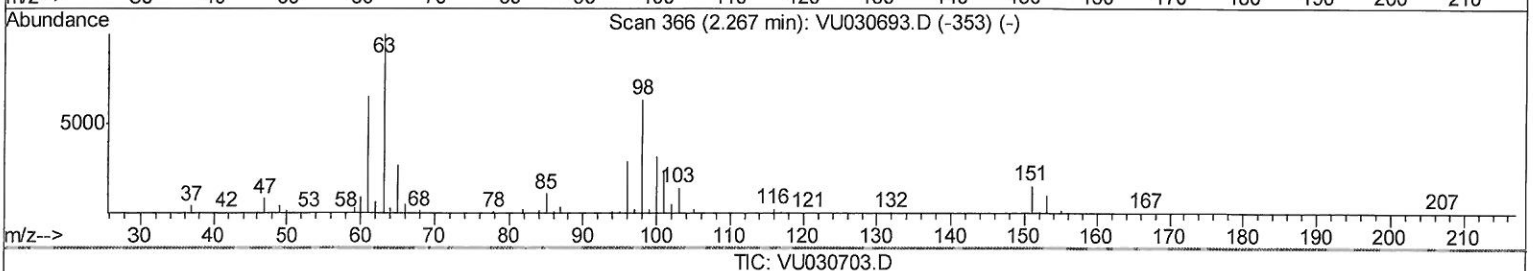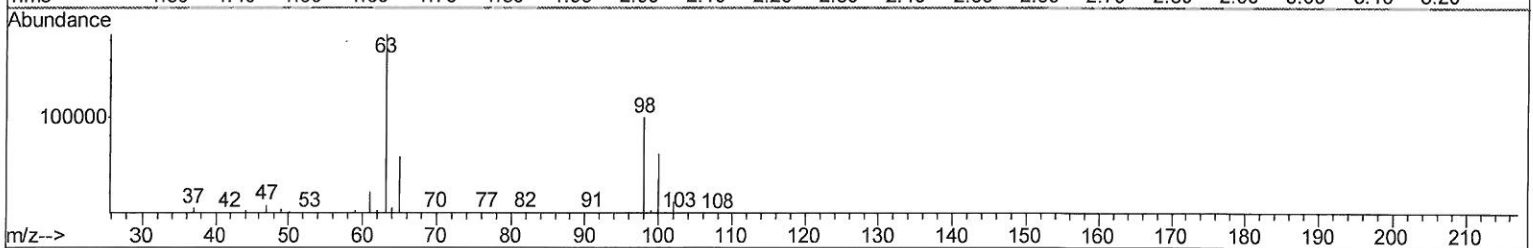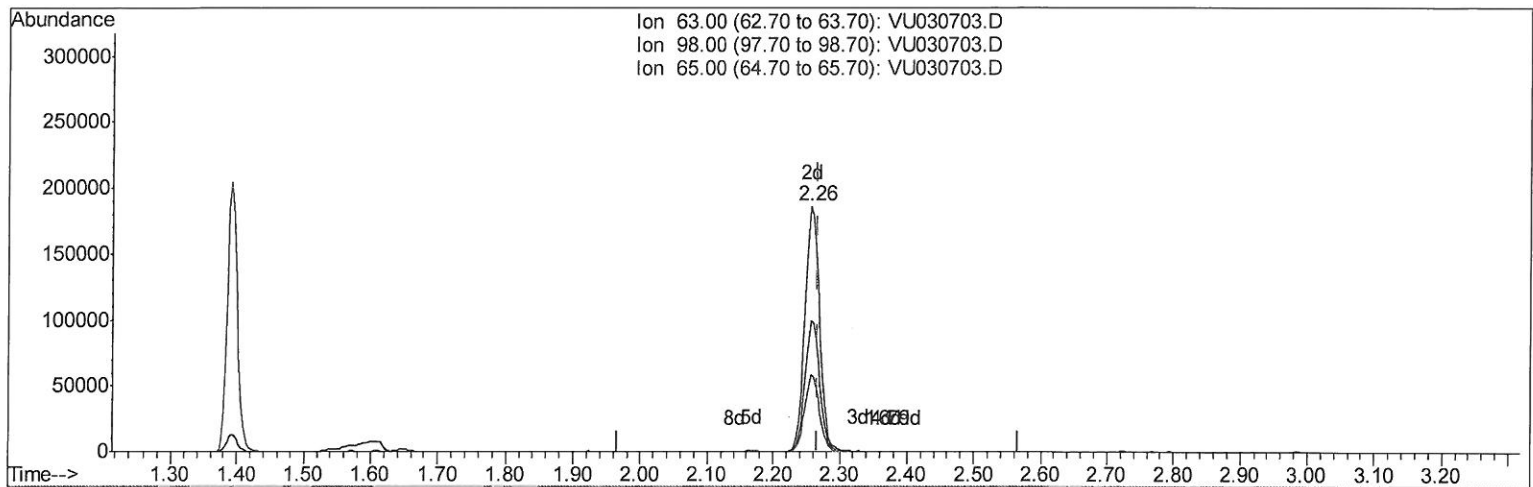

TIC: VU030703.D

(11) 1,1-Dichloroethene-d2 (S)

2.257min (-0.010) 33.13ug/L m

response 284843

Ion	Exp%	Act%
63.00	100	100
98.00	67.20	0.04#
65.00	24.00	0.02#
0.00	0.00	0.00

7MO
4/6/19

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\UU040519\
 Data File : VU030703.D
 Acq On : 04 Apr 2019 23:14
 Operator : JC/SP
 Sample : K2168-13DL 5X
 Misc : 6.26µ/5mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF638DL

Manual Integrations
 APPROVED

MMDadoda
 4/5/2019 10:21:13 AM

Quant Time: Apr 05 03:50:49 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Apr 05 02:15:56 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	532576	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	511336	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	242011	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.39	65	206168	43.37	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	86.74%		
7) Chloroethane-d5	1.65	69	157971	43.78	ug/L	-0.02
Spiked Amount 50.000	Range 70 - 130		Recovery =	87.56%		
11) 1,1-Dichloroethene-d2	2.26	63	284843m	33.13	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	66.26%		
21) 2-Butanone-d5	4.17	46	369551	98.08	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	98.08%		
24) Chloroform-d	4.64	84	317391	43.70	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	87.40%		
26) 1,2-Dichloroethane-d4	5.30	65	225274	45.46	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	90.92%		
32) Benzene-d6	5.33	84	692488	46.39	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	92.78%		
36) 1,2-Dichloropropane-d6	6.32	67	243229	47.55	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	95.10%		
41) Toluene-d8	7.56	98	622492	47.05	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	94.10%		
43) trans-1,3-Dichloropropene-	7.85	79	106399	45.61	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	91.22%		
47) 2-Hexanone-d5	8.31	63	238400	101.96	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	101.96%		
57) 1,1,2,2-Tetrachloroethane-	10.43	84	320385	46.43	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	92.86%		
64) 1,2-Dichlorobenzene-d4	11.85	152	224956	47.26	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	94.52%		

7 MD
 4/6/19

Target Compounds					Ovalue
29) Cyclohexane	4.98	56	222957	30.593	ug/L 87
33) Benzene	5.39	78	35867	2.143	ug/L 100
35) Methylcyclohexane	6.41	83	334500	52.812	ug/L 96
42) Toluene	7.64	91	24541	1.437	ug/L 99
52) Ethylbenzene	9.25	91	247856	13.312	ug/L 98
53) m,p-Xylene	9.37	106	173237	26.679	ug/L 99
54) o-xylene	9.77	106	22706	3.515	ug/L 94
56) Isopropylbenzene	10.16	105	49184	2.892	ug/L 98

(#) = qualifier out of range (m) = manual integration (+) = signals summed