


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU040519\
Data File : VU030733.D
Acq On : 05 Apr 2019 11:14
Operator : JC/SP
Sample : K2271-21
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 50 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DB7E2

Manual Integrations
APPROVED

MMDadoda
4/6/2019 11:08:08 AM

Quant Time: Apr 06 00:43:22 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Apr 05 23:39:17 2019
Response via : Initial Calibration

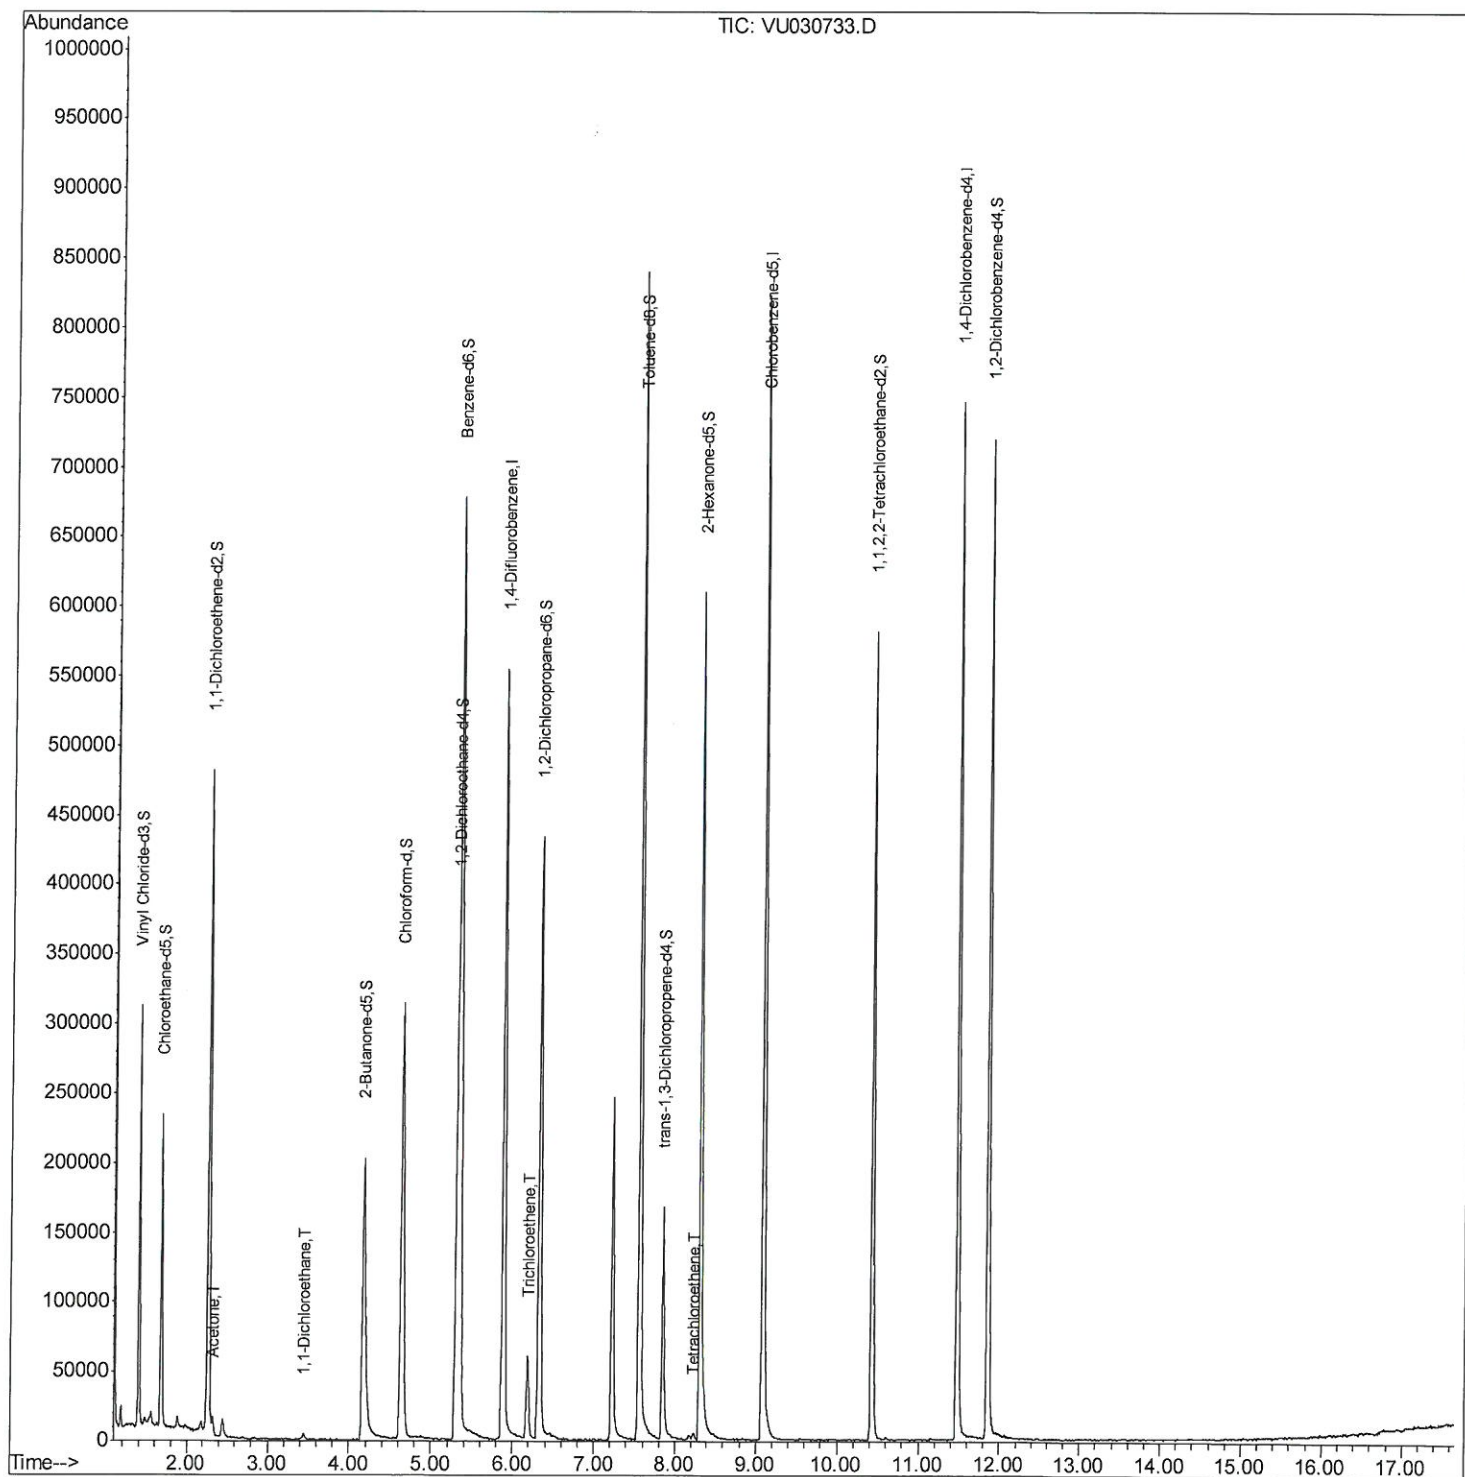

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU040519\
 Data File : VU030733.D
 Acq On : 05 Apr 2019 11:14
 Operator : JC/SP
 Sample : K2271-21
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DB7E2

Manual Integrations
 APPROVED

MMDadoda
 4/6/2019 11:08:08 AM

Quant Time: Apr 05 23:45:42 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Apr 05 23:39:17 2019
 Response via : Initial Calibration

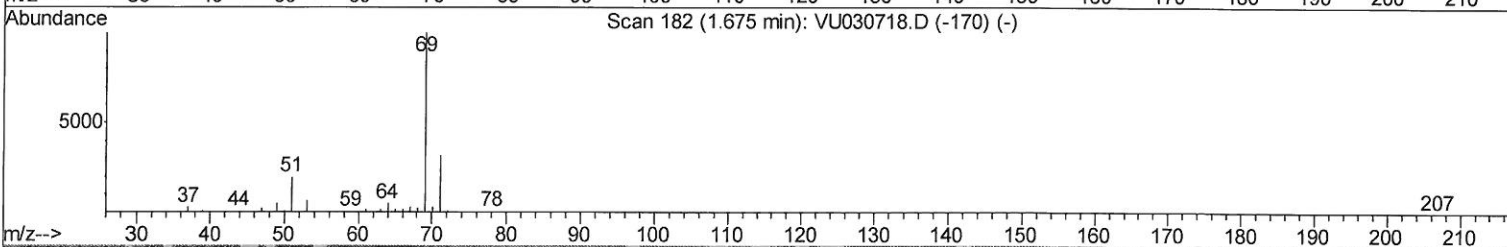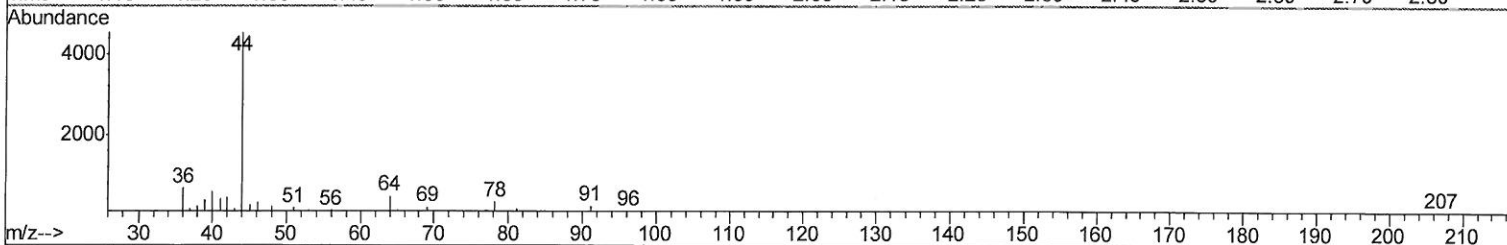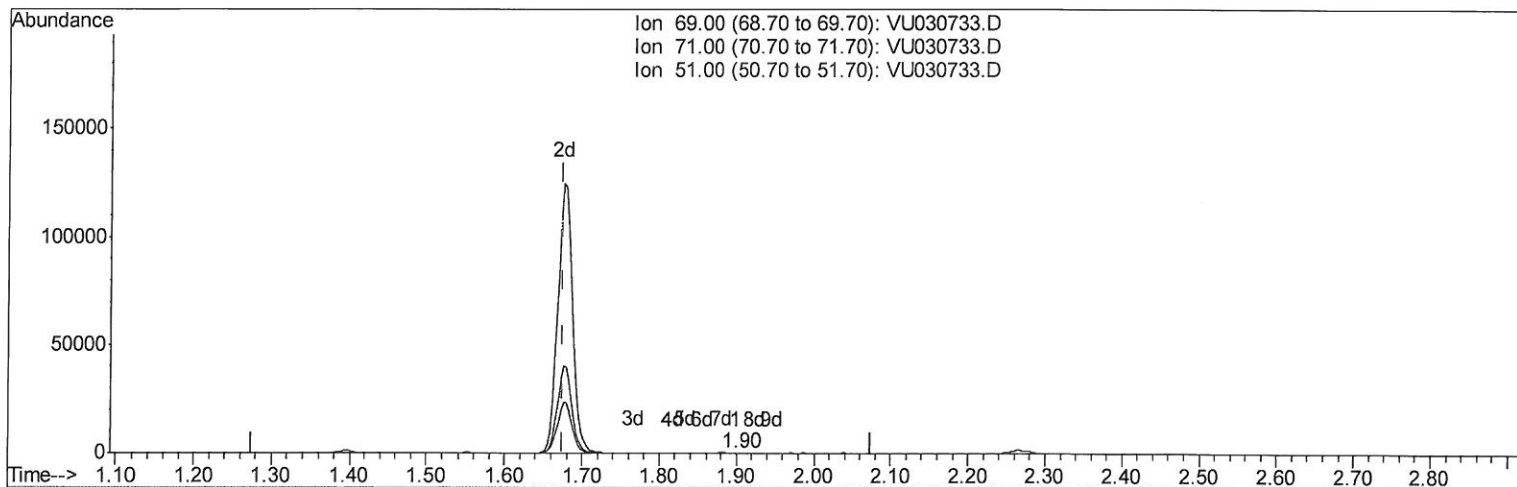

TIC: VU030733.D

(7) Chloroethane-d5 (S)
 1.900min (+0.225) 0.04ug/L
 response 111

Ion	Exp%	Act%
69.00	100	100
71.00	31.60	37.84
51.00	27.70	22.52
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU040519\
Data File : VU030733.D
Acq On : 05 Apr 2019 11:14
Operator : JC/SP
Sample : K2271-21
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 50 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DB7E2

Manual Integrations
APPROVED

MMDadoda
4/6/2019 11:08:08 AM

Quant Time: Apr 05 23:45:42 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Apr 05 23:39:17 2019
Response via : Initial Calibration

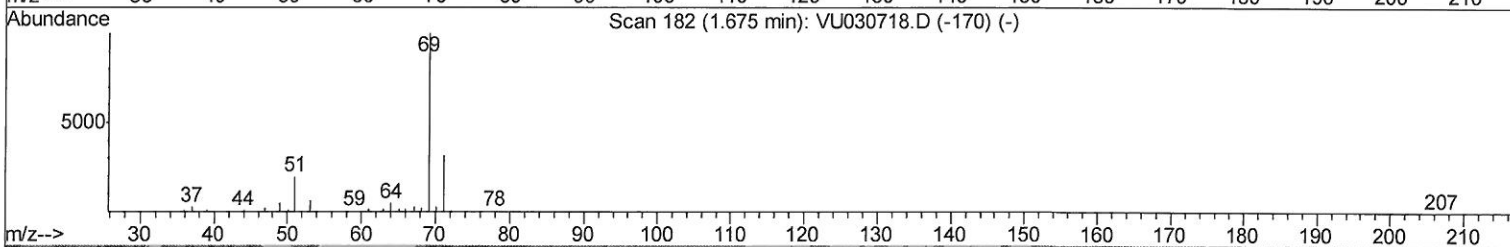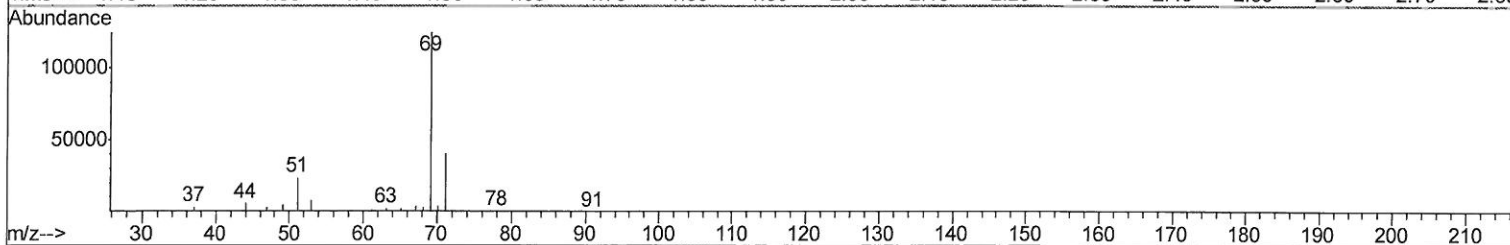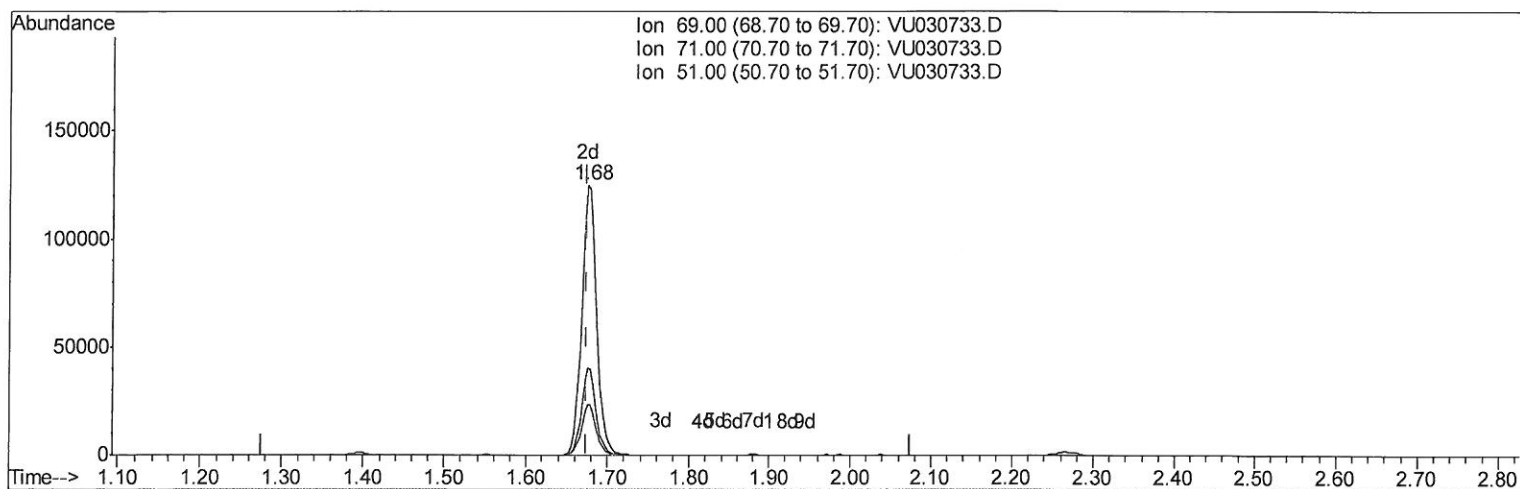

TIC: VU030733.D

(7) Chloroethane-d5 (S)

1.675min (-0.000) 52.24ug/L m

response 160648

Ion	Exp%	Act%
69.00	100	100
71.00	31.60	0.03#
51.00	27.70	0.02#
0.00	0.00	0.00

7 MD
4/6/19

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU040519\
 Data File : VU030733.D
 Acq On : 05 Apr 2019 11:14
 Operator : JC/SP
 Sample : K2271-21
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DB7E2

Manual Integrations
 APPROVED

MMDadoda
 4/6/2019 11:08:08 AM

Quant Time: Apr 06 00:43:22 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Apr 05 23:39:17 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Difluorobenzene	5.88	114	453891	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	450557	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	186449	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	199808	49.31	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	98.62%
7) Chloroethane-d5	1.68	69	160648m	52.24	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	104.48%
11) 1,1-Dichloroethene-d2	2.27	63	283720	38.71	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	77.42%
21) 2-Butanone-d5	4.17	46	351107	109.34	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	109.34%
24) Chloroform-d	4.64	84	307301	49.65	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	99.30%
26) 1,2-Dichloroethane-d4	5.30	65	218046	51.63	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	103.26%
32) Benzene-d6	5.34	84	658823	50.09	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	100.18%
36) 1,2-Dichloropropane-d6	6.32	67	228322	50.65	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	101.30%
41) Toluene-d8	7.56	98	562235	48.23	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	96.46%
43) trans-1,3-Dichloropropene-	7.85	79	101769	49.51	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	99.02%
47) 2-Hexanone-d5	8.31	63	207388	100.66	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	100.66%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	299041	49.18	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	98.36%
64) 1,2-Dichlorobenzene-d4	11.86	152	189920	51.79	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	103.58%

> MO
 4/6/19

Target Compounds

					Ovalue
13) Acetone	2.32	43	9325	2.838	ug/L 98
19) 1,1-Dichloroethane	3.44	63	4406	0.641	ug/L # 89
34) Trichloroethene	6.18	95	23755	6.569	ug/L 99
46) Tetrachloroethene	8.23	164	1089	0.414	ug/L 94

(#) = qualifier out of range (m) = manual integration (+) = signals summed