

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU040519\
 Data File : VU030713.D
 Acq On : 05 Apr 2019 03:03
 Operator : JC/SP
 Sample : K2271-04 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DB7C7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.180	24	28	35	rVB	15501	14542	0.65%	0.086%
2	1.395	87	95	107	rBV	375121	397571	17.64%	2.355%
3	1.675	174	182	197	rVB	270836	347953	15.43%	2.061%
4	2.267	355	366	380	rVB	564259	856121	37.98%	5.070%
5	2.366	395	397	401	rVB2	1886	1077	0.05%	0.006%
6	2.588	464	466	471	rBV3	924	774	0.03%	0.005%
7	2.694	495	499	502	rBV4	1704	1674	0.07%	0.010%
8	3.122	627	632	636	rVB3	658	547	0.02%	0.003%
9	3.360	700	706	708	rBV3	622	678	0.03%	0.004%
10	3.460	734	737	741	rVB3	596	453	0.02%	0.003%
11	3.492	744	747	753	rBV4	512	588	0.03%	0.003%
12	3.704	810	813	818	rVB3	850	697	0.03%	0.004%
13	3.781	833	837	840	rBV3	1297	1116	0.05%	0.007%
14	3.897	866	873	878	rBV3	754	906	0.04%	0.005%
15	3.961	890	893	895	rBV2	693	458	0.02%	0.003%
16	4.170	945	958	997	rBV	222119	609816	27.05%	3.612%
17	4.643	1088	1105	1132	rBV	333621	855648	37.95%	5.068%
18	5.045	1227	1230	1237	rVB3	778	755	0.03%	0.004%
19	5.157	1261	1265	1267	rBV3	505	423	0.02%	0.003%
20	5.254	1290	1295	1297	rBV3	815	773	0.03%	0.005%
21	5.334	1297	1320	1344	rBV2	765011	2254391	100.00%	13.352%
22	5.672	1423	1425	1427	rBV2	755	431	0.02%	0.003%
23	5.726	1440	1442	1448	rVV6	680	525	0.02%	0.003%
24	5.829	1470	1474	1476	rBV4	968	479	0.02%	0.003%
25	5.881	1476	1490	1515	rBV	620580	1248183	55.37%	7.392%
26	6.093	1554	1556	1558	rVB2	1162	502	0.02%	0.003%
27	6.189	1573	1586	1604	rVB4	20750	45746	2.03%	0.271%
28	6.254	1604	1606	1609	rVB3	1256	717	0.03%	0.004%
29	6.270	1609	1611	1614	rBV3	788	507	0.02%	0.003%
30	6.324	1614	1628	1657	rBV	498309	1026556	45.54%	6.080%
31	6.652	1726	1730	1733	rVB4	599	494	0.02%	0.003%
32	6.675	1733	1737	1738	rVV2	628	441	0.02%	0.003%
33	6.701	1741	1745	1748	rVB2	762	685	0.03%	0.004%
34	6.726	1748	1753	1754	rBV3	587	479	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU040519\
 Data File : VU030713.D
 Acq On : 05 Apr 2019 03:03
 Operator : JC/SP
 Sample : K2271-04 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DB7C7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Title : VOC Analysis

35	6.759	1760	1763	1769	rBV3	517	641	0.03%	0.004%
36	7.019	1840	1844	1848	rBV2	820	820	0.04%	0.005%
37	7.054	1850	1855	1857	rBV2	691	563	0.02%	0.003%
38	7.225	1895	1908	1942	rBV	263165	504820	22.39%	2.990%
39	7.562	2000	2013	2053	rBV	976257	1773775	78.68%	10.505%
40	7.845	2091	2101	2121	rBV	180388	327042	14.51%	1.937%
41	8.125	2184	2188	2191	rBV3	542	513	0.02%	0.003%
42	8.222	2214	2218	2229	rBV8	2146	3427	0.15%	0.020%
43	8.308	2233	2245	2289	rBV	674704	1283133	56.92%	7.599%
44	8.675	2354	2359	2361	rBV5	1054	875	0.04%	0.005%
45	8.845	2408	2412	2414	rBV3	882	614	0.03%	0.004%
46	8.974	2448	2452	2458	rVB4	810	652	0.03%	0.004%
47	9.086	2474	2487	2517	rBV	890439	1553609	68.91%	9.201%
48	9.382	2575	2579	2582	rBV3	885	569	0.03%	0.003%
49	9.402	2582	2585	2587	rBV3	731	495	0.02%	0.003%
50	9.511	2616	2619	2621	rVV2	817	455	0.02%	0.003%
51	9.614	2647	2651	2656	rVB2	784	787	0.03%	0.005%
52	9.643	2656	2660	2665	rBV3	753	689	0.03%	0.004%
53	9.942	2749	2753	2754	rBV2	812	502	0.02%	0.003%
54	10.077	2790	2795	2797	rBV3	751	589	0.03%	0.003%
55	10.164	2820	2822	2826	rBV	666	531	0.02%	0.003%
56	10.241	2841	2846	2849	rBV4	422	464	0.02%	0.003%
57	10.257	2849	2851	2860	rVB4	1025	893	0.04%	0.005%
58	10.292	2860	2862	2865	rBV	682	430	0.02%	0.003%
59	10.318	2865	2870	2871	rBV2	705	589	0.03%	0.003%
60	10.427	2891	2904	2927	rBV	626869	1042348	46.24%	6.173%
61	10.665	2974	2978	2984	rBV4	622	761	0.03%	0.005%
62	10.697	2984	2988	2990	rVV2	903	685	0.03%	0.004%
63	10.710	2990	2992	2996	rVV2	844	531	0.02%	0.003%
64	10.771	3005	3011	3014	rBV3	772	844	0.04%	0.005%
65	10.794	3014	3018	3023	rVV3	697	724	0.03%	0.004%
66	10.829	3026	3029	3034	rVV4	811	744	0.03%	0.004%
67	10.855	3034	3037	3040	rVB	884	493	0.02%	0.003%
68	10.996	3076	3081	3083	rBV3	570	547	0.02%	0.003%
69	11.038	3091	3094	3098	rVB3	824	511	0.02%	0.003%
70	11.077	3098	3106	3112	rBV6	1104	1748	0.08%	0.010%
71	11.106	3112	3115	3117	rBV2	1084	778	0.03%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU040519\
 Data File : VU030713.D
 Acq On : 05 Apr 2019 03:03
 Operator : JC/SP
 Sample : K2271-04 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DB7C7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Title : VOC Analysis

72	11.260	3157	3163	3165	rBV2	697	643	0.03%	0.004%
73	11.286	3165	3171	3174	rBV4	483	481	0.02%	0.003%
74	11.308	3175	3178	3182	rVB3	747	532	0.02%	0.003%
75	11.356	3189	3193	3197	rBV	782	593	0.03%	0.004%
76	11.482	3219	3232	3256	rBV	787806	1320367	58.57%	7.820%
77	11.855	3337	3348	3371	rBV	815714	1363575	60.49%	8.076%
78	12.356	3499	3504	3509	rBV5	1135	1128	0.05%	0.007%
79	12.382	3509	3512	3514	rBV3	1033	583	0.03%	0.003%
80	12.424	3523	3525	3530	rBV3	600	505	0.02%	0.003%
81	12.482	3541	3543	3547	rBV2	783	566	0.03%	0.003%
82	12.572	3568	3571	3575	rVB3	925	709	0.03%	0.004%
83	12.607	3579	3582	3590	rVB2	1379	1383	0.06%	0.008%
84	12.646	3591	3594	3598	rBV2	1048	850	0.04%	0.005%
85	12.713	3613	3615	3619	rVB3	830	476	0.02%	0.003%
86	12.752	3625	3627	3631	rBV3	862	549	0.02%	0.003%
87	12.954	3688	3690	3694	rVB3	682	465	0.02%	0.003%
88	13.135	3744	3746	3751	rBV2	867	782	0.03%	0.005%
89	13.253	3780	3783	3786	rBV	850	682	0.03%	0.004%
90	13.308	3795	3800	3805	rBV5	1444	1453	0.06%	0.009%
91	13.334	3805	3808	3812	rVB4	1077	923	0.04%	0.005%
92	13.360	3812	3816	3819	rBV3	788	811	0.04%	0.005%
93	13.427	3831	3837	3839	rBV4	876	871	0.04%	0.005%
94	13.462	3846	3848	3852	rVB2	1063	698	0.03%	0.004%
95	13.485	3852	3855	3859	rVB2	668	484	0.02%	0.003%
96	13.536	3869	3871	3876	rBV2	618	688	0.03%	0.004%
97	13.620	3895	3897	3903	rVB3	1006	999	0.04%	0.006%
98	13.774	3943	3945	3951	rBV2	656	505	0.02%	0.003%
99	14.321	4112	4115	4118	rBV	913	626	0.03%	0.004%
100	15.093	4352	4355	4357	rBV3	1214	864	0.04%	0.005%


Sum of corrected areas: 16884688

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU040519\
Data File : VU030713.D
Acq On : 05 Apr 2019 03:03
Operator : JC/SP
Sample : K2271-04 50X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DB7C7

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

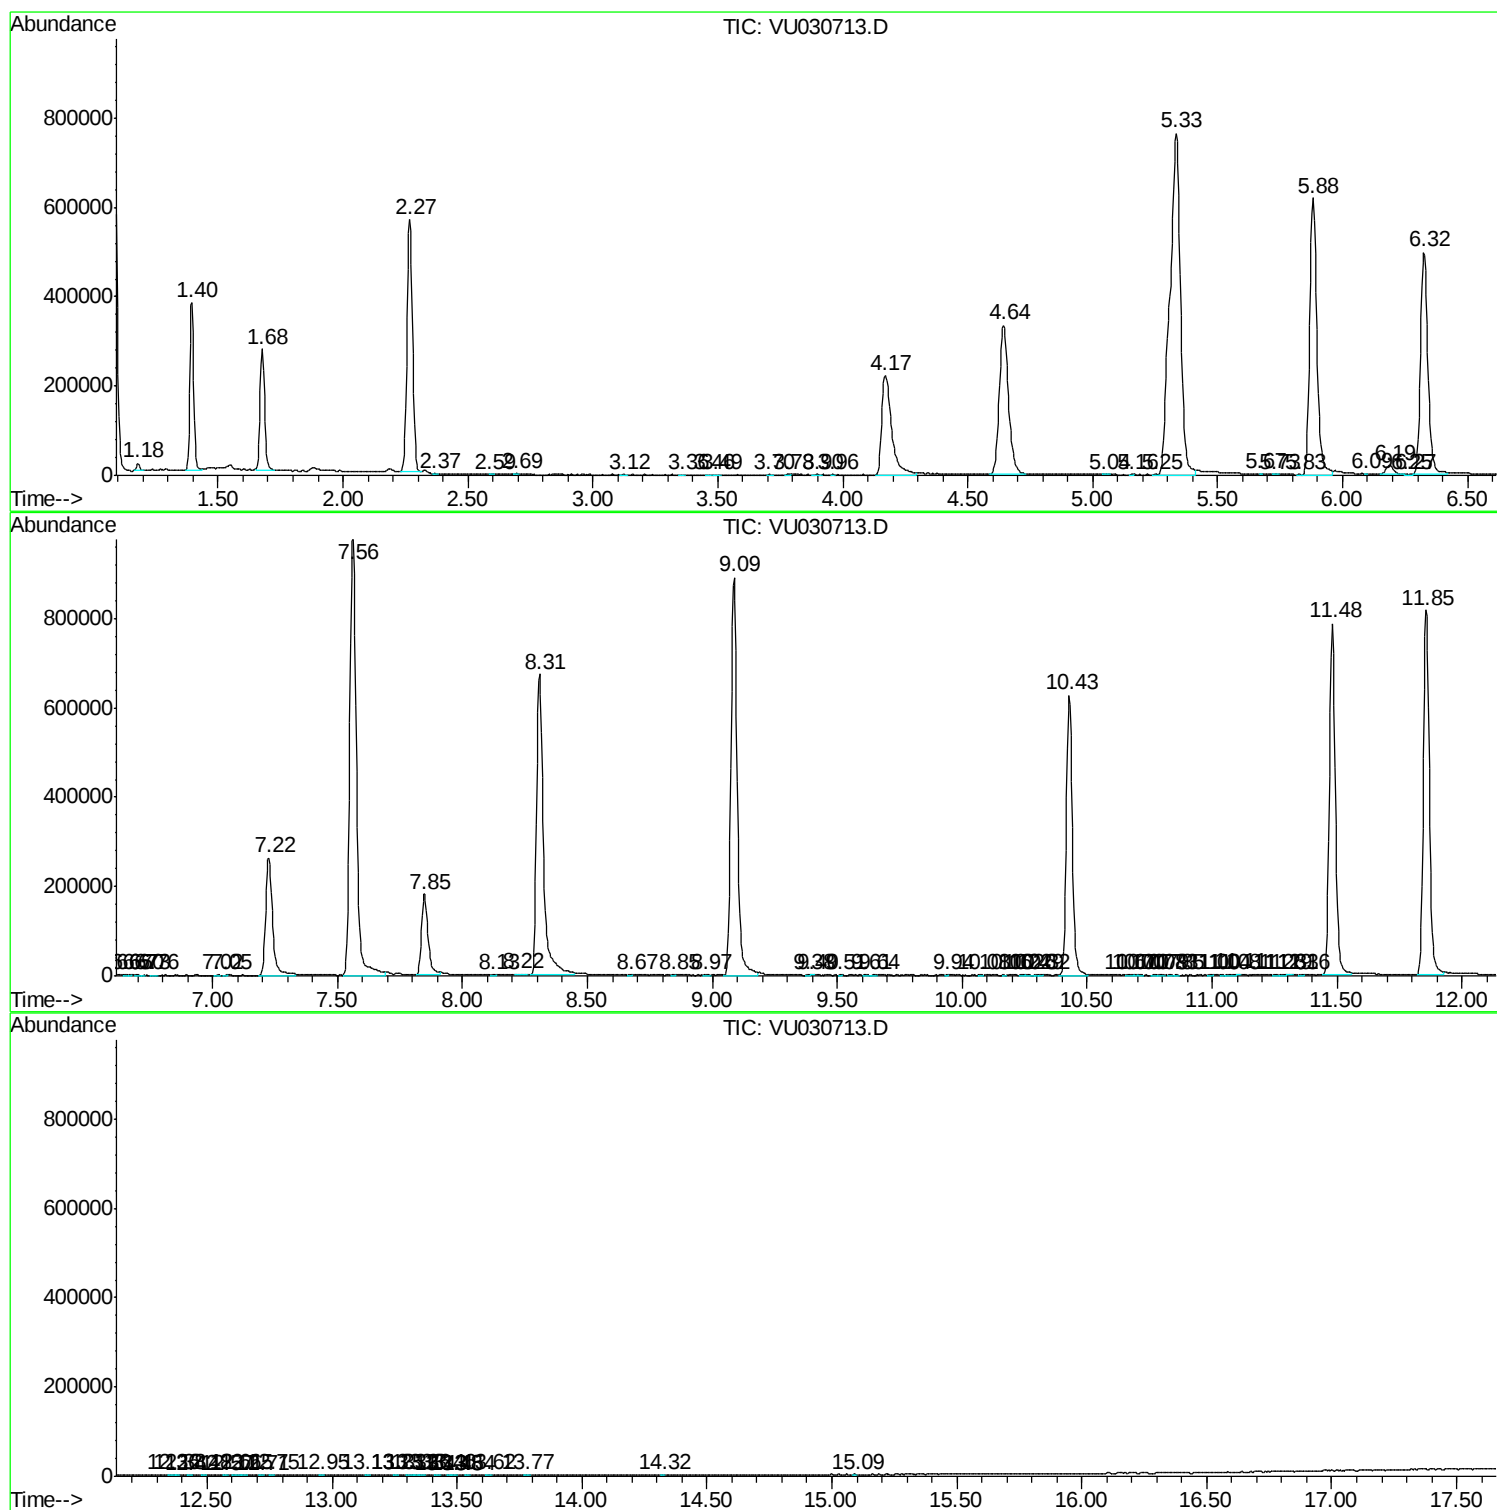

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU040519\
Data File : VU030713.D
Acq On : 05 Apr 2019 03:03
Operator : JC/SP
Sample : K2271-04 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DB7C7

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU040519\
Data File : VU030713.D
Acq On : 05 Apr 2019 03:03
Operator : JC/SP
Sample : K2271-04 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DB7C7

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc