

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU040519\
 Data File : VU030714.D
 Acq On : 05 Apr 2019 03:26
 Operator : JC/SP
 Sample : K2271-21 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DB7E2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.180	24	28	35	rVB2	16536	14693	0.66%	0.089%
2	1.395	87	95	106	rBV	374440	391322	17.62%	2.380%
3	1.675	174	182	196	rVB	263564	339224	15.27%	2.063%
4	2.267	355	366	379	rVB	539039	816232	36.75%	4.965%
5	2.440	415	420	421	rBV3	1158	936	0.04%	0.006%
6	2.540	446	451	455	rBV3	1037	1240	0.06%	0.008%
7	2.624	475	477	480	rBV3	774	432	0.02%	0.003%
8	2.701	488	501	508	rBV7	3223	5989	0.27%	0.036%
9	2.752	514	517	522	rVB4	736	495	0.02%	0.003%
10	2.810	532	535	537	rVV3	561	397	0.02%	0.002%
11	2.826	537	540	545	rVV5	690	584	0.03%	0.004%
12	3.128	631	634	637	rBV3	748	427	0.02%	0.003%
13	3.225	659	664	665	rBV3	548	460	0.02%	0.003%
14	3.260	670	675	678	rVB3	755	665	0.03%	0.004%
15	3.289	678	684	686	rBV3	559	562	0.03%	0.003%
16	3.331	694	697	700	rVB4	676	471	0.02%	0.003%
17	3.418	720	724	731	rBV2	555	664	0.03%	0.004%
18	3.453	731	735	740	rVV3	555	439	0.02%	0.003%
19	3.518	748	755	758	rBV3	671	699	0.03%	0.004%
20	3.546	759	764	765	rVV2	864	619	0.03%	0.004%
21	3.608	780	783	787	rBV3	560	452	0.02%	0.003%
22	3.701	808	812	814	rBV3	762	443	0.02%	0.003%
23	3.752	822	828	829	rBV	601	547	0.02%	0.003%
24	3.884	858	869	870	rBV3	451	570	0.03%	0.003%
25	3.942	881	887	893	rBV2	953	1106	0.05%	0.007%
26	4.099	932	936	939	rBV3	501	385	0.02%	0.002%
27	4.170	945	958	988	rBV	224412	595472	26.81%	3.622%
28	4.643	1088	1105	1133	rBV	333040	838842	37.77%	5.102%
29	5.022	1220	1223	1225	rBV2	603	415	0.02%	0.003%
30	5.115	1245	1252	1256	rBV4	785	1084	0.05%	0.007%
31	5.215	1281	1283	1288	rVB2	706	464	0.02%	0.003%
32	5.334	1294	1320	1352	rBV2	750633	2220807	100.00%	13.508%
33	5.704	1433	1435	1438	rBV3	737	474	0.02%	0.003%
34	5.804	1463	1466	1469	rVB2	789	456	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU040519\
 Data File : VU030714.D
 Acq On : 05 Apr 2019 03:26
 Operator : JC/SP
 Sample : K2271-21 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DB7E2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Title : VOC Analysis

35	5.881	1477	1490	1517	rBV	607531	1220258	54.95%	7.422%
36	6.160	1575	1577	1579	rBV2	881	553	0.02%	0.003%
37	6.186	1582	1585	1593	rVB9	2051	2438	0.11%	0.015%
38	6.324	1615	1628	1648	rBV	495286	996999	44.89%	6.064%
39	6.675	1735	1737	1742	rVB3	807	453	0.02%	0.003%
40	6.752	1757	1761	1766	rVB4	498	515	0.02%	0.003%
41	6.781	1766	1770	1778	rBV2	1796	2537	0.11%	0.015%
42	6.842	1786	1789	1793	rBV	450	440	0.02%	0.003%
43	6.903	1804	1808	1813	rVB3	439	445	0.02%	0.003%
44	6.939	1817	1819	1823	rBV3	920	714	0.03%	0.004%
45	6.964	1823	1827	1831	rVB2	566	429	0.02%	0.003%
46	7.225	1894	1908	1924	rBV	264205	479472	21.59%	2.916%
47	7.562	1999	2013	2035	rBV	946936	1685339	75.89%	10.251%
48	7.845	2091	2101	2126	rBV	173032	321325	14.47%	1.954%
49	8.070	2169	2171	2177	rVB3	927	633	0.03%	0.004%
50	8.128	2185	2189	2195	rVV5	595	688	0.03%	0.004%
51	8.176	2202	2204	2208	rVB3	1163	605	0.03%	0.004%
52	8.308	2233	2245	2295	rBV	656292	1272224	57.29%	7.738%
53	8.739	2375	2379	2382	rBV3	651	425	0.02%	0.003%
54	8.758	2382	2385	2389	rBV3	715	598	0.03%	0.004%
55	8.810	2397	2401	2404	rBV3	674	654	0.03%	0.004%
56	8.893	2424	2427	2432	rVB3	1342	1084	0.05%	0.007%
57	9.086	2474	2487	2514	rBV	879352	1517967	68.35%	9.233%
58	9.257	2534	2540	2548	rVB7	934	1490	0.07%	0.009%
59	9.411	2586	2588	2590	rBV	612	419	0.02%	0.003%
60	9.495	2612	2614	2617	rVB	742	398	0.02%	0.002%
61	9.514	2617	2620	2623	rBV2	691	423	0.02%	0.003%
62	9.588	2637	2643	2647	rBV2	835	822	0.04%	0.005%
63	9.614	2648	2651	2654	rVB	700	435	0.02%	0.003%
64	9.639	2654	2659	2662	rBV3	984	987	0.04%	0.006%
65	9.701	2673	2678	2683	rBV3	517	554	0.02%	0.003%
66	10.022	2775	2778	2781	rVB3	920	568	0.03%	0.003%
67	10.112	2803	2806	2808	rBV	540	404	0.02%	0.002%
68	10.167	2820	2823	2824	rBV	819	440	0.02%	0.003%
69	10.237	2843	2845	2849	rVB2	939	541	0.02%	0.003%
70	10.295	2860	2863	2867	rBV2	386	432	0.02%	0.003%
71	10.353	2879	2881	2885	rVB2	699	433	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU040519\
 Data File : VU030714.D
 Acq On : 05 Apr 2019 03:26
 Operator : JC/SP
 Sample : K2271-21 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DB7E2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Title : VOC Analysis

72	10.427	2892	2904	2934	rBV	616226	1025422	46.17%	6.237%
73	10.540	2934	2939	2942	rBV4	802	747	0.03%	0.005%
74	10.578	2948	2951	2954	rBV2	855	483	0.02%	0.003%
75	10.819	3024	3026	3030	rVB2	813	484	0.02%	0.003%
76	10.855	3033	3037	3039	rBV	476	423	0.02%	0.003%
77	10.961	3068	3070	3072	rBV	718	446	0.02%	0.003%
78	11.083	3105	3108	3112	rVV4	826	618	0.03%	0.004%
79	11.125	3119	3121	3125	rVB4	891	517	0.02%	0.003%
80	11.266	3162	3165	3168	rBV2	547	503	0.02%	0.003%
81	11.482	3219	3232	3259	rBV	792098	1303062	58.68%	7.926%
82	11.855	3336	3348	3377	rBV	796951	1342963	60.47%	8.168%
83	12.295	3481	3485	3489	rBV4	905	667	0.03%	0.004%
84	12.353	3501	3503	3508	rVB3	1087	720	0.03%	0.004%
85	12.417	3521	3523	3529	rVB4	961	639	0.03%	0.004%
86	12.530	3555	3558	3561	rBV2	542	412	0.02%	0.003%
87	12.707	3611	3613	3620	rVB4	786	570	0.03%	0.003%
88	12.768	3629	3632	3636	rVB2	1291	929	0.04%	0.006%
89	12.790	3636	3639	3640	rBV	804	427	0.02%	0.003%
90	13.016	3707	3709	3715	rVB3	1074	865	0.04%	0.005%
91	13.089	3730	3732	3737	rVB2	890	553	0.02%	0.003%
92	13.270	3785	3788	3791	rBV3	1100	732	0.03%	0.004%
93	13.311	3798	3801	3806	rBV3	928	891	0.04%	0.005%
94	13.437	3838	3840	3843	rBV2	515	394	0.02%	0.002%
95	13.614	3890	3895	3898	rBV3	979	935	0.04%	0.006%
96	13.745	3934	3936	3940	rBV2	832	507	0.02%	0.003%
97	14.051	4029	4031	4033	rBV2	719	441	0.02%	0.003%
98	14.263	4094	4097	4099	rBV3	864	599	0.03%	0.004%
99	14.356	4124	4126	4128	rBV	984	598	0.03%	0.004%
100	16.179	4690	4693	4695	rBV3	2288	1433	0.06%	0.009%


Sum of corrected areas: 16441188

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU040519\
Data File : VU030714.D
Acq On : 05 Apr 2019 03:26
Operator : JC/SP
Sample : K2271-21 50X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DB7E2

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

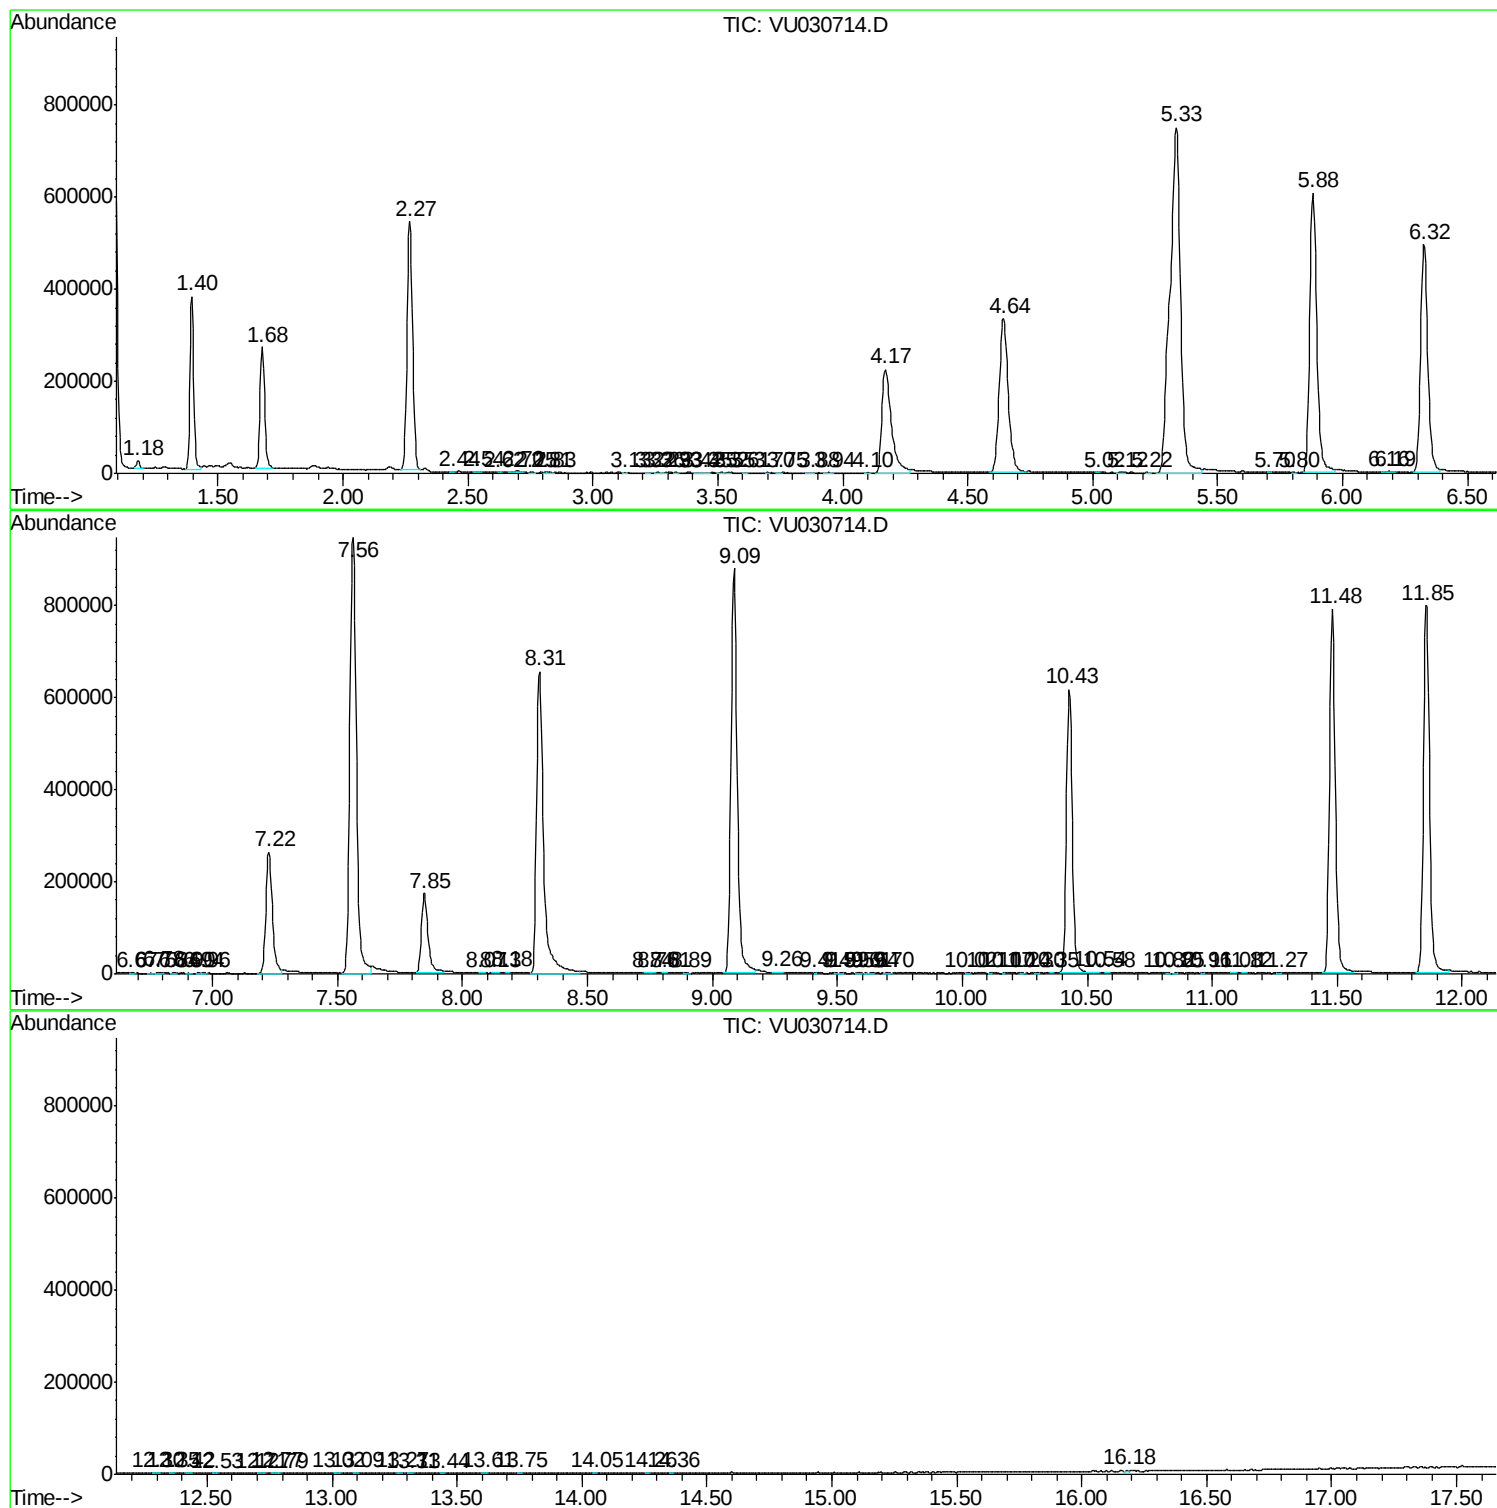

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU040519\
Data File : VU030714.D
Acq On : 05 Apr 2019 03:26
Operator : JC/SP
Sample : K2271-21 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DB7E2

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU040519\
Data File : VU030714.D
Acq On : 05 Apr 2019 03:26
Operator : JC/SP
Sample : K2271-21 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DB7E2

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc