

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU040519\
 Data File : VU030727.D
 Acq On : 05 Apr 2019 08:46
 Operator : JC/SP
 Sample : K2249-06
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E3YD5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.180	24	28	35	rVB3	17695	15671	0.06%	0.023%
2	1.399	88	96	116	rBV	5039946	5326701	20.91%	7.886%
3	1.694	175	188	202	rVB2	325362	668194	2.62%	0.989%
4	2.270	356	367	382	rBV3	598999	1051172	4.13%	1.556%
5	2.440	414	420	432	rBV2	8006	14384	0.06%	0.021%
6	2.640	476	482	484	rVB5	1084	1009	0.00%	0.001%
7	2.662	487	489	493	rVB4	1104	628	0.00%	0.001%
8	2.694	493	499	500	rBV5	2847	2924	0.01%	0.004%
9	2.791	518	529	532	rBV6	5268	9429	0.04%	0.014%
10	2.981	574	588	610	rBV	322478	606545	2.38%	0.898%
11	3.087	619	621	623	rVB	1270	635	0.00%	0.001%
12	3.109	623	628	631	rBV6	1179	1153	0.00%	0.002%
13	3.154	637	642	645	rBV6	670	455	0.00%	0.001%
14	3.254	670	673	675	rBV2	672	466	0.00%	0.001%
15	3.305	684	689	690	rVV2	585	488	0.00%	0.001%
16	3.360	703	706	708	rBV	885	448	0.00%	0.001%
17	3.440	708	731	759	rBV	6920000	15328783	60.17%	22.694%
18	4.218	948	973	1010	rBV	10348316	25475944	100.00%	37.717%
19	4.643	1093	1105	1133	rVB	309824	787737	3.09%	1.166%
20	4.910	1169	1188	1212	rBV	2133162	5155218	20.24%	7.632%
21	5.334	1298	1320	1333	rBV2	671254	1985539	7.79%	2.940%
22	5.746	1446	1448	1450	rBV2	875	552	0.00%	0.001%
23	5.781	1456	1459	1461	rBV3	792	491	0.00%	0.001%
24	5.881	1476	1490	1514	rBV	572785	1147515	4.50%	1.699%
25	6.183	1571	1584	1606	rBV	216646	437409	1.72%	0.648%
26	6.328	1615	1629	1648	rBV	437634	889823	3.49%	1.317%
27	6.617	1710	1719	1738	rVB3	12481	26007	0.10%	0.039%
28	6.714	1747	1749	1754	rVB3	1177	681	0.00%	0.001%
29	6.759	1758	1763	1764	rBV3	906	562	0.00%	0.001%
30	6.820	1781	1782	1785	rVB	957	420	0.00%	0.001%
31	6.971	1826	1829	1830	rBV	717	380	0.00%	0.001%
32	7.032	1845	1848	1850	rVV2	725	436	0.00%	0.001%
33	7.103	1863	1870	1872	rBV4	496	542	0.00%	0.001%
34	7.225	1896	1908	1934	rBV	226598	430733	1.69%	0.638%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU040519\
 Data File : VU030727.D
 Acq On : 05 Apr 2019 08:46
 Operator : JC/SP
 Sample : K2249-06
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E3YD5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Title : VOC Analysis

35	7.463	1979	1982	1992	rVB7	2032	3136	0.01%	0.005%
36	7.562	1999	2013	2032	rBV	840335	1513663	5.94%	2.241%
37	7.849	2090	2102	2130	rBV	156558	289285	1.14%	0.428%
38	8.067	2160	2170	2183	rBV4	18314	34254	0.13%	0.051%
39	8.170	2194	2202	2207	rBV8	4028	6217	0.02%	0.009%
40	8.225	2207	2219	2234	rVV	218640	375614	1.47%	0.556%
41	8.308	2235	2245	2287	rVV	586624	1098162	4.31%	1.626%
42	8.726	2372	2375	2379	rVB5	979	823	0.00%	0.001%
43	8.746	2379	2381	2385	rBV	535	385	0.00%	0.001%
44	8.775	2386	2390	2393	rVB4	1127	782	0.00%	0.001%
45	8.842	2408	2411	2413	rVB2	786	424	0.00%	0.001%
46	8.922	2434	2436	2440	rVB3	978	762	0.00%	0.001%
47	8.958	2444	2447	2451	rVB4	1255	718	0.00%	0.001%
48	8.984	2451	2455	2458	rBV3	729	632	0.00%	0.001%
49	9.086	2474	2487	2509	rBV	839662	1428771	5.61%	2.115%
50	9.376	2574	2577	2581	rVB3	748	441	0.00%	0.001%
51	9.395	2581	2583	2586	rVB4	818	491	0.00%	0.001%
52	9.453	2599	2601	2608	rVB5	919	724	0.00%	0.001%
53	9.485	2608	2611	2615	rVB2	747	548	0.00%	0.001%
54	9.508	2615	2618	2622	rBV2	853	641	0.00%	0.001%
55	9.694	2670	2676	2677	rBV2	898	821	0.00%	0.001%
56	9.713	2680	2682	2685	rVB2	1011	600	0.00%	0.001%
57	9.758	2692	2696	2698	rBV4	504	437	0.00%	0.001%
58	9.913	2741	2744	2746	rBV2	700	497	0.00%	0.001%
59	9.938	2750	2752	2759	rVB4	723	669	0.00%	0.001%
60	9.993	2766	2769	2772	rBV2	667	442	0.00%	0.001%
61	10.019	2772	2777	2780	rBV3	534	524	0.00%	0.001%
62	10.067	2787	2792	2796	rBV4	1152	1302	0.01%	0.002%
63	10.196	2828	2832	2835	rVB2	580	408	0.00%	0.001%
64	10.257	2849	2851	2855	rVB2	1419	942	0.00%	0.001%
65	10.279	2855	2858	2860	rBV2	910	549	0.00%	0.001%
66	10.427	2889	2904	2929	rBV	564750	945702	3.71%	1.400%
67	10.607	2952	2960	2969	rVB7	2994	5104	0.02%	0.008%
68	10.903	3049	3052	3057	rVB3	723	621	0.00%	0.001%
69	10.948	3062	3066	3071	rVV4	728	818	0.00%	0.001%
70	10.967	3071	3072	3077	rVV3	966	452	0.00%	0.001%
71	11.080	3104	3107	3113	rBV4	937	1058	0.00%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU040519\
 Data File : VU030727.D
 Acq On : 05 Apr 2019 08:46
 Operator : JC/SP
 Sample : K2249-06
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E3YD5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Title : VOC Analysis

72	11.231	3151	3154	3157	rBV3	673	460	0.00%	0.001%
73	11.321	3178	3182	3185	rVB4	795	584	0.00%	0.001%
74	11.389	3194	3203	3205	rBV6	1240	1709	0.01%	0.003%
75	11.479	3220	3231	3259	rBV	743825	1224976	4.81%	1.814%
76	11.678	3291	3293	3296	rBV3	1342	704	0.00%	0.001%
77	11.858	3335	3349	3367	rBV	724333	1217518	4.78%	1.803%
78	12.299	3482	3486	3487	rBV3	523	414	0.00%	0.001%
79	12.392	3512	3515	3519	rBV4	715	448	0.00%	0.001%
80	12.427	3522	3526	3529	rBV3	685	636	0.00%	0.001%
81	12.549	3560	3564	3567	rBV2	683	675	0.00%	0.001%
82	12.659	3593	3598	3599	rBV4	667	531	0.00%	0.001%
83	12.681	3603	3605	3609	rVB3	1005	693	0.00%	0.001%
84	12.758	3625	3629	3631	rBV2	754	580	0.00%	0.001%
85	12.884	3664	3668	3671	rVV4	726	603	0.00%	0.001%
86	13.089	3728	3732	3735	rBV2	875	674	0.00%	0.001%
87	13.118	3738	3741	3743	rVB2	682	412	0.00%	0.001%
88	13.141	3745	3748	3749	rBV2	746	406	0.00%	0.001%
89	13.208	3765	3769	3772	rVB3	1067	765	0.00%	0.001%
90	13.231	3772	3776	3778	rBV3	934	710	0.00%	0.001%
91	13.260	3783	3785	3790	rVB2	790	590	0.00%	0.001%
92	13.507	3859	3862	3866	rBV3	687	489	0.00%	0.001%
93	13.617	3892	3896	3898	rBV3	751	467	0.00%	0.001%
94	13.832	3959	3963	3964	rBV2	742	594	0.00%	0.001%
95	14.057	4030	4033	4034	rBV2	722	433	0.00%	0.001%
96	14.163	4061	4066	4070	rBV4	1039	992	0.00%	0.001%
97	14.324	4114	4116	4118	rBV2	704	419	0.00%	0.001%
98	14.446	4152	4154	4157	rBV3	773	602	0.00%	0.001%
99	14.527	4176	4179	4180	rBV2	816	437	0.00%	0.001%
100	14.855	4278	4281	4282	rBV3	794	464	0.00%	0.001%


Sum of corrected areas: 67545478

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU040519\
Data File : VU030727.D
Acq On : 05 Apr 2019 08:46
Operator : JC/SP
Sample : K2249-06
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E3YD5

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

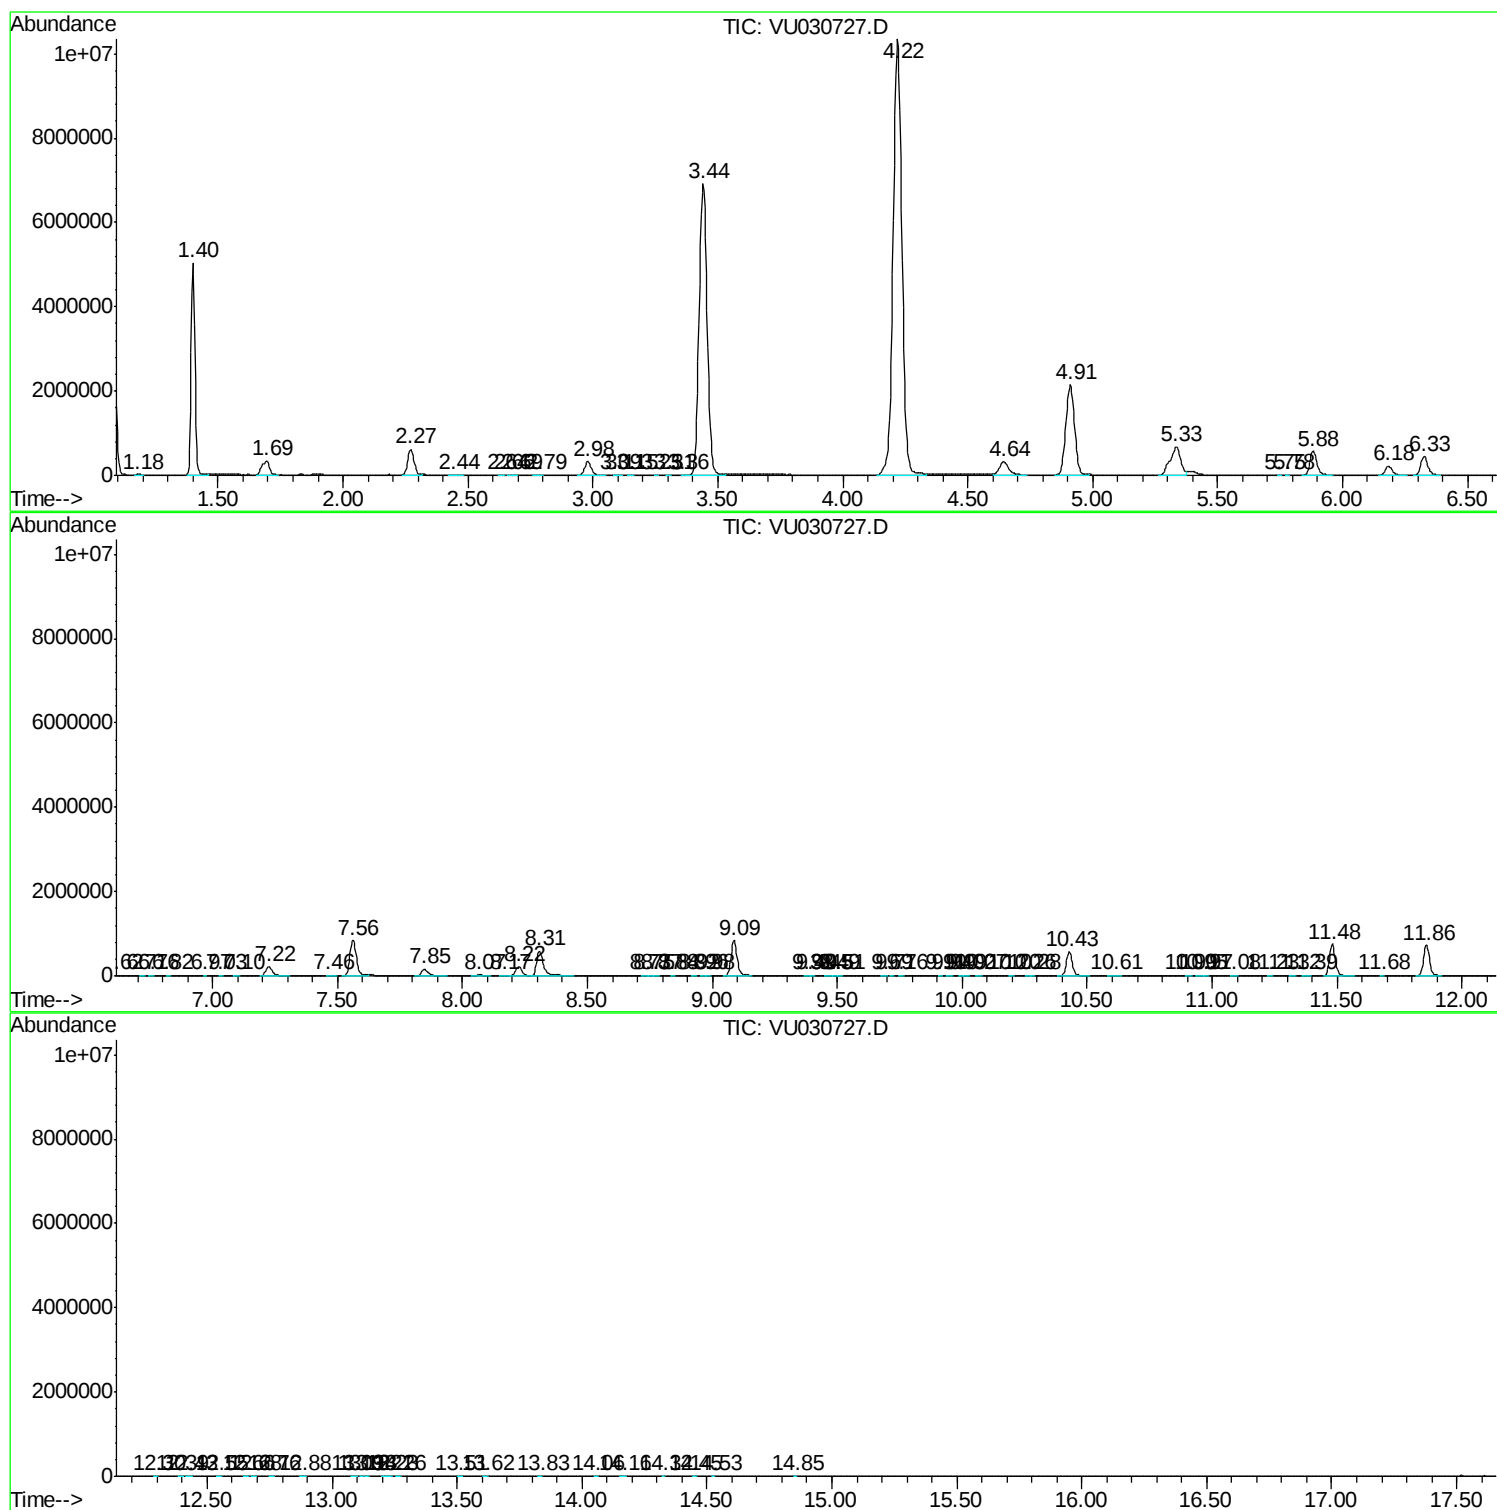

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU040519\
Data File : VU030727.D
Acq On : 05 Apr 2019 08:46
Operator : JC/SP
Sample : K2249-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E3YD5

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU040519\
Data File : VU030727.D
Acq On : 05 Apr 2019 08:46
Operator : JC/SP
Sample : K2249-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E3YD5

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc