

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU040519\
 Data File : VU030739.D
 Acq On : 05 Apr 2019 13:32
 Operator : JC/SP
 Sample : K2249-07 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E3YE0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.180	22	28	36	rBV	28307	27819	1.49%	0.199%
2	1.396	87	95	108	rBV	308921	329677	17.63%	2.356%
3	1.675	174	182	197	rVB	214517	277808	14.85%	1.985%
4	2.183	336	340	341	rBV3	5262	3672	0.20%	0.026%
5	2.267	355	366	380	rBV	459567	698694	37.36%	4.993%
6	2.605	469	471	477	rVB4	1245	1005	0.05%	0.007%
7	2.637	477	481	482	rVB3	729	390	0.02%	0.003%
8	2.659	485	488	491	rBV4	652	450	0.02%	0.003%
9	2.695	491	499	510	rBV6	2502	4748	0.25%	0.034%
10	2.785	522	527	530	rVB4	736	743	0.04%	0.005%
11	3.051	607	610	615	rVB2	564	431	0.02%	0.003%
12	3.077	615	618	620	rBV3	692	445	0.02%	0.003%
13	3.270	674	678	683	rVB3	571	545	0.03%	0.004%
14	3.441	722	731	750	rVB2	9675	22435	1.20%	0.160%
15	3.515	751	754	759	rBV2	493	539	0.03%	0.004%
16	3.540	759	762	769	rVB2	622	595	0.03%	0.004%
17	3.788	835	839	841	rBV2	497	442	0.02%	0.003%
18	3.804	841	844	846	rVV	704	473	0.03%	0.003%
19	3.826	846	851	854	rVV3	514	630	0.03%	0.005%
20	4.170	943	958	971	rBV	187172	496791	26.56%	3.550%
21	4.643	1088	1105	1133	rBV	288081	713847	38.17%	5.101%
22	4.907	1173	1187	1206	rVB2	26560	64954	3.47%	0.464%
23	5.019	1220	1222	1225	rBV3	790	466	0.02%	0.003%
24	5.129	1250	1256	1259	rBV4	770	621	0.03%	0.004%
25	5.219	1276	1284	1288	rBV4	774	863	0.05%	0.006%
26	5.334	1295	1320	1348	rBV2	637081	1870162	100.00%	13.363%
27	5.678	1423	1427	1429	rBV2	915	744	0.04%	0.005%
28	5.833	1472	1475	1477	rBV3	672	441	0.02%	0.003%
29	5.881	1477	1490	1517	rBV	526296	1058753	56.61%	7.565%
30	6.061	1544	1546	1549	rBV3	977	608	0.03%	0.004%
31	6.190	1577	1586	1592	rBV10	3107	4860	0.26%	0.035%
32	6.325	1613	1628	1655	rBV	417665	857187	45.83%	6.125%
33	6.563	1699	1702	1706	rVV4	1113	715	0.04%	0.005%
34	6.585	1706	1709	1714	rVB4	744	628	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU040519\
 Data File : VU030739.D
 Acq On : 05 Apr 2019 13:32
 Operator : JC/SP
 Sample : K2249-07 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E3YE0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Title : VOC Analysis

35	6.842	1784	1789	1792	rBV2	543	497	0.03%	0.004%
36	6.881	1798	1801	1807	rVB4	615	535	0.03%	0.004%
37	6.945	1817	1821	1824	rBV3	473	459	0.02%	0.003%
38	7.038	1846	1850	1855	rVB5	540	490	0.03%	0.004%
39	7.090	1863	1866	1870	rVB2	594	389	0.02%	0.003%
40	7.225	1895	1908	1929	rBV	205694	384625	20.57%	2.748%
41	7.392	1957	1960	1962	rBV3	612	418	0.02%	0.003%
42	7.476	1981	1986	1990	rVB4	589	570	0.03%	0.004%
43	7.505	1992	1995	1999	rBV3	1027	552	0.03%	0.004%
44	7.563	1999	2013	2042	rBV	776730	1406178	75.19%	10.048%
45	7.849	2091	2102	2126	rBV2	140713	263497	14.09%	1.883%
46	8.177	2198	2204	2209	rBV4	1545	1720	0.09%	0.012%
47	8.228	2211	2220	2231	rBV5	10409	17341	0.93%	0.124%
48	8.309	2234	2245	2290	rBV	552996	1063767	56.88%	7.601%
49	8.534	2312	2315	2321	rVB4	1263	1027	0.05%	0.007%
50	8.598	2331	2335	2338	rBV4	1024	771	0.04%	0.006%
51	8.675	2355	2359	2364	rBV4	648	616	0.03%	0.004%
52	8.698	2364	2366	2370	rVB4	697	500	0.03%	0.004%
53	8.730	2370	2376	2381	rVB6	977	1259	0.07%	0.009%
54	8.755	2381	2384	2390	rVB3	626	479	0.03%	0.003%
55	8.804	2395	2399	2402	rBV3	748	490	0.03%	0.004%
56	8.823	2402	2405	2408	rBV3	669	390	0.02%	0.003%
57	8.868	2412	2419	2421	rBV4	717	801	0.04%	0.006%
58	8.958	2445	2447	2452	rBV2	667	555	0.03%	0.004%
59	9.087	2474	2487	2534	rBV	748350	1319388	70.55%	9.428%
60	9.321	2558	2560	2564	rVB4	946	468	0.03%	0.003%
61	9.585	2635	2642	2644	rBV4	428	411	0.02%	0.003%
62	9.807	2708	2711	2714	rVB2	793	534	0.03%	0.004%
63	9.829	2714	2718	2720	rBV2	575	451	0.02%	0.003%
64	9.897	2736	2739	2742	rBV2	506	400	0.02%	0.003%
65	9.964	2756	2760	2763	rBV4	570	491	0.03%	0.004%
66	10.048	2783	2786	2791	rVB3	943	724	0.04%	0.005%
67	10.083	2794	2797	2801	rBV2	528	388	0.02%	0.003%
68	10.128	2806	2811	2815	rBV2	966	967	0.05%	0.007%
69	10.199	2829	2833	2836	rBV3	420	399	0.02%	0.003%
70	10.302	2861	2865	2867	rBV2	608	463	0.02%	0.003%
71	10.350	2876	2880	2885	rBV4	971	946	0.05%	0.007%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU040519\
 Data File : VU030739.D
 Acq On : 05 Apr 2019 13:32
 Operator : JC/SP
 Sample : K2249-07 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E3YE0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Title : VOC Analysis

72	10.427	2890	2904	2929	rBV	529976	873248	46.69%	6.240%
73	10.691	2981	2986	2988	rVB2	913	736	0.04%	0.005%
74	10.710	2988	2992	2993	rBV	615	428	0.02%	0.003%
75	10.797	3015	3019	3021	rBV2	792	396	0.02%	0.003%
76	10.820	3021	3026	3028	rBV2	604	531	0.03%	0.004%
77	10.858	3034	3038	3040	rBV	1052	803	0.04%	0.006%
78	11.238	3153	3156	3159	rBV	725	512	0.03%	0.004%
79	11.308	3174	3178	3183	rBV2	828	675	0.04%	0.005%
80	11.418	3206	3212	3214	rBV2	839	834	0.04%	0.006%
81	11.479	3219	3231	3255	rBV	657513	1087621	58.16%	7.772%
82	11.858	3336	3349	3373	rBV	649278	1100268	58.83%	7.862%
83	12.550	3561	3564	3565	rBV	676	441	0.02%	0.003%
84	12.884	3665	3668	3671	rBV3	825	685	0.04%	0.005%
85	13.218	3770	3772	3775	rVB3	971	541	0.03%	0.004%
86	13.305	3794	3799	3802	rBV2	587	525	0.03%	0.004%
87	13.328	3803	3806	3811	rVB3	955	791	0.04%	0.006%
88	13.357	3811	3815	3818	rBV2	684	703	0.04%	0.005%
89	13.447	3840	3843	3846	rBV3	661	480	0.03%	0.003%
90	13.588	3884	3887	3891	rBV3	837	824	0.04%	0.006%
91	13.784	3945	3948	3950	rBV2	933	538	0.03%	0.004%
92	14.096	4042	4045	4046	rBV	853	534	0.03%	0.004%
93	14.176	4067	4070	4074	rBV2	758	528	0.03%	0.004%
94	14.295	4104	4107	4109	rBV2	804	420	0.02%	0.003%
95	14.424	4145	4147	4152	rVB3	980	673	0.04%	0.005%
96	15.141	4367	4370	4373	rBV3	1125	885	0.05%	0.006%
97	15.160	4374	4376	4380	rVB3	1137	740	0.04%	0.005%
98	15.180	4380	4382	4385	rBV2	1171	699	0.04%	0.005%
99	15.238	4398	4400	4403	rBV3	1193	810	0.04%	0.006%
100	15.495	4477	4480	4481	rBV3	1397	839	0.04%	0.006%


Sum of corrected areas: 13994845

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU040519\
Data File : VU030739.D
Acq On : 05 Apr 2019 13:32
Operator : JC/SP
Sample : K2249-07 50X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 56 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E3YE0

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

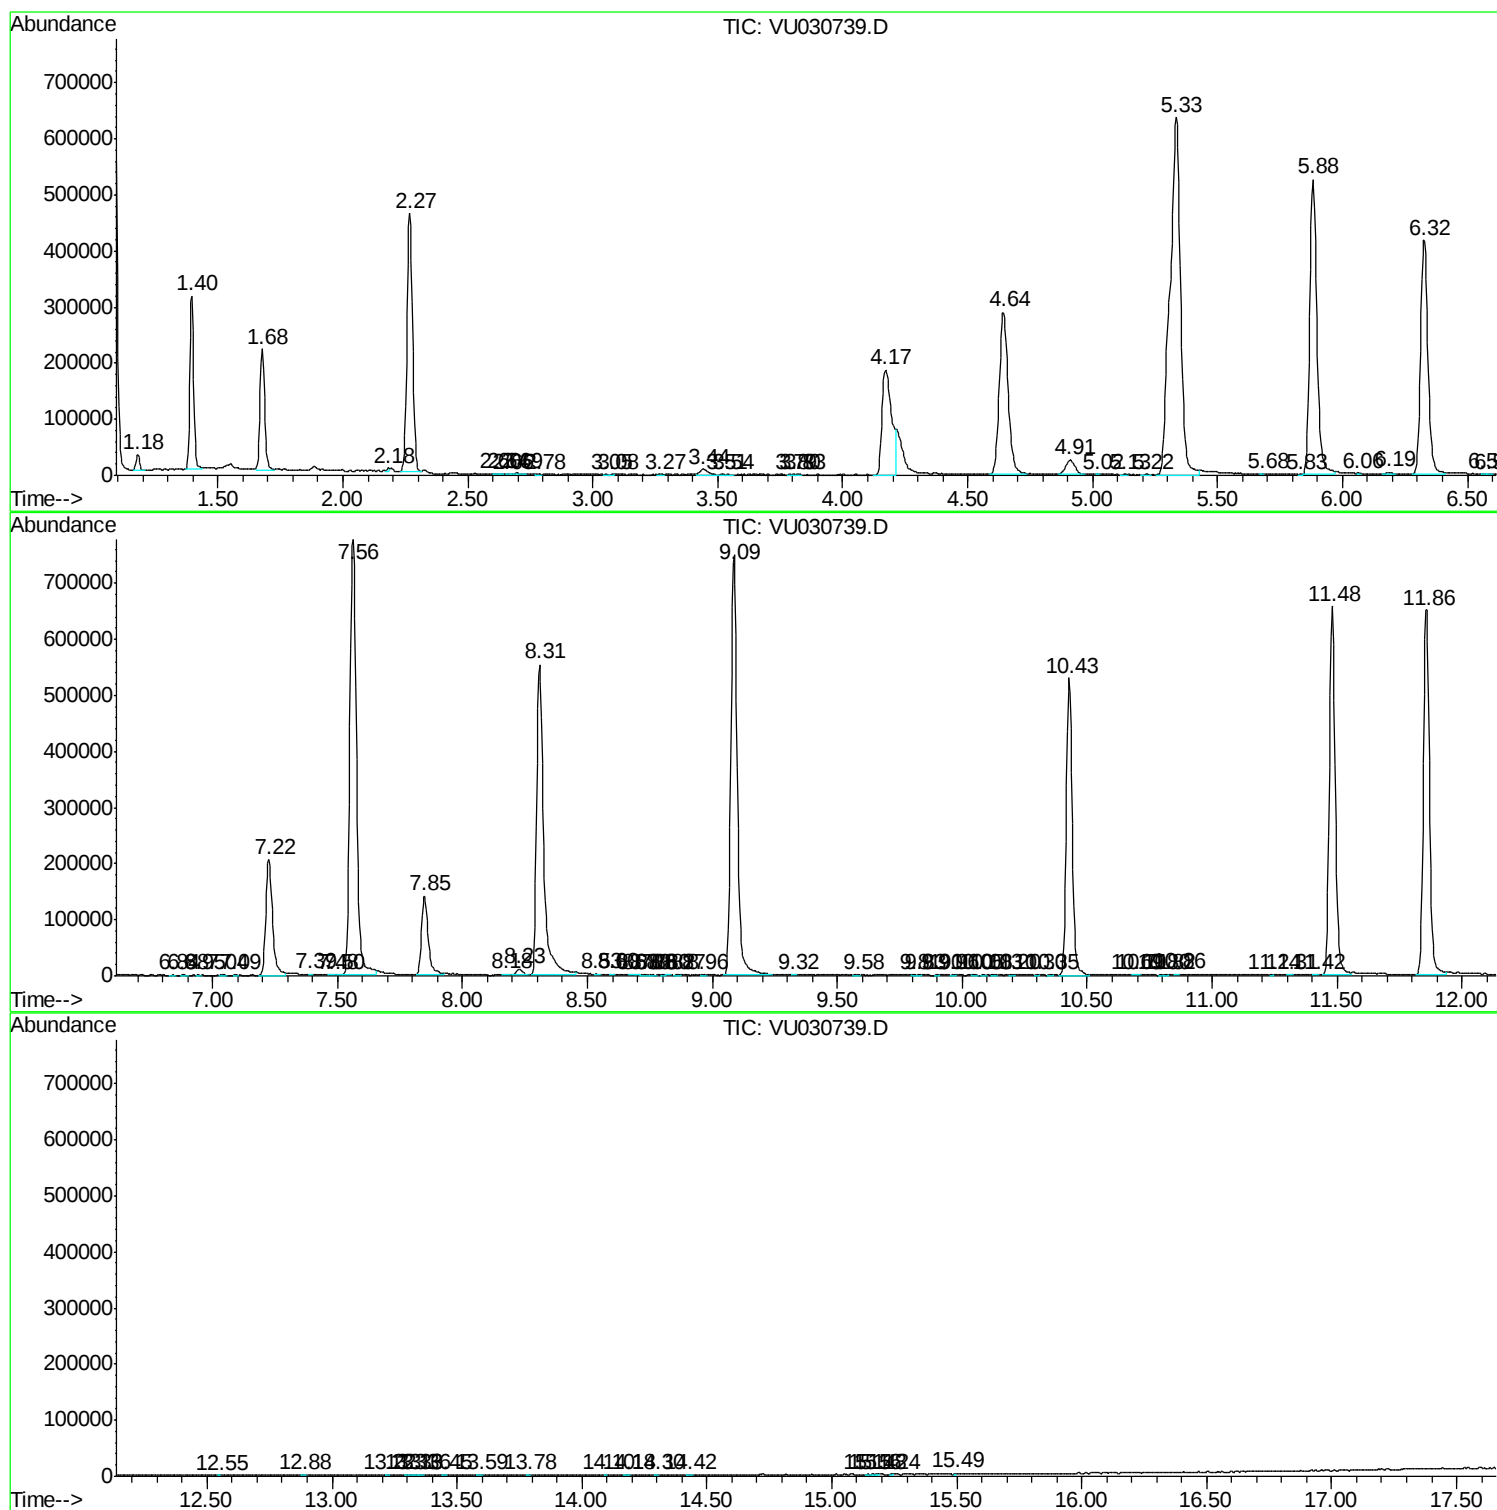

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU040519\
Data File : VU030739.D
Acq On : 05 Apr 2019 13:32
Operator : JC/SP
Sample : K2249-07 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 56 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E3YE0

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU040519\
Data File : VU030739.D
Acq On : 05 Apr 2019 13:32
Operator : JC/SP
Sample : K2249-07 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 56 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E3YE0

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc