


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU040519\
 Data File : VU030686.D
 Acq On : 04 Apr 2019 15:59
 Operator : JC/SP
 Sample : BFB50
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB50

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Title : VOC Analysis
 Last Update : Mon Apr 08 07:03:53 2019

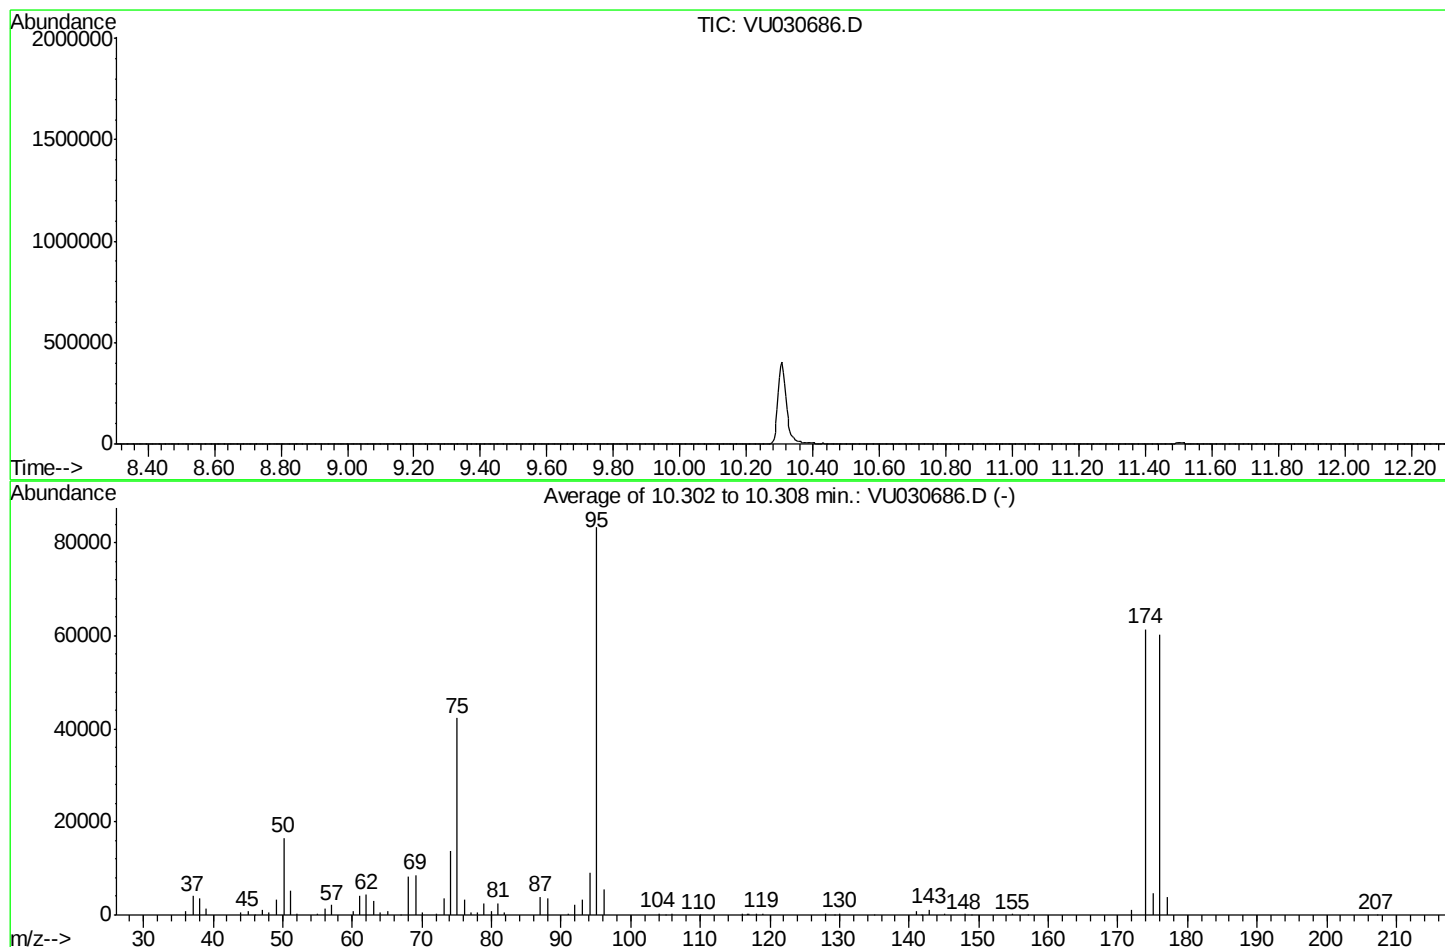

AutoFind: Scans 2865, 2866, 2867; Background Corrected with Scan 2854

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.0	16650	PASS
75	95	30	80	50.8	42336	PASS
95	95	100	100	100.0	83325	PASS
96	95	5	9	6.8	5636	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	73.8	61472	PASS
175	174	5	9	7.8	4771	PASS
176	174	95	101	98.2	60384	PASS
177	176	5	9	6.4	3852	PASS

Scan 2854 (10.266 min): VU030686.D
BFB50

m/z	Abundance
40.00	579.0
41.10	117.0
43.10	105.0
44.10	874.0

Instrument :
MSVOA_U
ClientSampleId :
BFB50

m/z	Abundance
36.10	847.0
37.00	4276.0
38.10	3453.0
39.00	1184.0
40.00	541.0
44.00	1402.0
45.00	835.0
46.00	148.0
47.00	989.0
48.00	570.0
49.00	3062.0
50.10	16584.0
51.10	4820.0
52.00	204.0
55.00	271.0
56.10	1148.0
57.10	2222.0
60.00	883.0
61.10	4220.0
62.10	4153.0
63.00	3018.0
64.00	453.0
65.10	636.0
66.90	128.0
68.10	8059.0
69.10	8360.0
70.00	803.0
72.00	326.0
73.10	3303.0
74.10	13595.0
75.10	42168.0
76.00	3462.0
77.00	653.0
78.00	592.0
78.90	2467.0
80.00	737.0
81.00	2617.0
81.90	644.0
87.00	3961.0
88.00	3338.0
90.90	201.0
92.00	2264.0
93.00	3265.0
94.10	9140.0
95.10	80192.0
96.10	5608.0
104.00	344.0
106.00	300.0
116.00	228.0
116.80	488.0
118.00	235.0
118.90	401.0
128.00	329.0
130.10	311.0
141.00	689.0
141.80	161.0
143.00	1144.0
145.10	316.0
148.00	171.0
154.90	262.0
157.00	135.0
172.00	1060.0
174.00	57712.0
175.00	4557.0
176.00	58112.0
177.00	3718.0
207.20	100.0

Instrument :
MSVOA_U
ClientSampleId :
BFB50

m/z	Abundance
36.10	895.0
37.10	4087.0
38.10	3726.0
39.00	1414.0
40.00	572.0
44.00	1497.0
45.00	744.0
46.00	149.0
47.10	1210.0
48.00	628.0
49.00	3262.0
50.10	16984.0
51.10	5197.0
52.00	256.0
55.10	308.0
56.10	1306.0
57.10	2141.0
60.00	790.0
61.10	4379.0
62.10	4494.0
63.00	3247.0
64.00	475.0
65.00	753.0
68.10	8499.0
69.10	8762.0
70.00	643.0
72.00	402.0
73.10	3695.0
74.10	14128.0
75.10	43648.0
76.00	3362.0
77.00	642.0
78.00	563.0
78.90	2491.0
80.00	711.0
80.90	2674.0
81.90	562.0
87.00	4205.0
88.00	3727.0
90.90	256.0
92.00	2423.0
93.00	3274.0
94.10	9416.0
95.10	86384.0
96.10	5858.0
104.00	355.0
104.90	142.0
106.00	335.0
116.00	223.0
117.00	421.0
118.10	231.0
118.90	412.0
128.00	320.0
130.10	448.0
141.00	694.0
141.80	131.0
143.00	1177.0
145.10	328.0
148.00	179.0
149.00	118.0
154.90	242.0
157.00	133.0
172.00	1157.0
174.00	62848.0
175.00	4932.0
176.00	62208.0
177.00	3977.0

Instrument :
MSVOA_U
ClientSampleId :
BFB50

m/z	Abundance
36.10	830.0
37.10	3645.0
38.10	3827.0
39.00	1577.0
40.00	559.0
44.00	1537.0
45.00	556.0
46.00	102.0
47.10	1205.0
48.00	639.0
49.10	3246.0
50.10	16384.0
51.10	5335.0
52.00	284.0
55.10	354.0
56.10	1323.0
57.00	2016.0
60.10	658.0
61.10	3910.0
62.00	4421.0
63.00	3095.0
64.00	428.0
65.00	876.0
68.10	8338.0
69.10	8660.0
70.00	554.0
72.00	498.0
73.10	3949.0
74.10	13866.0
75.10	41192.0
76.10	3379.0
77.10	593.0
78.00	464.0
78.90	2198.0
80.00	737.0
80.90	2541.0
81.90	464.0
87.10	3800.0
88.00	3521.0
91.00	320.0
92.00	2334.0
93.10	3116.0
94.10	8990.0
95.10	83400.0
96.10	5442.0
104.00	332.0
105.00	223.0
106.00	319.0
109.90	105.0
116.00	295.0
117.00	488.0
118.10	222.0
119.00	345.0
128.00	233.0
129.20	143.0
130.10	450.0
134.90	101.0
141.00	733.0
141.90	145.0
142.90	1084.0
145.00	304.0
147.90	197.0
149.00	139.0
154.80	220.0
172.00	994.0
174.00	63856.0
175.10	4826.0
176.00	60832.0
177.10	3862.0

Instrument :
MSVOA_U
ClientSampleId :
BFB50