

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_U\Data\VU040521\  
 Data File : VU042931.D  
 Acq On : 05 Apr 2021 15:25  
 Operator : SY/MD  
 Sample : M1903-02  
 Misc : 5.0mL/MSVOA\_U/WATER  
 ALS Vial : 11 Sample Multiplier: 1

Instrument :  
 MSVOA\_U  
 ClientSampleId :

Quant Time: Apr 06 01:19:27 2021  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_U\Method\82U032421W.M  
 Quant Title : SW846 8260  
 QLast Update : Thu Mar 25 05:42:00 2021  
 Response via : Initial Calibration


| Compound                      | R.T.   | QIon | Response | Conc      | Units  | Dev(Min) |
|-------------------------------|--------|------|----------|-----------|--------|----------|
| Internal Standards            |        |      |          |           |        |          |
| 1) Pentafluorobenzene         | 5.382  | 168  | 124029   | 50.00     | ug/l   | 0.00     |
| 34) 1,4-Difluorobenzene       | 6.256  | 114  | 197110   | 50.00     | ug/l   | 0.00     |
| 63) Chlorobenzene-d5          | 9.423  | 117  | 187765   | 50.00     | ug/l   | 0.00     |
| 72) 1,4-Dichlorobenzene-d4    | 11.819 | 152  | 97301    | 50.00     | ug/l   | 0.00     |
| System Monitoring Compounds   |        |      |          |           |        |          |
| 33) 1,2-Dichloroethane-d4     | 5.710  | 65   | 97880    | 49.50     | ug/l   | 0.00     |
| Spiked Amount                 | 50.000 |      | Recovery | =         | 99.00% |          |
| 35) Dibromofluoromethane      | 5.298  | 113  | 69681    | 47.37     | ug/l   | 0.00     |
| Spiked Amount                 | 50.000 |      | Recovery | =         | 94.74% |          |
| 50) Toluene-d8                | 7.906  | 98   | 247467   | 47.82     | ug/l   | 0.00     |
| Spiked Amount                 | 50.000 |      | Recovery | =         | 95.64% |          |
| 62) 4-Bromofluorobenzene      | 10.639 | 95   | 92991    | 46.24     | ug/l   | 0.00     |
| Spiked Amount                 | 50.000 |      | Recovery | =         | 92.48% |          |
| Target Compounds              |        |      |          |           |        |          |
|                               |        |      |          |           | Qvalue |          |
| 3) Chloromethane              | 1.523  | 50   | 372      | 0.24      | ug/l # | 86       |
| 5) Bromomethane               | 1.867  | 94   | 209      | Below Cal |        | 84       |
| 6) Chloroethane               | 1.932  | 64   | 96       | Below Cal | #      | 43       |
| 10) Methyl Iodide             | 2.732  | 142  | 354      | 0.22      | ug/l # | 52       |
| 11) Tert butyl alcohol        | 3.221  | 59   | 10261    | 24.27     | ug/l # | 88       |
| 13) Acrolein                  | 2.494  | 56   | 718      | 0.72      | ug/l # | 64       |
| 16) Acetone                   | 2.646  | 43   | 21122    | 8.05      | ug/l   | 97       |
| 18) Methyl Acetate            | 2.967  | 43   | 1124     | 0.50      | ug/l # | 68       |
| 25) 2-Butanone                | 4.729  | 43   | 3480     | 2.16      | ug/l   | 99       |
| 31) Cyclohexane               | 5.379  | 56   | 3039     | 1.23      | ug/l # | 12       |
| 36) 1,1-Dichloropropene       | 5.382  | 75   | 10586    | 5.43      | ug/l # | 47       |
| 37) Ethyl Acetate             | 4.729  | 43   | 3480     | 1.15      | ug/l # | 72       |
| 38) Carbon Tetrachloride      | 5.385  | 117  | 12301    | 5.53      | ug/l # | 16       |
| 40) Benzene                   | 5.787  | 78   | 2188     | 0.38      | ug/l   | 96       |
| 48) Methyl methacrylate       | 6.887  | 41   | 2587     | 1.18      | ug/l # | 48       |
| 51) 4-Methyl-2-Pentanone      | 7.806  | 43   | 815      | 0.26      | ug/l # | 84       |
| 52) Toluene                   | 7.977  | 92   | 4401     | 1.23      | ug/l   | 96       |
| 59) 2-Hexanone                | 8.703  | 43   | 592      | 0.23      | ug/l # | 51       |
| 68) m/p-Xylenes               | 9.700  | 106  | 1961     | 0.78      | ug/l   | 84       |
| 69) o-Xylene                  | 10.108 | 106  | 606      | 0.25      | ug/l   | 48       |
| 70) Styrene                   | 10.118 | 104  | 883      | 0.21      | ug/l # | 89       |
| 76) 1,2,3-Trichloropropane    | 10.639 | 75   | 53631    | 21.67     | ug/l # | 37       |
| 81) trans-1,4-Dichloro-2-b... | 10.639 | 75   | 53631    | 64.21     | ug/l # | 6        |
| 84) 1,2,4-Trimethylbenzene    | 11.475 | 105  | 3575     | 0.66      | ug/l   | 85       |
| 85) sec-Butylbenzene          | 11.475 | 105  | 3575     | 0.59      | ug/l # | 57       |
| 95) Naphthalene               | 14.095 | 128  | 6750     | 3.55      | ug/l   | 97       |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_U\Data\VU040521\  
Data File : VU042931.D  
Acq On : 05 Apr 2021 15:25  
Operator : SY/MD  
Sample : M1903-02  
Misc : 5.0mL/MSVOA\_U/WATER  
ALS Vial : 11 Sample Multiplier: 1

Instrument :  
MSVOA\_U  
ClientSampleId :

Quant Time: Apr 06 01:19:27 2021  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_U\Method\82U032421W.M  
Quant Title : SW846 8260  
QLast Update : Thu Mar 25 05:42:00 2021  
Response via : Initial Calibration




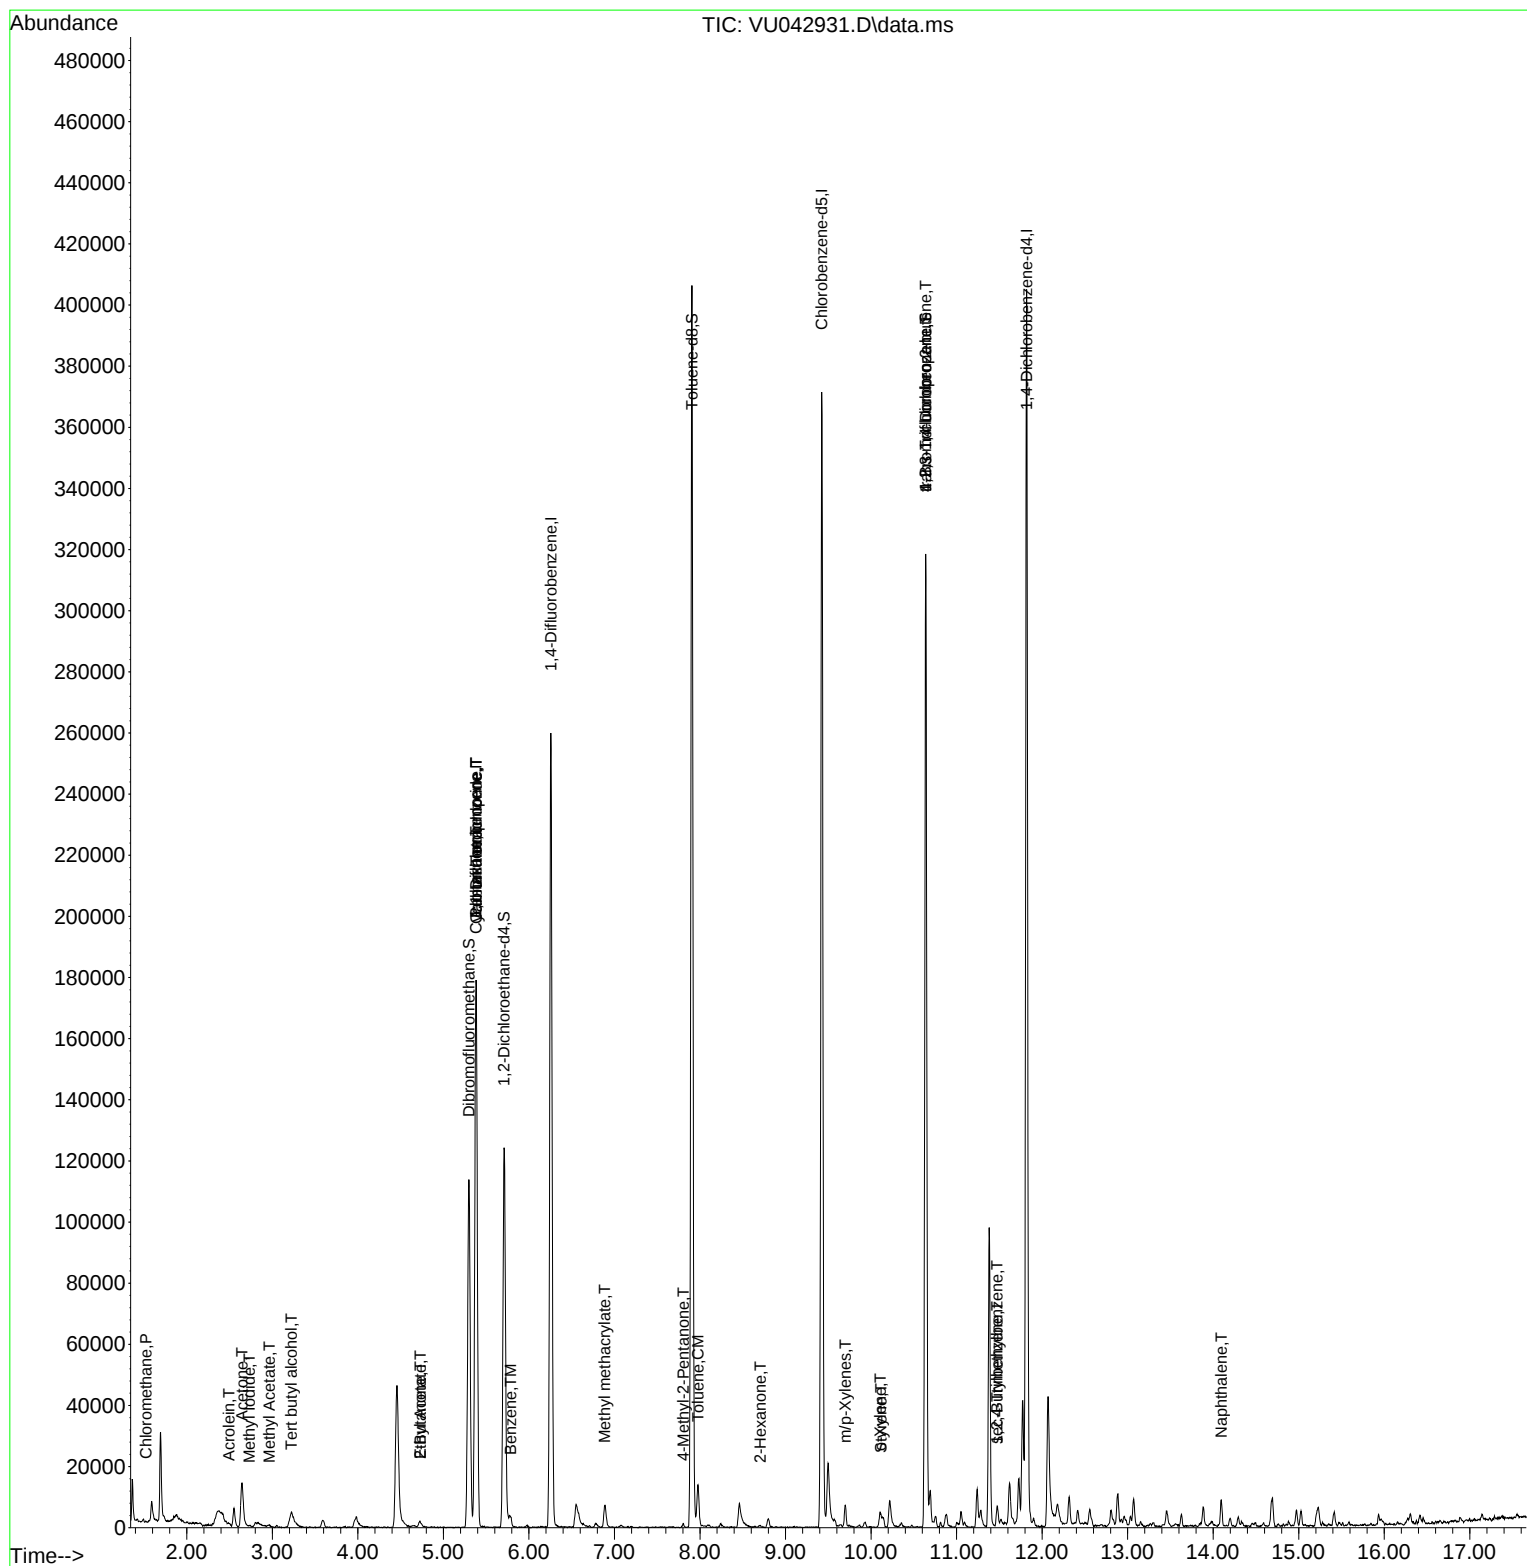




#1  
Pentafluorobenzene  
Concen: 50.00 ug/l  
RT: 5.382 min Scan# 1257  
Delta R.T. -0.003 min  
Lab File: VU042931.D  
Acq: 05 Apr 2021 15:25




Instrument :  
MSVOA\_U  
ClientSampleId :


Tgt Ion:168 Resp: 124029  
Ion Ratio Lower Upper  
168 100  
99 59.4 46.4 69.6

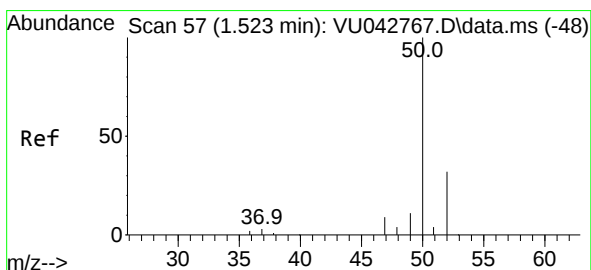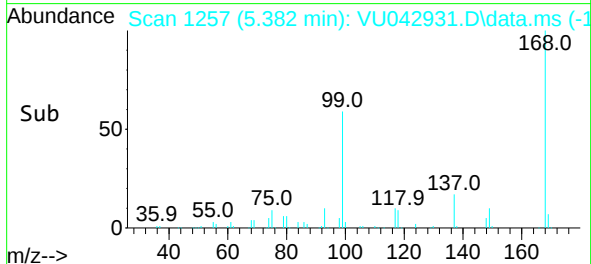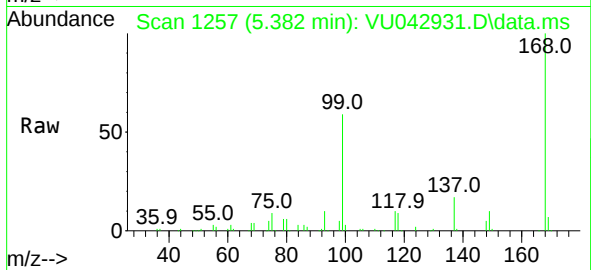

#3  
Chloromethane  
Concen: 0.24 ug/l  
RT: 1.523 min Scan# 57  
Delta R.T. 0.000 min  
Lab File: VU042931.D  
Acq: 05 Apr 2021 15:25

Tgt Ion: 50 Resp: 372  
Ion Ratio Lower Upper  
50 100  
52 39.5 25.4 38.0#


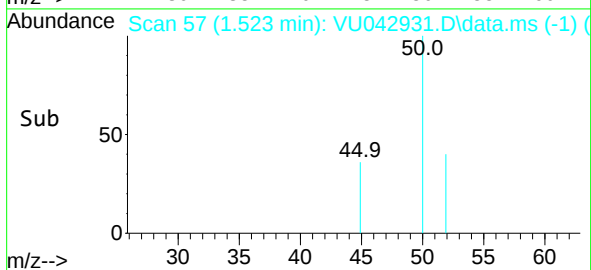

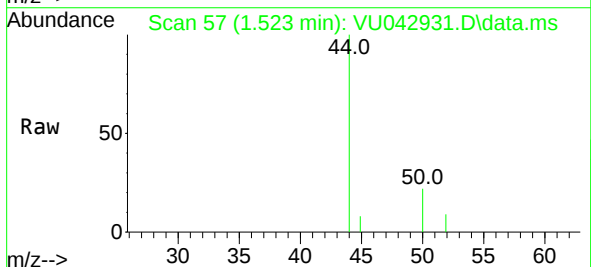


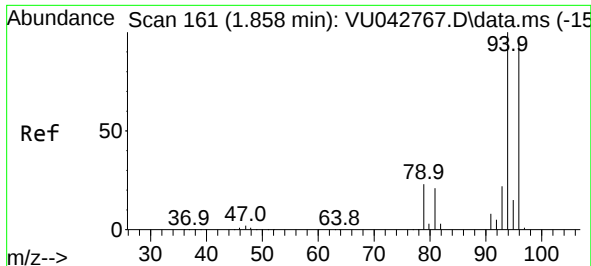

#5  
Bromomethane  
Concen: Below Cal  
RT: 1.867 min Scan# 164  
Delta R.T. 0.009 min  
Lab File: VU042931.D  
Acq: 05 Apr 2021 15:25




Instrument :  
MSVOA\_U  
ClientSampleId :


Tgt Ion: 94 Resp: 209  
Ion Ratio Lower Upper  
94 100  
96 80.3 77.1 115.7

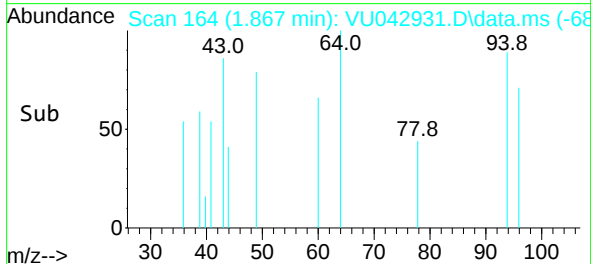

#6  
Chloroethane  
Concen: Below Cal  
RT: 1.932 min Scan# 184  
Delta R.T. -0.000 min  
Lab File: VU042931.D  
Acq: 05 Apr 2021 15:25


Tgt Ion: 64 Resp: 96  
Ion Ratio Lower Upper  
64 100  
66 0.0 25.0 37.6#

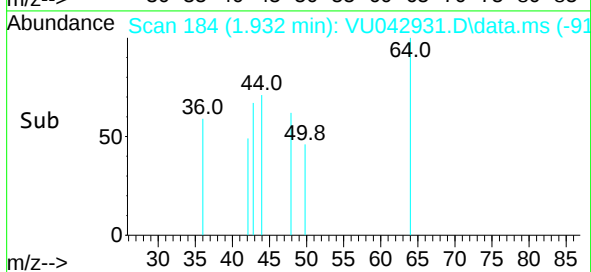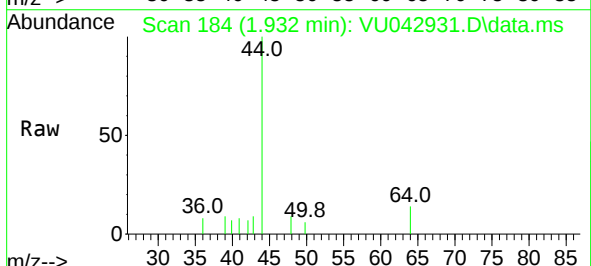






#10  
Methyl Iodide  
Concen: 0.22 ug/l  
RT: 2.732 min Scan# 433  
Delta R.T. 0.003 min  
Lab File: VU042931.D  
Acq: 05 Apr 2021 15:25

Instrument :  
MSVOA\_U  
ClientSampled :



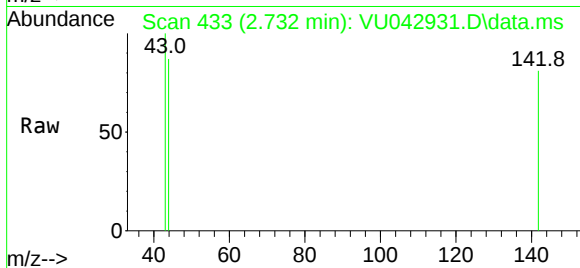



Tgt Ion:142 Resp: 354  
Ion Ratio Lower Upper  
142 100  
127 13.3 38.7 58.1#  
141 0.0 12.0 18.0#



#11  
Tert butyl alcohol  
Concen: 24.27 ug/l  
RT: 3.221 min Scan# 585  
Delta R.T. -0.000 min  
Lab File: VU042931.D  
Acq: 05 Apr 2021 15:25

Tgt Ion: 59 Resp: 10261  
Ion Ratio Lower Upper  
59 100  
57 4.8 7.4 11.2#


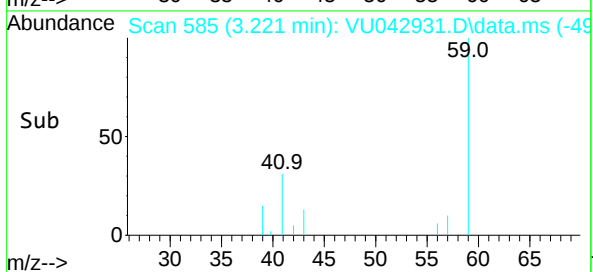

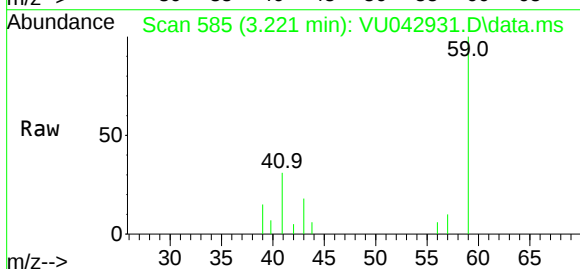




#13  
Acrolein  
Concen: 0.72 ug/l  
RT: 2.494 min Scan# 359  
Delta R.T. 0.000 min  
Lab File: VU042931.D  
Acq: 05 Apr 2021 15:25




Instrument :  
MSVOA\_U  
ClientSampleId :


Tgt Ion: 56 Resp: 718  
Ion Ratio Lower Upper  
56 100  
55 40.3 55.8 83.8#

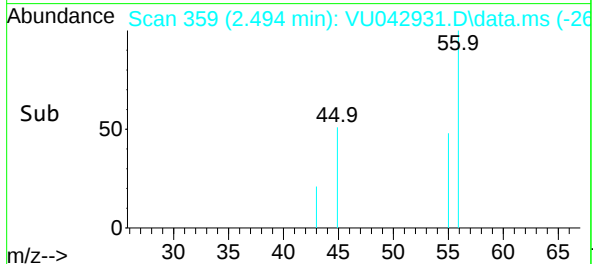

#16  
Acetone  
Concen: 8.05 ug/l  
RT: 2.646 min Scan# 406  
Delta R.T. 0.007 min  
Lab File: VU042931.D  
Acq: 05 Apr 2021 15:25

Tgt Ion: 43 Resp: 21122  
Ion Ratio Lower Upper  
43 100  
58 28.3 21.6 32.4


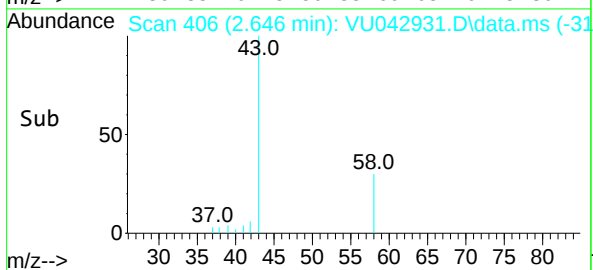

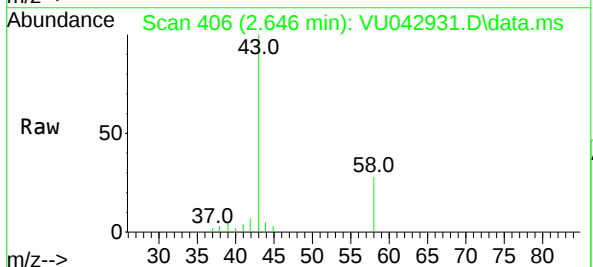




#18  
Methyl Acetate  
Concen: 0.50 ug/l  
RT: 2.967 min Scan# 506  
Delta R.T. 0.013 min  
Lab File: VU042931.D  
Acq: 05 Apr 2021 15:25




Instrument :  
MSVOA\_U  
ClientSampled :


Tgt Ion: 43 Resp: 1124  
Ion Ratio Lower Upper  
43 100  
74 5.7 16.2 24.4#

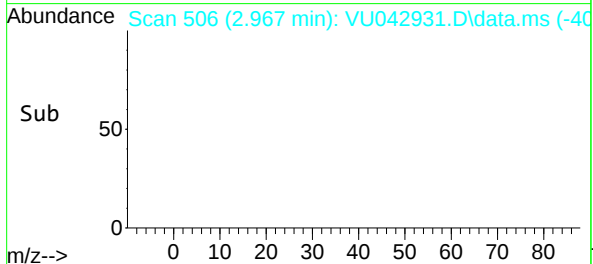

#25  
2-Butanone  
Concen: 2.16 ug/l  
RT: 4.729 min Scan# 1054  
Delta R.T. 0.016 min  
Lab File: VU042931.D  
Acq: 05 Apr 2021 15:25

Tgt Ion: 43 Resp: 3480  
Ion Ratio Lower Upper  
43 100  
72 21.8 17.7 26.5

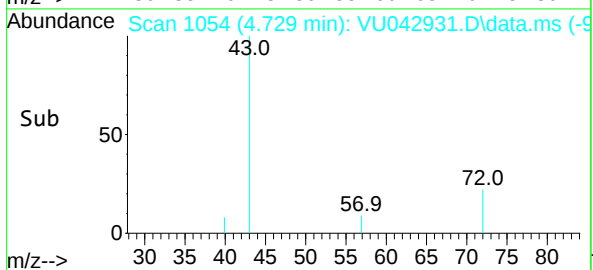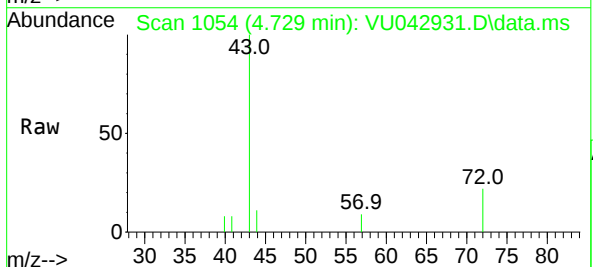



#31

Cyclohexane

Concen: 1.23 ug/l





RT: 5.379 min Scan# 1256

Delta R.T. -0.019 min

Lab File: VU042931.D

Acq: 05 Apr 2021 15:25

|          |       |       |       |
|----------|-------|-------|-------|
| Tgt Ion: | 56    | Resp: | 3039  |
| Ion      | Ratio | Lower | Upper |
| 56       | 100   |       |       |
| 69       | 156.9 | 23.3  | 34.9# |
| 84       | 105.8 | 62.2  | 93.4# |



#33

1,2-Dichloroethane-d4

Concen: 49.50 ug/l




RT: 5.710 min Scan# 1359


Delta R.T. -0.000 min

Lab File: VU042931.D

Acq: 05 Apr 2021 15:25

|          |       |       |       |
|----------|-------|-------|-------|
| Tgt Ion: | 65    | Resp: | 97880 |
| Ion      | Ratio | Lower | Upper |
| 65       | 100   |       |       |
| 67       | 50.8  | 0.0   | 98.8  |

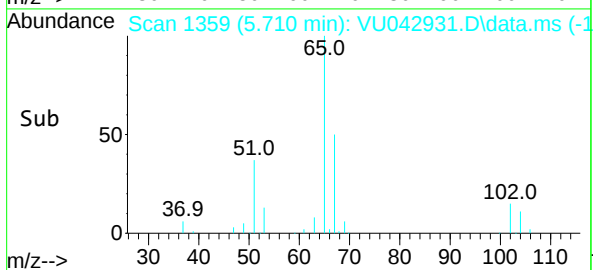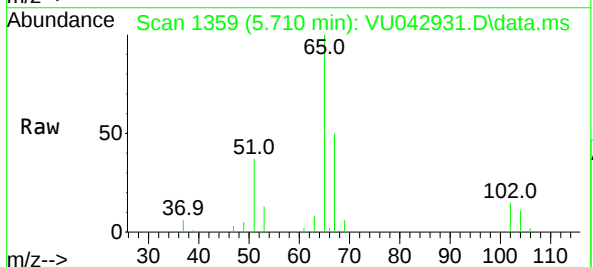



#34

1,4-Difluorobenzene

Concen: 50.00 ug/l

RT: 6.256 min Scan# 1529

Delta R.T. -0.004 min

Lab File: VU042931.D

Acq: 05 Apr 2021 15:25





Tgt Ion:114 Resp: 197110

Ion Ratio Lower Upper

114 100

63 22.8 0.0 46.8

88 16.1 0.0 32.2

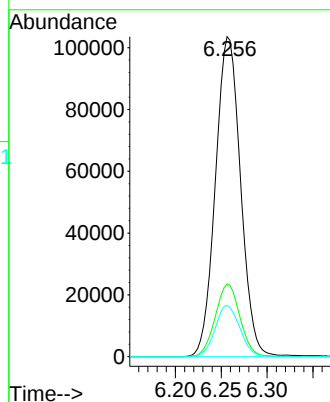

#35

Dibromofluoromethane

Concen: 47.37 ug/l

RT: 5.298 min Scan# 1231

Delta R.T. -0.000 min

Lab File: VU042931.D

Acq: 05 Apr 2021 15:25




Tgt Ion:113 Resp: 69681


Ion Ratio Lower Upper

113 100

111 103.0 82.1 123.1


192 21.1 17.6 26.4

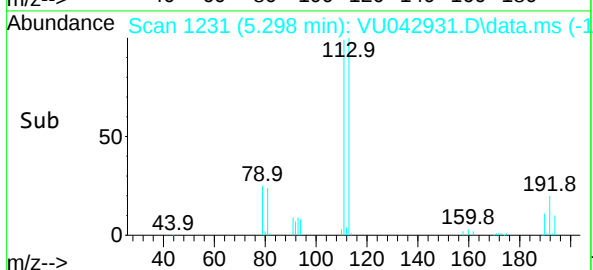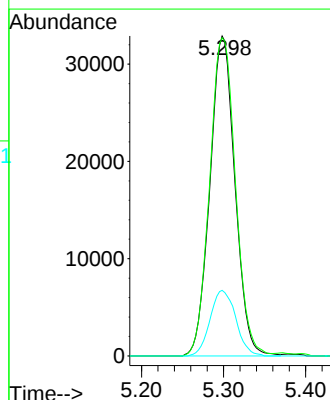






#36  
1,1-Dichloropropene  
Concen: 5.43 ug/l  
RT: 5.382 min Scan# 1257  
Delta R.T. -0.154 min  
Lab File: VU042931.D  
Acq: 05 Apr 2021 15:25


Instrument :  
MSVOA\_U  
ClientSampleId :

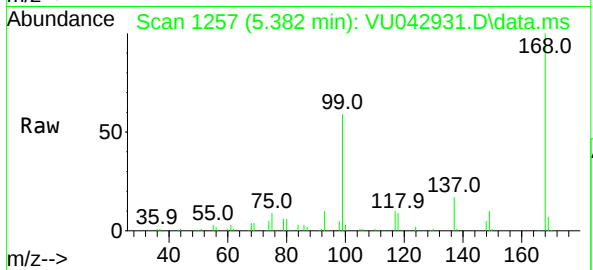



Tgt Ion: 75 Resp: 10586  
Ion Ratio Lower Upper  
75 100  
110 4.6 16.6 49.7#  
77 0.0 24.7 37.1#

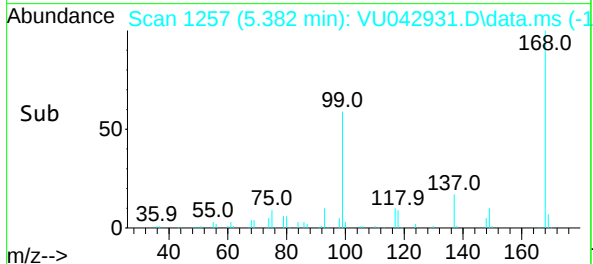


#37  
Ethyl Acetate  
Concen: 1.15 ug/l  
RT: 4.729 min Scan# 1054  
Delta R.T. -0.084 min  
Lab File: VU042931.D  
Acq: 05 Apr 2021 15:25

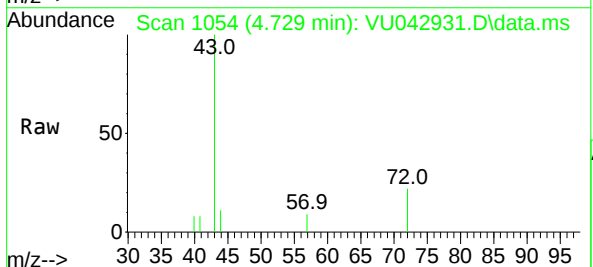


Tgt Ion: 43 Resp: 3480  
Ion Ratio Lower Upper  
43 100  
61 0.0 9.7 14.5#  
70 0.0 6.6 9.8#

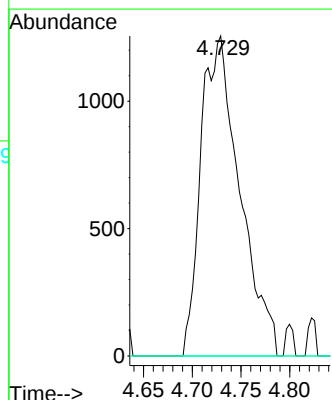






#38  
Carbon Tetrachloride  
Concen: 5.53 ug/l  
RT: 5.385 min Scan# 1258  
Delta R.T. -0.148 min  
Lab File: VU042931.D  
Acq: 05 Apr 2021 15:25

Instrument :  
MSVOA\_U  
ClientSampleId :







Tgt Ion:117 Resp: 12301  
Ion Ratio Lower Upper  
117 100  
119 3.7 75.2 112.8#  
121 0.0 24.2 36.4#

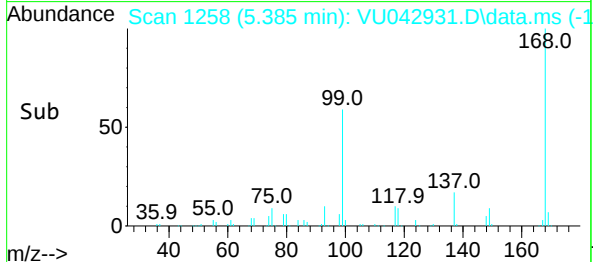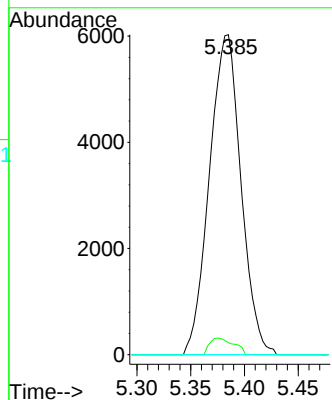

#40  
Benzene  
Concen: 0.38 ug/l  
RT: 5.787 min Scan# 1383  
Delta R.T. 0.003 min  
Lab File: VU042931.D  
Acq: 05 Apr 2021 15:25

Tgt Ion: 78 Resp: 2188  
Ion Ratio Lower Upper  
78 100  
77 26.9 19.9 29.9

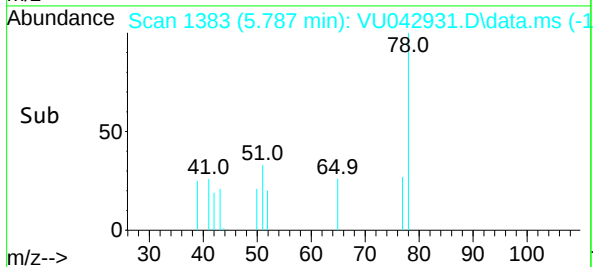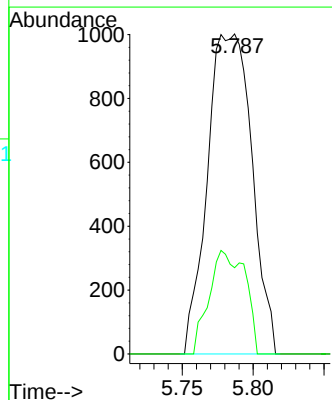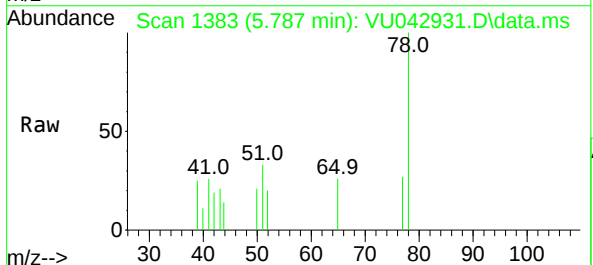



#48

Methyl methacrylate

Concen: 1.18 ug/l

RT: 6.887 min Scan# 1725





Delta R.T. -0.080 min

Lab File: VU042931.D

Acq: 05 Apr 2021 15:25

|             |             |
|-------------|-------------|
| Tgt Ion: 41 | Resp: 2587  |
| Ion Ratio   | Lower Upper |
| 41 100      |             |
| 69 0.0      | 55.9 83.9#  |
| 39 50.9     | 49.7 74.5   |

Instrument :  
MSVOA\_U  
ClientSampled :

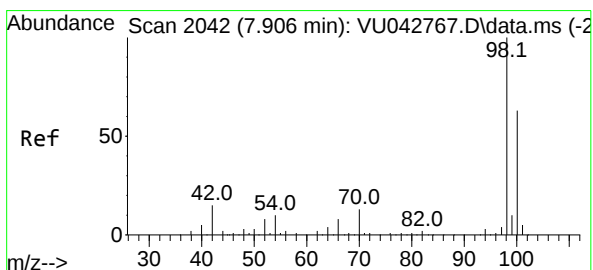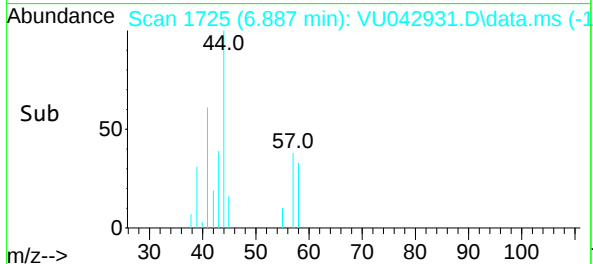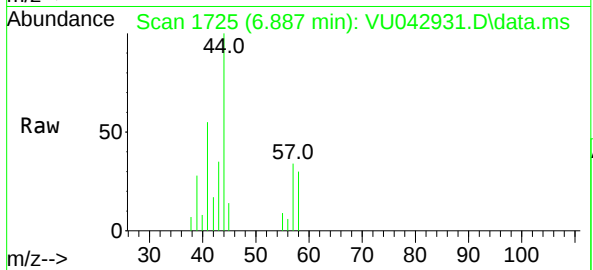

#50

Toluene-d8

Concen: 47.82 ug/l




RT: 7.906 min Scan# 2042


Delta R.T. -0.000 min

Lab File: VU042931.D

Acq: 05 Apr 2021 15:25

|             |              |
|-------------|--------------|
| Tgt Ion: 98 | Resp: 247467 |
| Ion Ratio   | Lower Upper  |
| 98 100      |              |
| 100 63.3    | 50.4 75.6    |



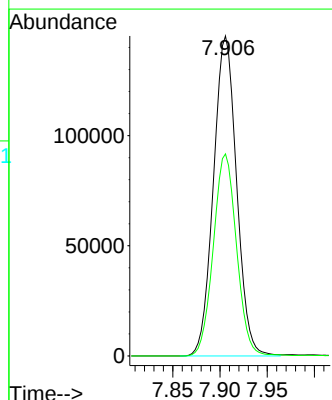
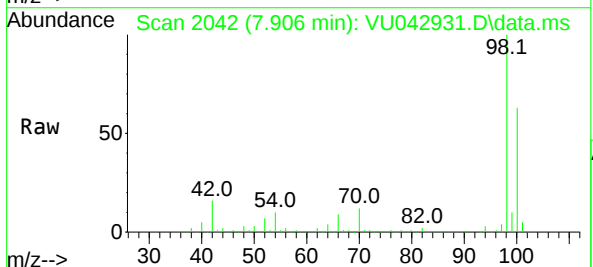




#51  
4-Methyl-2-Pentanone  
Concen: 0.26 ug/l  
RT: 7.806 min Scan# 2011  
Delta R.T. 0.006 min  
Lab File: VU042931.D  
Acq: 05 Apr 2021 15:25




Instrument :  
MSVOA\_U  
ClientSampled :


Tgt Ion: 43 Resp: 815  
Ion Ratio Lower Upper  
43 100  
58 25.3 27.4 41.2#

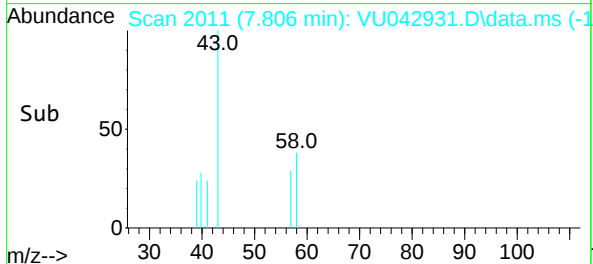

#52  
Toluene  
Concen: 1.23 ug/l  
RT: 7.977 min Scan# 2064  
Delta R.T. -0.000 min  
Lab File: VU042931.D  
Acq: 05 Apr 2021 15:25

Tgt Ion: 92 Resp: 4401  
Ion Ratio Lower Upper  
92 100  
91 180.6 140.6 210.8


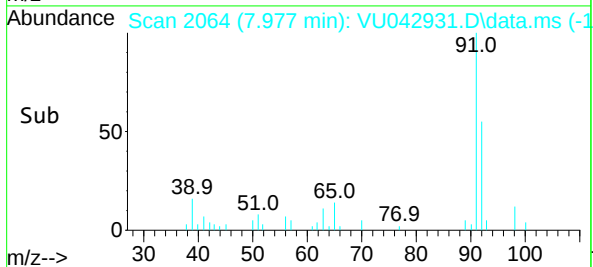

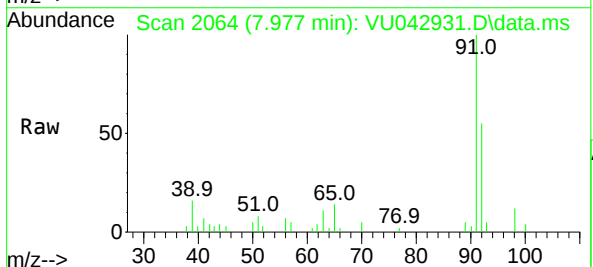


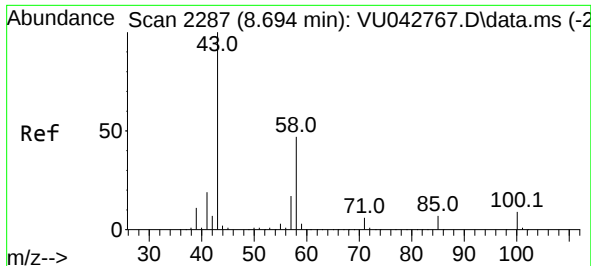

#59  
2-Hexanone  
Concen: 0.23 ug/l  
RT: 8.703 min Scan# 2290  
Delta R.T. 0.010 min  
Lab File: VU042931.D  
Acq: 05 Apr 2021 15:25




Instrument :  
MSVOA\_U  
ClientSampled :


Tgt Ion: 43 Resp: 592  
Ion Ratio Lower Upper  
43 100  
58 14.5 23.8 71.2#

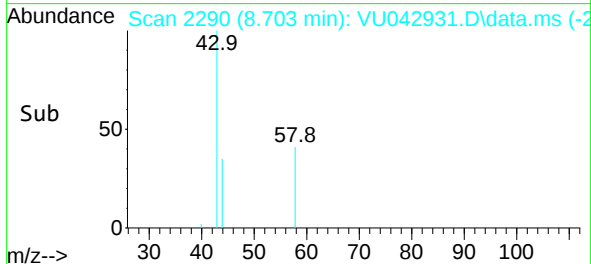

#62  
4-Bromofluorobenzene  
Concen: 46.24 ug/l  
RT: 10.639 min Scan# 2892  
Delta R.T. -0.000 min  
Lab File: VU042931.D  
Acq: 05 Apr 2021 15:25

Tgt Ion: 95 Resp: 92991  
Ion Ratio Lower Upper  
95 100  
174 88.9 0.0 175.2  
176 83.5 0.0 167.4


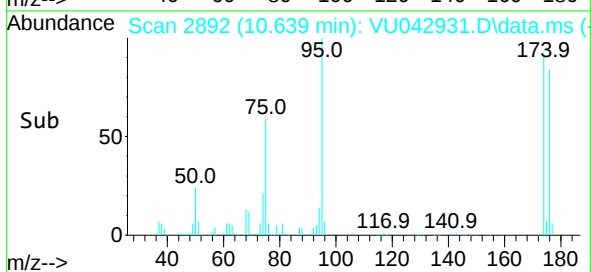

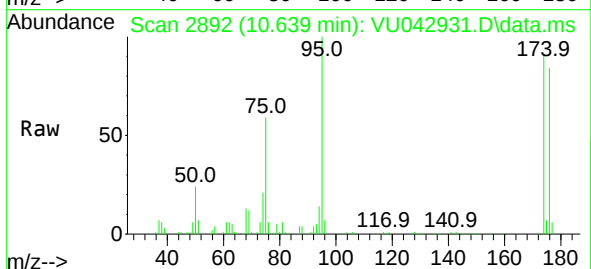




#63  
Chlorobenzene-d5  
Concen: 50.00 ug/l  
RT: 9.423 min Scan# 2514  
Delta R.T. -0.003 min  
Lab File: VU042931.D  
Acq: 05 Apr 2021 15:25




Instrument :  
MSVOA\_U  
ClientSampleId :


Tgt Ion:117 Resp: 187765  
Ion Ratio Lower Upper  
117 100  
82 57.8 45.5 68.3  
119 30.9 26.2 39.4

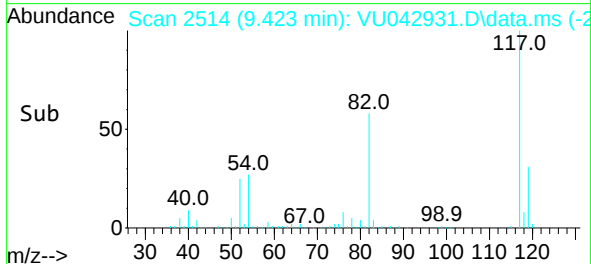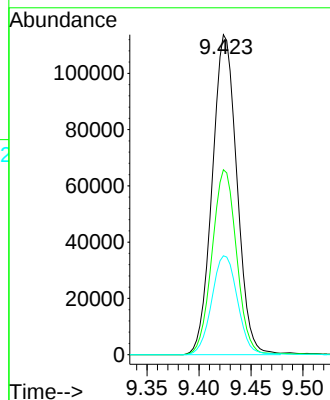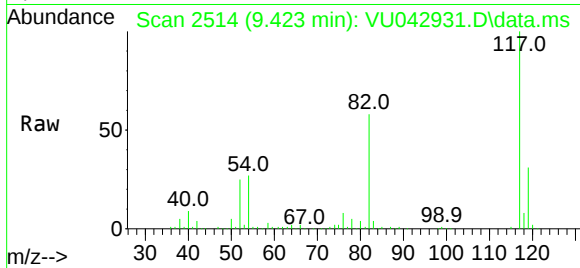

#68  
m/p-Xylenes  
Concen: 0.78 ug/l  
RT: 9.700 min Scan# 2600  
Delta R.T. -0.000 min  
Lab File: VU042931.D  
Acq: 05 Apr 2021 15:25

Tgt Ion:106 Resp: 1961  
Ion Ratio Lower Upper  
106 100  
91 185.8 168.3 252.5



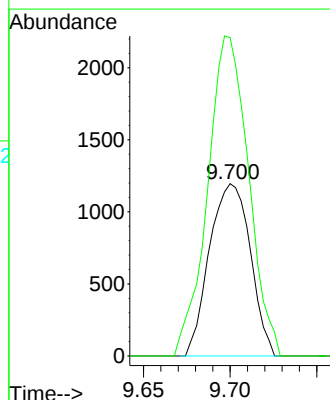
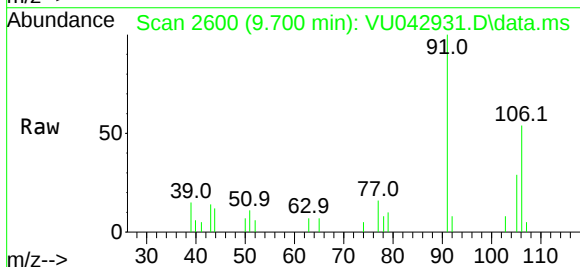




#69  
o-Xylene  
Concen: 0.25 ug/l  
RT: 10.108 min Scan# 2727  
Delta R.T. -0.000 min  
Lab File: VU042931.D  
Acq: 05 Apr 2021 15:25




Instrument :  
MSVOA\_U  
ClientSampled :


Tgt Ion:106 Resp: 606  
Ion Ratio Lower Upper  
106 100  
91 303.0 109.9 329.7

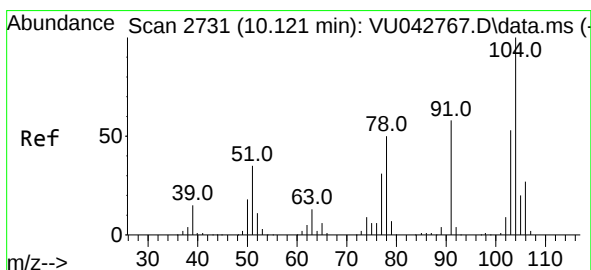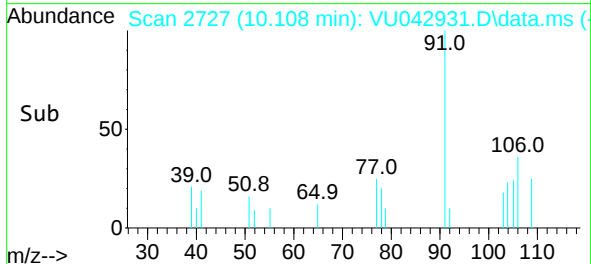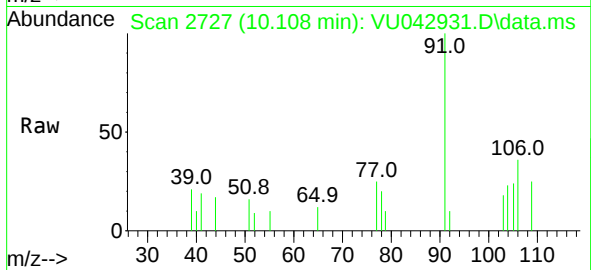

#70  
Styrene  
Concen: 0.21 ug/l  
RT: 10.118 min Scan# 2730  
Delta R.T. -0.003 min  
Lab File: VU042931.D  
Acq: 05 Apr 2021 15:25

Tgt Ion:104 Resp: 883  
Ion Ratio Lower Upper  
104 100  
78 66.7 43.2 64.8#  
103 60.0 45.0 67.4


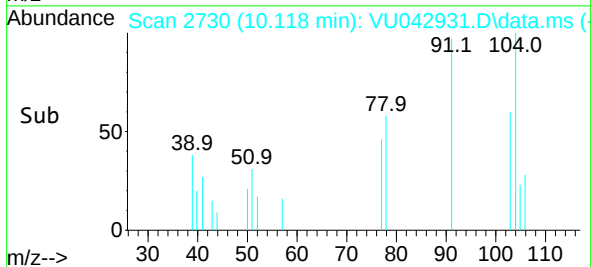

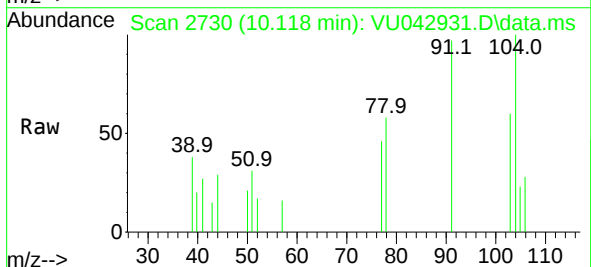


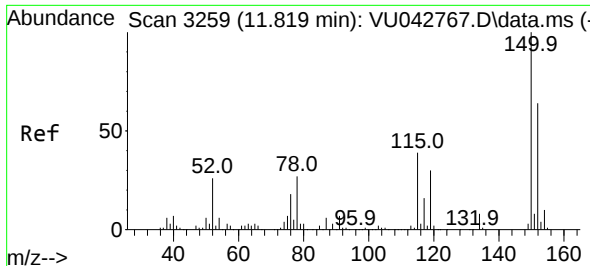

#72  
 1,4-Dichlorobenzene-d4  
 Concen: 50.00 ug/l  
 RT: 11.819 min Scan# 3259  
 Delta R.T. -0.000 min  
 Lab File: VU042931.D  
 Acq: 05 Apr 2021 15:25




Instrument :  
 MSVOA\_U  
 ClientSampleId :


Tgt Ion:152 Resp: 97301  
 Ion Ratio Lower Upper  
 152 100  
 115 59.0 41.0 123.0  
 150 160.0 0.0 341.0

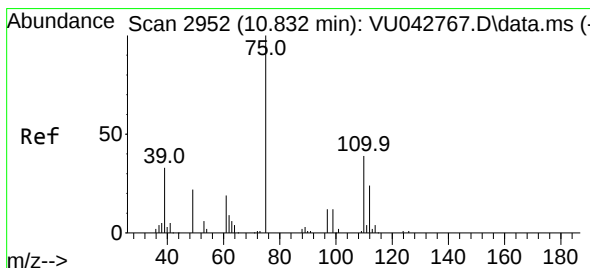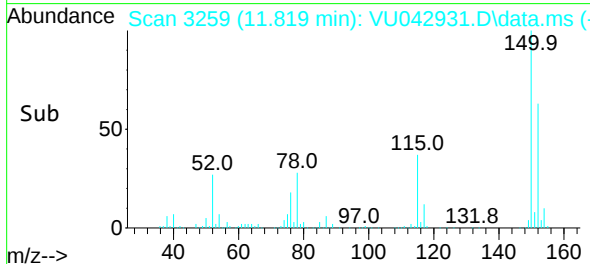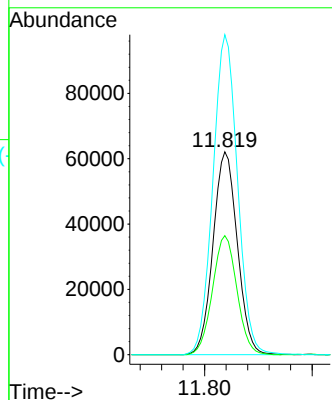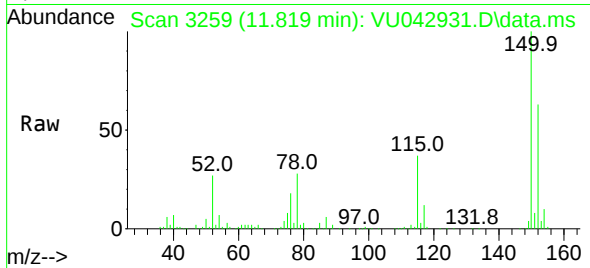

#76  
 1,2,3-Trichloropropane  
 Concen: 21.67 ug/l  
 RT: 10.639 min Scan# 2892  
 Delta R.T. -0.193 min  
 Lab File: VU042931.D  
 Acq: 05 Apr 2021 15:25

Tgt Ion: 75 Resp: 53631  
 Ion Ratio Lower Upper  
 75 100  
 77 0.9 19.6 58.8#


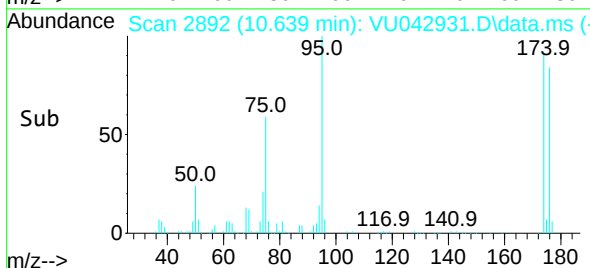
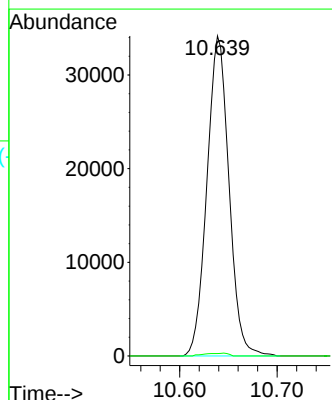
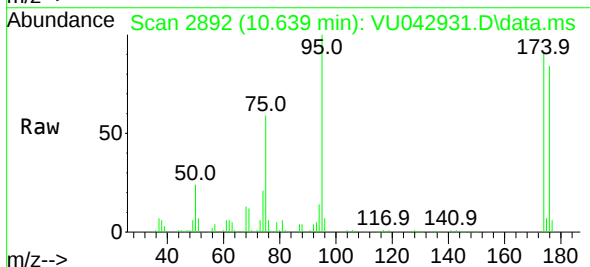


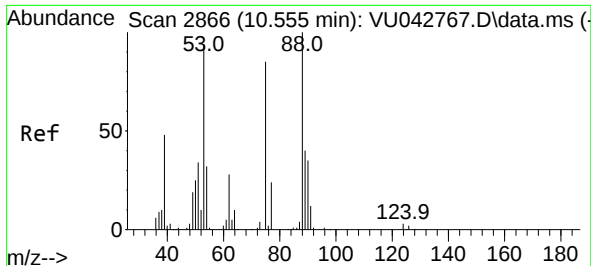

#81  
trans-1,4-Dichloro-2-butene  
Concen: 64.21 ug/l  
RT: 10.639 min Scan# 2892  
Delta R.T. 0.084 min  
Lab File: VU042931.D  
Acq: 05 Apr 2021 15:25




Instrument :  
MSVOA\_U  
ClientSampleId :


Tgt Ion: 75 Resp: 53631  
Ion Ratio Lower Upper  
75 100  
53 0.0 88.3 132.5#  
89 0.0 35.7 53.5#

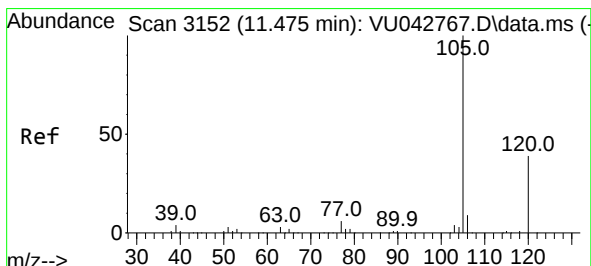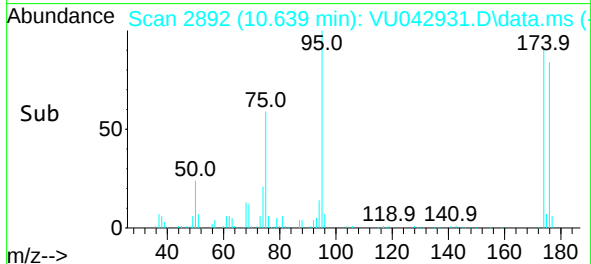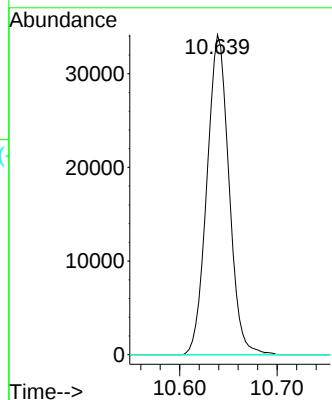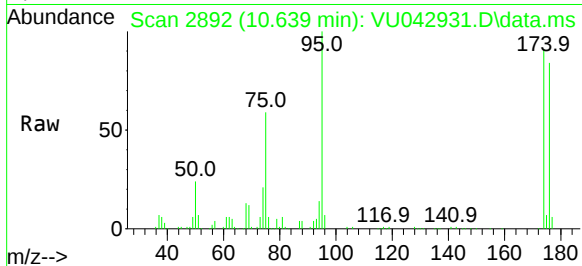

#84  
1,2,4-Trimethylbenzene  
Concen: 0.66 ug/l  
RT: 11.475 min Scan# 3152  
Delta R.T. -0.000 min  
Lab File: VU042931.D  
Acq: 05 Apr 2021 15:25

Tgt Ion: 105 Resp: 3575  
Ion Ratio Lower Upper  
105 100  
120 34.8 22.3 66.8


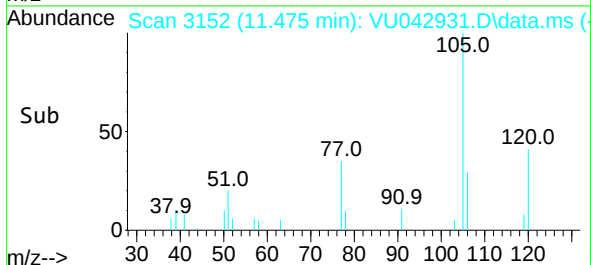
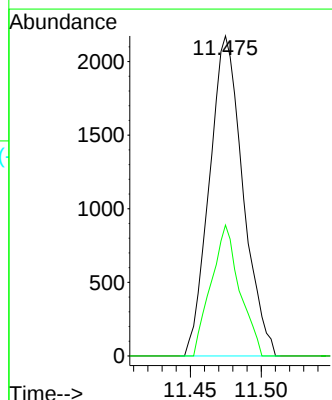
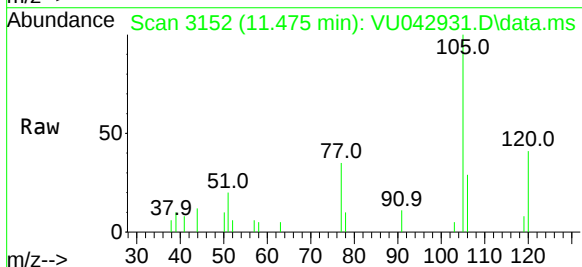


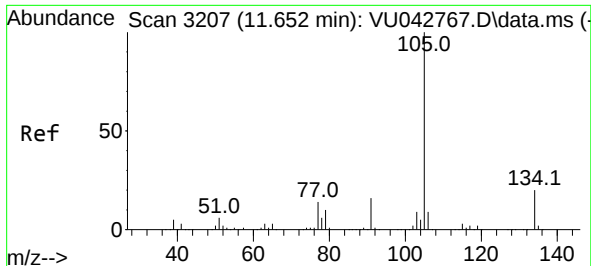

#85  
 sec-Butylbenzene  
 Concen: 0.59 ug/l  
 RT: 11.475 min Scan# 3152  
 Delta R.T. -0.177 min  
 Lab File: VU042931.D  
 Acq: 05 Apr 2021 15:25

Instrument :  
 MSVOA\_U  
 ClientSampleId :

Tgt Ion:105 Resp: 3575  
 Ion Ratio Lower Upper  
 105 100  
 134 0.0 9.8 29.5#

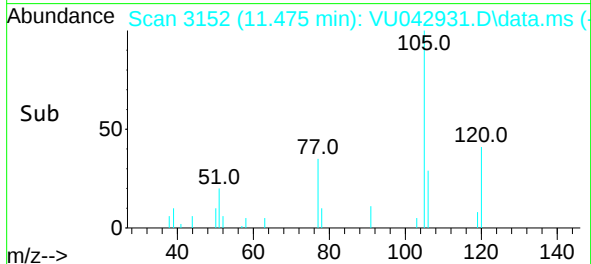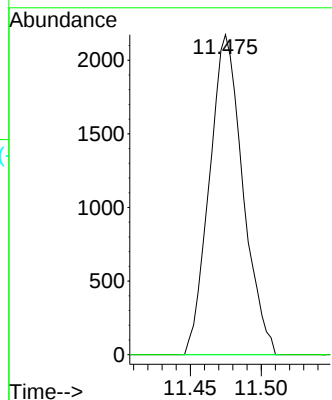

#95  
 Naphthalene  
 Concen: 3.55 ug/l  
 RT: 14.095 min Scan# 3967  
 Delta R.T. 0.000 min  
 Lab File: VU042931.D  
 Acq: 05 Apr 2021 15:25

Tgt Ion:128 Resp: 6750  
 Ion Ratio Lower Upper  
 128 100  
 127 11.6 10.9 16.3  
 129 11.3 8.7 13.1

