


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040521\
Data File : VU042921.D
Acq On : 05 Apr 2021 10:32
Operator : SY/MD
Sample : BFB
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U032421W.M
Title : SW846 8260
Last Update : Thu Mar 25 05:42:00 2021

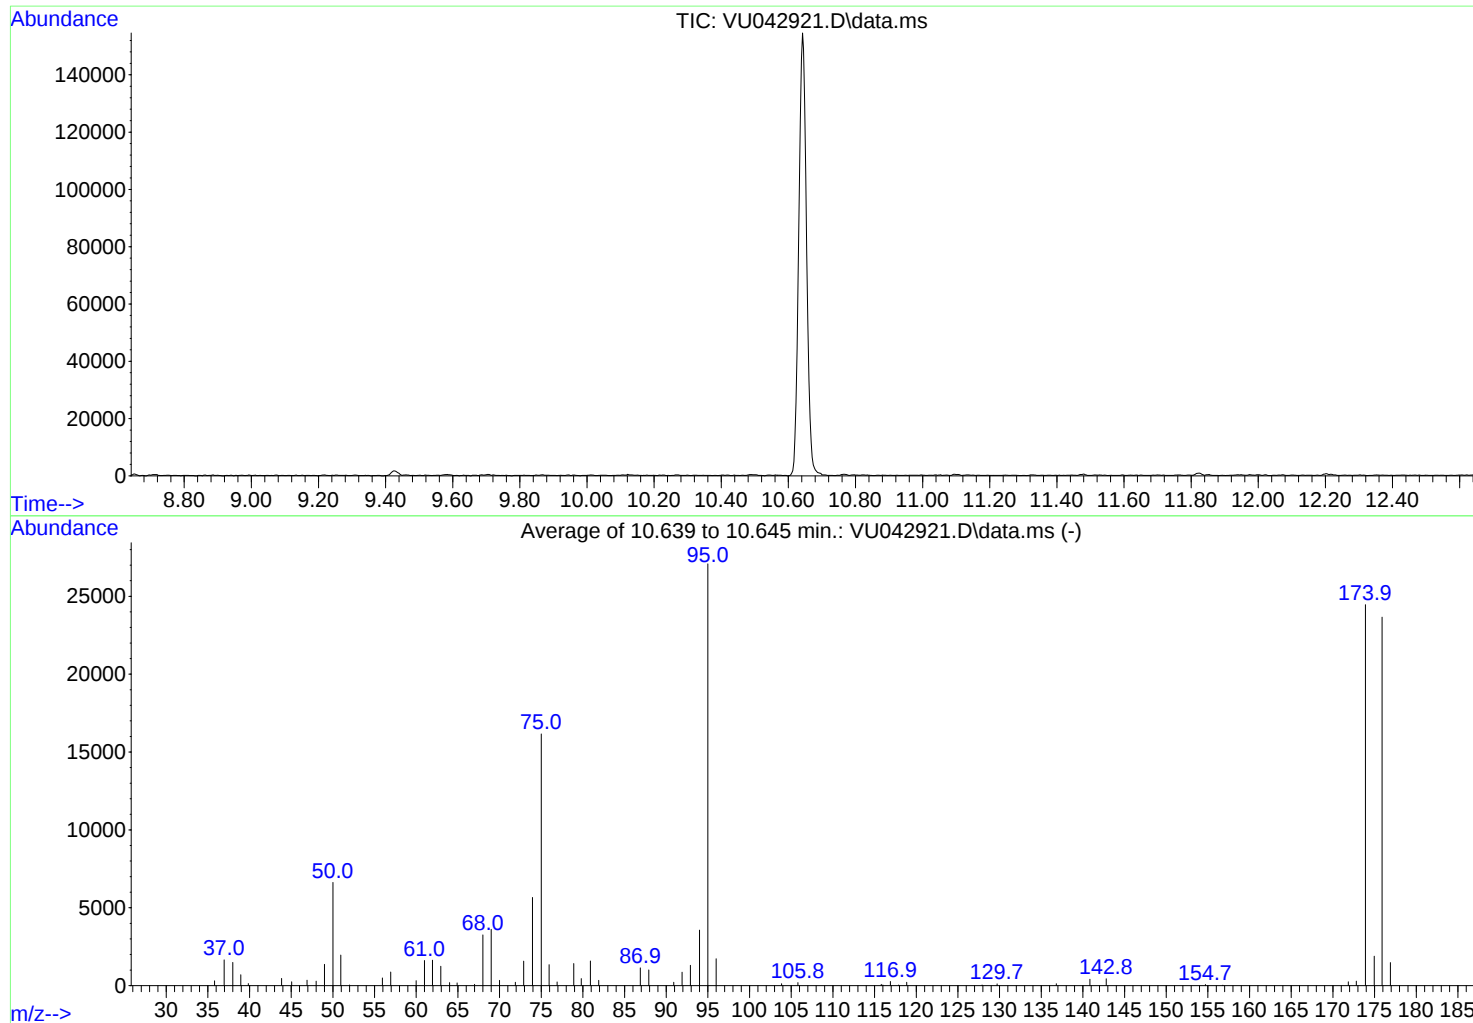

AutoFind: Scans 2892, 2893, 2894; Background Corrected with Scan 2880

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	24.5	6626	PASS
75	95	30	60	59.7	16163	PASS
95	95	100	100	100.0	27083	PASS
96	95	5	9	6.4	1727	PASS
173	174	0.00	2	1.2	292	PASS
174	95	50	100	90.3	24459	PASS
175	174	5	9	7.7	1887	PASS
176	174	95	101	96.7	23661	PASS
177	176	5	9	6.3	1479	PASS