

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040522\
 Data File : VU047819.D
 Acq On : 05 Apr 2022 12:28
 Operator : SY/MD
 Sample : N2179-01ME
 Misc : 5.72g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0R21ME

Quant Time: Apr 06 03:35:55 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Apr 06 03:35:05 2022
 Response via : Initial Calibration

Manual Integrations APPROVED

Reviewed By : John Carlone 04/06/2022
 Supervised By : Mahesh Dadoda 04/06/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.250	114	363940	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.423	117	379703	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.819	152	215088	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	124886	47.320	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	94.640%		
7) Chloroethane-d5	1.896	69	82074	39.440	ug/L	-0.02
Spiked Amount 50.000	Range 70 - 130		Recovery =	78.880%		
11) 1,1-Dichloroethene-d2	2.549	63	169583	35.121	ug/L	-0.02
Spiked Amount 50.000	Range 60 - 125		Recovery =	70.240%		
21) 2-Butanone-d5	4.639	46	190230	83.977	ug/L	0.01
Spiked Amount 100.000	Range 40 - 130		Recovery =	83.980%		
24) Chloroform-d	5.063	84	224557	46.502	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	93.000%		
26) 1,2-Dichloroethane-d4	5.703	65	145341	49.073	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	98.140%		
32) Benzene-d6	5.726	84	474509	49.664	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	99.320%		
36) 1,2-Dichloropropane-d6	6.694	67	146194	49.824	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	99.640%		
41) Toluene-d8	7.899	98	434132	46.637	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	93.280%		
43) trans-1,3-Dichloroprop...	8.185	79	64719	43.537	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	87.080%		
47) 2-Hexanone-d5	8.661	63	153709	89.485	ug/L	0.03
Spiked Amount 100.000	Range 45 - 130		Recovery =	89.490%		
56) 1,1,2,2-Tetrachloroeth...	10.767	84	234222	46.513	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	93.020%		
66) 1,2-Dichlorobenzene-d4	12.198	152	194963	50.949	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	101.900%		
Target Compounds					Qvalue	
13) Acetone	2.649	43	4763m	2.259	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040522\
Data File : VU047819.D
Acq On : 05 Apr 2022 12:28
Operator : SY/MD
Sample : N2179-01ME
Misc : 5.72g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 5 Sample Multiplier: 1


Instrument :
MSVOA_U
ClientSampleId :
C0R21ME

Quant Time: Apr 06 03:35:55 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Apr 06 03:35:05 2022
Response via : Initial Calibration

Manual Integrations
APPROVED

Reviewed By : John Carlone 04/06/2022
Supervised By : Mahesh Dadoda 04/06/2022

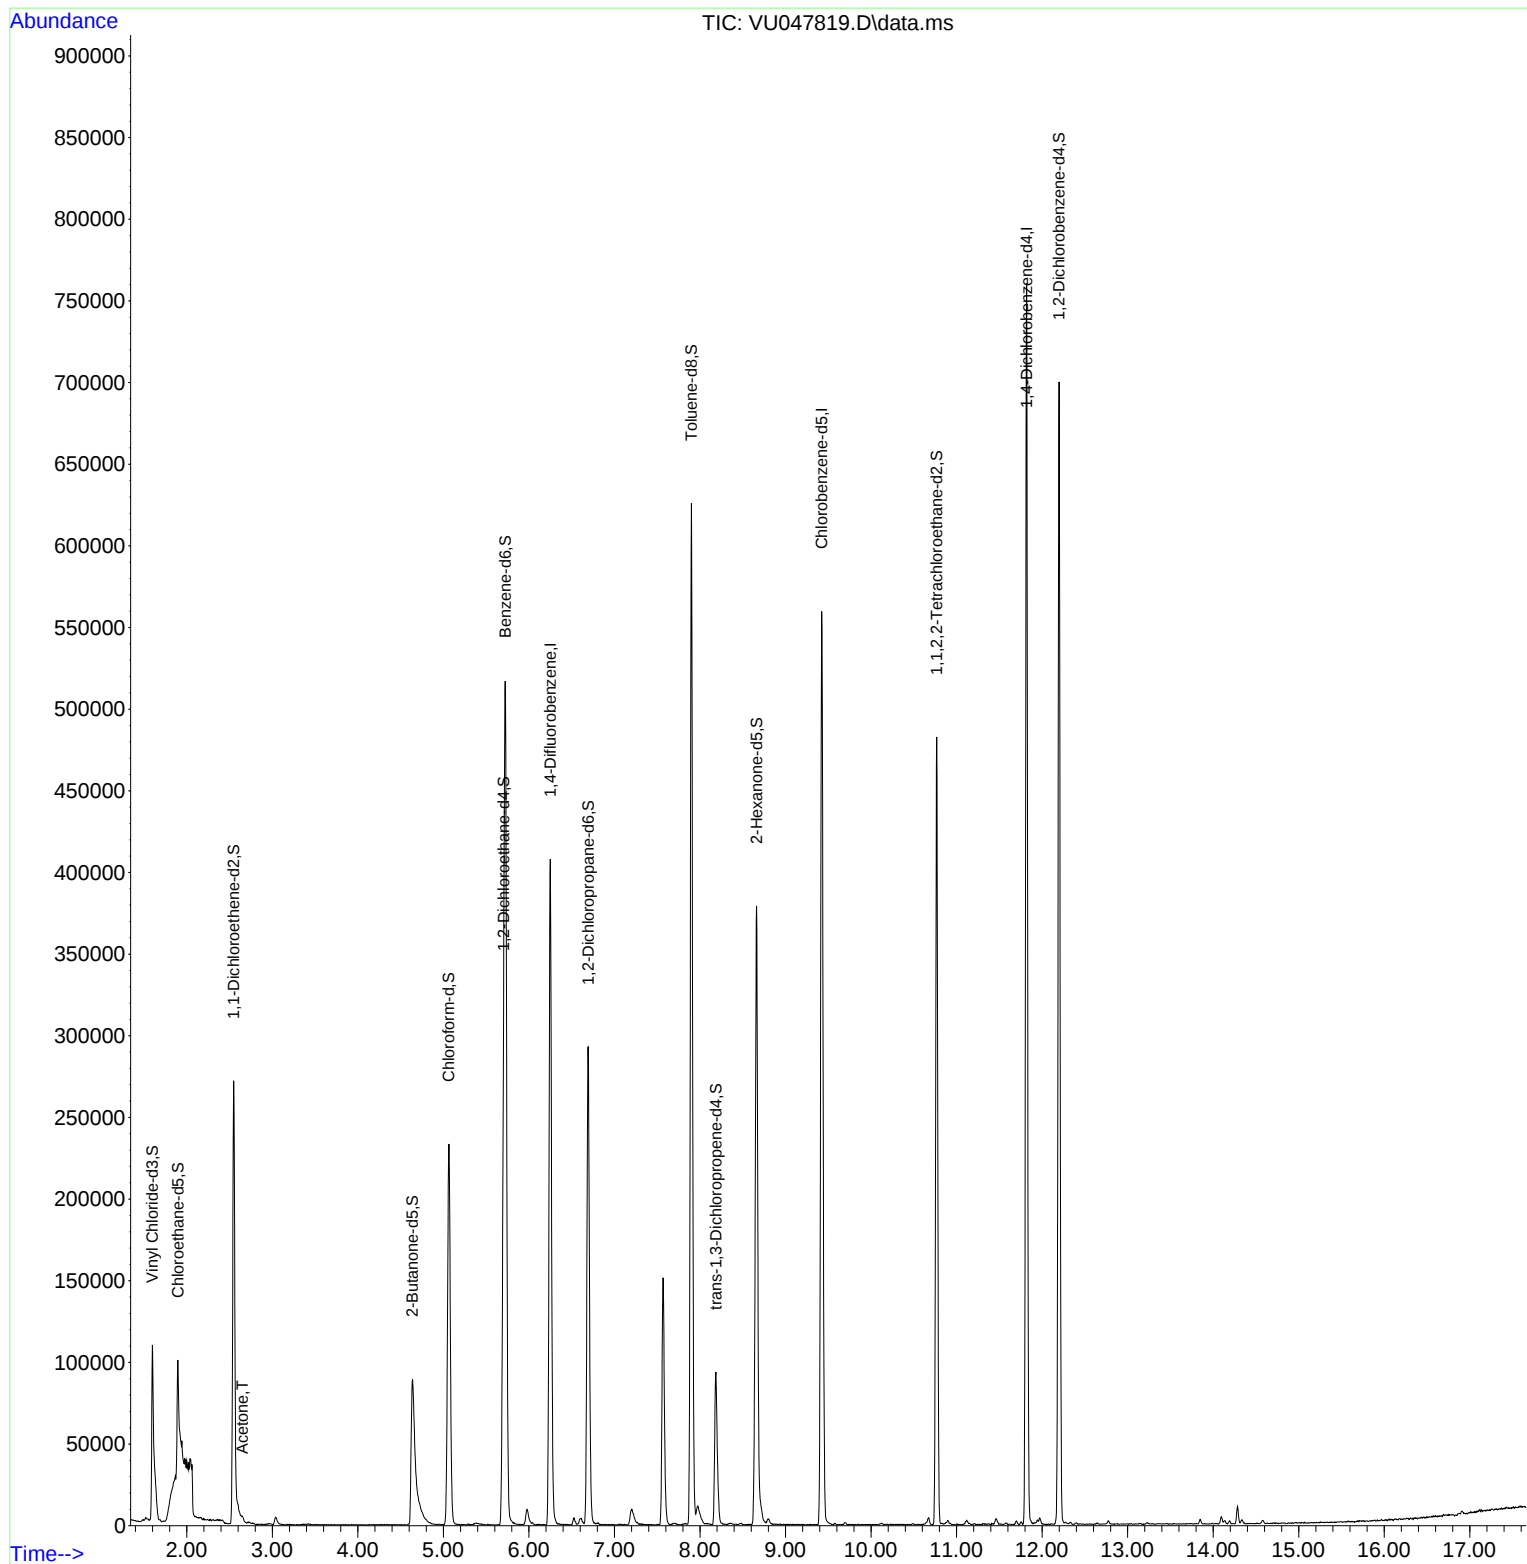

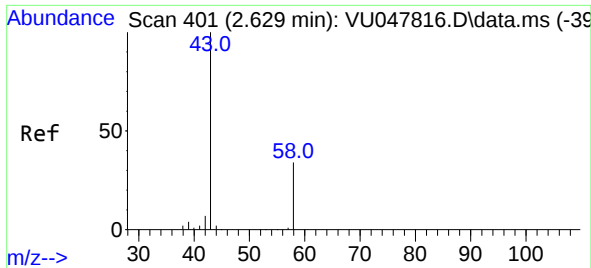

#13
Acetone
Concen: 2.259 ug/L m
RT: 2.649 min Scan# 407
Delta R.T. 0.019 min
Lab File: VU047819.D
Acq: 05 Apr 2022 12:28

Instrument :
MSVOA_U
ClientSampleId :
C0R21ME

Tgt Ion: 43 Resp: 476
Ion Ratio Lower Upper
43 100
58 0.0 0.0 70.0

Manual Integrations
APPROVED

Reviewed By :John Carlone 04/06/2022
Supervised By :Mahesh Dadoda 04/06/2022

