


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040522\
Data File : VU047815.D
Acq On : 05 Apr 2022 09:04
Operator : SY/MD
Sample : BFB059
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB059

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Title : VOC Analysis
Last Update : Wed Apr 06 03:35:05 2022

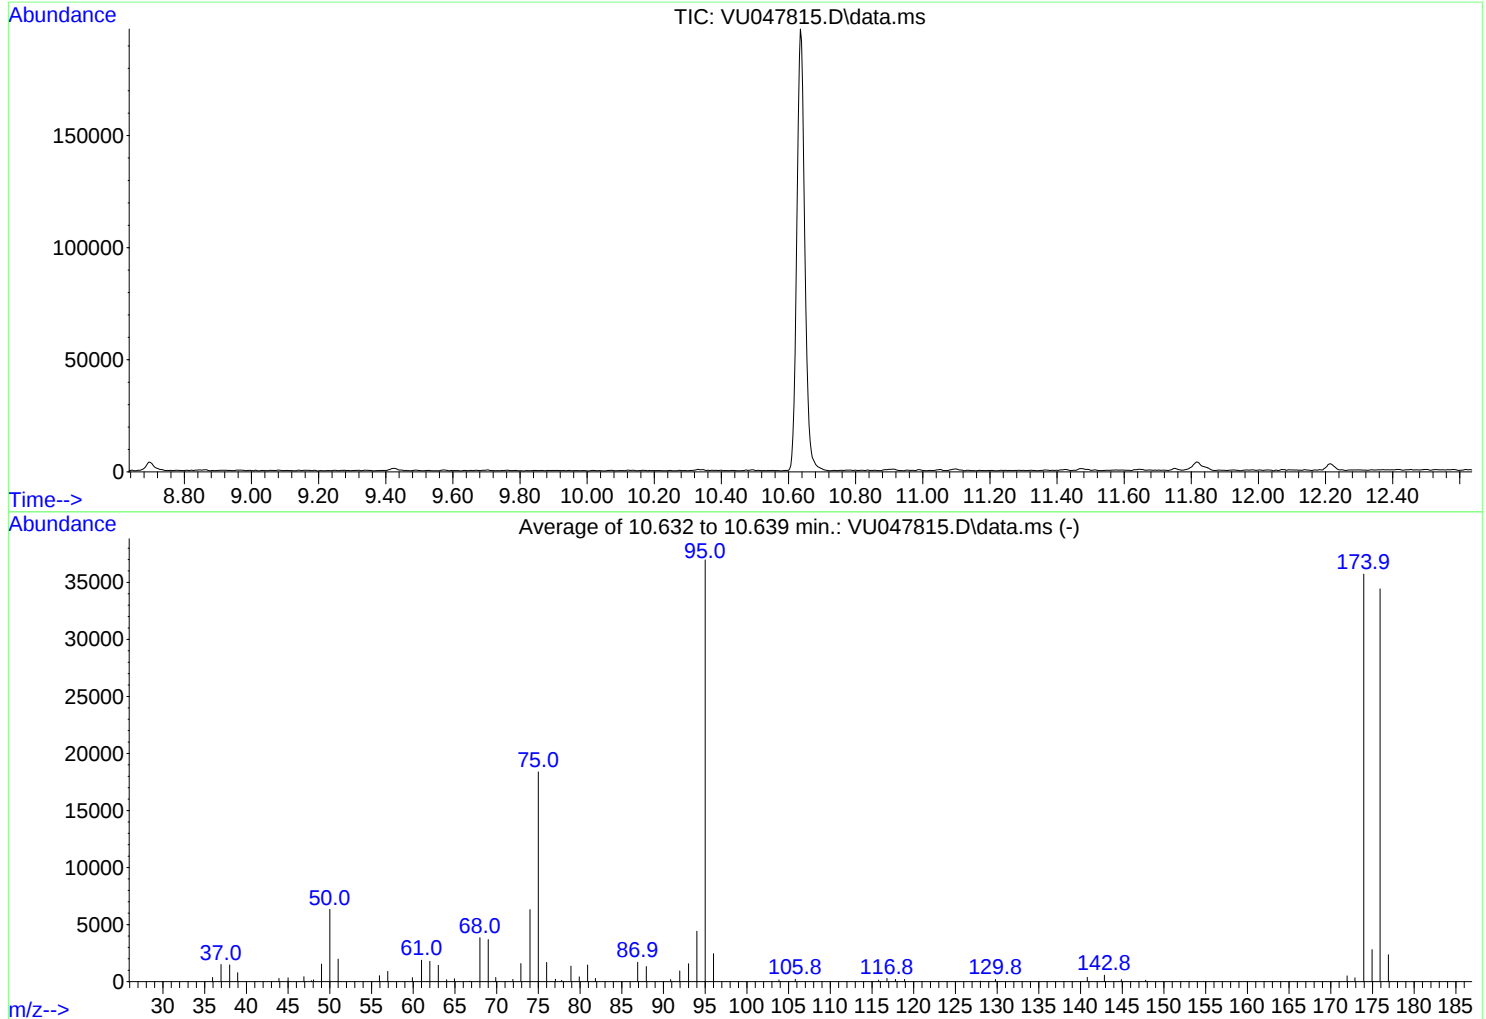

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2878

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.1	6337	PASS
75	95	30	80	49.7	18392	PASS
95	95	100	100	100.0	36973	PASS
96	95	5	9	6.6	2452	PASS
173	174	0.00	2	1.0	341	PASS
174	95	50	120	96.6	35720	PASS
175	174	5	9	7.9	2811	PASS
176	174	95	101	96.4	34435	PASS
177	176	5	9	6.8	2354	PASS

m/z	Abundance
35.90	338.0
37.00	1555.0
38.00	1458.0
38.90	758.0
40.00	154.0
43.90	700.0
44.90	240.0
46.90	434.0
48.10	244.0
49.00	1554.0
50.00	6155.0
51.00	1935.0
56.00	567.0
57.00	903.0
59.90	342.0
61.00	1814.0
62.00	1766.0
63.00	1370.0
64.00	208.0
65.00	265.0
68.00	3896.0
69.00	3639.0
69.90	347.0
71.90	165.0
72.90	1638.0
74.00	6306.0
75.00	18432.0
76.00	1512.0
77.10	197.0
77.80	121.0
78.90	1349.0
79.90	414.0
80.90	1419.0
81.80	289.0
86.90	1717.0
87.90	1316.0
90.80	186.0
91.90	839.0
93.00	1499.0
94.00	4508.0
95.00	37336.0
96.00	2291.0
103.80	134.0
105.80	224.0
115.80	156.0
116.80	298.0
117.80	208.0
118.90	190.0
128.00	120.0
129.80	212.0
140.80	360.0
142.80	521.0
144.90	151.0
172.00	518.0
173.00	434.0
174.00	36688.0
174.90	2851.0
175.90	34704.0
176.90	2294.0

Instrument :
MSVOA_U
ClientSampleId :
BFB059

m/z	Abundance
39.80	192.0
43.90	466.0

Instrument :
MSVOA_U
ClientSampleId :
BFB059

m/z	Abundance
36.00	381.0
36.90	1431.0
38.00	1438.0
39.00	774.0
40.00	118.0
43.90	772.0
45.00	412.0
46.90	412.0
47.80	238.0
49.00	1481.0
50.00	6339.0
51.00	1958.0
55.90	475.0
56.90	867.0
59.90	375.0
61.00	1862.0
62.00	1744.0
63.00	1433.0
64.00	151.0
64.90	247.0
66.80	120.0
68.00	3666.0
69.00	3603.0
69.90	337.0
72.00	212.0
72.90	1459.0
74.00	6108.0
75.00	17696.0
76.00	1812.0
77.00	204.0
77.80	112.0
78.90	1322.0
79.90	413.0
80.90	1435.0
81.90	254.0
86.90	1679.0
88.00	1288.0
90.90	184.0
92.00	1040.0
93.00	1573.0
94.00	4252.0
95.00	35456.0
96.00	2529.0
103.90	163.0
105.80	184.0
115.80	120.0
116.80	258.0
117.80	180.0
118.90	193.0
129.80	175.0
140.80	386.0
142.90	581.0
144.90	220.0
147.80	197.0
172.00	472.0
172.80	265.0
173.90	33632.0
175.00	2657.0
175.90	33032.0
176.90	2333.0

Instrument :
MSVOA_U
ClientSampleId :
BFB059

m/z	Abundance
35.90	367.0
36.90	1507.0
38.00	1532.0
39.00	817.0
40.00	132.0
43.90	747.0
45.00	345.0
46.90	480.0
48.00	225.0
49.00	1591.0
50.00	6518.0
51.00	2027.0
55.90	529.0
57.00	918.0
59.90	359.0
61.00	1960.0
62.00	1844.0
63.00	1478.0
64.00	166.0
65.00	264.0
68.00	4007.0
69.00	3814.0
69.90	396.0
72.00	201.0
72.90	1649.0
74.00	6530.0
75.00	19048.0
76.00	1737.0
77.00	227.0
77.80	120.0
78.90	1390.0
79.90	428.0
80.90	1514.0
81.80	293.0
86.90	1720.0
87.90	1351.0
90.80	196.0
92.00	927.0
93.00	1631.0
94.00	4509.0
95.00	38128.0
96.00	2536.0
103.90	150.0
105.80	211.0
115.80	144.0
116.80	280.0
117.80	204.0
118.90	207.0
129.80	208.0
140.80	387.0
142.80	588.0
144.90	188.0
147.80	169.0
171.90	525.0
172.90	325.0
173.90	36840.0
174.90	2926.0
175.90	35568.0
176.90	2435.0

Instrument :
MSVOA_U
ClientSampleId :
BFB059