

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040523\
 Data File : VU053578.D
 Acq On : 05 Apr 2023 11:02
 Operator : JC/MD
 Sample : VU0405MBL01
 Misc : 5.0g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK069

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

Signal : TIC: VU053578.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	93	rBV	94614	108178	13.61%	1.635%
2	1.909	170	177	194	rVB	82335	112731	14.18%	1.703%
3	2.565	369	381	400	rBV	153445	247224	31.11%	3.736%
4	3.044	524	530	539	rVB4	2262	3382	0.43%	0.051%
5	3.256	593	596	598	rBV	370	179	0.02%	0.003%
6	3.350	620	625	630	rBV3	728	1050	0.13%	0.016%
7	3.398	637	640	642	rBV2	337	234	0.03%	0.004%
8	3.433	648	651	654	rBV	334	226	0.03%	0.003%
9	4.488	976	979	985	rBV	268	215	0.03%	0.003%
10	4.559	999	1001	1004	rBV	202	82	0.01%	0.001%
11	4.613	1006	1018	1047	rBV	75449	186897	23.52%	2.824%
12	5.057	1141	1156	1180	rBV	153637	334439	42.08%	5.054%
13	5.285	1224	1227	1232	rBV2	473	431	0.05%	0.007%
14	5.327	1238	1240	1241	rBV2	157	88	0.01%	0.001%
15	5.491	1287	1291	1292	rBV	211	137	0.02%	0.002%
16	5.530	1300	1303	1306	rVB	356	217	0.03%	0.003%
17	5.584	1318	1320	1324	rBV	273	226	0.03%	0.003%
18	5.645	1337	1339	1341	rBV2	173	91	0.01%	0.001%
19	5.719	1341	1362	1387	rBV2	286189	794781	100.00%	12.010%
20	5.935	1425	1429	1435	rBV3	331	419	0.05%	0.006%
21	5.980	1442	1443	1446	rBV	216	100	0.01%	0.002%
22	6.034	1458	1460	1461	rBV	286	77	0.01%	0.001%
23	6.243	1512	1525	1547	rBV	292675	556244	69.99%	8.405%
24	6.494	1601	1603	1605	rBV	243	116	0.01%	0.002%
25	6.530	1605	1614	1626	rVB7	4695	9157	1.15%	0.138%
26	6.687	1649	1663	1684	rBV	184653	363032	45.68%	5.486%
27	7.182	1812	1817	1820	rBV2	659	631	0.08%	0.010%
28	7.263	1839	1842	1843	rBV2	151	67	0.01%	0.001%
29	7.279	1845	1847	1852	rVB	235	105	0.01%	0.002%
30	7.520	1918	1922	1923	rBV	208	162	0.02%	0.002%
31	7.562	1923	1935	1950	rBV2	106230	186805	23.50%	2.823%
32	7.748	1990	1993	1996	rBV2	276	209	0.03%	0.003%
33	7.893	2024	2038	2060	rBV	359850	628911	79.13%	9.503%
34	8.121	2106	2109	2113	rVB2	240	148	0.02%	0.002%
35	8.176	2113	2126	2147	rBV2	74289	129018	16.23%	1.950%
36	8.314	2166	2169	2170	rBV	203	109	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040523\
 Data File : VU053578.D
 Acq On : 05 Apr 2023 11:02
 Operator : JC/MD
 Sample : VU0405MBL01
 Misc : 5.0g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK069

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

37	8.343	2176	2178	2180	rVB	169	47	0.01%	0.001%
38	8.378	2187	2189	2194	rBV	225	142	0.02%	0.002%
39	8.475	2214	2219	2222	rVB	365	284	0.04%	0.004%
40	8.501	2222	2227	2228	rBV	276	223	0.03%	0.003%
41	8.529	2233	2236	2237	rBV	220	137	0.02%	0.002%
42	8.552	2237	2243	2250	rVB4	1555	2185	0.27%	0.033%
43	8.626	2255	2266	2295	rBV	223879	417729	52.56%	6.312%
44	8.906	2348	2353	2354	rBV	268	232	0.03%	0.004%
45	8.954	2366	2368	2371	rBV2	271	167	0.02%	0.003%
46	9.031	2389	2392	2394	rBV	220	135	0.02%	0.002%
47	9.192	2440	2442	2446	rVB	397	140	0.02%	0.002%
48	9.272	2465	2467	2472	rVB	253	144	0.02%	0.002%
49	9.414	2497	2511	2534	rBV	400414	672200	84.58%	10.158%
50	9.642	2577	2582	2583	rBV	335	272	0.03%	0.004%
51	9.735	2610	2611	2614	rVB	269	68	0.01%	0.001%
52	10.041	2703	2706	2712	rVB	254	188	0.02%	0.003%
53	10.070	2713	2715	2718	rBV	212	88	0.01%	0.001%
54	10.240	2764	2768	2771	rBV2	317	277	0.03%	0.004%
55	10.484	2837	2844	2852	rBV2	994	1448	0.18%	0.022%
56	10.539	2859	2861	2865	rBV	240	140	0.02%	0.002%
57	10.632	2887	2890	2897	rBV3	763	848	0.11%	0.013%
58	10.751	2914	2927	2947	rBV	295555	470820	59.24%	7.115%
59	10.857	2958	2960	2966	rBV2	341	222	0.03%	0.003%
60	10.886	2966	2969	2970	rBV2	296	142	0.02%	0.002%
61	10.931	2980	2983	2986	rBV	251	142	0.02%	0.002%
62	11.240	3077	3079	3080	rBV	153	48	0.01%	0.001%
63	11.272	3086	3089	3091	rBV	239	126	0.02%	0.002%
64	11.404	3129	3130	3131	rBV	236	53	0.01%	0.001%
65	11.471	3143	3151	3158	rBV2	903	1219	0.15%	0.018%
66	11.751	3228	3238	3243	rBV5	2705	3879	0.49%	0.059%
67	11.809	3243	3256	3274	rBV	429102	689807	86.79%	10.424%
68	11.928	3290	3293	3296	rBV5	478	425	0.05%	0.006%
69	12.188	3361	3374	3392	rBV	395506	651254	81.94%	9.841%
70	12.536	3480	3482	3486	rBV	152	96	0.01%	0.001%
71	13.227	3689	3697	3704	rBV5	1892	2660	0.33%	0.040%
72	13.841	3879	3888	3900	rVB5	8481	13654	1.72%	0.206%
73	13.954	3920	3923	3926	rBV	526	436	0.05%	0.007%
74	14.092	3958	3966	3977	rBV3	7248	11310	1.42%	0.171%
75	14.330	4032	4040	4051	rBV3	4736	8215	1.03%	0.124%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040523\
Data File : VU053578.D
Acq On : 05 Apr 2023 11:02
Operator : JC/MD
Sample : VU0405MBL01
Misc : 5.0g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK069

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M

Title : VOC Analysis




Sum of corrected areas: 6617720

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040523\
Data File : VU053578.D
Acq On : 05 Apr 2023 11:02
Operator : JC/MD
Sample : VU0405MBL01
Misc : 5.0g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK069

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

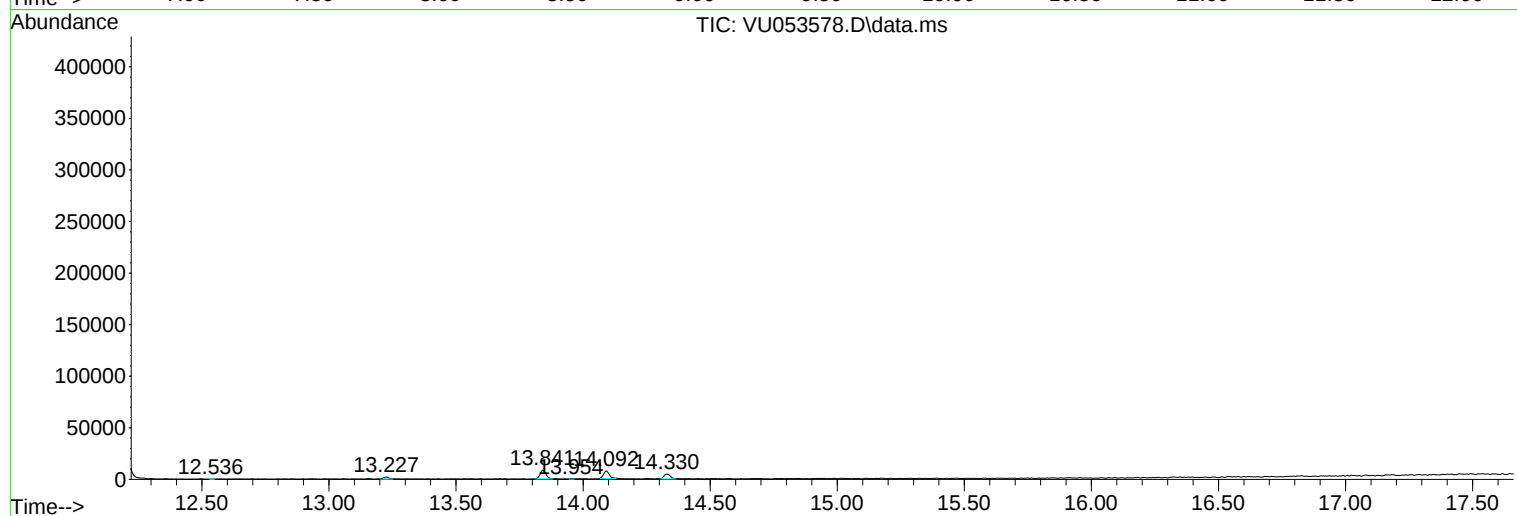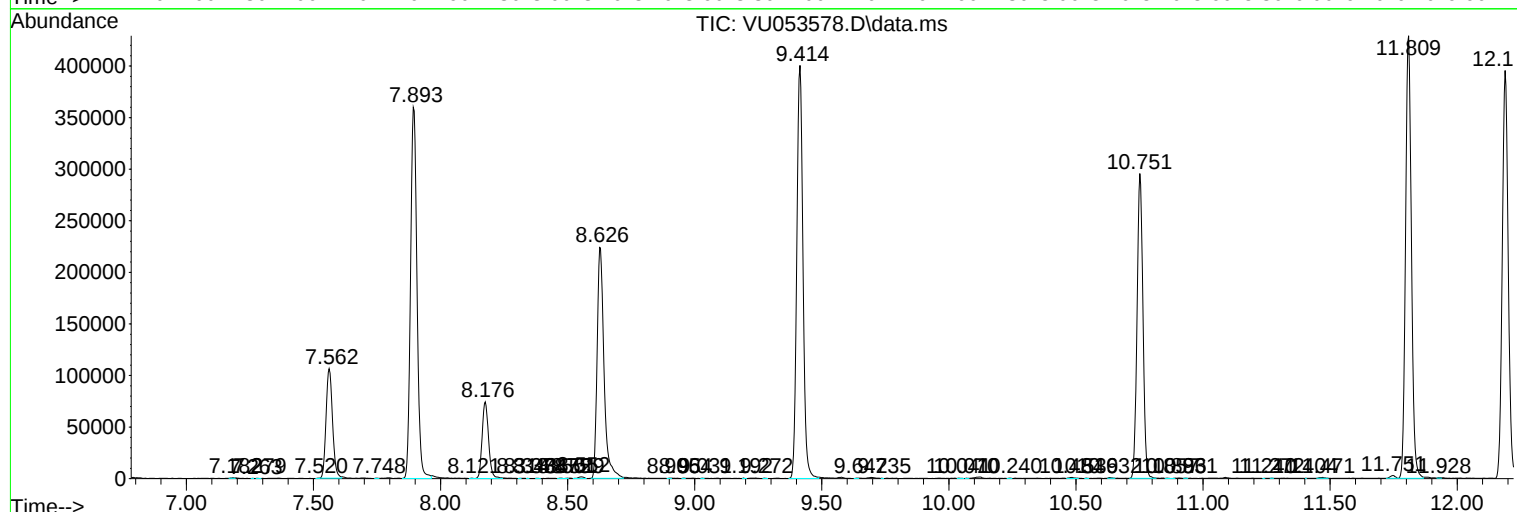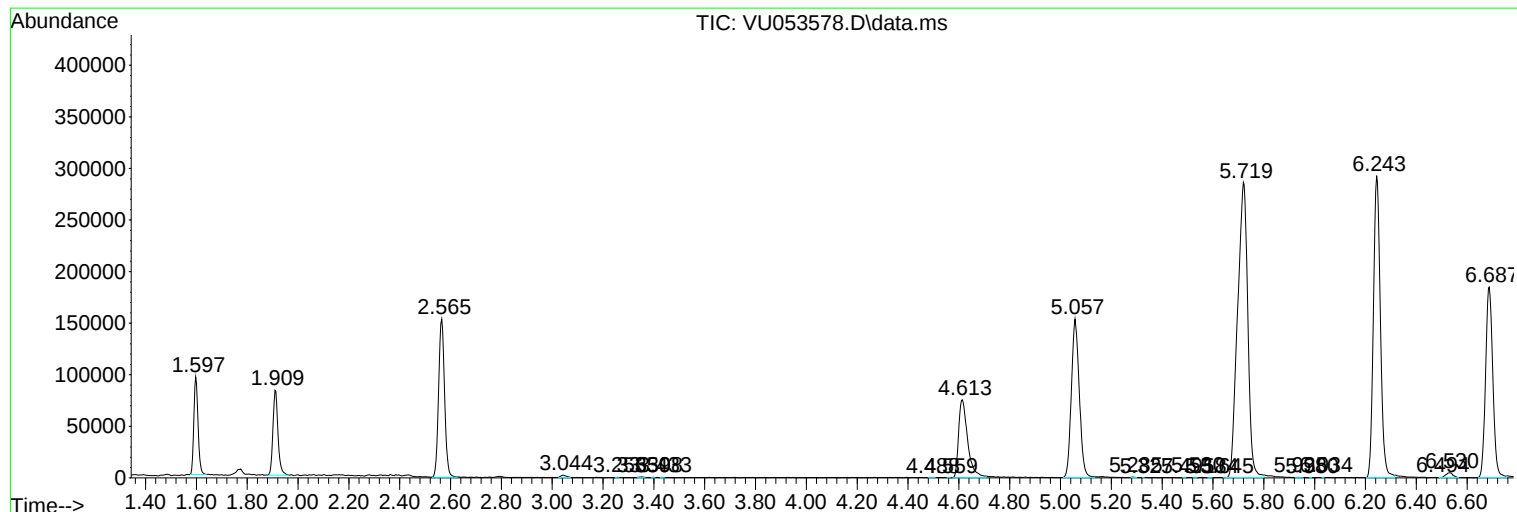

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040523\
Data File : VU053578.D
Acq On : 05 Apr 2023 11:02
Operator : JC/MD
Sample : VU0405MBL01
Misc : 5.0g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK069

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040523\
Data File : VU053578.D
Acq On : 05 Apr 2023 11:02
Operator : JC/MD
Sample : VU0405MBL01
Misc : 5.0g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK069

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc