

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040523\
 Data File : VU053580.D
 Acq On : 05 Apr 2023 13:10
 Operator : JC/MD
 Sample : 02158-06DL 200X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 PMW-5(20230329)DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

Signal : TIC: VU053580.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	94	rVB	93182	106134	10.10%	1.118%
2	1.909	169	177	193	rBV	79184	107478	10.23%	1.132%
3	2.565	369	381	396	rBV	149171	242950	23.12%	2.559%
4	2.761	440	442	443	rBV	269	107	0.01%	0.001%
5	3.047	522	531	538	rBV2	1633	2801	0.27%	0.030%
6	3.170	568	569	570	rBV2	320	73	0.01%	0.001%
7	3.272	598	601	603	rBV	207	110	0.01%	0.001%
8	3.337	620	621	622	rBV	165	39	0.00%	0.000%
9	3.346	622	624	627	rBV2	377	226	0.02%	0.002%
10	3.485	664	667	668	rBV	215	99	0.01%	0.001%
11	3.613	705	707	712	rVB	246	151	0.01%	0.002%
12	3.793	761	763	764	rBV	220	91	0.01%	0.001%
13	3.919	798	802	805	rBV	324	251	0.02%	0.003%
14	4.060	843	846	848	rBV	157	113	0.01%	0.001%
15	4.086	852	854	857	rBV	162	83	0.01%	0.001%
16	4.260	905	908	910	rBV2	280	174	0.02%	0.002%
17	4.613	1007	1018	1024	rBV	70752	140230	13.35%	1.477%
18	4.909	1107	1110	1113	rBV	323	217	0.02%	0.002%
19	4.935	1116	1118	1123	rBV	232	194	0.02%	0.002%
20	4.983	1132	1133	1136	rBV	130	66	0.01%	0.001%
21	5.060	1140	1157	1178	rBV	151969	331211	31.52%	3.489%
22	5.279	1223	1225	1226	rBV	336	166	0.02%	0.002%
23	5.382	1254	1257	1260	rBV2	258	190	0.02%	0.002%
24	5.514	1296	1298	1300	rBV	173	60	0.01%	0.001%
25	5.719	1341	1362	1392	rBV2	287428	793936	75.57%	8.364%
26	6.157	1496	1498	1503	rBV	186	134	0.01%	0.001%
27	6.247	1512	1526	1549	rBV	306746	584680	55.65%	6.159%
28	6.539	1604	1617	1632	rVB4	37903	75816	7.22%	0.799%
29	6.594	1632	1634	1637	rBV	233	127	0.01%	0.001%
30	6.687	1650	1663	1680	rBV2	185064	363820	34.63%	3.833%
31	6.854	1713	1715	1719	rVB2	325	160	0.02%	0.002%
32	6.928	1736	1738	1740	rVB	160	58	0.01%	0.001%
33	7.118	1794	1797	1798	rBV	196	122	0.01%	0.001%
34	7.124	1798	1799	1800	rVV	166	48	0.00%	0.001%
35	7.163	1810	1811	1812	rBV	127	34	0.00%	0.000%
36	7.182	1812	1817	1820	rBV2	558	482	0.05%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040523\
 Data File : VU053580.D
 Acq On : 05 Apr 2023 13:10
 Operator : JC/MD
 Sample : 02158-06DL 200X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 PMW-5(20230329)DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

37	7.372	1873	1876	1879	rBV	176	85	0.01%	0.001%
38	7.401	1882	1885	1888	rVB	207	99	0.01%	0.001%
39	7.562	1922	1935	1949	rBV	104614	184407	17.55%	1.943%
40	7.761	1995	1997	2000	rVB	200	89	0.01%	0.001%
41	7.812	2009	2013	2014	rBV	196	156	0.01%	0.002%
42	7.896	2025	2039	2050	rBV	365223	626439	59.62%	6.599%
43	7.967	2051	2061	2080	rVB	346391	603555	57.45%	6.358%
44	8.176	2115	2126	2142	rBV	73057	126759	12.06%	1.335%
45	8.449	2209	2211	2213	rBV2	240	133	0.01%	0.001%
46	8.552	2230	2243	2256	rBV	218484	370117	35.23%	3.899%
47	8.629	2257	2267	2299	rVB	207327	381989	36.36%	4.024%
48	8.787	2313	2316	2319	rVB	185	85	0.01%	0.001%
49	8.809	2320	2323	2327	rVV3	354	248	0.02%	0.003%
50	8.931	2358	2361	2363	rBV	140	85	0.01%	0.001%
51	9.012	2385	2386	2387	rBV	126	36	0.00%	0.000%
52	9.150	2427	2429	2432	rVB	344	207	0.02%	0.002%
53	9.414	2498	2511	2538	rBV	427416	737490	70.19%	7.769%
54	9.568	2551	2559	2575	rVB	16333	27157	2.58%	0.286%
55	9.690	2586	2597	2611	rBV	58688	96997	9.23%	1.022%
56	9.800	2629	2631	2635	rBV	262	173	0.02%	0.002%
57	9.845	2643	2645	2653	rVB	229	193	0.02%	0.002%
58	10.099	2713	2724	2740	rBV2	20581	34261	3.26%	0.361%
59	10.295	2782	2785	2790	rBV	283	174	0.02%	0.002%
60	10.378	2810	2811	2813	rBV	213	73	0.01%	0.001%
61	10.407	2818	2820	2821	rBV	169	50	0.00%	0.001%
62	10.484	2838	2844	2852	rVB2	2455	3065	0.29%	0.032%
63	10.639	2890	2892	2897	rVB2	560	405	0.04%	0.004%
64	10.681	2903	2905	2910	rBV	259	187	0.02%	0.002%
65	10.751	2915	2927	2945	rVV	282933	449843	42.82%	4.739%
66	10.902	2966	2974	2985	rVB	2646	4039	0.38%	0.043%
67	10.947	2986	2988	2991	rVV2	216	141	0.01%	0.001%
68	10.999	2995	3004	3021	rVV2	7741	15466	1.47%	0.163%
69	11.086	3025	3031	3041	rVB4	4063	5828	0.55%	0.061%
70	11.224	3071	3074	3075	rBV	331	182	0.02%	0.002%
71	11.291	3088	3095	3106	rVB2	3580	5034	0.48%	0.053%
72	11.356	3112	3115	3118	rBV2	284	205	0.02%	0.002%
73	11.468	3141	3150	3162	rVB2	11729	16473	1.57%	0.174%
74	11.742	3226	3235	3244	rBV2	24163	37906	3.61%	0.399%
75	11.809	3245	3256	3276	rVV2	502508	975718	92.87%	10.279%
76	12.092	3337	3344	3351	rBV4	2614	3900	0.37%	0.041%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040523\
 Data File : VU053580.D
 Acq On : 05 Apr 2023 13:10
 Operator : JC/MD
 Sample : 02158-06DL 200X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 PMW-5(20230329)DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M

Title : VOC Analysis

77	12.189	3362	3374	3394	rBV	432812	754047	71.77%	7.943%
78	12.311	3409	3412	3413	rBV	398	194	0.02%	0.002%
79	12.465	3453	3460	3465	rBV2	990	1349	0.13%	0.014%
80	12.571	3486	3493	3503	rBV3	1699	2877	0.27%	0.030%
81	12.770	3553	3555	3559	rBV	267	180	0.02%	0.002%
82	12.912	3597	3599	3601	rBV2	373	105	0.01%	0.001%
83	12.967	3612	3616	3627	rBV2	902	1169	0.11%	0.012%
84	13.095	3654	3656	3659	rBV	409	245	0.02%	0.003%
85	13.838	3871	3887	3904	rBV	657474	1050646	100.00%	11.068%
86	14.089	3958	3965	3973	rVB2	6960	9582	0.91%	0.101%
87	14.327	4028	4039	4055	rBV	131089	210277	20.01%	2.215%




Sum of corrected areas: 9492751

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040523\
Data File : VU053580.D
Acq On : 05 Apr 2023 13:10
Operator : JC/MD
Sample : 02158-06DL 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PMW-5(20230329)DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

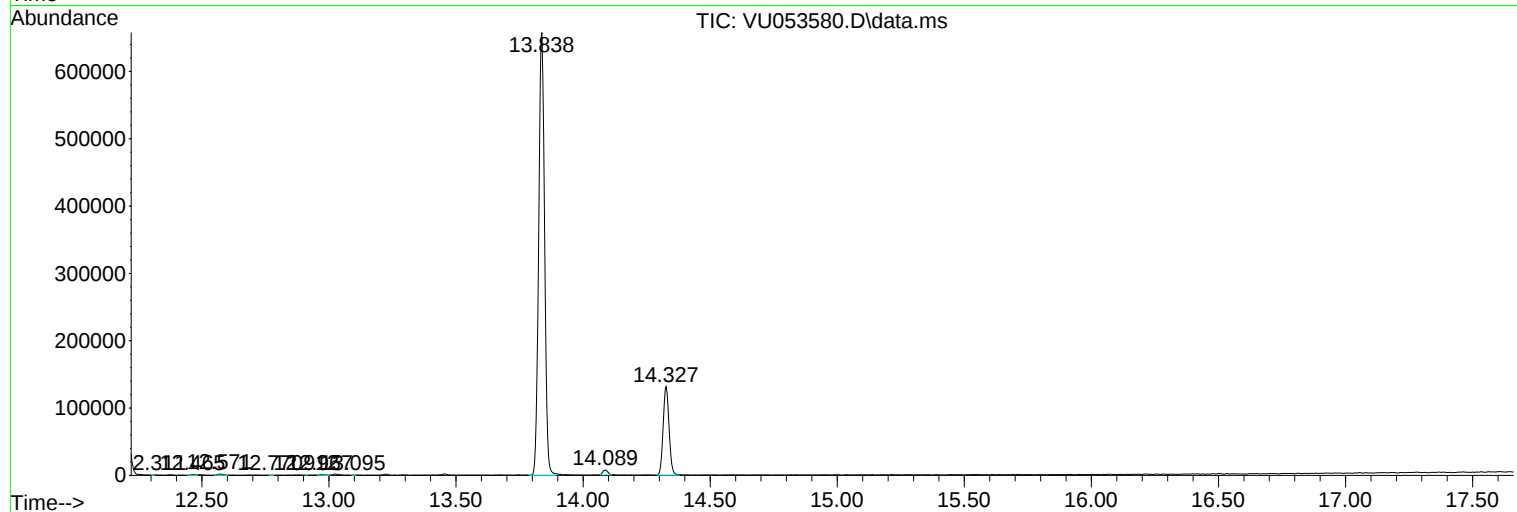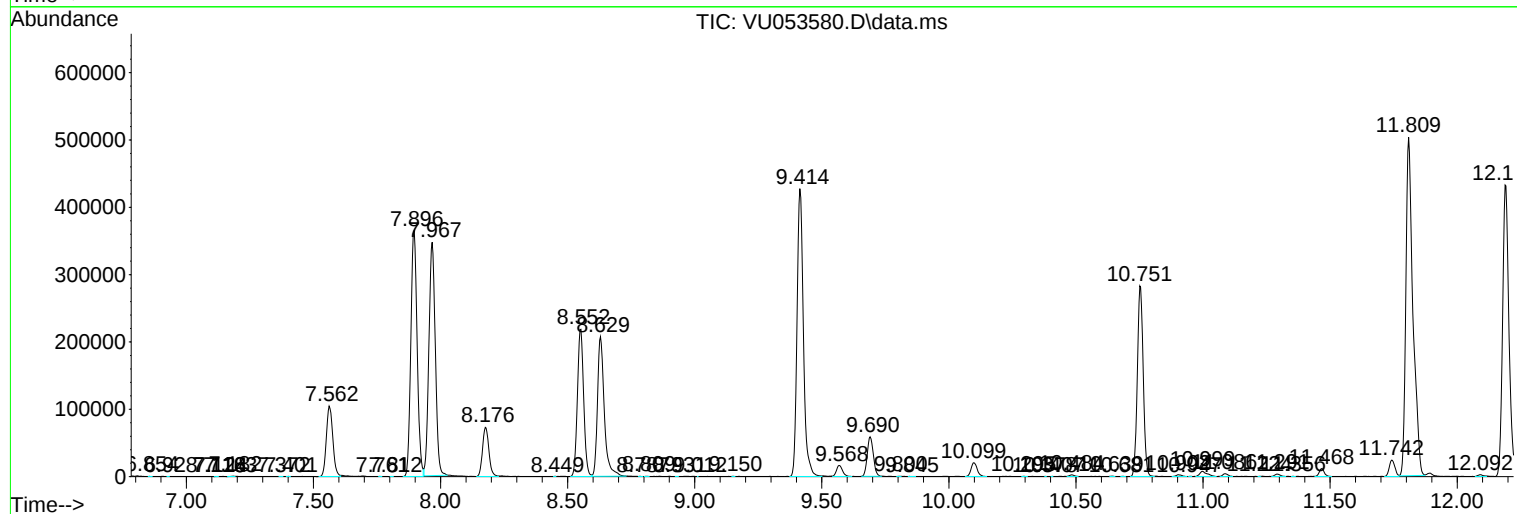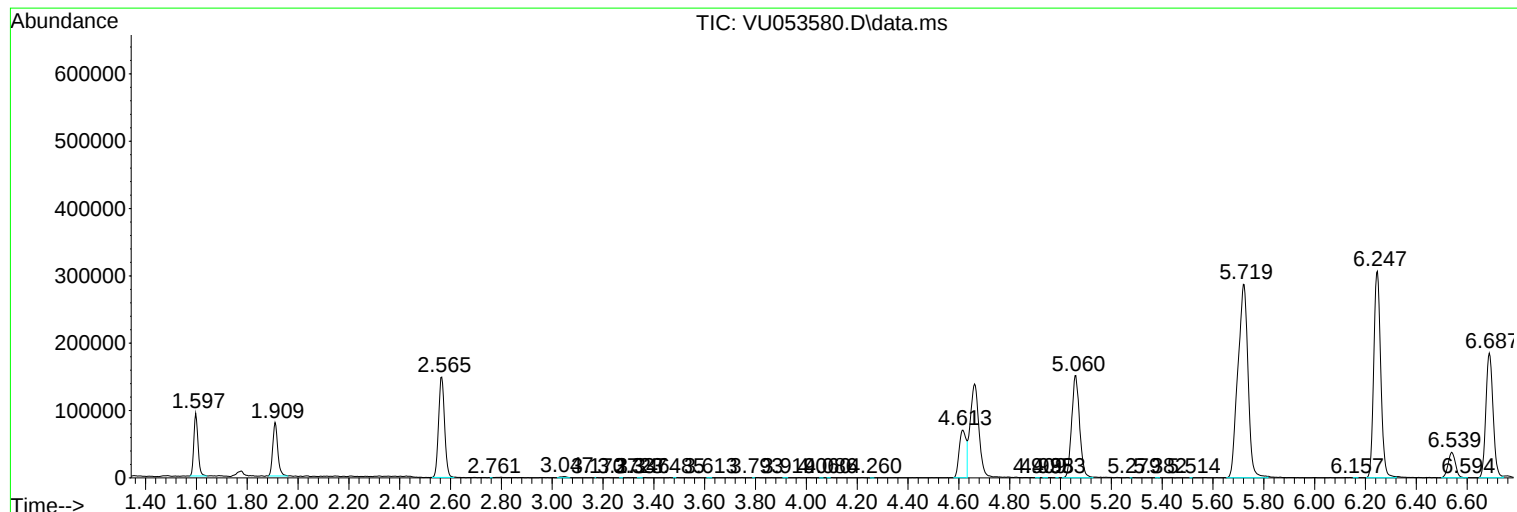

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040523\
Data File : VU053580.D
Acq On : 05 Apr 2023 13:10
Operator : JC/MD
Sample : 02158-06DL 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PMW-5(20230329)DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040523\
Data File : VU053580.D
Acq On : 05 Apr 2023 13:10
Operator : JC/MD
Sample : 02158-06DL 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PMW-5(20230329)DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------