

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040523\
 Data File : VU053581.D
 Acq On : 05 Apr 2023 13:37
 Operator : JC/MD
 Sample : 02158-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 PMW-6(20230329)

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

Signal : TIC: VU053581.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	74	80	94	rVB	90299	104708	2.92%	0.710%
2	1.909	170	177	194	rVB	82198	114920	3.20%	0.779%
3	2.565	369	381	395	rBV	148447	240681	6.71%	1.632%
4	2.751	434	439	443	rBV2	663	677	0.02%	0.005%
5	2.787	447	450	451	rBV2	338	241	0.01%	0.002%
6	2.909	487	488	492	rVB2	243	85	0.00%	0.001%
7	3.047	520	531	542	rBV4	2728	5716	0.16%	0.039%
8	3.166	564	568	570	rBV2	626	528	0.01%	0.004%
9	3.356	623	627	630	rBV2	306	239	0.01%	0.002%
10	3.472	661	663	665	rBV	200	101	0.00%	0.001%
11	3.626	708	711	717	rVB	300	180	0.01%	0.001%
12	3.771	754	756	757	rBV	275	77	0.00%	0.001%
13	3.941	806	809	812	rBV	231	177	0.00%	0.001%
14	4.452	967	968	969	rBV	164	54	0.00%	0.000%
15	4.520	987	989	991	rVB	196	93	0.00%	0.001%
16	4.536	991	994	997	rBV	171	136	0.00%	0.001%
17	4.613	1007	1018	1048	rBV	76948	190185	5.30%	1.289%
18	5.060	1140	1157	1175	rBV	167030	361623	10.08%	2.452%
19	5.275	1219	1224	1225	rBV2	307	293	0.01%	0.002%
20	5.391	1257	1260	1262	rBV2	257	160	0.00%	0.001%
21	5.446	1275	1277	1279	rBV	190	66	0.00%	0.000%
22	5.475	1284	1286	1289	rBV	181	68	0.00%	0.000%
23	5.494	1289	1292	1295	rVB2	199	143	0.00%	0.001%
24	5.626	1330	1333	1337	rBV	350	171	0.00%	0.001%
25	5.722	1341	1363	1398	rBV2	302084	878100	24.47%	5.953%
26	5.964	1435	1438	1442	rBV2	463	355	0.01%	0.002%
27	6.012	1449	1453	1455	rBV	291	224	0.01%	0.002%
28	6.192	1507	1509	1511	rBV	136	49	0.00%	0.000%
29	6.247	1511	1526	1546	rBV	324177	621218	17.31%	4.211%
30	6.529	1604	1614	1625	rVB6	6425	12130	0.34%	0.082%
31	6.687	1649	1663	1683	rBV	202130	391427	10.91%	2.654%
32	6.857	1713	1716	1719	rVB	243	120	0.00%	0.001%
33	6.941	1741	1742	1743	rBB	103	20	0.00%	0.000%
34	6.951	1743	1745	1746	rBV	188	100	0.00%	0.001%
35	7.012	1761	1764	1769	rBV2	308	294	0.01%	0.002%
36	7.153	1805	1808	1811	rBV2	223	168	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040523\
 Data File : VU053581.D
 Acq On : 05 Apr 2023 13:37
 Operator : JC/MD
 Sample : 02158-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 PMW-6(20230329)

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

37	7.192	1814	1820	1825	rBV3	702	894	0.02%	0.006%
38	7.269	1839	1844	1848	rVB2	254	226	0.01%	0.002%
39	7.314	1856	1858	1861	rBV	176	113	0.00%	0.001%
40	7.562	1923	1935	1958	rBV	115513	203225	5.66%	1.378%
41	7.690	1971	1975	1976	rBV2	731	575	0.02%	0.004%
42	7.758	1994	1996	1997	rBV2	203	90	0.00%	0.001%
43	7.796	2005	2008	2010	rBV	201	127	0.00%	0.001%
44	7.896	2026	2039	2056	rBV	381163	670640	18.69%	4.546%
45	8.092	2098	2100	2102	rBV	168	62	0.00%	0.000%
46	8.176	2113	2126	2141	rBV3	81631	137132	3.82%	0.930%
47	8.362	2182	2184	2187	rBV	196	76	0.00%	0.001%
48	8.468	2212	2217	2222	rBV	802	706	0.02%	0.005%
49	8.552	2236	2243	2251	rBV3	2956	4728	0.13%	0.032%
50	8.629	2255	2267	2297	rBV	231114	422654	11.78%	2.865%
51	8.893	2347	2349	2354	rBV	226	131	0.00%	0.001%
52	9.005	2381	2384	2391	rBV2	238	221	0.01%	0.001%
53	9.443	2498	2520	2554	rBV2	1722417	3589145	100.00%	24.332%
54	9.690	2592	2597	2607	rVB6	1473	2491	0.07%	0.017%
55	9.761	2616	2619	2624	rVB	351	257	0.01%	0.002%
56	9.793	2627	2629	2631	rVB	249	71	0.00%	0.000%
57	9.918	2667	2668	2670	rBV	205	56	0.00%	0.000%
58	10.028	2700	2702	2706	rBV	143	53	0.00%	0.000%
59	10.070	2713	2715	2721	rVB	246	164	0.00%	0.001%
60	10.108	2721	2727	2733	rBV5	988	1229	0.03%	0.008%
61	10.439	2829	2830	2835	rBV	188	140	0.00%	0.001%
62	10.465	2835	2838	2839	rBV	263	162	0.00%	0.001%
63	10.526	2855	2857	2858	rBV	187	65	0.00%	0.000%
64	10.568	2866	2870	2872	rBV2	366	252	0.01%	0.002%
65	10.751	2915	2927	2943	rBV	310588	499497	13.92%	3.386%
66	10.877	2961	2966	2968	rBV4	449	393	0.01%	0.003%
67	11.047	3016	3019	3022	rBV	260	222	0.01%	0.002%
68	11.648	3202	3206	3208	rBV2	264	204	0.01%	0.001%
69	11.741	3223	3235	3246	rBV	559341	882968	24.60%	5.986%
70	11.831	3246	3263	3290	rVB2	1447411	3046429	84.88%	20.652%
71	12.053	3330	3332	3333	rBV	272	88	0.00%	0.001%
72	12.095	3343	3345	3347	rBV	191	90	0.00%	0.001%
73	12.192	3362	3375	3398	rBV2	497604	1007648	28.07%	6.831%
74	13.012	3628	3630	3633	rBV	260	171	0.00%	0.001%
75	13.227	3689	3697	3704	rBV4	2418	3331	0.09%	0.023%
76	13.381	3743	3745	3748	rBV2	413	259	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040523\
Data File : VU053581.D
Acq On : 05 Apr 2023 13:37
Operator : JC/MD
Sample : 02158-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PMW-6(20230329)

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Title : VOC Analysis

77	13.835	3874	3886	3910	rBV	811373	1291177	35.97%	8.753%
78	14.089	3961	3965	3974	rVB3	2423	2856	0.08%	0.019%
79	14.327	4029	4039	4053	rBV3	35347	54370	1.51%	0.369%




Sum of corrected areas: 14750915

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040523\
Data File : VU053581.D
Acq On : 05 Apr 2023 13:37
Operator : JC/MD
Sample : 02158-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PMW-6(20230329)

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

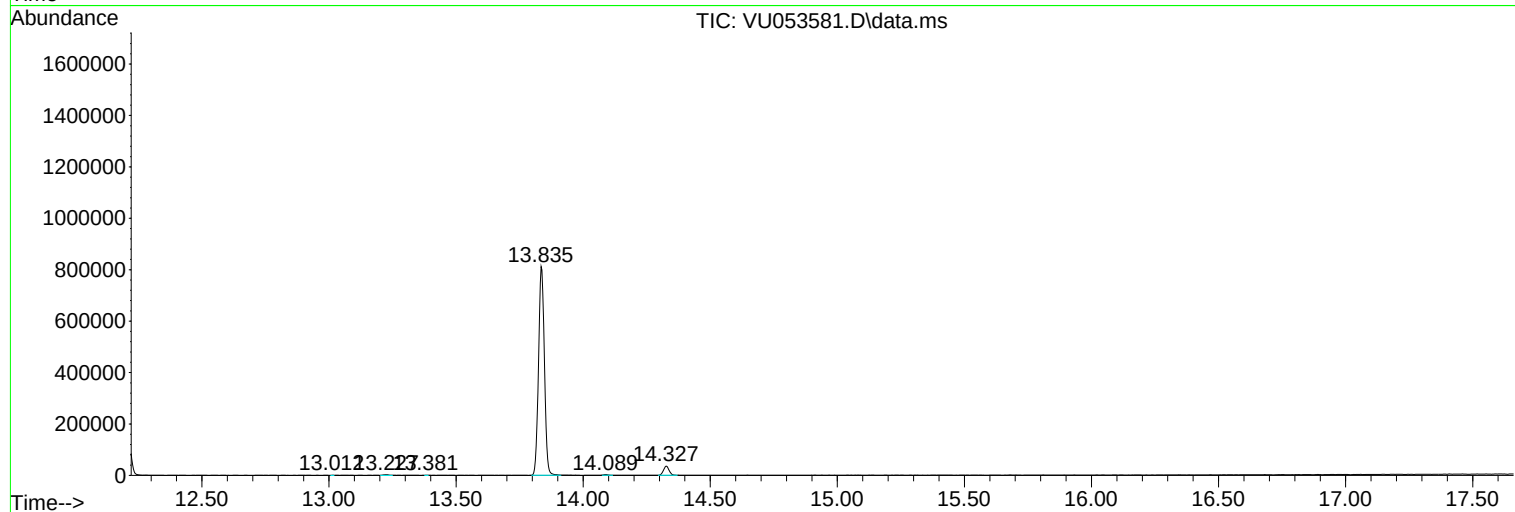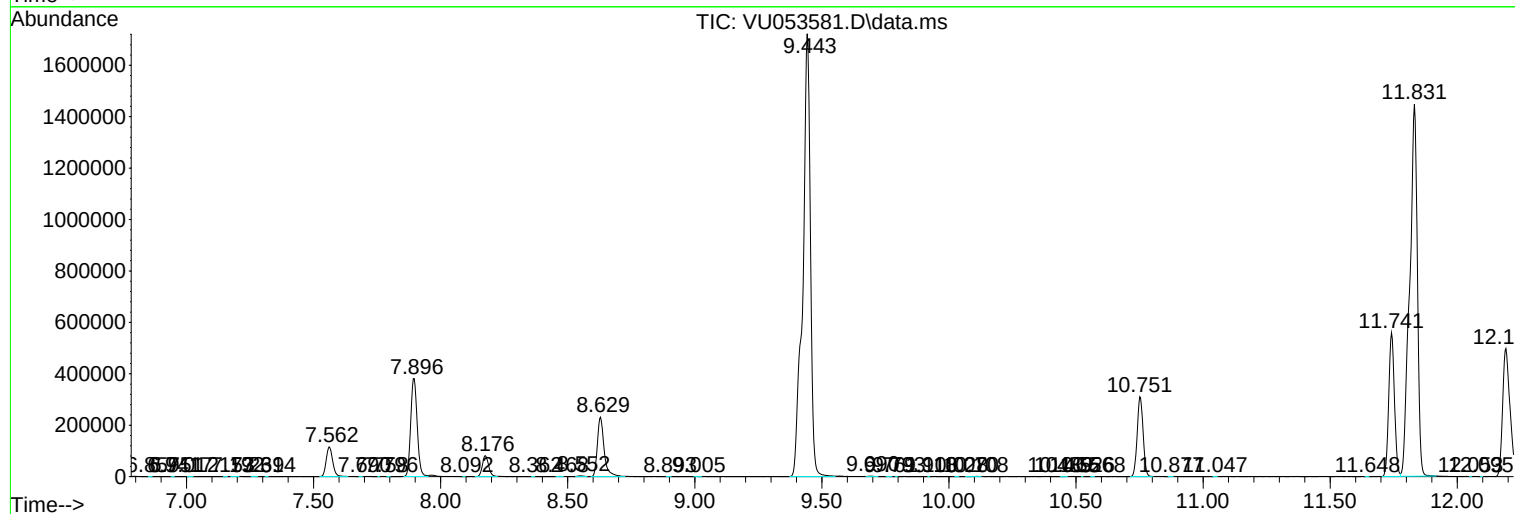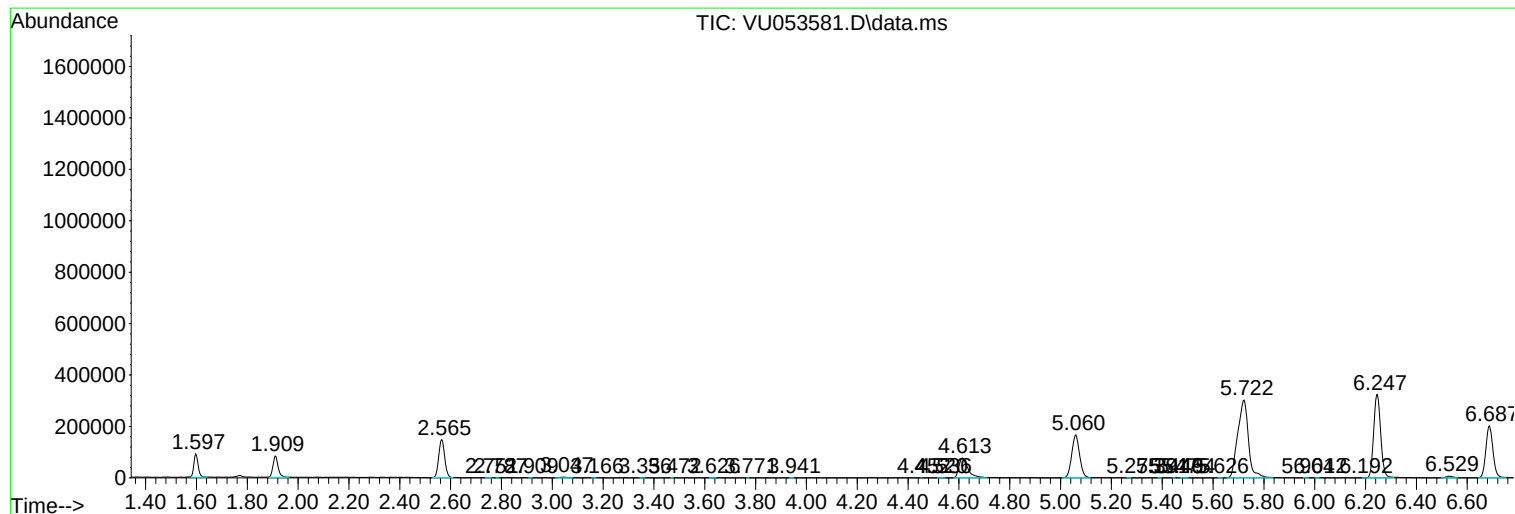

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040523\
Data File : VU053581.D
Acq On : 05 Apr 2023 13:37
Operator : JC/MD
Sample : 02158-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PMW-6(20230329)

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040523\
Data File : VU053581.D
Acq On : 05 Apr 2023 13:37
Operator : JC/MD
Sample : 02158-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PMW-6(20230329)

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------