

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040523\
 Data File : VU053582.D
 Acq On : 05 Apr 2023 15:02
 Operator : JC/MD
 Sample : 02158-28
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

Signal : TIC: VU053582.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	97	rVB	150306	171292	17.82%	2.262%
2	1.909	169	177	192	rBV	111046	153172	15.93%	2.022%
3	2.565	368	381	403	rBV	213703	347100	36.11%	4.583%
4	2.687	416	419	423	rBV3	508	333	0.03%	0.004%
5	2.777	445	447	451	rBV2	526	406	0.04%	0.005%
6	3.044	521	530	547	rBV4	2824	5242	0.55%	0.069%
7	3.208	578	581	584	rBV	254	177	0.02%	0.002%
8	3.362	626	629	632	rVB2	221	156	0.02%	0.002%
9	3.896	791	795	796	rBV	222	135	0.01%	0.002%
10	4.054	842	844	846	rBV	185	102	0.01%	0.001%
11	4.234	899	900	901	rBV	143	45	0.00%	0.001%
12	4.391	947	949	951	rBV	143	38	0.00%	0.001%
13	4.414	952	956	959	rVV2	207	185	0.02%	0.002%
14	4.446	961	966	972	rBV	366	493	0.05%	0.007%
15	4.613	1007	1018	1046	rBV2	69159	170075	17.69%	2.245%
16	4.980	1130	1132	1135	rVB	227	94	0.01%	0.001%
17	5.060	1141	1157	1178	rBV	178825	392630	40.85%	5.184%
18	5.301	1230	1232	1233	rBV	271	118	0.01%	0.002%
19	5.356	1246	1249	1253	rVB	205	109	0.01%	0.001%
20	5.375	1253	1255	1256	rBV	145	68	0.01%	0.001%
21	5.488	1288	1290	1295	rVB	247	159	0.02%	0.002%
22	5.536	1300	1305	1308	rBV2	306	330	0.03%	0.004%
23	5.568	1312	1315	1316	rBV2	167	79	0.01%	0.001%
24	5.600	1322	1325	1328	rBV2	166	125	0.01%	0.002%
25	5.645	1336	1339	1342	rVB	197	125	0.01%	0.002%
26	5.722	1342	1363	1385	rBV2	349120	961252	100.00%	12.691%
27	5.983	1442	1444	1446	rVB	133	54	0.01%	0.001%
28	6.009	1448	1452	1453	rBV	220	157	0.02%	0.002%
29	6.076	1469	1473	1476	rVB	276	219	0.02%	0.003%
30	6.247	1510	1526	1546	rBV	302350	579359	60.27%	7.649%
31	6.529	1604	1614	1627	rVB4	4881	9068	0.94%	0.120%
32	6.584	1627	1631	1636	rVB2	249	199	0.02%	0.003%
33	6.687	1649	1663	1688	rBV	218610	425758	44.29%	5.621%
34	6.800	1695	1698	1704	rVB6	1229	1008	0.10%	0.013%
35	7.047	1772	1775	1778	rBV	156	135	0.01%	0.002%
36	7.182	1813	1817	1819	rBV	617	490	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040523\
 Data File : VU053582.D
 Acq On : 05 Apr 2023 15:02
 Operator : JC/MD
 Sample : 02158-28
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

37	7.272	1842	1845	1852	rVB	223	177	0.02%	0.002%
38	7.314	1855	1858	1861	rBV	244	157	0.02%	0.002%
39	7.562	1923	1935	1961	rBV	123461	222561	23.15%	2.938%
40	7.687	1971	1974	1981	rVB3	581	712	0.07%	0.009%
41	7.783	2000	2004	2005	rBV3	268	153	0.02%	0.002%
42	7.800	2006	2009	2011	rVV2	236	167	0.02%	0.002%
43	7.841	2019	2022	2024	rBV	204	98	0.01%	0.001%
44	7.896	2025	2039	2072	rBV	469582	819734	85.28%	10.823%
45	8.108	2103	2105	2107	rVB	171	61	0.01%	0.001%
46	8.176	2115	2126	2149	rBV	89481	150420	15.65%	1.986%
47	8.359	2180	2183	2185	rBV	142	87	0.01%	0.001%
48	8.417	2198	2201	2205	rBB	179	116	0.01%	0.002%
49	8.446	2208	2210	2212	rBV	164	77	0.01%	0.001%
50	8.555	2237	2244	2249	rVB4	1392	1602	0.17%	0.021%
51	8.629	2255	2267	2297	rBV	210075	390731	40.65%	5.159%
52	8.870	2339	2342	2345	rBV2	402	270	0.03%	0.004%
53	9.005	2382	2384	2387	rBV2	186	120	0.01%	0.002%
54	9.095	2410	2412	2414	rBV	203	107	0.01%	0.001%
55	9.127	2420	2422	2423	rBV	150	36	0.00%	0.000%
56	9.189	2439	2441	2445	rBV2	225	140	0.01%	0.002%
57	9.314	2478	2480	2484	rBV2	243	138	0.01%	0.002%
58	9.414	2499	2511	2537	rBV	423318	714964	74.38%	9.440%
59	9.664	2586	2589	2593	rBV2	273	173	0.02%	0.002%
60	9.690	2594	2597	2600	rBV3	375	319	0.03%	0.004%
61	9.754	2616	2617	2621	rVB	336	189	0.02%	0.002%
62	9.819	2635	2637	2638	rBV	196	86	0.01%	0.001%
63	9.954	2678	2679	2681	rBV	149	65	0.01%	0.001%
64	10.082	2717	2719	2720	rBV	216	76	0.01%	0.001%
65	10.561	2865	2868	2873	rBV	367	322	0.03%	0.004%
66	10.751	2914	2927	2949	rBV	296339	477852	49.71%	6.309%
67	10.877	2964	2966	2968	rBV	174	124	0.01%	0.002%
68	11.462	3145	3148	3149	rBV	320	172	0.02%	0.002%
69	11.500	3159	3160	3161	rBV	187	41	0.00%	0.001%
70	11.745	3229	3236	3243	rBV5	3113	4445	0.46%	0.059%
71	11.809	3244	3256	3277	rBV	469421	761611	79.23%	10.055%
72	12.188	3362	3374	3395	rBV	479735	774126	80.53%	10.221%
73	12.356	3419	3426	3431	rBV2	387	552	0.06%	0.007%
74	12.651	3515	3518	3522	rVB2	440	313	0.03%	0.004%
75	12.848	3576	3579	3581	rBV	283	196	0.02%	0.003%
76	13.841	3879	3888	3905	rVB2	17564	30031	3.12%	0.396%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040523\
Data File : VU053582.D
Acq On : 05 Apr 2023 15:02
Operator : JC/MD
Sample : 02158-28
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Title : VOC Analysis

77	14.089	3962	3965	3966	rBV2	627	361	0.04%	0.005%
----	--------	------	------	------	------	-----	-----	-------	--------




Sum of corrected areas: 7574169

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040523\
Data File : VU053582.D
Acq On : 05 Apr 2023 15:02
Operator : JC/MD
Sample : 02158-28
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

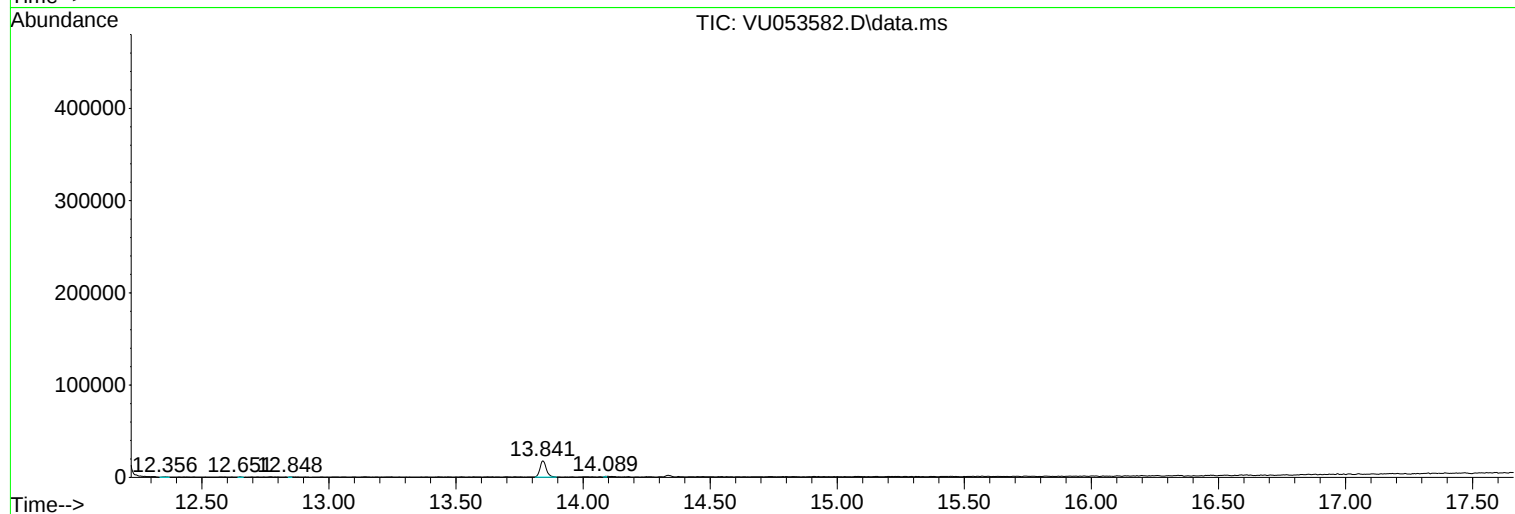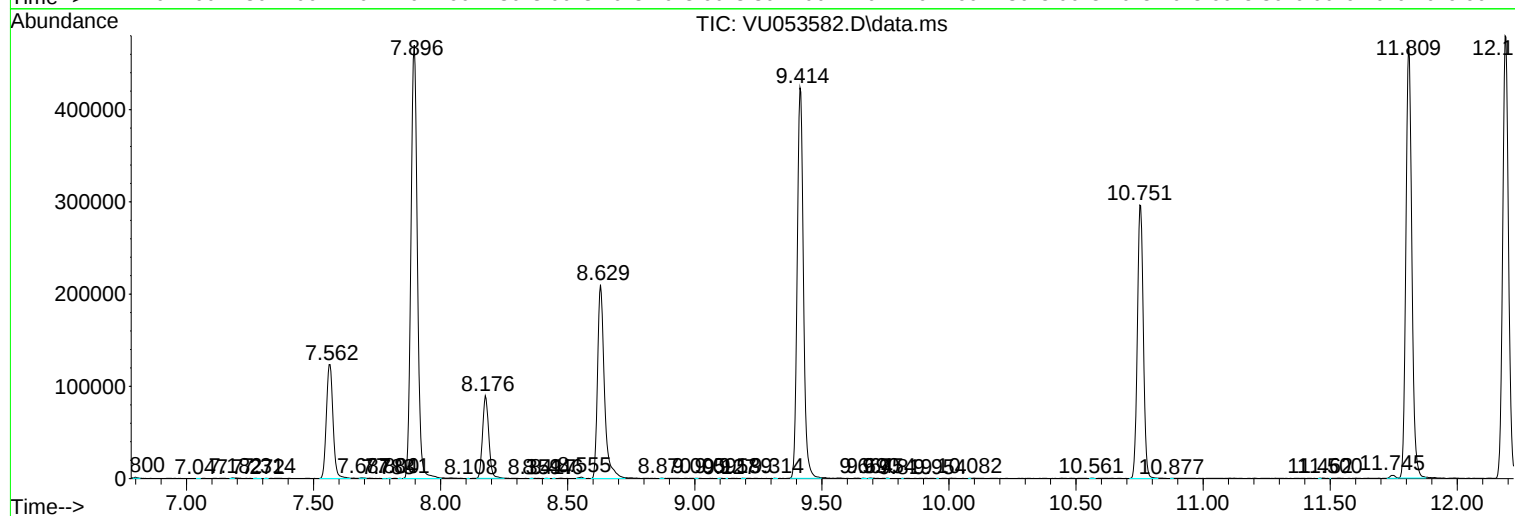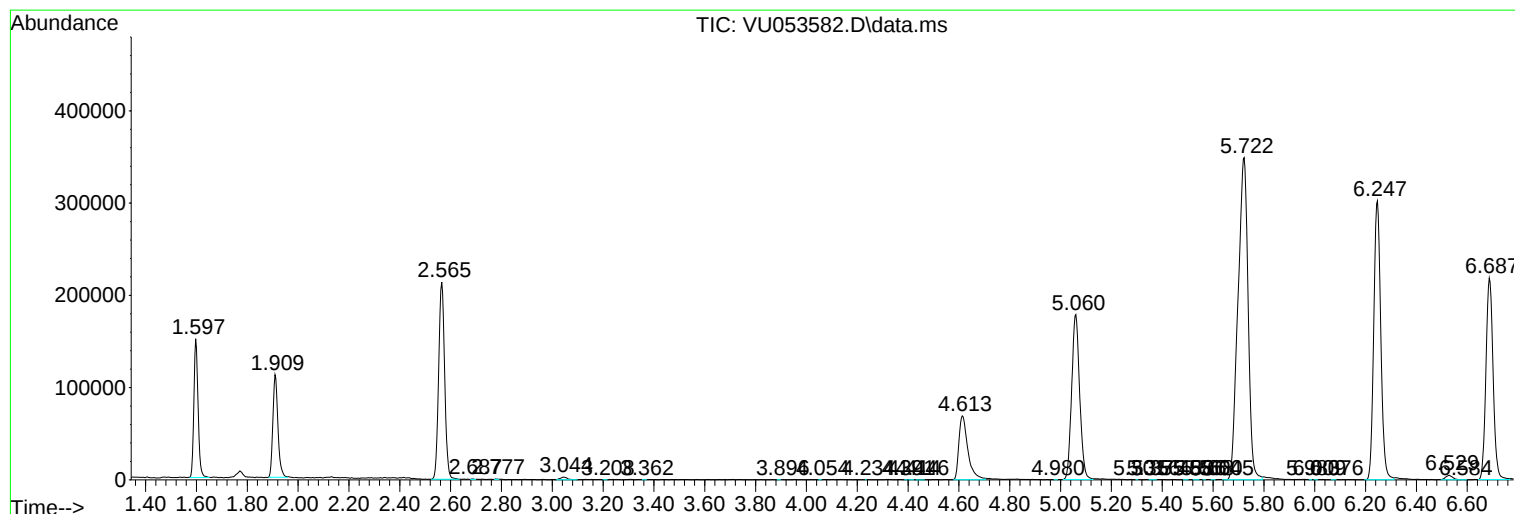

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040523\
Data File : VU053582.D
Acq On : 05 Apr 2023 15:02
Operator : JC/MD
Sample : 02158-28
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040523\
Data File : VU053582.D
Acq On : 05 Apr 2023 15:02
Operator : JC/MD
Sample : 02158-28
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------