


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040523\
Data File : VU053576.D
Acq On : 05 Apr 2023 09:42
Operator : JC/MD
Sample : BFB174
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB174

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Title : VOC Analysis
Last Update : Sat Apr 01 04:51:17 2023

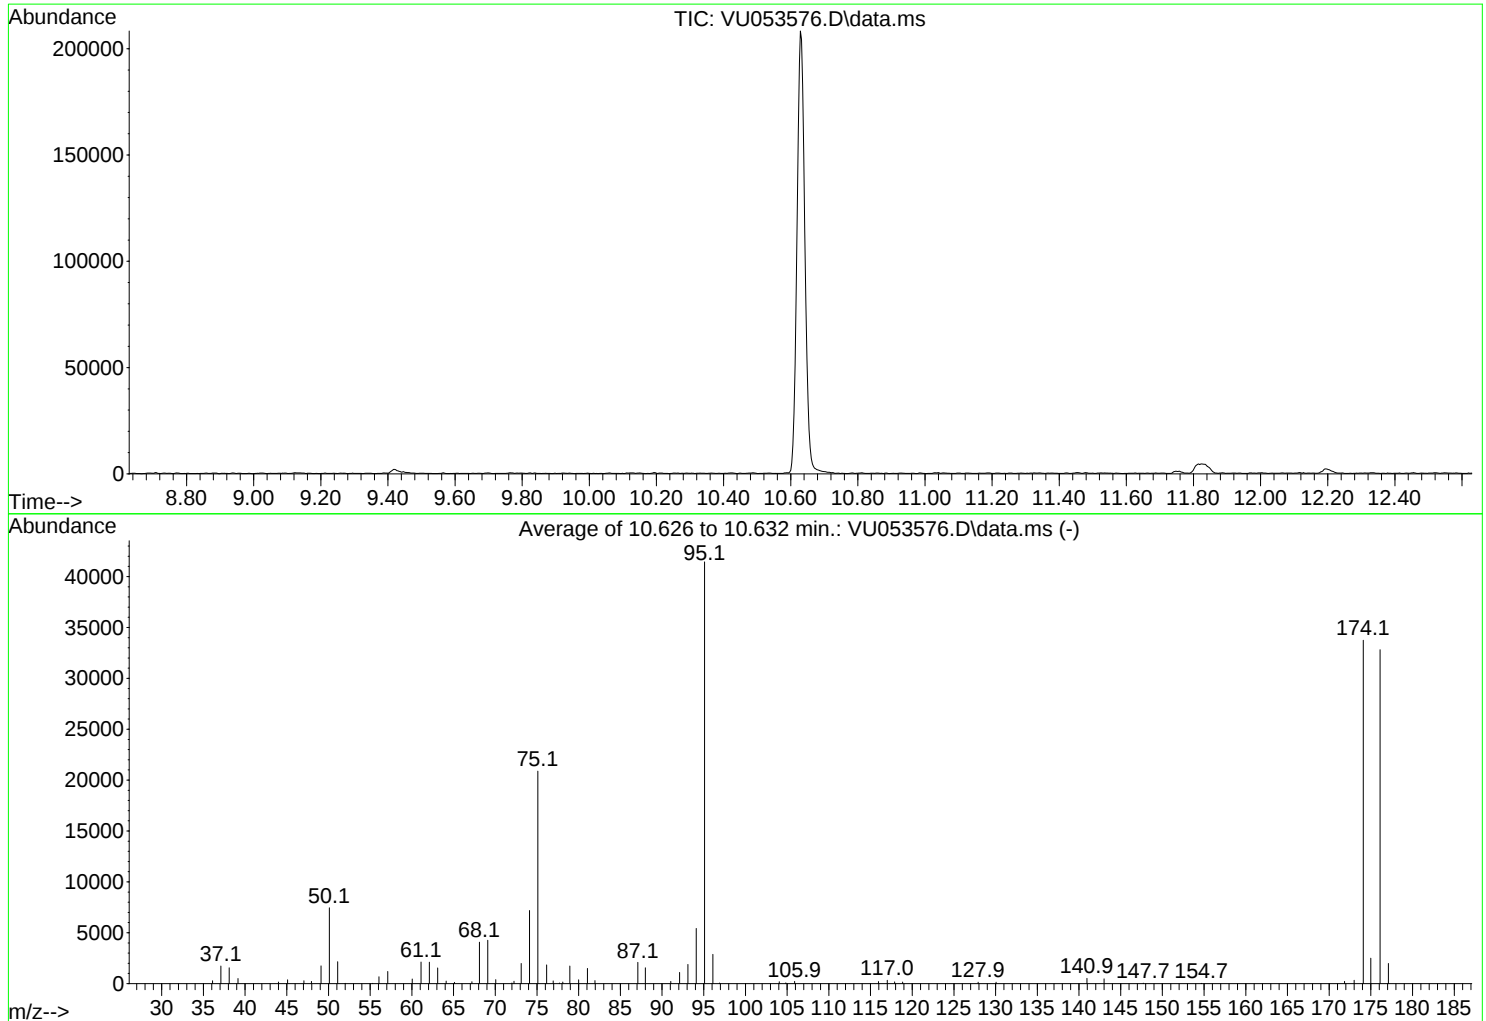

AutoFind: Scans 2888, 2889, 2890; Background Corrected with Scan 2877

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.0	7454	PASS
75	95	30	80	50.4	20880	PASS
95	95	100	100	100.0	41448	PASS
96	95	5	9	6.9	2874	PASS
173	174	0.00	2	1.0	334	PASS
174	95	50	120	81.4	33741	PASS
175	174	5	9	7.4	2503	PASS
176	174	95	101	97.2	32813	PASS
177	176	5	9	6.0	1985	PASS

Scan 2877 (10.590 min): VU053576.D\data.ms
BFB174

m/z	Abundance
39.80	151.0
44.00	356.0

Instrument :
MSVOA_U
ClientSampleId :
BFB174

m/z	Abundance
36.10	278.0
37.10	1660.0
38.10	1526.0
39.10	479.0
40.00	149.0
44.00	431.0
45.10	362.0
47.00	269.0
47.90	263.0
49.10	1639.0
50.10	7163.0
51.10	2058.0
55.30	106.0
56.00	732.0
57.10	1146.0
60.10	483.0
61.10	2086.0
62.10	1973.0
63.10	1531.0
64.10	220.0
65.00	114.0
67.20	216.0
68.10	4148.0
69.10	4208.0
70.00	465.0
72.00	181.0
72.30	198.0
73.10	2043.0
74.10	7064.0
75.10	20624.0
76.10	1706.0
76.90	261.0
77.70	180.0
78.10	147.0
79.00	1706.0
79.90	338.0
81.10	1390.0
82.00	309.0
87.10	1886.0
88.00	1623.0
91.10	266.0
92.10	1125.0
93.10	1731.0
94.10	5130.0
95.10	39512.0
96.10	2905.0
96.90	101.0
104.10	186.0
105.90	199.0
116.00	159.0
117.00	383.0
117.90	173.0
118.80	159.0
127.90	157.0
130.10	146.0
140.90	497.0
143.00	376.0
171.80	173.0
173.00	295.0
174.10	31584.0
175.00	2385.0
176.10	30304.0
177.10	1915.0

Instrument :
MSVOA_U
ClientSampleId :
BFB174

m/z	Abundance
36.10	283.0
37.10	1779.0
38.10	1597.0
39.20	503.0
40.00	131.0
44.00	523.0
45.10	402.0
47.10	293.0
48.00	233.0
49.10	1818.0
50.10	7779.0
51.10	2270.0
56.10	701.0
57.10	1237.0
60.10	440.0
61.10	2177.0
62.10	2180.0
63.10	1545.0
64.10	249.0
65.10	123.0
67.20	210.0
68.10	4193.0
69.10	4373.0
70.10	420.0
72.30	247.0
73.10	2051.0
74.10	7324.0
75.10	21296.0
76.20	1951.0
77.00	286.0
78.10	174.0
79.00	1766.0
80.00	368.0
81.10	1511.0
81.90	285.0
87.10	2169.0
88.00	1626.0
91.00	241.0
92.10	1158.0
93.10	1969.0
94.10	5677.0
95.10	42896.0
96.10	2991.0
96.90	101.0
104.00	175.0
104.80	103.0
105.90	226.0
116.00	199.0
117.00	350.0
117.90	186.0
118.80	166.0
128.00	136.0
130.00	137.0
140.90	549.0
143.00	489.0
154.70	108.0
171.90	232.0
173.00	356.0
174.10	34712.0
175.00	2590.0
176.10	34032.0
177.10	2007.0

Instrument :
MSVOA_U
ClientSampleId :
BFB174

m/z	Abundance
36.10	278.0
37.10	1755.0
38.10	1539.0
39.20	515.0
40.00	109.0
44.00	570.0
45.10	368.0
47.10	286.0
48.00	178.0
49.10	1774.0
50.10	7420.0
51.10	2155.0
52.00	105.0
56.10	609.0
57.10	1217.0
60.00	430.0
61.10	2097.0
62.10	2154.0
63.10	1525.0
64.10	272.0
65.20	132.0
67.10	139.0
68.10	3900.0
69.10	4225.0
70.00	312.0
72.20	253.0
73.10	1856.0
74.10	7150.0
75.10	20720.0
76.10	1879.0
77.00	259.0
78.10	157.0
78.90	1709.0
80.10	440.0
81.00	1571.0
82.00	306.0
87.10	2198.0
88.00	1429.0
91.00	165.0
92.10	1020.0
93.10	1979.0
94.10	5456.0
95.10	41936.0
96.10	2725.0
104.00	187.0
104.90	118.0
105.90	225.0
115.90	253.0
117.00	274.0
117.90	154.0
118.90	164.0
127.80	129.0
130.00	139.0
141.00	513.0
143.00	538.0
147.70	135.0
171.90	251.0
173.00	350.0
174.10	34928.0
175.00	2533.0
176.10	34104.0
177.10	2033.0

Instrument :
MSVOA_U
ClientSampleId :
BFB174