

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU040619\
Quantitation Report (QT Reviewed)


Data File : VU030764.D
Acq On : 06 Apr 2019 00:17
Operator : JC/SP
Sample : K2260-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ETJ57

Manual Integrations
APPROVED

MMDadoda
4/6/2019 10:32:57 AM

Quant Time: Apr 06 05:00:36 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Apr 06 02:16:29 2019
Response via : Initial Calibration

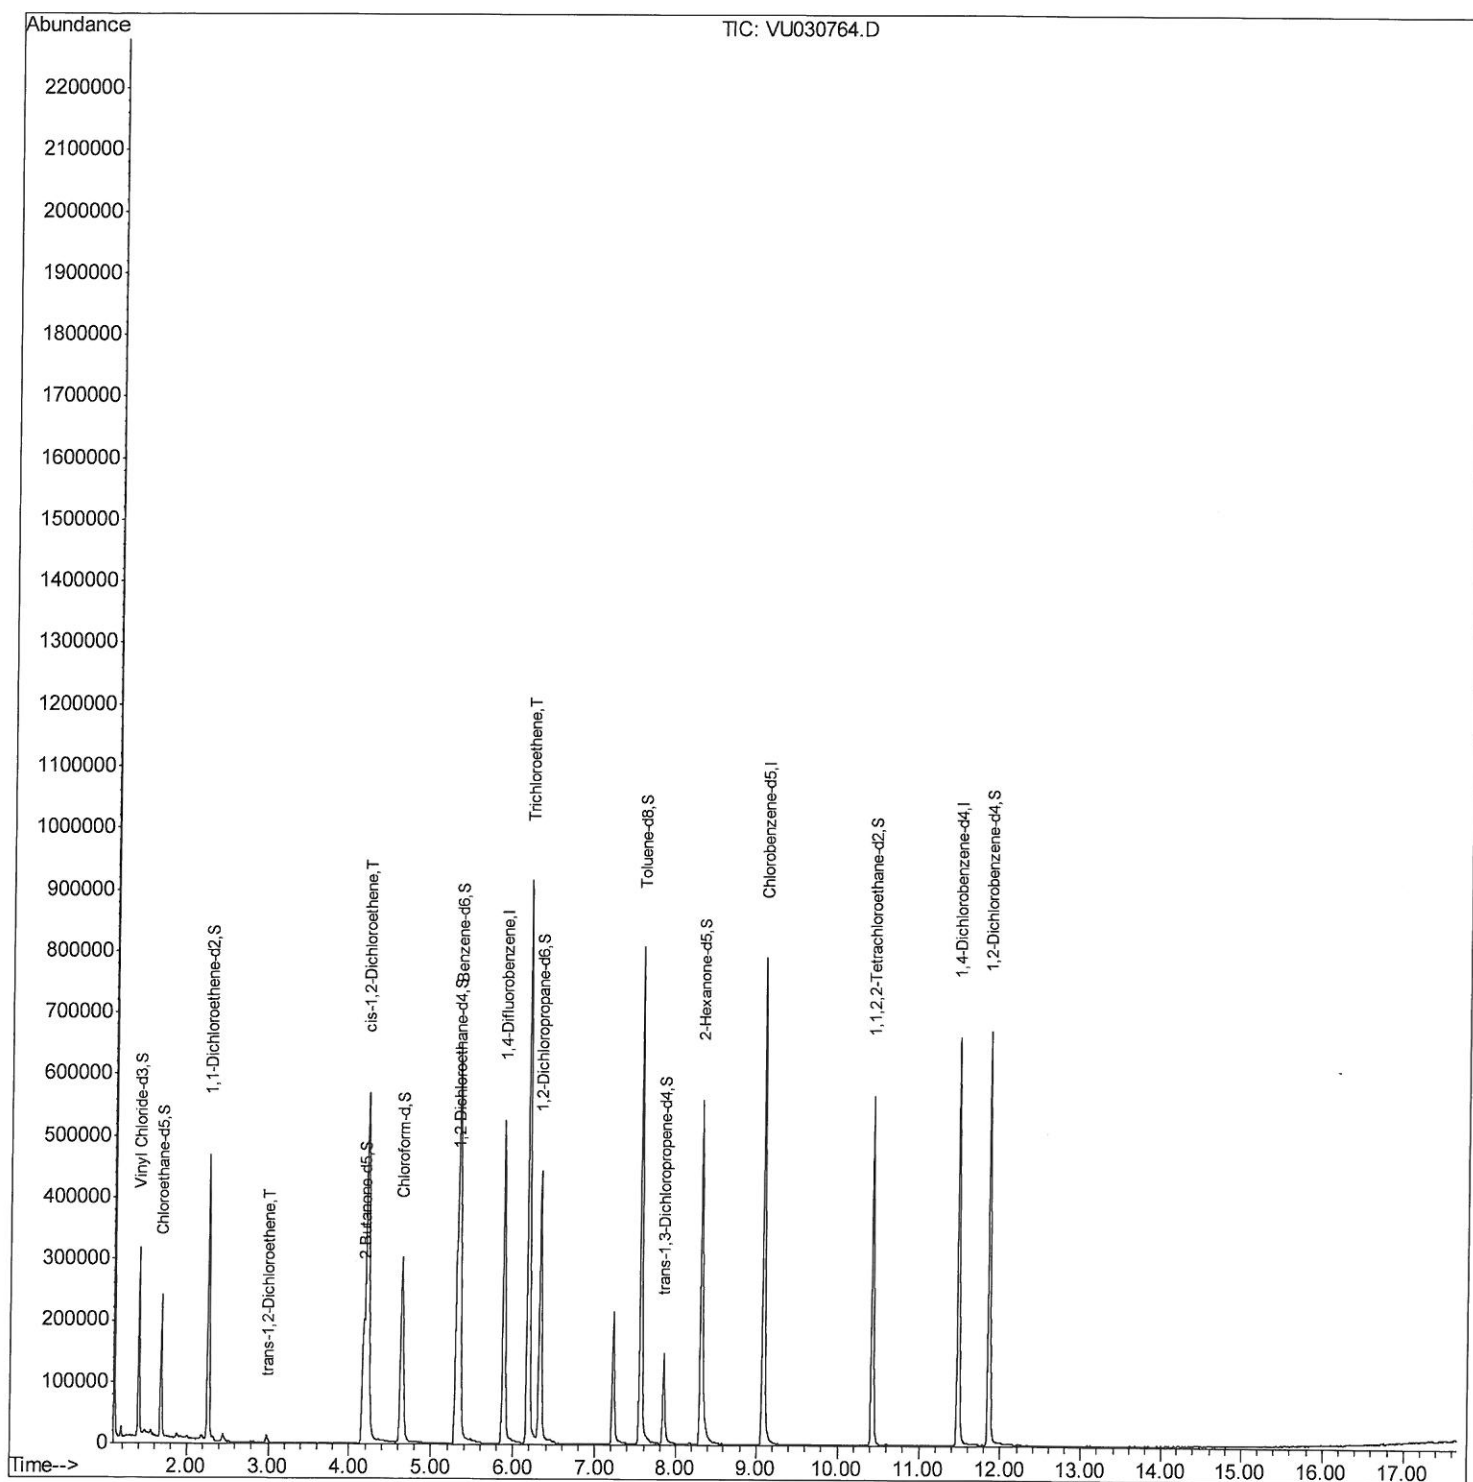

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU040619\
Quantitation Report (Qedit)




Data File : VU030764.D
Acq On : 06 Apr 2019 00:17
Operator : JC/SP
Sample : K2260-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ETJ57

Manual Integrations
APPROVED

MMDadoda
4/6/2019 10:32:57 AM

Quant Time: Apr 06 02:23:33 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Apr 06 02:16:29 2019
Response via : Initial Calibration

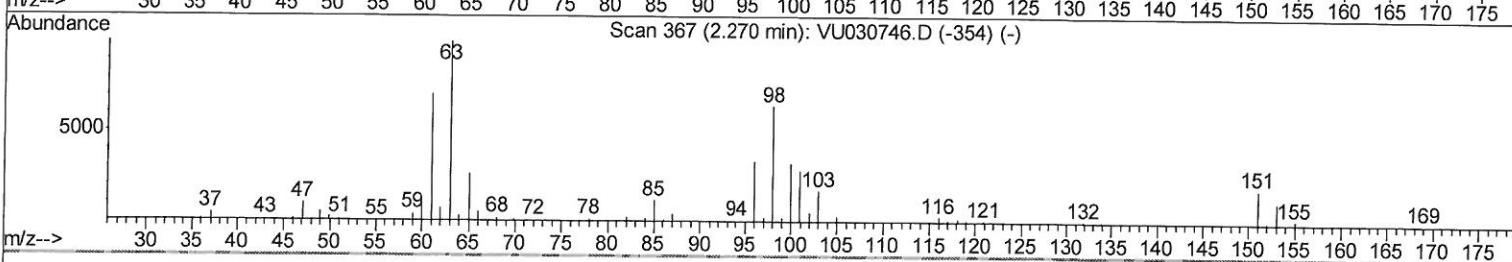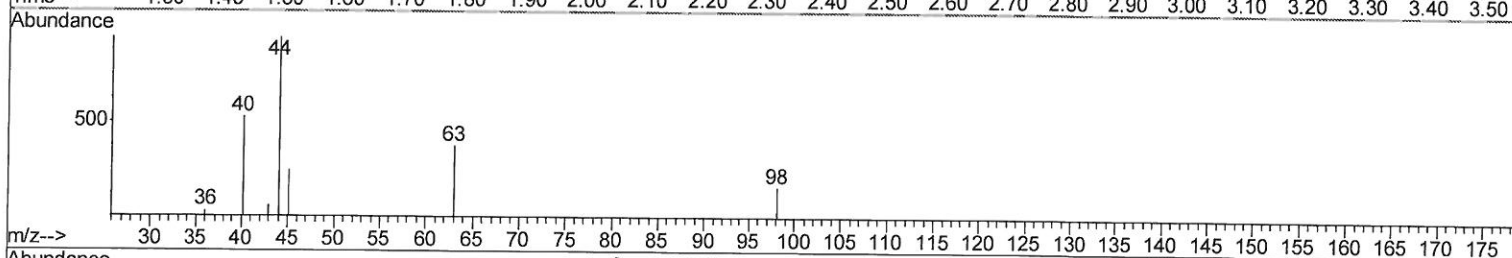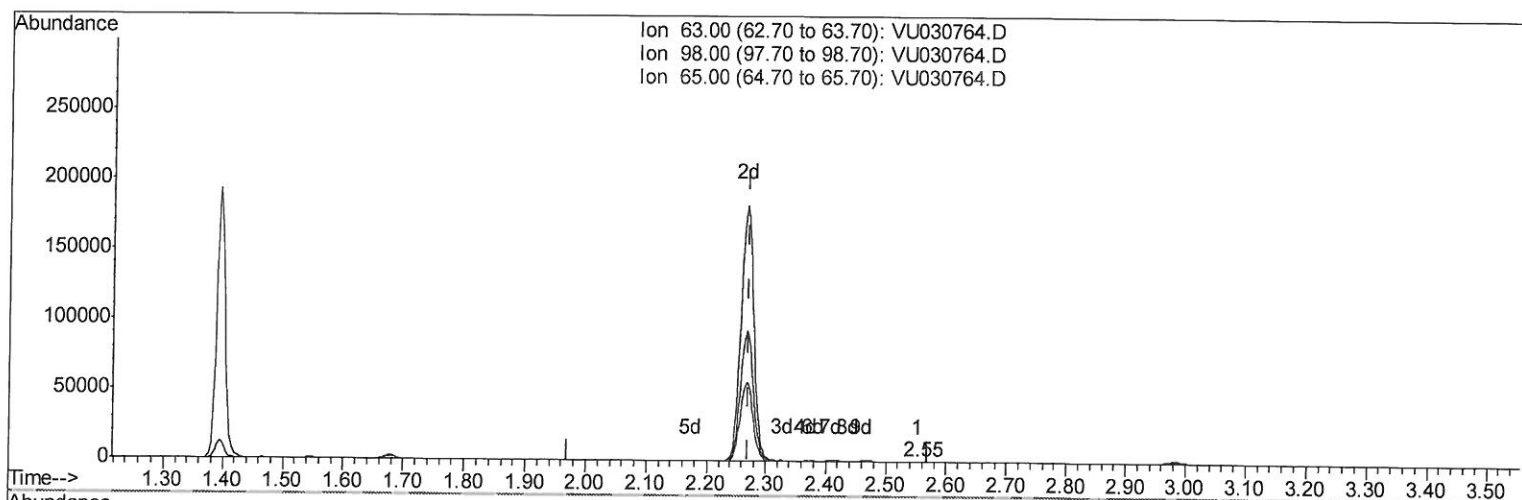

TIC: VU030764.D

(11) 1,1-Dichloroethene-d2 (S)

2.553min (+0.283) 0.03ug/L

response 190

Ion	Exp%	Act%
63.00	100	100
98.00	67.20	85.79
65.00	24.00	22.63
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU040619\
Quantitation Report (Qedit)




Data File : VU030764.D
Acq On : 06 Apr 2019 00:17
Operator : JC/SP
Sample : K2260-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ETJ57

Manual Integrations
APPROVED

MMDadoda
4/6/2019 10:32:57 AM

Quant Time: Apr 06 02:23:33 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Apr 06 02:16:29 2019
Response via : Initial Calibration

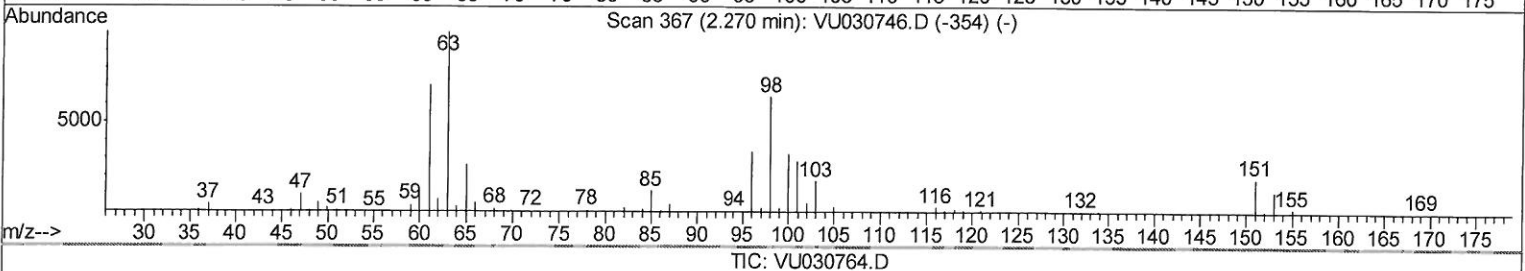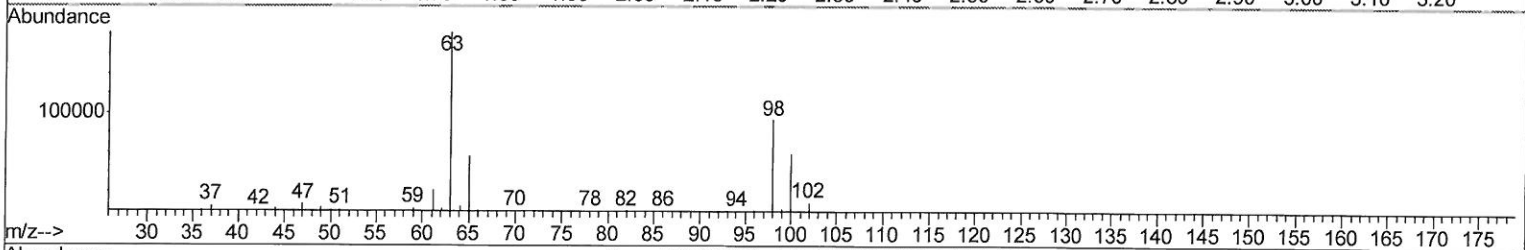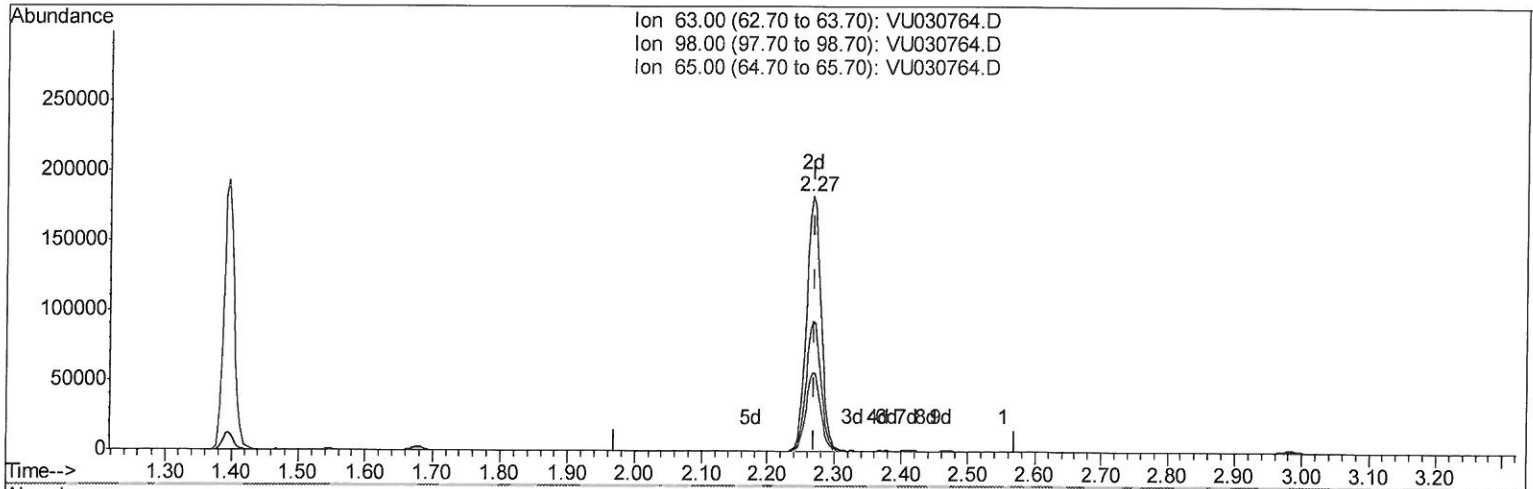

TIC: VU030764.D

(11) 1,1-Dichloroethene-d2 (S)

2.267min (-0.003) 39.47ug/L m

response 272040

Ion	Exp%	Act%
63.00	100	100
98.00	67.20	0.06#
65.00	24.00	0.02#
0.00	0.00	0.00

7 M Q
4/7/19

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU040619\
Quantitation Report (QT Reviewed)

Data File : VU030764.D
Acq On : 06 Apr 2019 00:17
Operator : JC/SP
Sample : K2260-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ETJ57

Manual Integrations
APPROVED

MMDadoda
4/6/2019 10:32:57 AM

Quant Time: Apr 06 05:00:36 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Apr 06 02:16:29 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	426833	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	424781	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	170919	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	197898	51.94	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	103.88%
7) Chloroethane-d5	1.68	69	159416	55.13	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	110.26%
11) 1,1-Dichloroethene-d2	2.27	63	272040m	39.47	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	78.94%
21) 2-Butanone-d5	4.17	46	328222	108.69	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	108.69%
24) Chloroform-d	4.64	84	302121	51.91	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	103.82%
26) 1,2-Dichloroethane-d4	5.31	65	217826	54.85	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	109.70%
32) Benzene-d6	5.34	84	634680	51.18	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	102.36%
36) 1,2-Dichloropropane-d6	6.33	67	223424	52.57	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	105.14%
41) Toluene-d8	7.56	98	538937	49.03	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	98.06%
43) trans-1,3-Dichloropropene-	7.85	79	90007	46.45	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	92.90%
47) 2-Hexanone-d5	8.31	63	182578	94.00	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	94.00%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	298540	52.08	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	104.16%
64) 1,2-Dichlorobenzene-d4	11.86	152	179827	53.50	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	107.00%

Target Compounds					Qvalue
17) trans-1,2-Dichloroethene	2.98	96	4688	1.496	ug/L 80
20) cis-1,2-Dichloroethene	4.22	96	305971	88.454	ug/L 96
34) Trichloroethene	6.18	95	341044	100.031	ug/L 99

(#) = qualifier out of range (m) = manual integration (+) = signals summed