

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU040619\
 Data File : VU030781.D
 Acq On : 06 Apr 2019 07:10
 Operator : JC/SP
 Sample : K2269-05
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0BR7

Quant Time: Apr 08 01:59:37 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon Apr 08 01:03:28 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	472079	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	463123	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	190916	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	222994	52.92	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	105.84%
7) Chloroethane-d5	1.68	69	176022	55.03	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	110.06%
11) 1,1-Dichloroethene-d2	2.27	63	305421	40.07	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	80.14%
21) 2-Butanone-d5	4.17	46	352399	105.51	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	105.51%
24) Chloroform-d	4.64	84	333918	51.87	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	103.74%
26) 1,2-Dichloroethane-d4	5.31	65	234888	53.47	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	106.94%
32) Benzene-d6	5.33	84	695522	51.44	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	102.88%
36) 1,2-Dichloropropane-d6	6.33	67	239257	51.64	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	103.28%
41) Toluene-d8	7.56	98	593226	49.50	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	99.00%
43) trans-1,3-Dichloropropene-	7.85	79	94699	44.82	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	89.64%
47) 2-Hexanone-d5	8.31	63	209975	99.15	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	99.15%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	320202	51.23	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	102.46%
64) 1,2-Dichlorobenzene-d4	11.86	152	201984	53.80	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	107.60%


Target Compounds					Ovalue
13) Acetone	2.32	43	11383	3.331 ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU040619\
Data File : VU030781.D
Acq On : 06 Apr 2019 07:10
Operator : JC/SP
Sample : K2269-05
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BR7

Quant Time: Apr 08 01:59:37 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Apr 08 01:03:28 2019
Response via : Initial Calibration

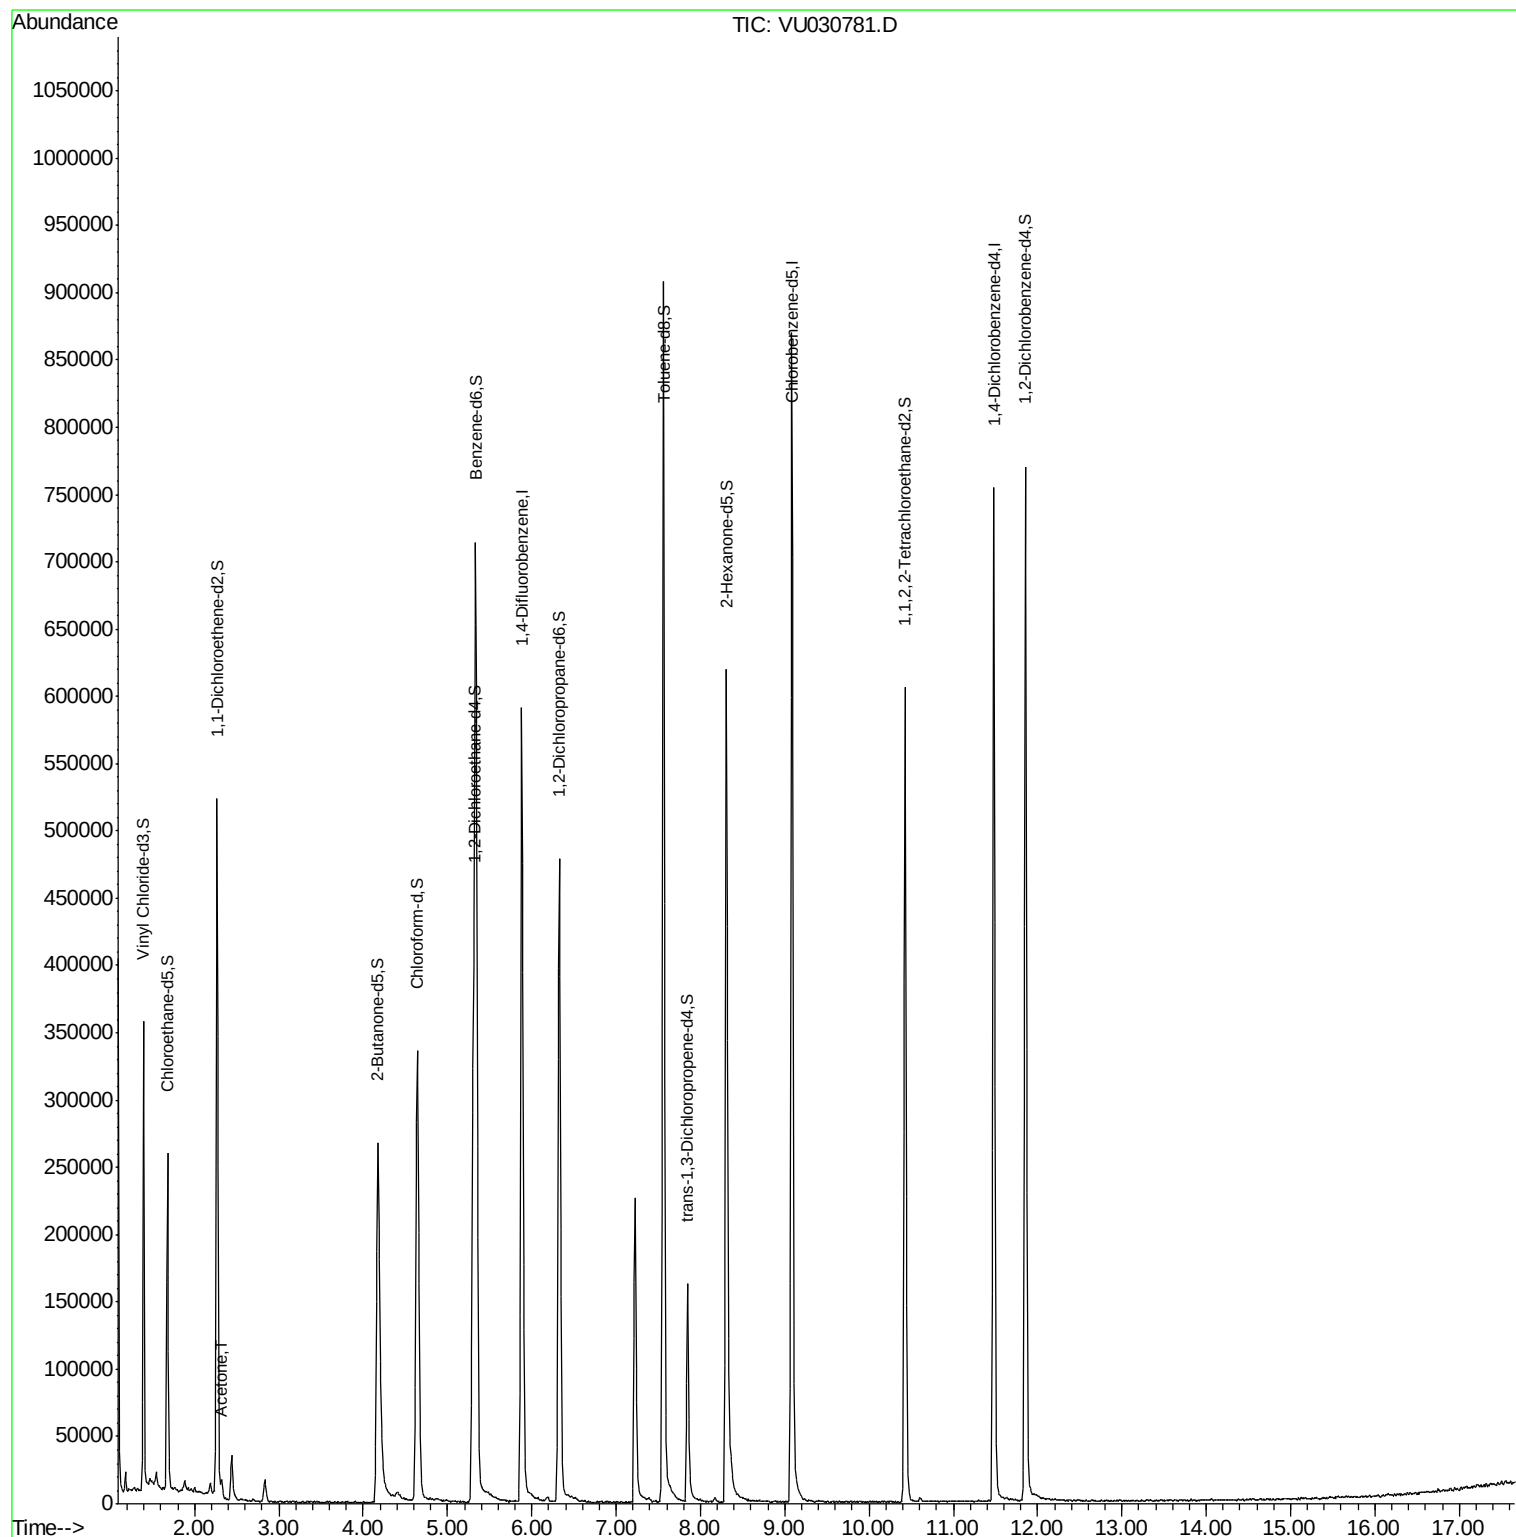

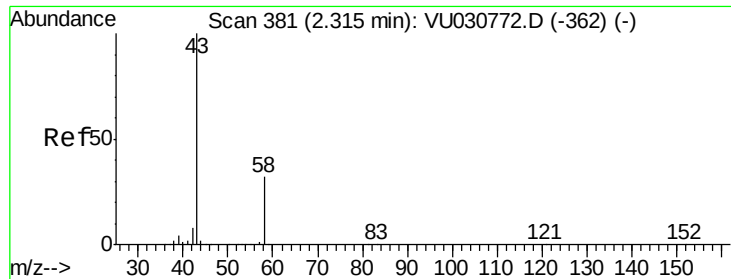

#13

Acetone

Concen: 3.331 ug/L

RT: 2.32 min Scan# 382

Delta R.T. 0.00 min

Lab File: VU030781.D

Acq: 06 Apr 2019 07:10

Instrument :

MSVOA_U

ClientSampleId :

C0BR7

Tot Ion: 43 Resp: 11383

Ion Ratio Lower Upper

43 100

58 35.4 0.0 64.0

