

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU040619\
 Data File : VU030759.D
 Acq On : 05 Apr 2019 22:23
 Operator : JC/SP
 Sample : K2215-06ME 40X
 Misc : 5.33q/5mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF2M7ME

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.180	23	28	35	rBV	16693	15806	0.86%	0.110%
2	1.395	88	95	104	rBV	268032	275774	14.93%	1.912%
3	1.672	173	181	195	rBV	196570	266423	14.43%	1.847%
4	2.267	355	366	380	rVB	427223	647004	35.04%	4.485%
5	2.431	414	417	419	rBV4	1270	907	0.05%	0.006%
6	2.534	446	449	451	rBV2	912	560	0.03%	0.004%
7	2.604	466	471	477	rVB5	872	1052	0.06%	0.007%
8	2.691	493	498	501	rBV6	1967	1964	0.11%	0.014%
9	2.932	570	573	577	rBV4	703	556	0.03%	0.004%
10	3.022	597	601	605	rVB2	828	502	0.03%	0.003%
11	3.122	629	632	638	rVB3	990	1111	0.06%	0.008%
12	3.183	647	651	654	rBV3	598	521	0.03%	0.004%
13	3.286	677	683	684	rVV2	568	531	0.03%	0.004%
14	3.296	684	686	689	rVV3	918	717	0.04%	0.005%
15	3.354	701	704	707	rVV3	901	639	0.03%	0.004%
16	3.553	762	766	771	rVV3	463	446	0.02%	0.003%
17	3.669	799	802	806	rBV2	629	521	0.03%	0.004%
18	3.698	806	811	815	rBV4	452	508	0.03%	0.004%
19	3.768	826	833	836	rVB3	736	774	0.04%	0.005%
20	3.797	836	842	844	rBV3	886	805	0.04%	0.006%
21	3.913	871	878	879	rBV3	798	695	0.04%	0.005%
22	3.958	887	892	897	rBV3	485	485	0.03%	0.003%
23	4.029	910	914	916	rBV2	614	504	0.03%	0.003%
24	4.067	924	926	931	rVB2	609	499	0.03%	0.003%
25	4.109	934	939	942	rBV	519	461	0.02%	0.003%
26	4.173	946	959	990	rBV	206457	551912	29.89%	3.826%
27	4.643	1085	1105	1136	rBV2	281611	726528	39.34%	5.036%
28	4.791	1149	1151	1154	rBV3	832	506	0.03%	0.004%
29	4.862	1169	1173	1175	rBV2	1142	708	0.04%	0.005%
30	4.993	1211	1214	1216	rBV3	884	486	0.03%	0.003%
31	5.045	1226	1230	1235	rVB5	537	474	0.03%	0.003%
32	5.334	1297	1320	1355	rBV3	615621	1846628	100.00%	12.801%
33	5.697	1431	1433	1437	rVB4	922	659	0.04%	0.005%
34	5.746	1444	1448	1453	rVV4	656	861	0.05%	0.006%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU040619\
 Data File : VU030759.D
 Acq On : 05 Apr 2019 22:23
 Operator : JC/SP
 Sample : K2215-06ME 40X
 Misc : 5.33q/5mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF2M7ME

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Title : VOC Analysis

35	5.788	1457	1461	1464	rBV5	555	486	0.03%	0.003%
36	5.881	1471	1490	1514	rBV	588145	1175575	63.66%	8.149%
37	6.135	1567	1569	1572	rBV2	715	476	0.03%	0.003%
38	6.167	1572	1579	1582	rBV6	2050	2454	0.13%	0.017%
39	6.263	1606	1609	1610	rBV2	1061	547	0.03%	0.004%
40	6.324	1613	1628	1648	rBV	422207	852694	46.18%	5.911%
41	6.688	1736	1741	1747	rVB5	673	692	0.04%	0.005%
42	6.881	1798	1801	1805	rBV3	655	538	0.03%	0.004%
43	6.974	1827	1830	1832	rVB2	1014	615	0.03%	0.004%
44	7.006	1834	1840	1845	rBV5	521	657	0.04%	0.005%
45	7.080	1859	1863	1869	rBV2	1263	1305	0.07%	0.009%
46	7.225	1895	1908	1935	rBV	217655	412607	22.34%	2.860%
47	7.466	1980	1983	1988	rBV3	843	675	0.04%	0.005%
48	7.562	2000	2013	2032	rBV	740991	1318301	71.39%	9.139%
49	7.845	2091	2101	2125	rBV	150858	277135	15.01%	1.921%
50	8.019	2152	2155	2159	rBV5	625	581	0.03%	0.004%
51	8.173	2199	2203	2206	rBV4	1350	1020	0.06%	0.007%
52	8.225	2206	2219	2232	rBV2	39199	65592	3.55%	0.455%
53	8.308	2234	2245	2281	rBV	611124	1154445	62.52%	8.003%
54	8.643	2345	2349	2353	rBV4	1159	859	0.05%	0.006%
55	8.803	2395	2399	2402	rBV4	612	587	0.03%	0.004%
56	8.897	2423	2428	2430	rBV3	1207	1030	0.06%	0.007%
57	8.958	2444	2447	2451	rBV4	759	519	0.03%	0.004%
58	8.984	2452	2455	2458	rBV	892	483	0.03%	0.003%
59	9.086	2474	2487	2517	rBV	848904	1455964	78.84%	10.093%
60	9.328	2558	2562	2566	rBV5	883	834	0.05%	0.006%
61	9.357	2569	2571	2574	rVV2	827	502	0.03%	0.003%
62	9.373	2574	2576	2581	rVV3	701	695	0.04%	0.005%
63	9.427	2589	2593	2596	rBV3	632	606	0.03%	0.004%
64	9.469	2601	2606	2607	rBV2	876	641	0.03%	0.004%
65	9.501	2614	2616	2622	rVB3	661	470	0.03%	0.003%
66	9.540	2622	2628	2630	rBV4	952	962	0.05%	0.007%
67	9.553	2630	2632	2636	rVB2	743	466	0.03%	0.003%
68	9.617	2649	2652	2656	rVB2	1024	609	0.03%	0.004%
69	9.729	2684	2687	2690	rBV5	1004	755	0.04%	0.005%
70	9.787	2701	2705	2710	rVB4	741	699	0.04%	0.005%
71	9.813	2710	2713	2716	rBV4	1188	756	0.04%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU040619\
 Data File : VU030759.D
 Acq On : 05 Apr 2019 22:23
 Operator : JC/SP
 Sample : K2215-06ME 40X
 Misc : 5.33g/5mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF2M7ME

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Title : VOC Analysis

72	9.993	2767	2769	2774	rVB2	700	478	0.03%	0.003%
73	10.099	2799	2802	2805	rBV2	940	580	0.03%	0.004%
74	10.135	2810	2813	2816	rBV3	746	498	0.03%	0.003%
75	10.263	2849	2853	2857	rBV3	721	501	0.03%	0.003%
76	10.427	2891	2904	2925	rBV	579112	937773	50.78%	6.501%
77	10.565	2944	2947	2949	rBV2	990	531	0.03%	0.004%
78	10.594	2952	2956	2959	rBV3	946	823	0.04%	0.006%
79	10.659	2972	2976	2980	rVB5	1165	981	0.05%	0.007%
80	10.684	2980	2984	2987	rBV3	1069	806	0.04%	0.006%
81	10.791	3013	3017	3020	rBV4	925	851	0.05%	0.006%
82	10.839	3028	3032	3036	rBV4	809	618	0.03%	0.004%
83	11.083	3103	3108	3111	rBV4	984	897	0.05%	0.006%
84	11.112	3111	3117	3124	rVB6	2110	2627	0.14%	0.018%
85	11.176	3134	3137	3140	rBV3	800	540	0.03%	0.004%
86	11.196	3140	3143	3152	rBV3	755	967	0.05%	0.007%
87	11.482	3219	3232	3261	rBV	753285	1235633	66.91%	8.566%
88	11.752	3313	3316	3319	rBV2	1146	731	0.04%	0.005%
89	11.858	3332	3349	3375	rBV	681143	1147978	62.17%	7.958%
90	12.099	3421	3424	3430	rBV5	1425	1243	0.07%	0.009%
91	12.356	3500	3504	3506	rBV3	937	835	0.05%	0.006%
92	12.398	3514	3517	3523	rVB4	838	699	0.04%	0.005%
93	12.469	3533	3539	3544	rBV5	1253	1551	0.08%	0.011%
94	12.601	3577	3580	3582	rBV4	1053	666	0.04%	0.005%
95	12.694	3607	3609	3615	rVB4	783	840	0.05%	0.006%
96	12.903	3671	3674	3678	rBV3	992	640	0.03%	0.004%
97	13.205	3765	3768	3771	rBV2	728	471	0.03%	0.003%
98	13.864	3971	3973	3977	rBV4	884	786	0.04%	0.005%
99	14.266	4096	4098	4100	rBV2	995	592	0.03%	0.004%
100	14.652	4215	4218	4223	rBV4	1206	881	0.05%	0.006%


Sum of corrected areas: 14425376

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU040619\
Data File : VU030759.D
Acq On : 05 Apr 2019 22:23
Operator : JC/SP
Sample : K2215-06ME 40X
Misc : 5.33q/5mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF2M7ME

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

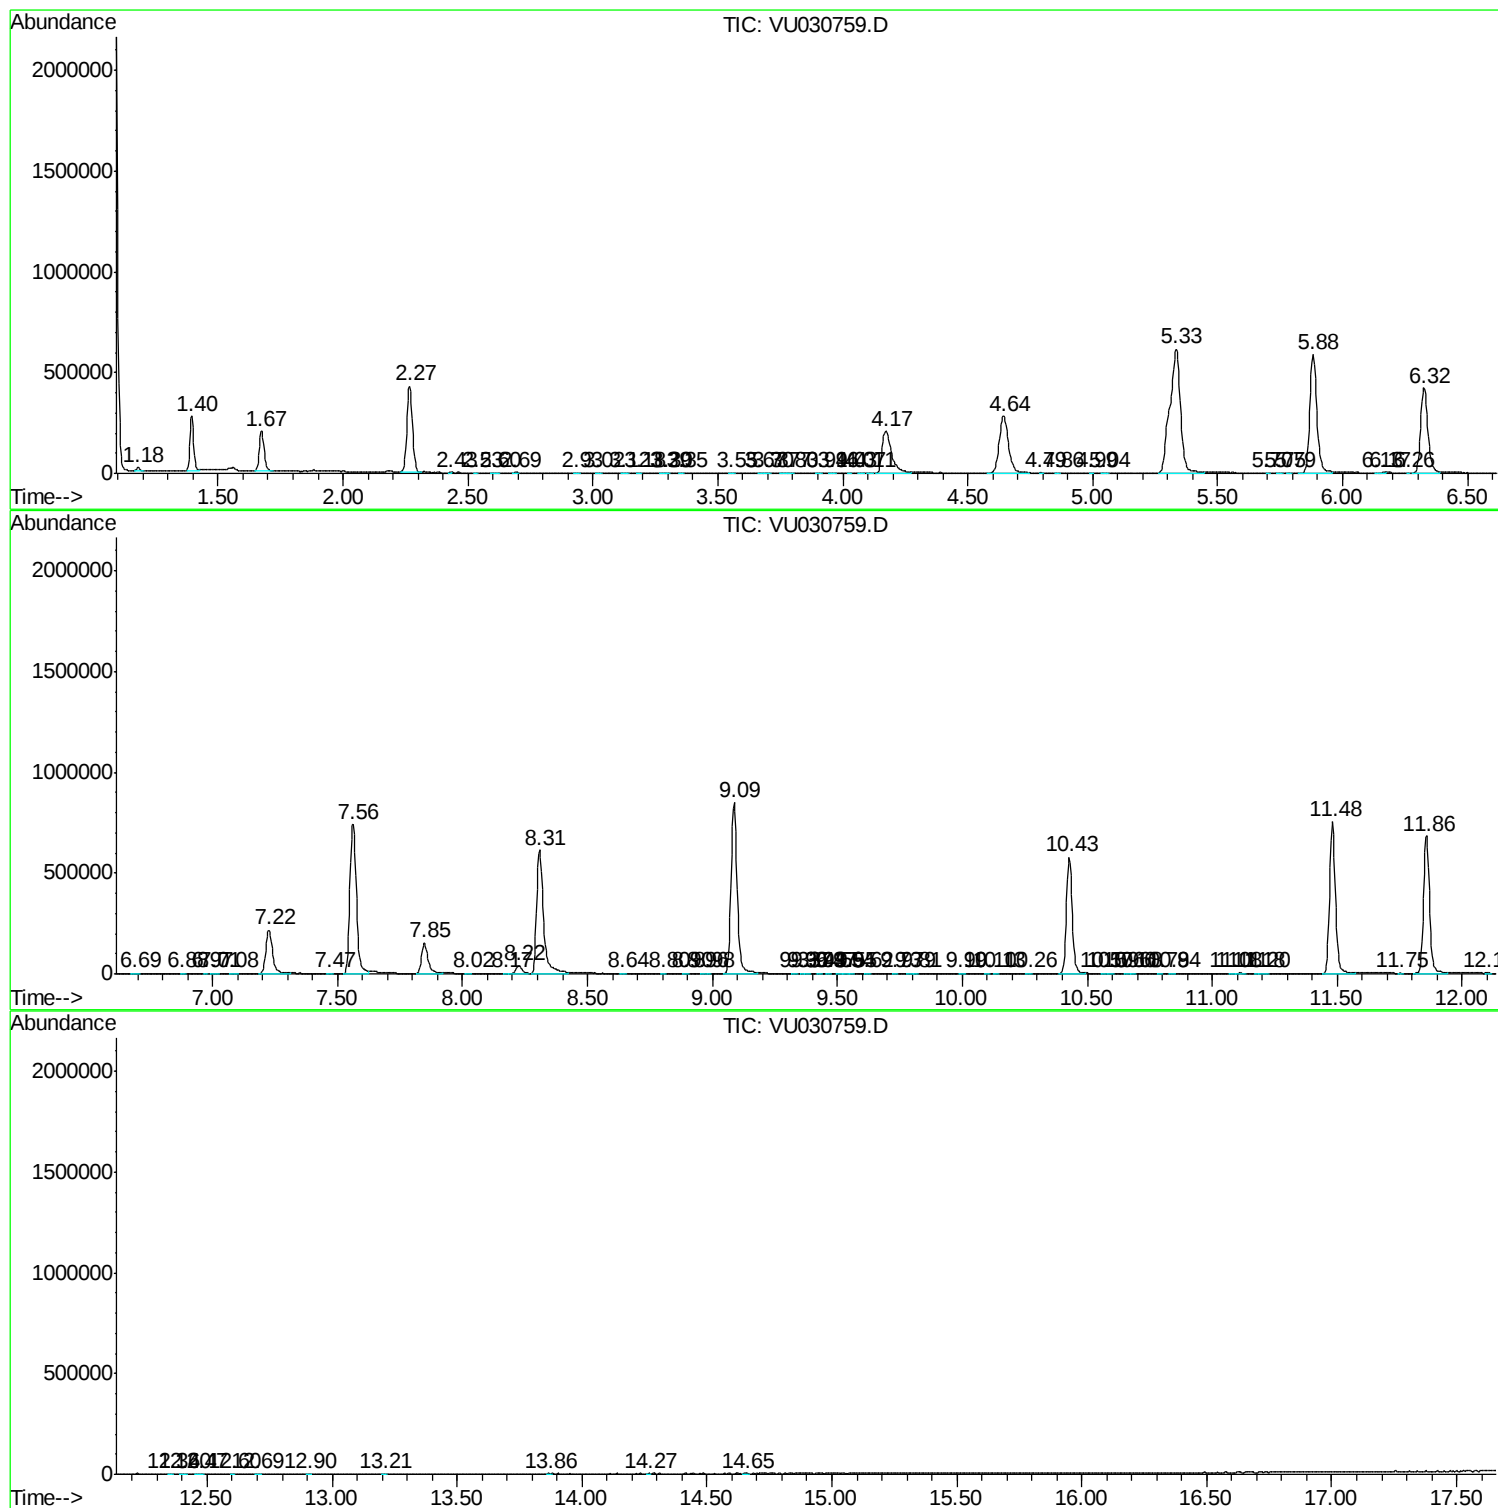

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU040619\
Data File : VU030759.D
Acq On : 05 Apr 2019 22:23
Operator : JC/SP
Sample : K2215-06ME 40X
Misc : 5.33g/5mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF2M7ME

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU040619\
Data File : VU030759.D
Acq On : 05 Apr 2019 22:23
Operator : JC/SP
Sample : K2215-06ME 40X
Misc : 5.33g/5mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF2M7ME

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc