

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU040619\
 Data File : VU030776.D
 Acq On : 06 Apr 2019 05:15
 Operator : JC/SP
 Sample : K2249-11DL 5X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E3YE5DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.180	23	28	34	rVB	14887	14283	0.73%	0.081%
2	1.396	88	95	105	rBV	326138	332116	17.09%	1.884%
3	1.675	174	182	195	rBV	234224	295790	15.22%	1.678%
4	2.270	355	367	391	rVB4	631990	1126915	57.98%	6.392%
5	2.440	412	420	432	rBV2	7447	13634	0.70%	0.077%
6	2.543	450	452	458	rVB5	1394	883	0.05%	0.005%
7	2.592	463	467	469	rBV3	650	487	0.03%	0.003%
8	2.653	482	486	490	rBV4	1385	1110	0.06%	0.006%
9	2.698	493	500	507	rVB6	3349	4892	0.25%	0.028%
10	2.788	521	528	531	rBV4	739	892	0.05%	0.005%
11	2.981	579	588	601	rVB3	9052	16963	0.87%	0.096%
12	3.112	625	629	632	rBV	582	522	0.03%	0.003%
13	3.154	638	642	648	rVB4	653	797	0.04%	0.005%
14	3.219	656	662	664	rBV2	558	460	0.02%	0.003%
15	3.366	706	708	712	rBV2	626	435	0.02%	0.002%
16	3.440	712	731	755	rBV	213435	476685	24.53%	2.704%
17	3.608	780	783	788	rVB2	894	645	0.03%	0.004%
18	3.640	788	793	794	rBV2	864	691	0.04%	0.004%
19	3.688	804	808	813	rBV3	727	902	0.05%	0.005%
20	3.945	884	888	892	rVB2	557	471	0.02%	0.003%
21	4.174	946	959	966	rBV	204058	474660	24.42%	2.692%
22	4.424	1035	1037	1039	rBV2	1150	500	0.03%	0.003%
23	4.453	1043	1046	1049	rBV4	1074	630	0.03%	0.004%
24	4.501	1058	1061	1065	rBV4	987	702	0.04%	0.004%
25	4.643	1088	1105	1136	rBV	304033	764386	39.33%	4.336%
26	4.910	1170	1188	1211	rBV2	657516	1604472	82.56%	9.101%
27	5.125	1251	1255	1259	rBV6	1115	1330	0.07%	0.008%
28	5.334	1297	1320	1342	rBV2	653201	1943477	100.00%	11.024%
29	5.604	1401	1404	1406	rVB2	1078	480	0.02%	0.003%
30	5.755	1449	1451	1454	rVB2	899	520	0.03%	0.003%
31	5.778	1454	1458	1462	rBV3	941	818	0.04%	0.005%
32	5.881	1476	1490	1515	rBV	567223	1132992	58.30%	6.427%
33	6.183	1572	1584	1605	rBV2	133511	270847	13.94%	1.536%
34	6.325	1613	1628	1653	rBV	433681	892767	45.94%	5.064%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU040619\
 Data File : VU030776.D
 Acq On : 06 Apr 2019 05:15
 Operator : JC/SP
 Sample : K2249-11DL 5X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E3YE5DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Title : VOC Analysis

35	6.794	1770	1774	1777	rBV3	736	534	0.03%	0.003%
36	6.855	1788	1793	1796	rVB3	637	700	0.04%	0.004%
37	6.894	1796	1805	1809	rBV5	811	1254	0.06%	0.007%
38	6.968	1825	1828	1832	rBV3	616	545	0.03%	0.003%
39	7.058	1852	1856	1862	rVB4	971	941	0.05%	0.005%
40	7.087	1862	1865	1868	rBV2	670	549	0.03%	0.003%
41	7.225	1894	1908	1932	rBV	223978	420798	21.65%	2.387%
42	7.440	1973	1975	1978	rVB2	1153	645	0.03%	0.004%
43	7.460	1978	1981	1983	rBV3	1573	1226	0.06%	0.007%
44	7.562	1999	2013	2033	rBV	810842	1444192	74.31%	8.192%
45	7.775	2075	2079	2081	rBV2	677	557	0.03%	0.003%
46	7.849	2087	2102	2124	rBV	153255	288007	14.82%	1.634%
47	7.987	2143	2145	2148	rVB3	889	518	0.03%	0.003%
48	8.067	2164	2170	2185	rVB10	4933	9308	0.48%	0.053%
49	8.173	2194	2203	2207	rBV5	3149	4771	0.25%	0.027%
50	8.225	2207	2219	2233	rVV2	166378	291389	14.99%	1.653%
51	8.308	2235	2245	2288	rVV	592677	1126950	57.99%	6.392%
52	8.656	2349	2353	2354	rBV2	558	446	0.02%	0.003%
53	8.681	2358	2361	2363	rVB2	821	487	0.03%	0.003%
54	8.778	2386	2391	2395	rBV3	983	935	0.05%	0.005%
55	8.919	2428	2435	2438	rBV4	977	1094	0.06%	0.006%
56	9.041	2469	2473	2475	rBV3	1455	1012	0.05%	0.006%
57	9.087	2475	2487	2513	rBV	810241	1393215	71.69%	7.903%
58	9.373	2574	2576	2580	rBV3	831	579	0.03%	0.003%
59	9.447	2597	2599	2602	rVV3	625	552	0.03%	0.003%
60	9.459	2602	2603	2610	rVB2	1267	763	0.04%	0.004%
61	9.511	2615	2619	2626	rBV3	532	562	0.03%	0.003%
62	9.662	2662	2666	2670	rVB3	709	628	0.03%	0.004%
63	9.720	2680	2684	2686	rBV3	770	709	0.04%	0.004%
64	9.746	2689	2692	2695	rVV2	548	439	0.02%	0.002%
65	9.829	2712	2718	2722	rVB3	1168	1097	0.06%	0.006%
66	9.894	2732	2738	2741	rBV	620	697	0.04%	0.004%
67	10.106	2801	2804	2808	rBV2	562	509	0.03%	0.003%
68	10.427	2889	2904	2925	rBV	566526	928236	47.76%	5.265%
69	10.575	2946	2950	2952	rBV2	726	554	0.03%	0.003%
70	10.723	2992	2996	2999	rBV3	768	590	0.03%	0.003%
71	10.787	3013	3016	3020	rBV4	1193	1046	0.05%	0.006%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU040619\
 Data File : VU030776.D
 Acq On : 06 Apr 2019 05:15
 Operator : JC/SP
 Sample : K2249-11DL 5X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E3YE5DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Title : VOC Analysis

72	10.855	3033	3037	3043	rVV3	978	1091	0.06%	0.006%
73	10.932	3057	3061	3065	rBV2	564	536	0.03%	0.003%
74	10.964	3066	3071	3072	rBV2	572	504	0.03%	0.003%
75	11.115	3115	3118	3120	rBV2	875	653	0.03%	0.004%
76	11.157	3128	3131	3132	rBV2	742	441	0.02%	0.003%
77	11.299	3170	3175	3179	rBV3	797	911	0.05%	0.005%
78	11.405	3203	3208	3209	rBV2	760	619	0.03%	0.004%
79	11.479	3218	3231	3252	rBV	700621	1156458	59.50%	6.560%
80	11.855	3336	3348	3371	rBV	679411	1144849	58.91%	6.494%
81	12.308	3486	3489	3492	rBV3	1136	672	0.03%	0.004%
82	12.353	3500	3503	3506	rVB5	1074	644	0.03%	0.004%
83	12.620	3584	3586	3589	rVB3	908	494	0.03%	0.003%
84	12.691	3605	3608	3611	rBV2	677	588	0.03%	0.003%
85	12.916	3676	3678	3682	rBV2	596	445	0.02%	0.003%
86	12.961	3690	3692	3698	rBV4	869	760	0.04%	0.004%
87	13.250	3777	3782	3784	rBV2	797	677	0.03%	0.004%
88	13.649	3904	3906	3908	rBV	848	511	0.03%	0.003%
89	13.688	3915	3918	3921	rBV2	1047	716	0.04%	0.004%
90	13.938	3992	3996	3997	rBV2	3079	1872	0.10%	0.011%
91	13.977	4005	4008	4009	rBV2	2046	1198	0.06%	0.007%
92	14.045	4025	4029	4034	rBV2	2952	2991	0.15%	0.017%
93	14.070	4035	4037	4039	rVB	1230	497	0.03%	0.003%
94	14.131	4053	4056	4062	rVB3	1305	1212	0.06%	0.007%
95	14.189	4070	4074	4080	rBV2	1034	1291	0.07%	0.007%
96	14.508	4170	4173	4177	rVB2	1333	870	0.04%	0.005%
97	14.874	4285	4287	4289	rBV	882	463	0.02%	0.003%
98	14.942	4306	4308	4310	rBV3	1216	631	0.03%	0.004%
99	15.035	4334	4337	4339	rBV3	1228	756	0.04%	0.004%
100	15.356	4434	4437	4440	rBV4	1383	1073	0.06%	0.006%


Sum of corrected areas: 17629611

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU040619\
Data File : VU030776.D
Acq On : 06 Apr 2019 05:15
Operator : JC/SP
Sample : K2249-11DL 5X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E3YE5DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

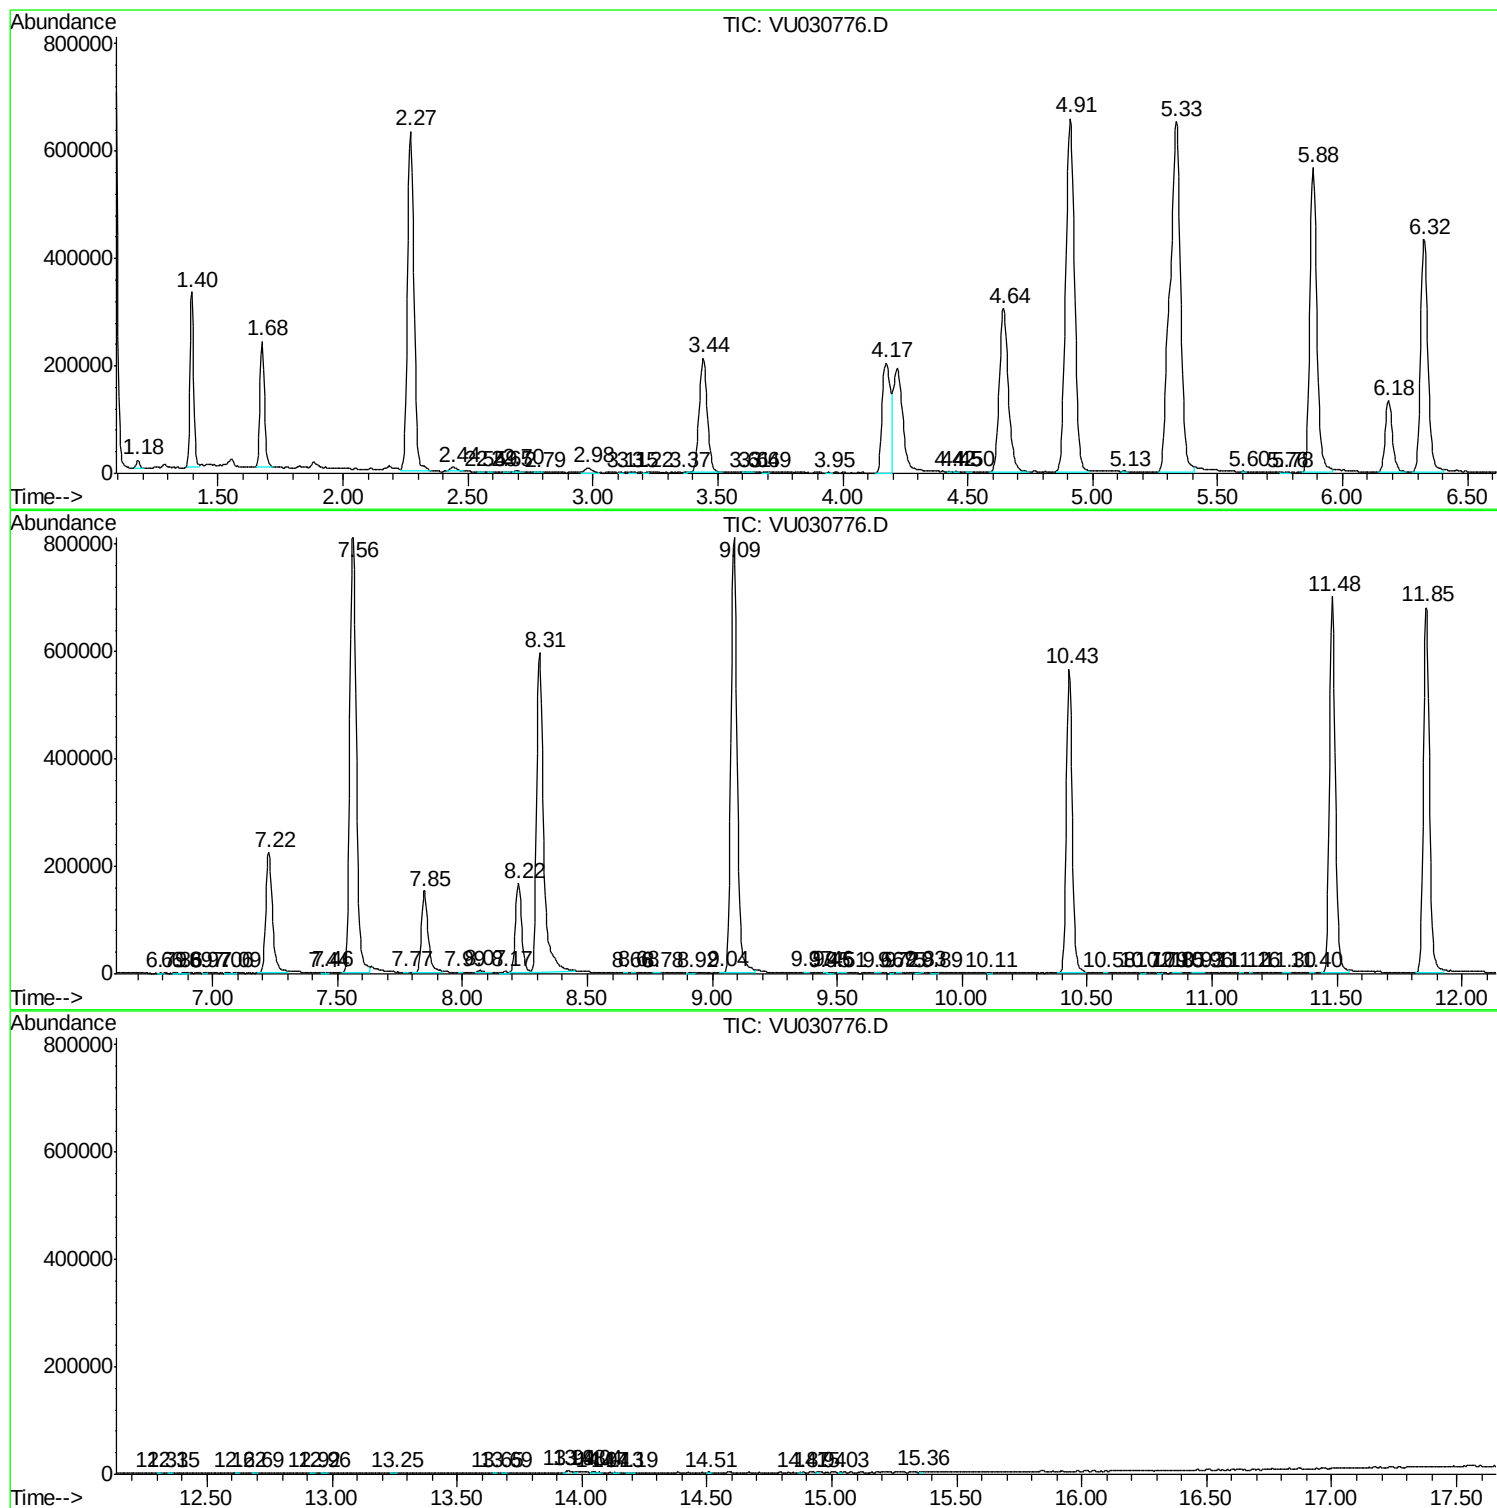

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU040619\
Data File : VU030776.D
Acq On : 06 Apr 2019 05:15
Operator : JC/SP
Sample : K2249-11DL 5X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E3YE5DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU040619\
Data File : VU030776.D
Acq On : 06 Apr 2019 05:15
Operator : JC/SP
Sample : K2249-11DL 5X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E3YE5DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc