

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU040619\
 Data File : VU030780.D
 Acq On : 06 Apr 2019 06:47
 Operator : JC/SP
 Sample : K2249-06DL 20X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E3YD5DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.180	23	28	33	rBV2	14491	13737	0.66%	0.083%
2	1.395	87	95	106	rBV2	539196	604964	29.22%	3.660%
3	1.675	174	182	201	rVB	235367	331890	16.03%	2.008%
4	1.881	240	246	254	rBV3	8142	11900	0.57%	0.072%
5	2.267	355	366	380	rBV	513511	783965	37.86%	4.743%
6	2.694	490	499	500	rBV6	2000	2331	0.11%	0.014%
7	2.817	532	537	544	rBV6	1093	1924	0.09%	0.012%
8	2.881	553	557	559	rBV2	723	476	0.02%	0.003%
9	2.900	559	563	566	rVV2	758	689	0.03%	0.004%
10	2.939	570	575	576	rBV2	615	542	0.03%	0.003%
11	2.981	576	588	605	rVB	17469	32129	1.55%	0.194%
12	3.170	642	647	653	rBV4	650	793	0.04%	0.005%
13	3.257	669	674	678	rBV3	763	866	0.04%	0.005%
14	3.315	689	692	695	rVB3	662	524	0.03%	0.003%
15	3.366	705	708	711	rBV	836	521	0.03%	0.003%
16	3.440	714	731	753	rBV2	339491	763210	36.86%	4.618%
17	3.601	779	781	788	rVB4	779	718	0.03%	0.004%
18	3.672	799	803	808	rBV5	1065	1141	0.06%	0.007%
19	3.698	808	811	818	rVV4	774	721	0.03%	0.004%
20	3.730	818	821	824	rBV5	674	472	0.02%	0.003%
21	3.887	865	870	875	rVB3	611	742	0.04%	0.004%
22	3.919	875	880	882	rBV4	1133	983	0.05%	0.006%
23	3.997	898	904	907	rBV3	517	470	0.02%	0.003%
24	4.173	944	959	963	rBV	211935	410583	19.83%	2.484%
25	4.643	1089	1105	1132	rBV	310502	784039	37.87%	4.744%
26	4.910	1170	1188	1205	rBV3	105873	257179	12.42%	1.556%
27	5.186	1271	1274	1277	rVB4	751	552	0.03%	0.003%
28	5.334	1297	1320	1358	rBV2	699143	2070555	100.00%	12.527%
29	5.736	1441	1445	1446	rBV2	850	467	0.02%	0.003%
30	5.755	1448	1451	1456	rVB5	924	600	0.03%	0.004%
31	5.791	1460	1462	1465	rVB3	1318	713	0.03%	0.004%
32	5.816	1465	1470	1472	rBV5	1064	969	0.05%	0.006%
33	5.881	1477	1490	1515	rBV	563675	1145476	55.32%	6.930%
34	6.103	1557	1559	1561	rBV3	1063	587	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU040619\
 Data File : VU030780.D
 Acq On : 06 Apr 2019 06:47
 Operator : JC/SP
 Sample : K2249-06DL 20X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E3YD5DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Title : VOC Analysis

35	6.189	1574	1586	1599	rBV7	12665	27411	1.32%	0.166%
36	6.324	1613	1628	1652	rBV	452170	926463	44.74%	5.605%
37	6.630	1721	1723	1727	rVB4	1131	705	0.03%	0.004%
38	6.939	1814	1819	1823	rBV3	839	713	0.03%	0.004%
39	6.961	1823	1826	1834	rVB6	968	937	0.05%	0.006%
40	7.225	1894	1908	1931	rBV	237830	440927	21.30%	2.668%
41	7.469	1980	1984	1991	rVB6	1311	1465	0.07%	0.009%
42	7.562	1999	2013	2032	rBV	872956	1542500	74.50%	9.333%
43	7.849	2091	2102	2125	rBV	163151	293958	14.20%	1.779%
44	8.090	2174	2177	2180	rVB2	840	458	0.02%	0.003%
45	8.125	2183	2188	2190	rVB2	681	619	0.03%	0.004%
46	8.144	2190	2194	2198	rBV4	916	870	0.04%	0.005%
47	8.170	2198	2202	2210	rVB6	1229	1571	0.08%	0.010%
48	8.225	2210	2219	2231	rVB5	11022	19446	0.94%	0.118%
49	8.308	2234	2245	2277	rBV	609985	1162322	56.14%	7.032%
50	8.611	2336	2339	2343	rVB3	959	725	0.04%	0.004%
51	8.662	2353	2355	2359	rVB4	1130	586	0.03%	0.004%
52	8.710	2367	2370	2374	rBV4	927	774	0.04%	0.005%
53	8.730	2374	2376	2382	rVB5	877	885	0.04%	0.005%
54	8.820	2398	2404	2408	rBV4	1367	1098	0.05%	0.007%
55	8.926	2434	2437	2443	rBV5	688	645	0.03%	0.004%
56	9.022	2462	2467	2470	rBV2	1077	908	0.04%	0.005%
57	9.086	2470	2487	2521	rBV	840117	1443868	69.73%	8.736%
58	9.382	2576	2579	2585	rVB6	1035	1033	0.05%	0.006%
59	9.411	2585	2588	2591	rVB2	575	429	0.02%	0.003%
60	9.440	2591	2597	2600	rBV4	1106	1071	0.05%	0.006%
61	9.684	2668	2673	2676	rBV5	861	841	0.04%	0.005%
62	10.003	2766	2772	2773	rBV3	559	471	0.02%	0.003%
63	10.045	2778	2785	2791	rVB3	610	806	0.04%	0.005%
64	10.077	2791	2795	2799	rBV3	661	649	0.03%	0.004%
65	10.102	2799	2803	2807	rVB3	673	524	0.03%	0.003%
66	10.241	2843	2846	2849	rBV3	893	586	0.03%	0.004%
67	10.299	2854	2864	2867	rBV2	906	1267	0.06%	0.008%
68	10.427	2891	2904	2926	rBV	589339	962223	46.47%	5.822%
69	10.520	2930	2933	2936	rVB3	956	650	0.03%	0.004%
70	10.768	3008	3010	3018	rVB3	827	837	0.04%	0.005%
71	10.900	3045	3051	3054	rBV3	640	598	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU040619\
 Data File : VU030780.D
 Acq On : 06 Apr 2019 06:47
 Operator : JC/SP
 Sample : K2249-06DL 20X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E3YD5DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Title : VOC Analysis

72	10.987	3075	3078	3083	rVB3	770	501	0.02%	0.003%
73	11.016	3083	3087	3090	rBV	596	458	0.02%	0.003%
74	11.135	3120	3124	3125	rBV2	1099	858	0.04%	0.005%
75	11.479	3220	3231	3253	rBV	724464	1204466	58.17%	7.287%
76	11.790	3325	3328	3333	rVB5	1224	1104	0.05%	0.007%
77	11.855	3336	3348	3372	rBV	724930	1235223	59.66%	7.473%
78	12.308	3486	3489	3491	rVB2	926	558	0.03%	0.003%
79	12.446	3529	3532	3535	rVB3	622	481	0.02%	0.003%
80	12.495	3544	3547	3551	rVB3	891	742	0.04%	0.004%
81	12.565	3566	3569	3571	rBV3	966	559	0.03%	0.003%
82	12.594	3575	3578	3584	rBV4	500	591	0.03%	0.004%
83	12.659	3595	3598	3604	rVB4	1212	1028	0.05%	0.006%
84	12.691	3604	3608	3611	rBV	949	690	0.03%	0.004%
85	12.842	3648	3655	3659	rBV5	836	962	0.05%	0.006%
86	13.006	3700	3706	3708	rBV2	705	726	0.04%	0.004%
87	13.186	3758	3762	3764	rBV	784	607	0.03%	0.004%
88	13.231	3771	3776	3779	rBV3	778	832	0.04%	0.005%
89	13.279	3789	3791	3796	rVB2	1025	528	0.03%	0.003%
90	13.597	3888	3890	3896	rVB2	815	533	0.03%	0.003%
91	13.633	3899	3901	3904	rVV4	836	460	0.02%	0.003%
92	13.710	3922	3925	3927	rBV2	906	625	0.03%	0.004%
93	13.745	3933	3936	3940	rVB2	918	721	0.03%	0.004%
94	13.890	3978	3981	3988	rVB4	1236	1139	0.06%	0.007%
95	13.967	4002	4005	4012	rBV5	1092	1033	0.05%	0.006%
96	14.250	4090	4093	4094	rBV	743	441	0.02%	0.003%
97	14.340	4118	4121	4123	rBV	840	583	0.03%	0.004%
98	14.578	4192	4195	4198	rBV	1202	847	0.04%	0.005%
99	14.900	4293	4295	4298	rBV3	900	658	0.03%	0.004%
100	15.922	4610	4613	4614	rBV2	1633	999	0.05%	0.006%


Sum of corrected areas: 16528220

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU040619\
Data File : VU030780.D
Acq On : 06 Apr 2019 06:47
Operator : JC/SP
Sample : K2249-06DL 20X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E3YD5DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

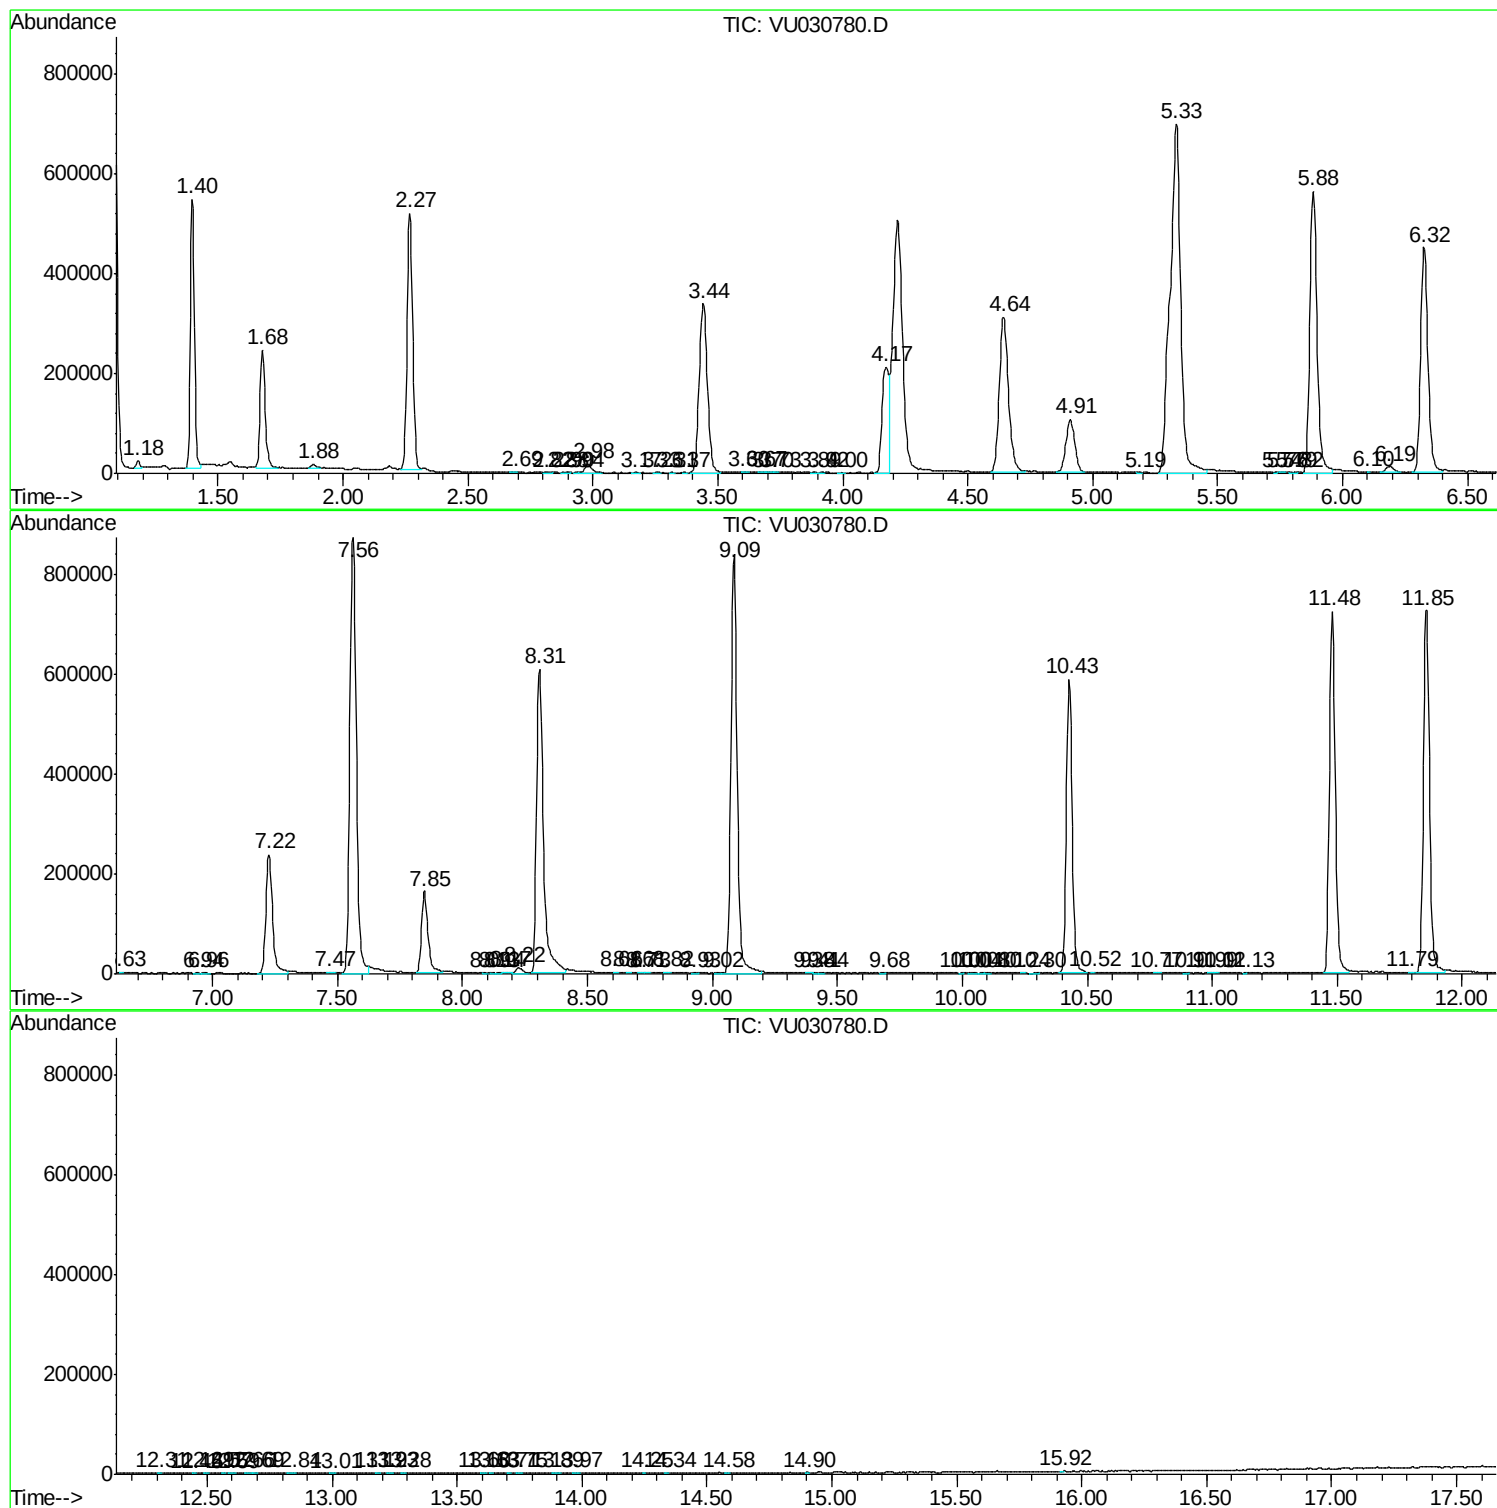

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU040619\
Data File : VU030780.D
Acq On : 06 Apr 2019 06:47
Operator : JC/SP
Sample : K2249-06DL 20X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E3YD5DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU040619\
Data File : VU030780.D
Acq On : 06 Apr 2019 06:47
Operator : JC/SP
Sample : K2249-06DL 20X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E3YD5DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc