


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU040619\
 Data File : VU030745.D
 Acq On : 05 Apr 2019 16:55
 Operator : JC/SP
 Sample : BFB51
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB51

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Title : VOC Analysis
 Last Update : Mon Apr 08 12:41:05 2019

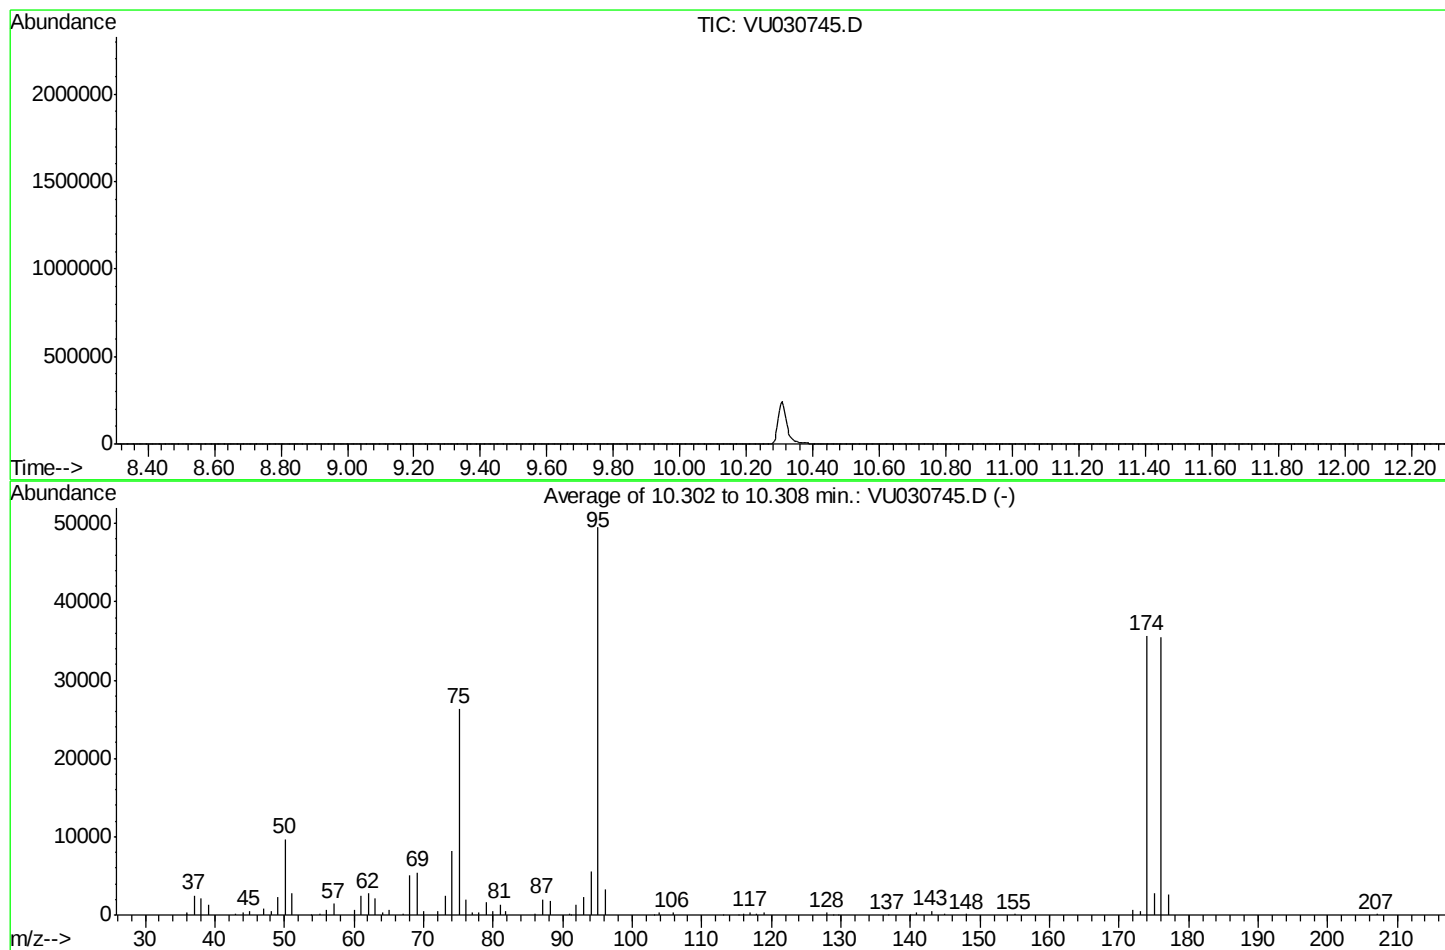

AutoFind: Scans 2865, 2866, 2867; Background Corrected with Scan 2854

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.5	9651	PASS
75	95	30	80	53.2	26357	PASS
95	95	100	100	100.0	49520	PASS
96	95	5	9	6.6	3271	PASS
173	174	0.00	2	1.5	531	PASS
174	95	50	120	72.1	35725	PASS
175	174	5	9	7.8	2794	PASS
176	174	95	101	99.4	35525	PASS
177	176	5	9	7.2	2546	PASS

Scan 2854 (10.266 min): VU030745.D
BFB51

m/z	Abundance
39.80	540.0
44.00	795.0

Instrument :
MSVOA_U
ClientSampleId :
BFB51

m/z	Abundance
35.90	420.0
37.10	2504.0
38.10	2332.0
39.00	1174.0
39.90	502.0
42.90	147.0
44.00	1130.0
44.90	439.0
47.00	792.0
48.00	471.0
49.00	2204.0
50.10	9316.0
51.00	2857.0
55.10	165.0
56.00	660.0
57.10	1355.0
60.10	653.0
61.00	2389.0
62.10	2561.0
63.10	2054.0
64.00	296.0
65.00	500.0
67.10	245.0
68.00	4647.0
69.10	5051.0
69.90	514.0
71.90	492.0
73.10	2377.0
74.10	7871.0
75.10	25544.0
76.20	2008.0
77.00	272.0
78.00	270.0
78.90	1623.0
80.00	417.0
81.00	1368.0
81.80	360.0
87.00	1966.0
88.10	1792.0
90.90	130.0
92.00	1290.0
93.00	2155.0
94.10	5430.0
95.10	48008.0
96.10	3018.0
104.00	247.0
105.90	227.0
113.00	141.0
115.20	103.0
115.90	132.0
117.00	286.0
117.90	173.0
118.80	333.0
128.00	305.0
128.80	105.0
136.80	126.0
141.00	343.0
143.00	542.0
145.00	125.0
148.10	113.0
155.00	233.0
172.00	542.0
174.00	33616.0
175.00	2816.0
176.00	33136.0
177.00	2419.0
207.10	177.0

Instrument :
MSVOA_U
ClientSampleId :
BFB51

m/z	Abundance
36.10	424.0
37.00	2400.0
38.10	2217.0
39.00	1307.0
39.90	469.0
42.90	118.0
44.00	1128.0
45.00	525.0
47.00	767.0
48.10	450.0
49.00	2308.0
50.10	9999.0
51.00	2841.0
53.90	105.0
55.10	176.0
56.10	693.0
57.00	1458.0
60.10	671.0
61.00	2485.0
62.10	2909.0
63.10	2169.0
64.10	308.0
65.00	686.0
67.00	213.0
68.00	5397.0
69.10	5586.0
69.90	432.0
71.90	435.0
73.10	2540.0
74.10	8318.0
75.10	27064.0
76.20	2009.0
77.00	281.0
77.90	359.0
79.00	1639.0
80.00	472.0
81.00	1431.0
81.80	428.0
86.10	127.0
87.10	2055.0
88.20	1874.0
90.90	172.0
92.00	1457.0
93.00	2288.0
94.10	5733.0
95.10	51000.0
96.10	3322.0
103.10	104.0
104.00	290.0
105.90	295.0
115.20	111.0
116.00	137.0
117.00	361.0
117.90	185.0
118.90	307.0
128.00	278.0
128.90	104.0
140.90	352.0
143.00	539.0
144.90	183.0
148.10	174.0
155.00	144.0
172.00	557.0
173.10	780.0
174.00	36696.0
175.00	2813.0
176.00	36768.0
177.00	2588.0
207.00	133.0

Instrument :
MSVOA_U
ClientSampleId :
BFB51

m/z	Abundance
36.00	417.0
37.00	2474.0
38.00	1975.0
39.10	1391.0
39.90	405.0
44.10	1083.0
45.00	571.0
46.90	719.0
48.10	347.0
49.10	2164.0
50.10	9640.0
51.10	2668.0
53.90	112.0
55.00	189.0
56.10	743.0
57.00	1424.0
60.10	624.0
61.00	2501.0
62.10	2778.0
63.10	2061.0
64.10	318.0
65.00	720.0
67.00	176.0
68.00	5410.0
69.10	5780.0
70.00	366.0
72.00	377.0
73.10	2426.0
74.10	8457.0
75.10	26464.0
76.10	1970.0
76.90	285.0
77.90	397.0
79.00	1623.0
79.90	503.0
81.00	1338.0
81.90	457.0
86.10	181.0
87.10	2039.0
88.10	1648.0
91.10	140.0
92.00	1361.0
93.10	2311.0
94.10	5716.0
95.10	49552.0
96.00	3474.0
103.90	225.0
105.90	282.0
115.90	178.0
117.00	364.0
117.90	189.0
119.00	310.0
128.10	233.0
129.70	101.0
139.90	143.0
140.90	432.0
143.00	527.0
144.90	257.0
148.10	166.0
172.00	646.0
173.10	814.0
174.00	36864.0
175.10	2753.0
176.00	36672.0
177.10	2631.0
207.00	127.0

Instrument :
MSVOA_U
ClientSampleId :
BFB51