

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU040620\
 Data File : VU037590.D
 Acq On : 06 Apr 2020 15:08
 Operator : JC/MD
 Sample : L2158-08 10X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0F05

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040320WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.613	78	85	103	rVB	90364	94983	10.41%	1.514%
2	1.906	169	176	189	rVB	66907	89011	9.76%	1.418%
3	2.584	375	387	404	rVB2	139762	235359	25.81%	3.751%
4	2.706	423	425	426	rBV2	424	183	0.02%	0.003%
5	3.047	528	531	533	rBV	263	176	0.02%	0.003%
6	3.073	534	539	541	rVV2	583	564	0.06%	0.009%
7	3.173	568	570	571	rBV2	220	77	0.01%	0.001%
8	3.279	601	603	607	rVB	157	63	0.01%	0.001%
9	3.436	651	652	656	rBV	229	105	0.01%	0.002%
10	3.571	692	694	696	rBV	209	92	0.01%	0.001%
11	3.642	714	716	721	rVB	153	72	0.01%	0.001%
12	3.735	741	745	747	rVB	364	195	0.02%	0.003%
13	3.848	778	780	786	rVB2	279	177	0.02%	0.003%
14	3.877	786	789	790	rBV	251	109	0.01%	0.002%
15	4.005	827	829	831	rBV	137	54	0.01%	0.001%
16	4.041	838	840	841	rBV	172	52	0.01%	0.001%
17	4.102	856	859	863	rVB	256	152	0.02%	0.002%
18	4.227	895	898	902	rVB2	219	141	0.02%	0.002%
19	4.259	904	908	914	rBV	359	385	0.04%	0.006%
20	4.314	922	925	928	rVV	173	81	0.01%	0.001%
21	4.337	930	932	934	rBV	232	112	0.01%	0.002%
22	4.366	939	941	942	rBV	220	88	0.01%	0.001%
23	4.407	949	954	958	rBV2	359	391	0.04%	0.006%
24	4.427	958	960	961	rBV2	153	70	0.01%	0.001%
25	4.530	990	992	996	rBV	220	124	0.01%	0.002%
26	4.668	1021	1035	1065	rBV2	68078	203683	22.33%	3.246%
27	4.838	1086	1088	1092	rBV	253	137	0.02%	0.002%
28	4.861	1094	1095	1097	rBV	255	82	0.01%	0.001%
29	4.890	1101	1104	1107	rBV	161	104	0.01%	0.002%
30	4.976	1129	1131	1139	rVB2	381	273	0.03%	0.004%
31	5.102	1154	1170	1191	rBV	116570	254753	27.93%	4.060%
32	5.198	1196	1200	1203	rBV2	321	201	0.02%	0.003%
33	5.333	1235	1242	1244	rBV3	596	660	0.07%	0.011%
34	5.420	1265	1269	1271	rBV	323	315	0.03%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU040620\
 Data File : VU037590.D
 Acq On : 06 Apr 2020 15:08
 Operator : JC/MD
 Sample : L2158-08 10X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0F05

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040320WMA.M
 Title : VOC Analysis

35	5.449	1276	1278	1280	rBV	196	97	0.01%	0.002%
36	5.549	1307	1309	1310	rBV	160	63	0.01%	0.001%
37	5.639	1335	1337	1339	rBV	203	83	0.01%	0.001%
38	5.758	1354	1374	1391	rBV2	246568	639402	70.11%	10.189%
39	5.870	1406	1409	1410	rBV	198	87	0.01%	0.001%
40	5.941	1429	1431	1434	rVB	188	64	0.01%	0.001%
41	6.147	1492	1495	1497	rBV	282	138	0.02%	0.002%
42	6.160	1497	1499	1504	rVV	229	156	0.02%	0.002%
43	6.279	1521	1536	1555	rVB	219039	405511	44.46%	6.462%
44	6.420	1578	1580	1585	rBV	195	138	0.02%	0.002%
45	6.504	1603	1606	1608	rBV	199	156	0.02%	0.002%
46	6.571	1612	1627	1646	rVV	497264	912002	100.00%	14.533%
47	6.722	1657	1674	1690	rBV	152751	296577	32.52%	4.726%
48	6.825	1703	1706	1709	rBV2	355	255	0.03%	0.004%
49	6.967	1748	1750	1753	rVB	217	69	0.01%	0.001%
50	6.999	1758	1760	1762	rVV	216	88	0.01%	0.001%
51	7.044	1772	1774	1777	rVB	329	160	0.02%	0.003%
52	7.369	1873	1875	1879	rVB	197	92	0.01%	0.001%
53	7.410	1886	1888	1892	rVB	220	102	0.01%	0.002%
54	7.481	1908	1910	1913	rVB	215	102	0.01%	0.002%
55	7.526	1922	1924	1927	rVB	251	105	0.01%	0.002%
56	7.590	1932	1944	1960	rVB	99328	168562	18.48%	2.686%
57	7.652	1960	1963	1964	rBV	169	70	0.01%	0.001%
58	7.674	1968	1970	1976	rBV	144	73	0.01%	0.001%
59	7.922	2033	2047	2061	rBV	310928	525871	57.66%	8.380%
60	8.121	2106	2109	2111	rBV	186	88	0.01%	0.001%
61	8.201	2122	2134	2146	rBV2	70705	114952	12.60%	1.832%
62	8.295	2161	2163	2165	rBV	177	63	0.01%	0.001%
63	8.574	2240	2250	2260	rVB2	33393	53856	5.91%	0.858%
64	8.655	2263	2275	2303	rBV	235409	400831	43.95%	6.387%
65	8.835	2328	2331	2333	rBV	198	134	0.01%	0.002%
66	8.912	2352	2355	2360	rBV2	220	168	0.02%	0.003%
67	8.979	2375	2376	2379	rBV2	237	113	0.01%	0.002%
68	9.275	2465	2468	2470	rBV	192	101	0.01%	0.002%
69	9.311	2477	2479	2484	rVB	210	110	0.01%	0.002%
70	9.436	2506	2518	2536	rBV	313579	512676	56.21%	8.170%
71	9.571	2557	2560	2561	rBV	325	140	0.02%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU040620\
 Data File : VU037590.D
 Acq On : 06 Apr 2020 15:08
 Operator : JC/MD
 Sample : L2158-08 10X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0F05

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040320WMA.M
 Title : VOC Analysis

72	9.587	2561	2565	2571	rVV3	790	998	0.11%	0.016%
73	9.709	2598	2603	2611	rVB	911	1169	0.13%	0.019%
74	9.848	2643	2646	2652	rVB	306	192	0.02%	0.003%
75	9.918	2666	2668	2671	rBV	161	70	0.01%	0.001%
76	10.111	2723	2728	2729	rBV2	867	673	0.07%	0.011%
77	10.500	2842	2849	2851	rBV2	722	709	0.08%	0.011%
78	10.658	2896	2898	2901	rVB	212	93	0.01%	0.001%
79	10.680	2902	2905	2908	rBV	210	158	0.02%	0.003%
80	10.700	2908	2911	2912	rBV	166	85	0.01%	0.001%
81	10.774	2921	2934	2947	rBV	217651	351444	38.54%	5.600%
82	10.950	2987	2989	2992	rBV2	218	125	0.01%	0.002%
83	11.044	3015	3018	3020	rBV	254	146	0.02%	0.002%
84	11.105	3031	3037	3042	rBV4	725	787	0.09%	0.013%
85	11.195	3063	3065	3068	rVB	234	88	0.01%	0.001%
86	11.291	3091	3095	3096	rBV	279	178	0.02%	0.003%
87	11.475	3148	3152	3161	rVB3	737	946	0.10%	0.015%
88	11.825	3249	3261	3275	rBV	327765	507757	55.67%	8.091%
89	12.079	3336	3340	3342	rVB2	422	265	0.03%	0.004%
90	12.105	3346	3348	3353	rVB	491	323	0.04%	0.005%
91	12.134	3355	3357	3360	rVB	276	116	0.01%	0.002%
92	12.153	3361	3363	3364	rBV	193	68	0.01%	0.001%
93	12.204	3366	3379	3393	rVB	310291	491802	53.93%	7.837%
94	13.057	3642	3644	3647	rBV	215	113	0.01%	0.002%
95	13.860	3891	3894	3896	rBV2	459	277	0.03%	0.004%
96	14.256	4015	4017	4020	rBV	313	168	0.02%	0.003%
97	14.876	4207	4210	4212	rBV	349	248	0.03%	0.004%


Sum of corrected areas: 6275277

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU040620\
Data File : VU037590.D
Acq On : 06 Apr 2020 15:08
Operator : JC/MD
Sample : L2158-08 10X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0F05

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

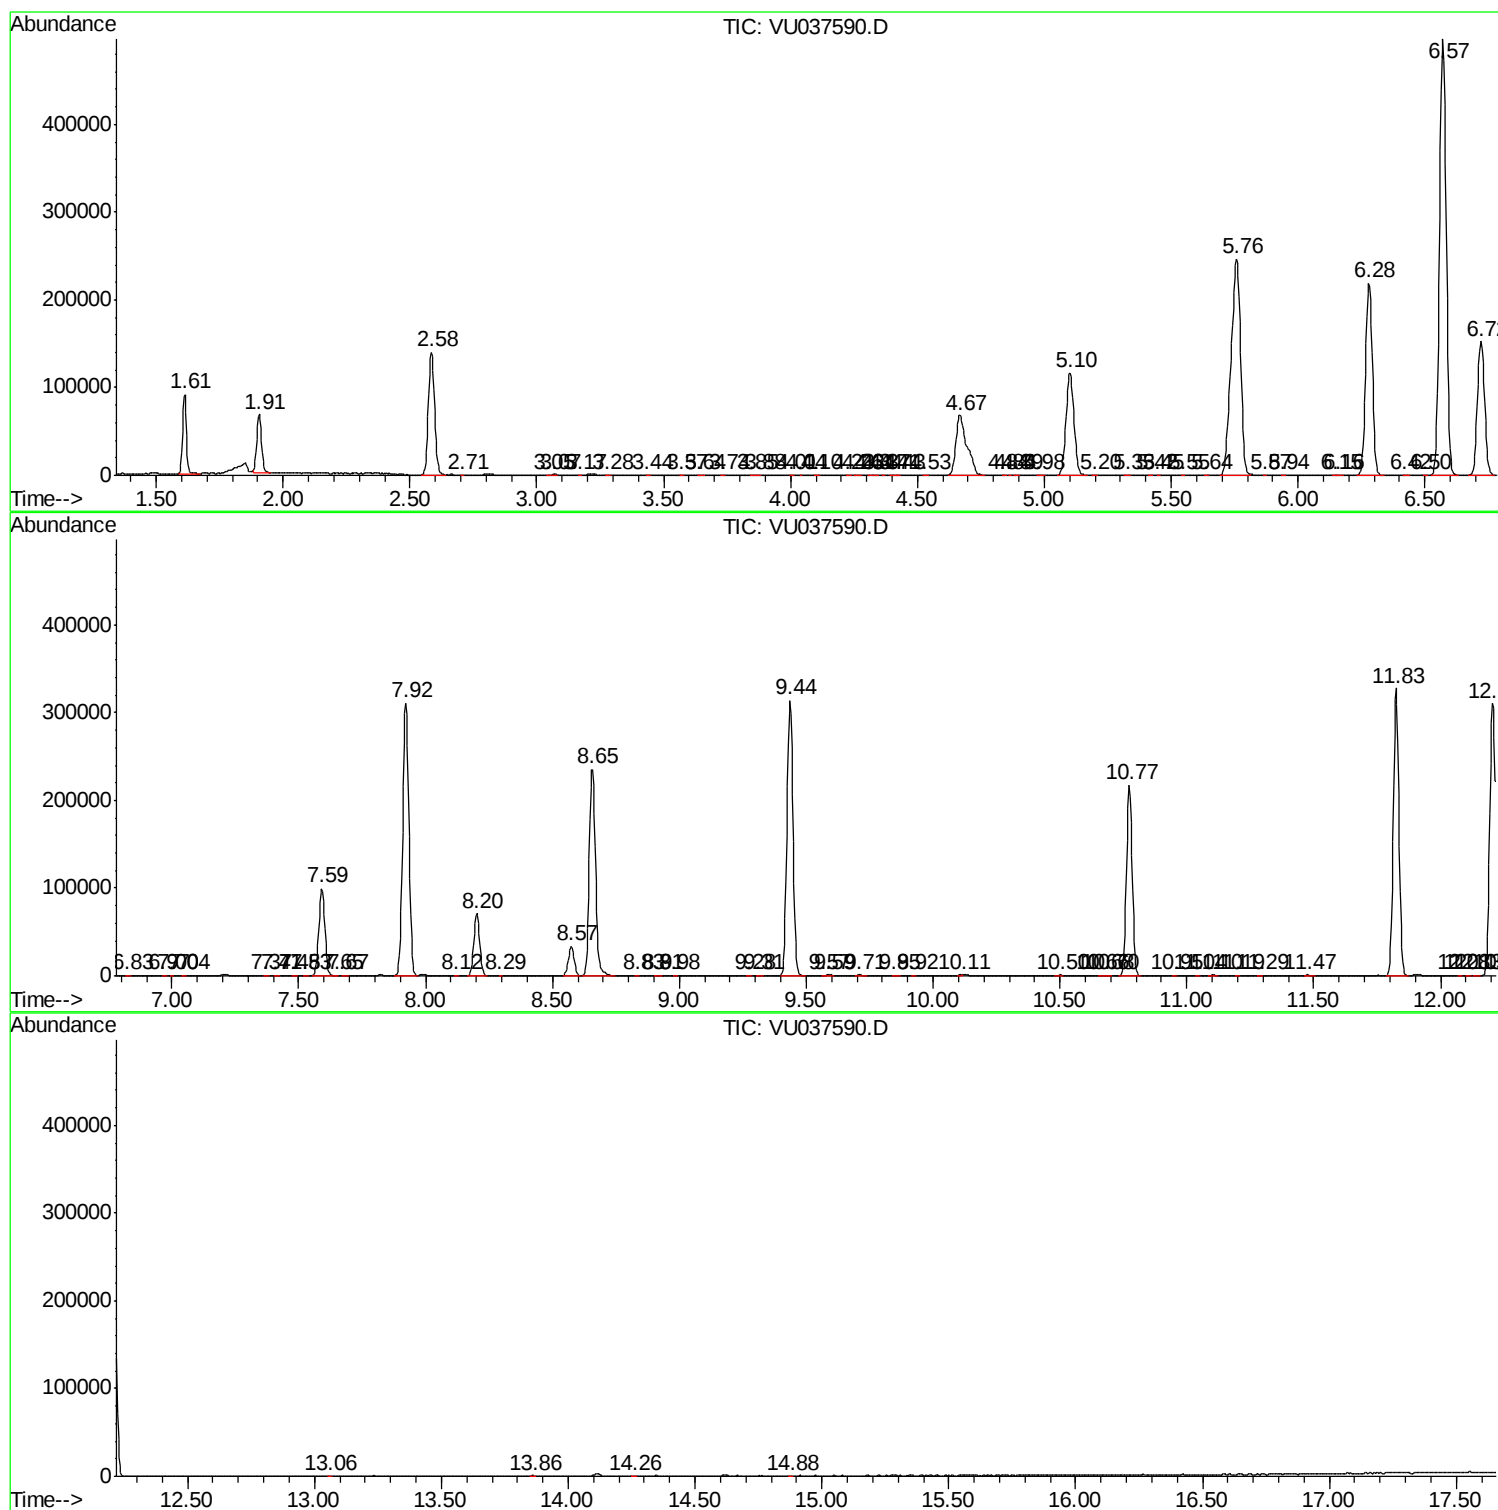

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU040620\
Data File : VU037590.D
Acq On : 06 Apr 2020 15:08
Operator : JC/MD
Sample : L2158-08 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0F05

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU040620\
Data File : VU037590.D
Acq On : 06 Apr 2020 15:08
Operator : JC/MD
Sample : L2158-08 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0F05

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
