

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU040620\
 Data File : VU037594.D
 Acq On : 06 Apr 2020 16:39
 Operator : JC/MD
 Sample : VIBLK40
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK40

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040320WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.613	78	85	96	rVB	86250	93712	14.93%	1.846%
2	1.928	176	183	195	rVB	68830	88452	14.09%	1.743%
3	2.591	377	389	406	rBV	133486	215134	34.27%	4.239%
4	2.954	500	502	504	rBV	264	118	0.02%	0.002%
5	3.044	528	530	534	rBV	368	186	0.03%	0.004%
6	3.063	534	536	539	rBV2	564	287	0.05%	0.006%
7	3.211	575	582	583	rBV	1089	1042	0.17%	0.021%
8	3.366	628	630	632	rVB	211	88	0.01%	0.002%
9	3.501	670	672	676	rBV	334	288	0.05%	0.006%
10	3.632	711	713	716	rVB	248	99	0.02%	0.002%
11	4.041	837	840	843	rVB	201	121	0.02%	0.002%
12	4.105	858	860	864	rVB	167	75	0.01%	0.001%
13	4.227	894	898	900	rVB	190	126	0.02%	0.002%
14	4.346	933	935	938	rBV	146	45	0.01%	0.001%
15	4.481	975	977	978	rBV	107	23	0.00%	0.000%
16	4.668	1020	1035	1062	rBV	71828	168546	26.85%	3.321%
17	4.832	1079	1086	1088	rBV2	236	305	0.05%	0.006%
18	4.861	1092	1095	1100	rBV	304	230	0.04%	0.005%
19	5.105	1153	1171	1190	rVB	111649	245817	39.16%	4.843%
20	5.179	1191	1194	1198	rBV	214	215	0.03%	0.004%
21	5.320	1230	1238	1244	rBV2	497	784	0.12%	0.015%
22	5.468	1283	1284	1285	rBV2	93	19	0.00%	0.000%
23	5.552	1307	1310	1316	rVB	182	130	0.02%	0.003%
24	5.597	1323	1324	1326	rBV	219	67	0.01%	0.001%
25	5.677	1347	1349	1353	rVB	139	41	0.01%	0.001%
26	5.761	1353	1375	1396	rBV3	239264	627764	100.00%	12.369%
27	5.880	1408	1412	1415	rBV	176	111	0.02%	0.002%
28	6.083	1469	1475	1478	rBV3	363	373	0.06%	0.007%
29	6.150	1494	1496	1501	rBV	178	124	0.02%	0.002%
30	6.282	1522	1537	1553	rBV	213856	392497	62.52%	7.733%
31	6.462	1591	1593	1595	rVB	215	83	0.01%	0.002%
32	6.568	1617	1626	1641	rVB8	7260	12869	2.05%	0.254%
33	6.722	1659	1674	1693	rBV	149451	288095	45.89%	5.676%
34	6.951	1744	1745	1748	rVB	228	63	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU040620\
 Data File : VU037594.D
 Acq On : 06 Apr 2020 16:39
 Operator : JC/MD
 Sample : VIBLK40
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK40

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040320WMA.M
 Title : VOC Analysis

35	7.047	1774	1775	1776	rBV	210	67	0.01%	0.001%
36	7.160	1806	1810	1814	rBV	182	184	0.03%	0.004%
37	7.201	1820	1823	1824	rBV	396	228	0.04%	0.004%
38	7.590	1932	1944	1959	rBV	95082	161405	25.71%	3.180%
39	7.703	1976	1979	1981	rBV2	515	335	0.05%	0.007%
40	7.783	2001	2004	2007	rBV	219	132	0.02%	0.003%
41	7.809	2007	2012	2013	rBV	408	258	0.04%	0.005%
42	7.922	2034	2047	2064	rVB	302780	511320	81.45%	10.074%
43	8.137	2112	2114	2116	rVB	270	86	0.01%	0.002%
44	8.201	2122	2134	2147	rBV	67617	110792	17.65%	2.183%
45	8.266	2151	2154	2161	rVB	301	250	0.04%	0.005%
46	8.362	2182	2184	2185	rBV	160	77	0.01%	0.002%
47	8.655	2263	2275	2298	rBV	226410	389784	62.09%	7.680%
48	8.819	2324	2326	2327	rBV	187	68	0.01%	0.001%
49	8.918	2355	2357	2358	rBV	180	49	0.01%	0.001%
50	8.931	2358	2361	2362	rBV	582	359	0.06%	0.007%
51	9.031	2390	2392	2393	rBV	153	67	0.01%	0.001%
52	9.307	2474	2478	2479	rBV2	275	138	0.02%	0.003%
53	9.356	2490	2493	2495	rBV2	170	99	0.02%	0.002%
54	9.436	2505	2518	2537	rBV	303160	486308	77.47%	9.582%
55	9.568	2557	2559	2562	rBV	141	39	0.01%	0.001%
56	9.587	2563	2565	2570	rVB	242	116	0.02%	0.002%
57	9.629	2575	2578	2581	rBV	260	188	0.03%	0.004%
58	9.703	2598	2601	2603	rBV	147	102	0.02%	0.002%
59	9.880	2654	2656	2658	rBV	129	30	0.00%	0.001%
60	9.951	2676	2678	2682	rBV	178	115	0.02%	0.002%
61	10.224	2760	2763	2766	rBV	274	161	0.03%	0.003%
62	10.642	2891	2893	2898	rVB	342	172	0.03%	0.003%
63	10.774	2922	2934	2950	rVB	207238	328076	52.26%	6.464%
64	11.571	3180	3182	3188	rVB	429	240	0.04%	0.005%
65	11.648	3203	3206	3208	rBV	242	133	0.02%	0.003%
66	11.825	3249	3261	3280	rVB	303378	478378	76.20%	9.425%
67	12.069	3334	3337	3341	rBV2	382	270	0.04%	0.005%
68	12.204	3367	3379	3395	rVB	292550	466645	74.33%	9.194%
69	12.330	3416	3418	3422	rBV2	273	145	0.02%	0.003%
70	12.571	3490	3493	3497	rBV	403	273	0.04%	0.005%
71	13.661	3829	3832	3835	rBV	553	288	0.05%	0.006%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU040620\
Data File : VU037594.D
Acq On : 06 Apr 2020 16:39
Operator : JC/MD
Sample : VIBLK40
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK40

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040320WMA.M
Title : VOC Analysis

72	14.188	3993	3996	3997	rBV	314	154	0.02%	0.003%
----	--------	------	------	------	-----	-----	-----	-------	--------


Sum of corrected areas: 5075460

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU040620\
Data File : VU037594.D
Acq On : 06 Apr 2020 16:39
Operator : JC/MD
Sample : VIBLK40
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK40

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

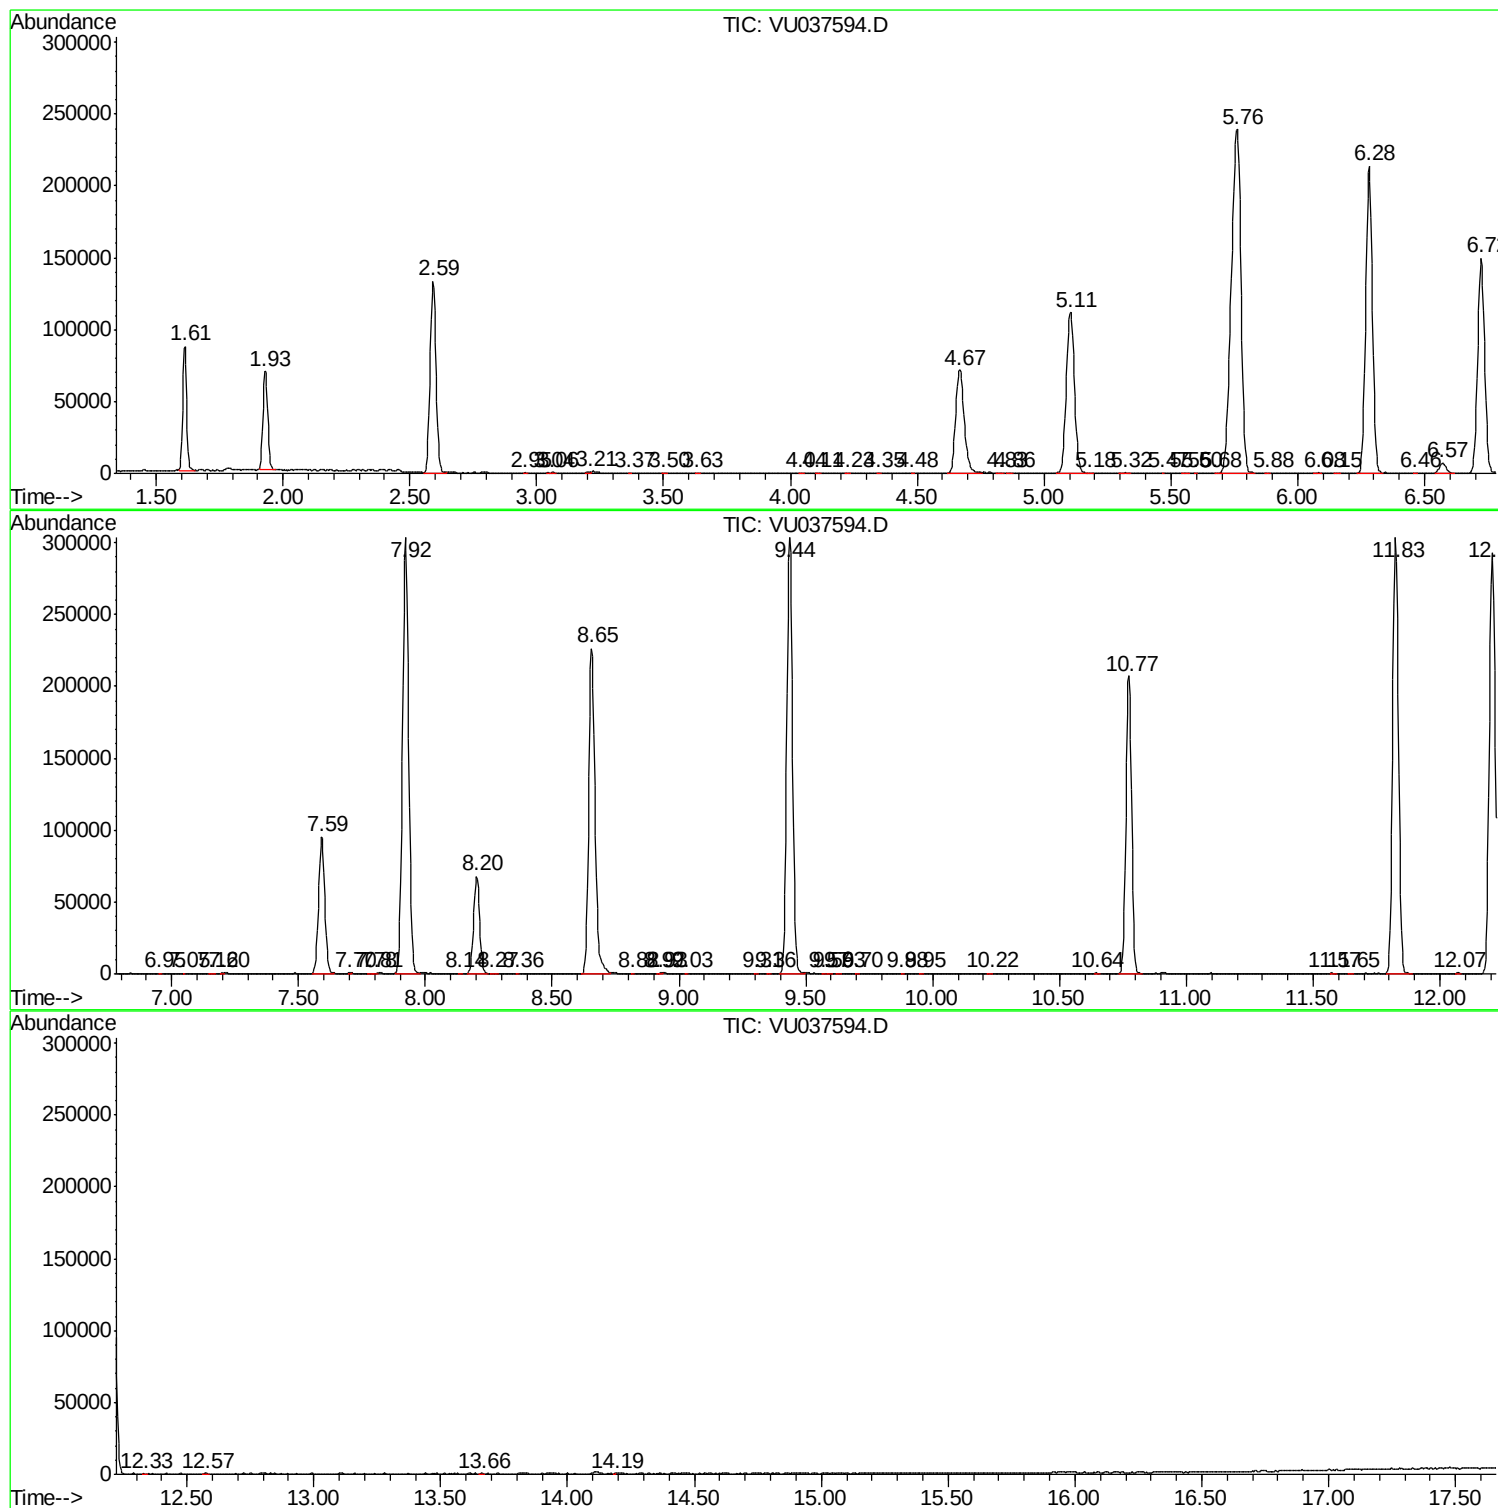

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU040620\
Data File : VU037594.D
Acq On : 06 Apr 2020 16:39
Operator : JC/MD
Sample : VIBLK40
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK40

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU040620\
Data File : VU037594.D
Acq On : 06 Apr 2020 16:39
Operator : JC/MD
Sample : VIBLK40
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK40

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc