

Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU040620\
 Data File : VU037595.D
 Acq On : 06 Apr 2020 17:25
 Operator : JC/MD
 Sample : L2158-11
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040320WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.613	78	85	96	rVB	78714	83937	14.39%	1.738%
2	1.928	176	183	201	rVB	62814	83361	14.29%	1.726%
3	2.591	377	389	406	rBV	120673	196174	33.64%	4.063%
4	2.723	426	430	433	rVB2	328	267	0.05%	0.006%
5	2.880	476	479	483	rVB	294	188	0.03%	0.004%
6	2.938	494	497	499	rBV	219	126	0.02%	0.003%
7	3.073	536	539	542	rVB3	409	242	0.04%	0.005%
8	3.108	548	550	551	rBV3	139	36	0.01%	0.001%
9	3.218	577	584	596	rBV2	1109	2048	0.35%	0.042%
10	3.311	611	613	614	rBV2	199	90	0.02%	0.002%
11	3.353	624	626	627	rBV2	165	53	0.01%	0.001%
12	3.497	668	671	673	rBV	195	100	0.02%	0.002%
13	3.571	691	694	695	rBV	156	95	0.02%	0.002%
14	3.703	733	735	737	rBV	143	62	0.01%	0.001%
15	3.732	743	744	745	rVB	120	23	0.00%	0.000%
16	3.751	748	750	753	rBV	125	60	0.01%	0.001%
17	3.800	763	765	767	rBV	238	135	0.02%	0.003%
18	4.182	882	884	887	rVB	223	85	0.01%	0.002%
19	4.404	950	953	954	rBV	144	82	0.01%	0.002%
20	4.668	1018	1035	1059	rBV	69347	163177	27.98%	3.379%
21	4.838	1085	1088	1091	rVB	164	77	0.01%	0.002%
22	4.867	1095	1097	1100	rVV	167	64	0.01%	0.001%
23	4.896	1103	1106	1109	rBV	254	124	0.02%	0.003%
24	4.935	1116	1118	1123	rVB	159	65	0.01%	0.001%
25	4.996	1134	1137	1142	rVB	316	185	0.03%	0.004%
26	5.022	1142	1145	1146	rBV	148	67	0.01%	0.001%
27	5.102	1155	1170	1191	rVB	106581	231931	39.77%	4.803%
28	5.173	1191	1192	1194	rBV	235	88	0.02%	0.002%
29	5.321	1236	1238	1240	rBV	221	109	0.02%	0.002%
30	5.449	1277	1278	1280	rBV	131	40	0.01%	0.001%
31	5.513	1297	1298	1301	rVB	344	129	0.02%	0.003%
32	5.533	1301	1304	1306	rBV	173	150	0.03%	0.003%
33	5.575	1314	1317	1321	rBV	140	121	0.02%	0.003%
34	5.761	1353	1375	1392	rBV2	224539	583234	100.00%	12.079%

Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU040620\
 Data File : VU037595.D
 Acq On : 06 Apr 2020 17:25
 Operator : JC/MD
 Sample : L2158-11
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040320WMA.M
 Title : VOC Analysis

35	5.883	1411	1413	1416	rVB	135	44	0.01%	0.001%
36	5.928	1424	1427	1434	rVB2	187	175	0.03%	0.004%
37	6.005	1449	1451	1455	rBV	199	104	0.02%	0.002%
38	6.099	1479	1480	1481	rBV	89	20	0.00%	0.000%
39	6.115	1481	1485	1490	rVB	196	144	0.02%	0.003%
40	6.282	1523	1537	1554	rBV	209943	388440	66.60%	8.045%
41	6.443	1584	1587	1589	rBV	231	144	0.02%	0.003%
42	6.533	1612	1615	1617	rVB	135	58	0.01%	0.001%
43	6.568	1617	1626	1631	rBV4	2314	3537	0.61%	0.073%
44	6.671	1656	1658	1659	rBV	208	86	0.01%	0.002%
45	6.722	1660	1674	1692	rVB	141657	267867	45.93%	5.548%
46	6.812	1700	1702	1704	rVB	139	35	0.01%	0.001%
47	6.832	1705	1708	1711	rBV3	302	198	0.03%	0.004%
48	6.893	1723	1727	1730	rBV	246	191	0.03%	0.004%
49	6.944	1741	1743	1744	rBV	173	79	0.01%	0.002%
50	7.079	1783	1785	1789	rVB	153	72	0.01%	0.001%
51	7.102	1790	1792	1798	rVB	322	302	0.05%	0.006%
52	7.131	1798	1801	1804	rBV	253	239	0.04%	0.005%
53	7.208	1821	1825	1831	rVB2	542	613	0.11%	0.013%
54	7.346	1866	1868	1870	rVB	131	34	0.01%	0.001%
55	7.365	1872	1874	1877	rBV	209	98	0.02%	0.002%
56	7.475	1906	1908	1910	rBV	163	70	0.01%	0.001%
57	7.591	1932	1944	1958	rBV	89935	154651	26.52%	3.203%
58	7.848	2023	2024	2026	rBV	224	78	0.01%	0.002%
59	7.861	2026	2028	2033	rVB	200	151	0.03%	0.003%
60	7.922	2033	2047	2062	rBV	274783	470084	80.60%	9.736%
61	8.201	2123	2134	2149	rBV	63612	103676	17.78%	2.147%
62	8.256	2149	2151	2153	rVB	231	88	0.02%	0.002%
63	8.375	2186	2188	2194	rVB	261	178	0.03%	0.004%
64	8.655	2263	2275	2301	rBV	216520	374462	64.20%	7.755%
65	8.777	2309	2313	2316	rBV2	379	286	0.05%	0.006%
66	8.806	2320	2322	2327	rVB	182	103	0.02%	0.002%
67	8.941	2355	2364	2373	rBV3	1187	2229	0.38%	0.046%
68	8.999	2380	2382	2384	rBV	263	104	0.02%	0.002%
69	9.336	2484	2487	2489	rBV	213	109	0.02%	0.002%
70	9.436	2505	2518	2537	rBV	299180	483509	82.90%	10.014%
71	10.774	2922	2934	2949	rVB	197214	315142	54.03%	6.527%

Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU040620\
Data File : VU037595.D
Acq On : 06 Apr 2020 17:25
Operator : JC/MD
Sample : L2158-11
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040320WMA.M
Title : VOC Analysis

72	11.002	3003	3005	3006	rBV	274	116	0.02%	0.002%
73	11.211	3068	3070	3072	rBV	183	84	0.01%	0.002%
74	11.745	3234	3236	3239	rBV	258	145	0.02%	0.003%
75	11.825	3249	3261	3277	rBV	306866	474669	81.39%	9.831%
76	11.896	3282	3283	3286	rBV	128	71	0.01%	0.001%
77	12.205	3368	3379	3394	rVB	274630	438519	75.19%	9.082%
78	13.549	3794	3797	3802	rBV2	307	264	0.05%	0.005%
79	14.195	3995	3998	4001	rBV	380	169	0.03%	0.004%
80	14.468	4080	4083	4088	rVB	615	353	0.06%	0.007%


Sum of corrected areas: 4828515

Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU040620\
Data File : VU037595.D
Acq On : 06 Apr 2020 17:25
Operator : JC/MD
Sample : L2158-11
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK01

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

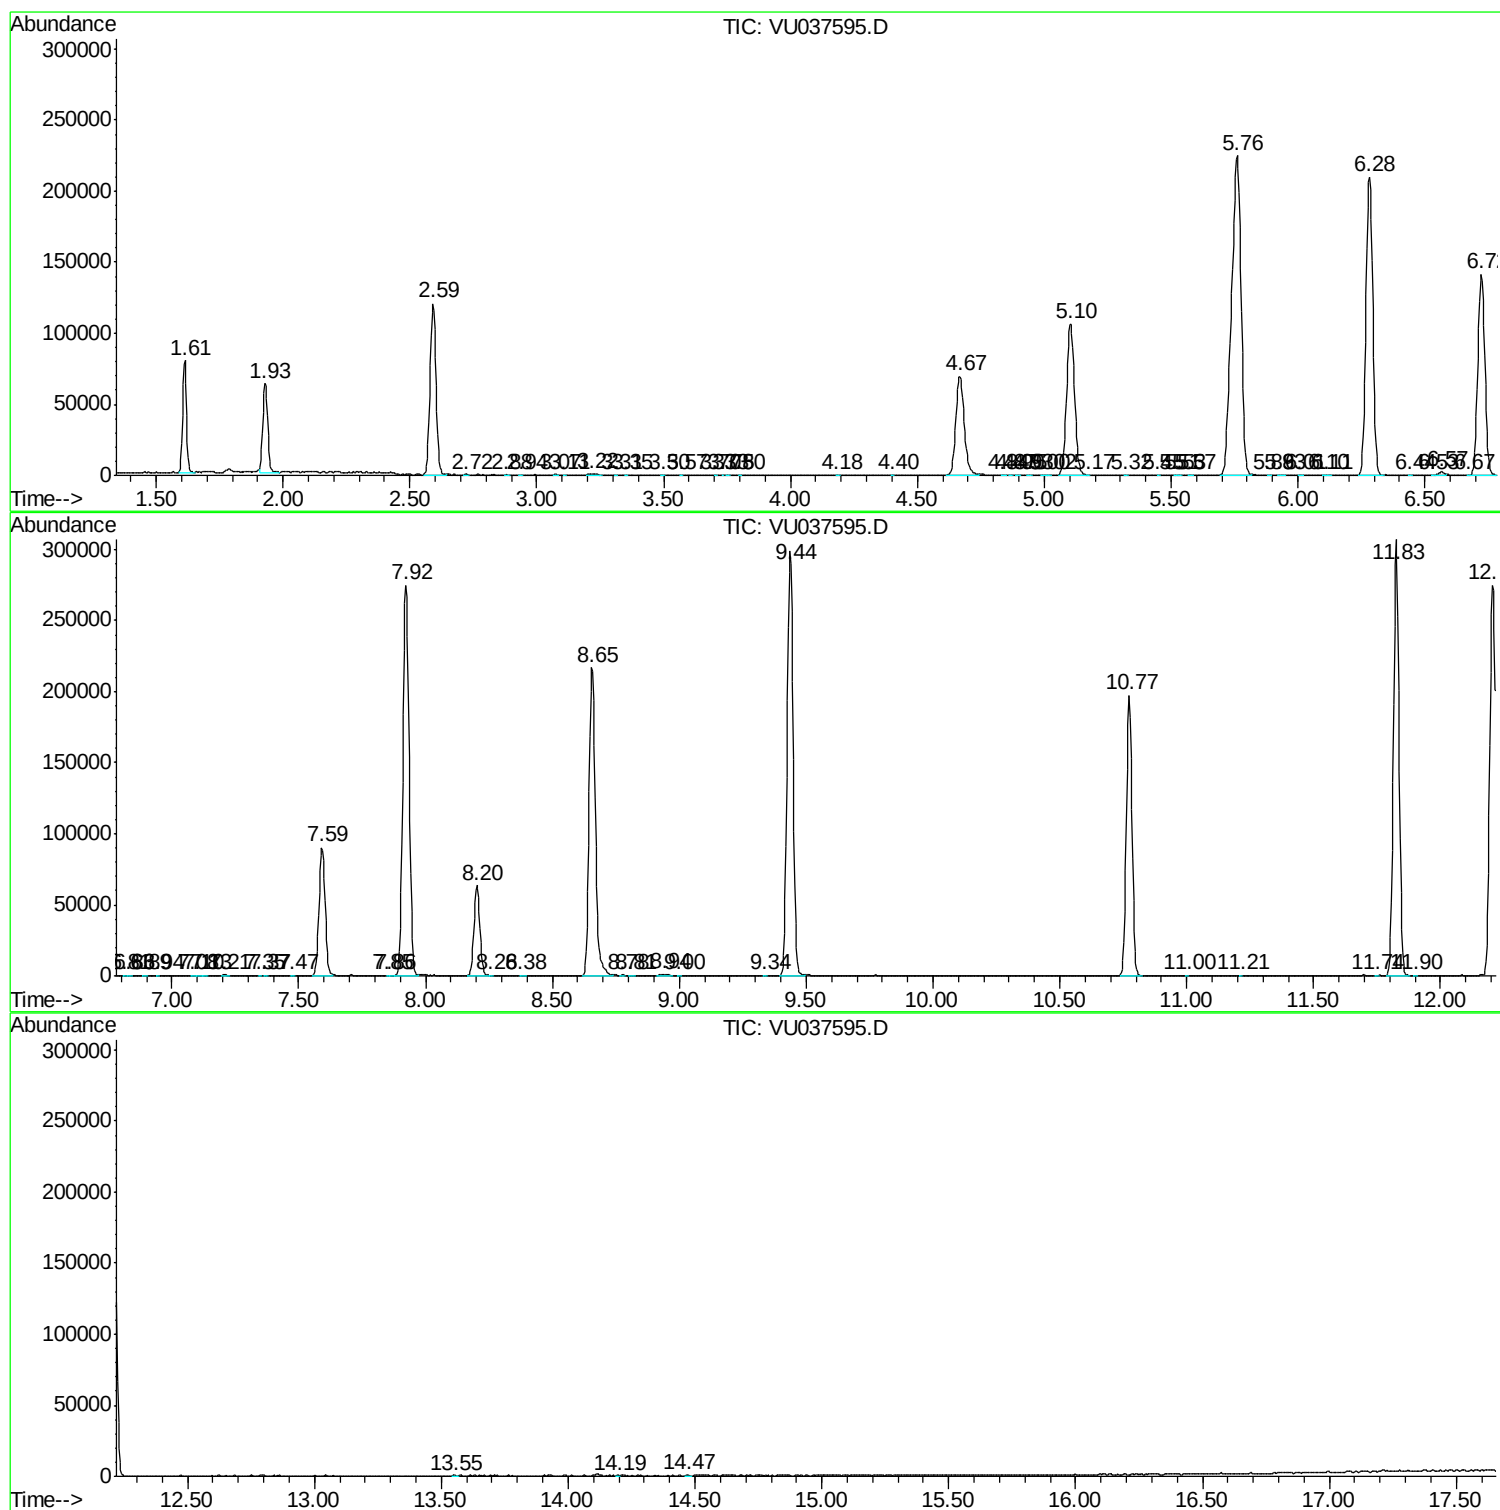

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040620\
Data File : VU037595.D
Acq On : 06 Apr 2020 17:25
Operator : JC/MD
Sample : L2158-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK01

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040620\
Data File : VU037595.D
Acq On : 06 Apr 2020 17:25
Operator : JC/MD
Sample : L2158-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK01

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc