


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU040620\
 Data File : VU037582.D
 Acq On : 06 Apr 2020 09:01
 Operator : JC/MD
 Sample : BFB36
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB36

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040320WMA.M
 Title : VOC Analysis
 Last Update : Tue Apr 07 00:48:05 2020

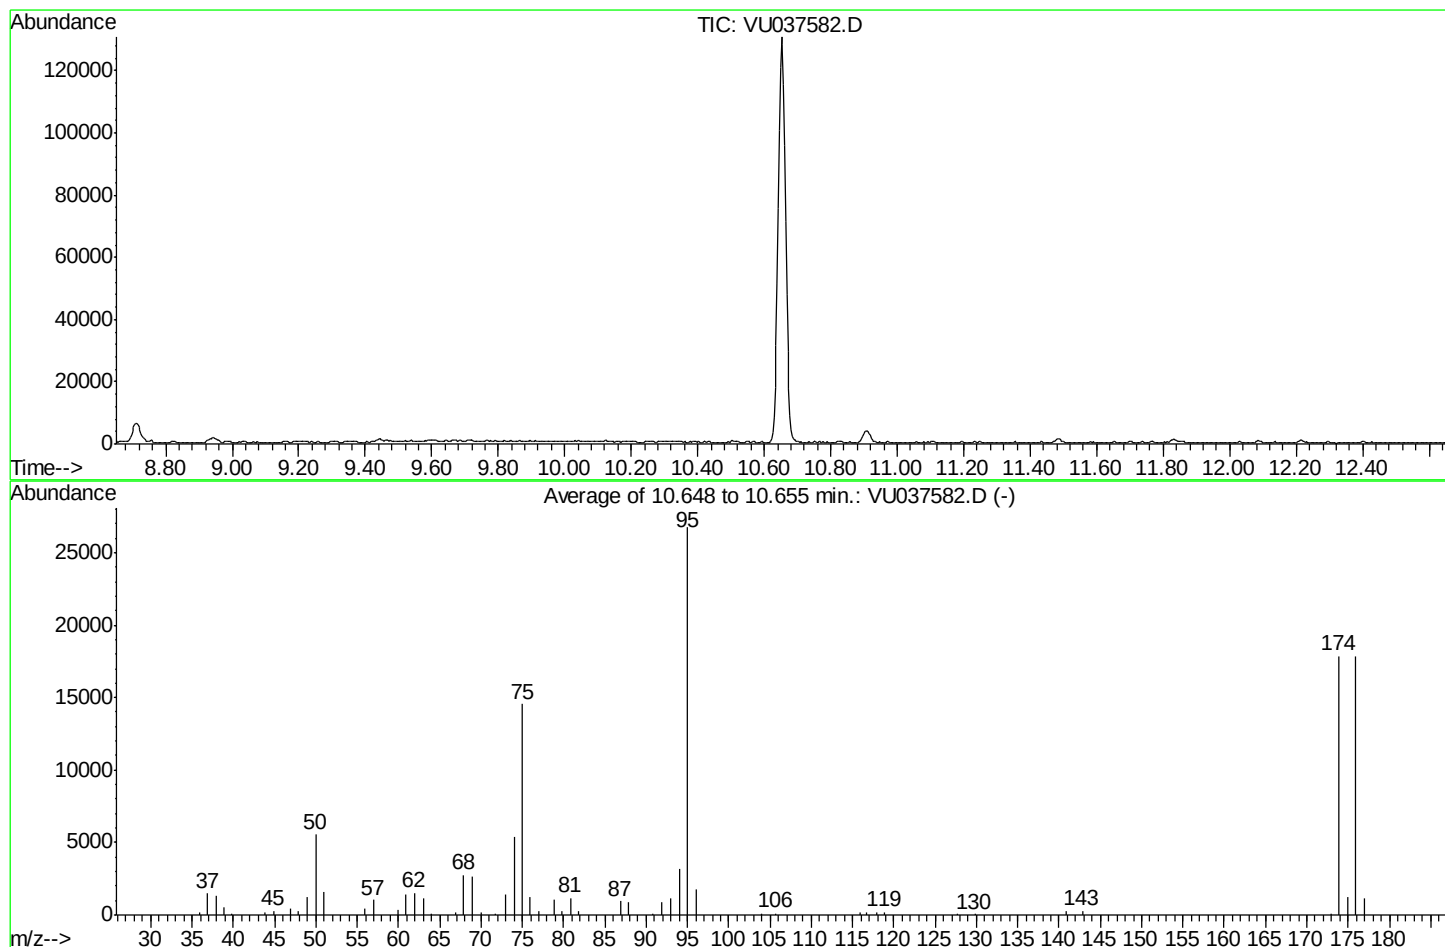

AutoFind: Scans 2895, 2896, 2897; Background Corrected with Scan 2884

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.7	5526	PASS
75	95	30	80	54.5	14565	PASS
95	95	100	100	100.0	26744	PASS
96	95	5	9	6.7	1799	PASS
173	174	0.00	2	0.5	92	PASS
174	95	50	120	66.7	17845	PASS
175	174	5	9	7.2	1276	PASS
176	174	95	101	99.9	17824	PASS
177	176	5	9	6.7	1190	PASS

m/z	Abundance
35.90	534.0
36.90	1351.0
38.00	1415.0
38.90	568.0
39.80	105.0
44.00	421.0
44.90	283.0
47.00	488.0
47.80	182.0
48.90	1123.0
50.00	5436.0
50.90	1432.0
55.90	433.0
56.90	938.0
59.90	405.0
60.90	1418.0
61.90	1392.0
63.00	1094.0
66.90	148.0
67.90	2820.0
69.00	2622.0
70.00	210.0
71.80	116.0
73.00	1340.0
74.00	4925.0
75.00	14103.0
75.90	1281.0
77.00	232.0
78.80	1094.0
79.70	302.0
80.80	1155.0
81.80	287.0
86.90	781.0
87.90	914.0
90.80	100.0
91.90	837.0
92.90	1142.0
94.00	3278.0
95.00	25480.0
96.00	1663.0
103.90	107.0
105.80	119.0
115.90	143.0
116.70	129.0
117.80	128.0
118.90	185.0
129.80	125.0
140.80	219.0
142.90	248.0
173.90	16736.0
174.90	1283.0
175.90	16624.0
176.90	1127.0

Instrument :
MSVOA_U
ClientSampleId :
BFB36

m/z	Abundance
35.90	493.0
36.90	1509.0
37.90	1422.0
38.90	586.0
39.90	108.0
44.00	443.0
44.90	278.0
47.00	495.0
47.80	250.0
48.90	1257.0
50.00	5649.0
50.90	1673.0
56.00	508.0
56.90	1058.0
59.90	403.0
60.90	1394.0
61.90	1560.0
63.00	1263.0
64.00	103.0
66.90	180.0
67.90	2835.0
69.00	2737.0
70.00	197.0
71.80	120.0
73.00	1410.0
74.00	5542.0
75.00	14998.0
76.00	1223.0
77.00	263.0
78.90	1086.0
79.70	299.0
80.80	1161.0
81.90	311.0
86.90	946.0
87.90	944.0
91.90	876.0
92.90	1209.0
94.00	3289.0
95.00	27664.0
96.00	1860.0
103.90	114.0
105.80	118.0
115.90	183.0
116.70	164.0
117.90	191.0
118.90	221.0
127.70	110.0
129.80	123.0
140.80	241.0
142.80	250.0
172.90	131.0
173.90	18432.0
174.90	1314.0
175.90	18408.0
176.90	1234.0

Instrument :
MSVOA_U
ClientSampleId :
BFB36

m/z	Abundance
35.90	457.0
36.90	1532.0
37.90	1267.0
38.90	557.0
44.00	425.0
44.90	272.0
47.00	388.0
47.80	268.0
48.90	1235.0
50.00	5495.0
50.90	1714.0
56.00	510.0
57.00	1098.0
59.90	310.0
60.90	1368.0
61.90	1598.0
63.00	1191.0
64.00	125.0
66.90	146.0
67.90	2578.0
69.00	2649.0
70.00	170.0
72.90	1371.0
74.00	5593.0
75.00	14595.0
76.00	1129.0
77.00	224.0
78.90	1056.0
79.80	305.0
80.80	1133.0
81.90	291.0
86.90	1081.0
87.90	888.0
90.80	115.0
91.90	872.0
92.90	1096.0
94.00	3017.0
95.00	27088.0
96.00	1876.0
103.90	105.0
105.70	120.0
115.90	210.0
116.70	164.0
117.90	214.0
118.90	223.0
127.70	122.0
140.80	282.0
142.80	311.0
172.90	147.0
173.90	18368.0
174.90	1232.0
175.90	18440.0
176.90	1209.0

Instrument :
MSVOA_U
ClientSampleId :
BFB36

Scan 2884 (10.613 min): VU037582.D
BFB36

m/z	Abundance
35.90	323.0
43.80	209.0

Instrument :
MSVOA_U
ClientSampleId :
BFB36