

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040622\
 Data File : VU047832.D
 Acq On : 06 Apr 2022 16:35
 Operator : SY/MD
 Sample : VU0406WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0406WBL01

Quant Time: Apr 07 06:40:00 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U040622DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Thu Apr 07 06:19:08 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Fluorobenzene	6.118	96	47912	1.000	ug/l	# 0.00
System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.636	95	14561	0.841	ug/l	0.00
Spiked Amount 1.000			Recovery	=	84.000%	
68) 1,2-Dichlorobenzene-d4	12.195	152	18230	0.872	ug/l	0.00
Spiked Amount 1.000			Recovery	=	87.000%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040622\
Data File : VU047832.D
Acq On : 06 Apr 2022 16:35
Operator : SY/MD
Sample : VU0406WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0406WBL01

Quant Time: Apr 07 06:40:00 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U040622DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Thu Apr 07 06:19:08 2022
Response via : Initial Calibration




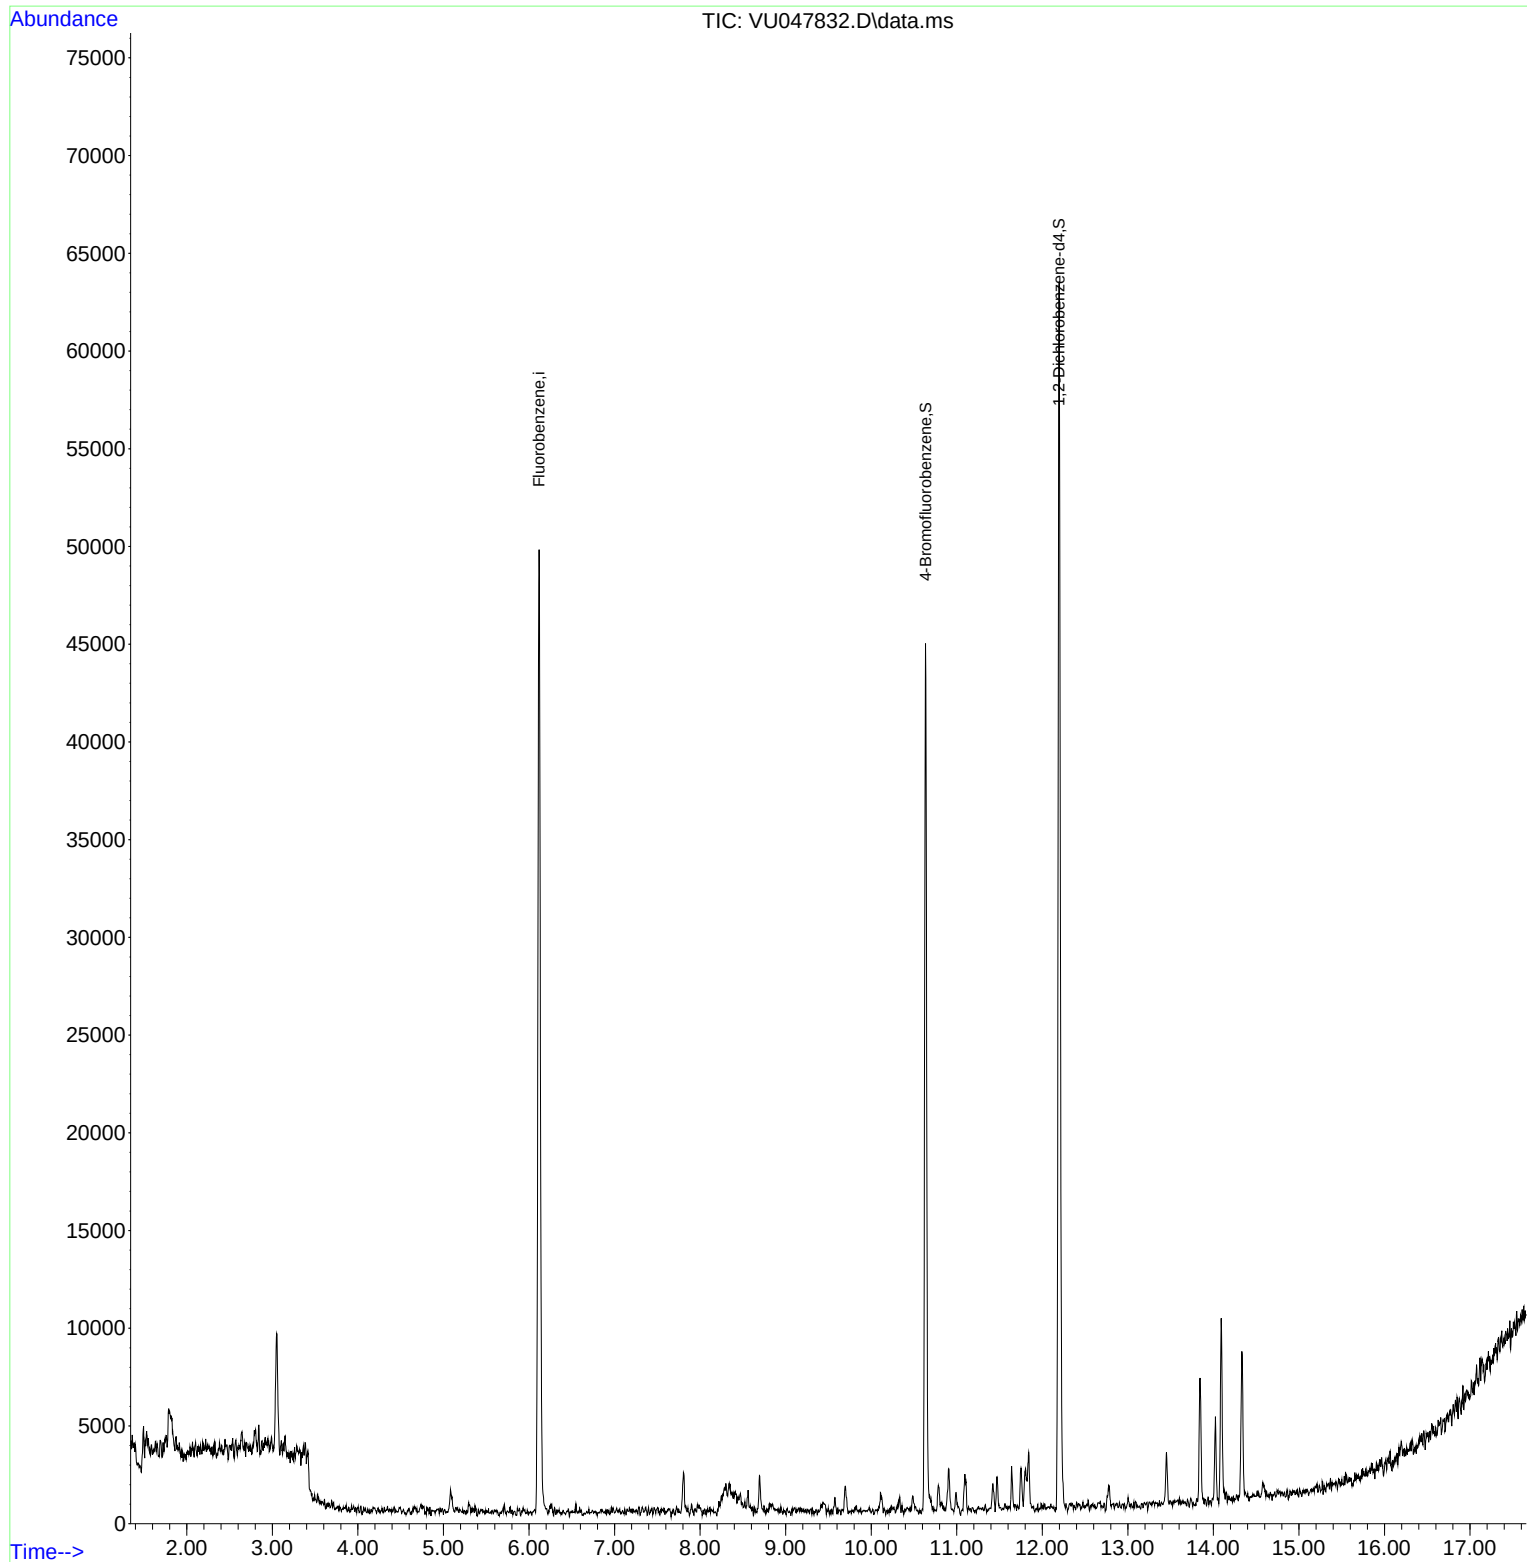


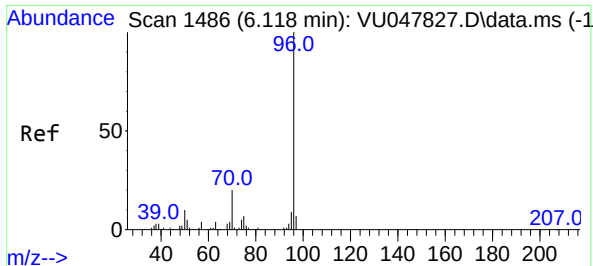

#1
Fluorobenzene
Concen: 1.000 ug/l
RT: 6.118 min Scan# 1486
Delta R.T. 0.000 min
Lab File: VU047832.D
Acq: 06 Apr 2022 16:35




Instrument :
MSVOA_U
ClientSampleId :
VU0406WBL01


Tgt Ion:	96	Resp:	47912
Ion	Ratio	Lower	Upper
96	100		
70	18.2	15.4	23.0
95	9.6	7.6	11.4
97	7.1	0.0	0.0

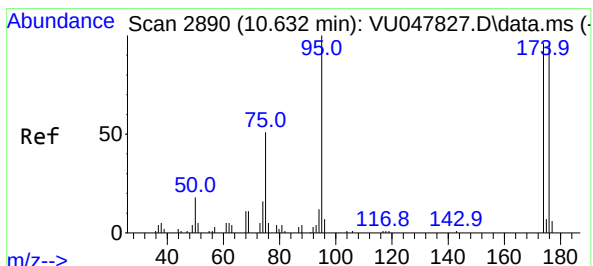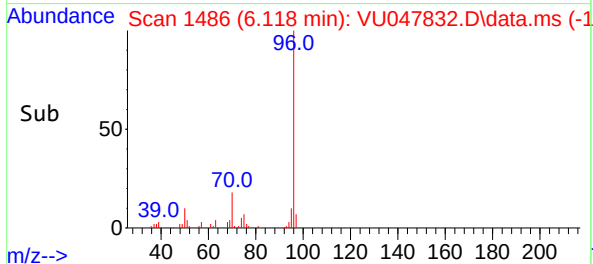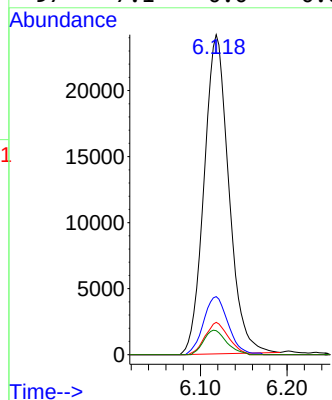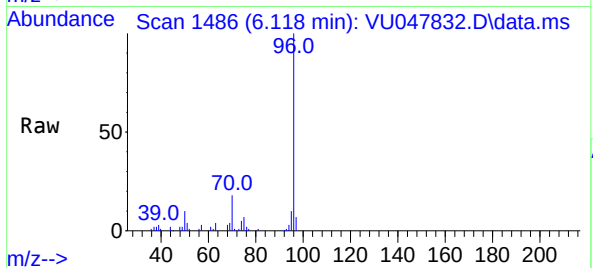

#57
4-Bromofluorobenzene
Concen: 0.841 ug/l
RT: 10.636 min Scan# 2891
Delta R.T. 0.003 min
Lab File: VU047832.D
Acq: 06 Apr 2022 16:35

Tgt Ion:	95	Resp:	14561
Ion	Ratio	Lower	Upper
95	100		
174	99.7	76.9	115.3
176	93.6	76.4	114.6

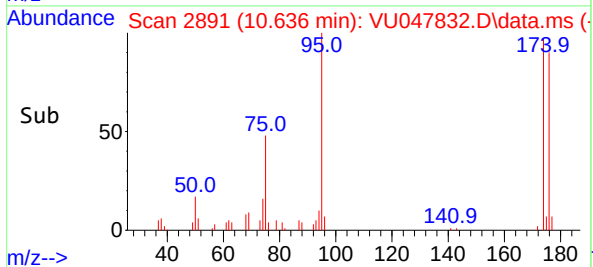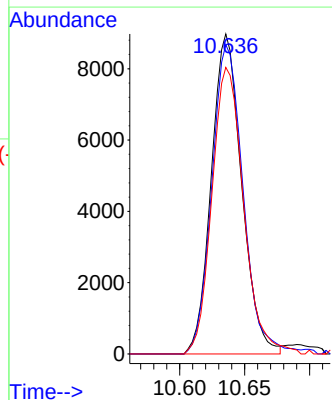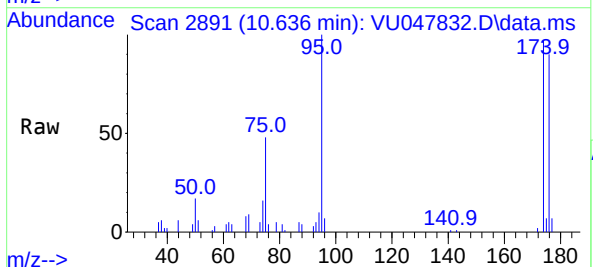

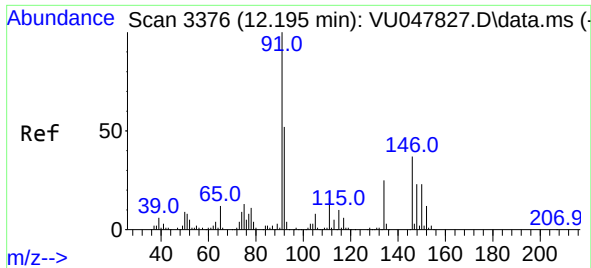

#68

1,2-Dichlorobenzene-d4

Concen: 0.872 ug/l

RT: 12.195 min Scan# 31

Delta R.T. 0.000 min

Lab File: VU047832.D


Acq: 06 Apr 2022 16:35

Instrument :

MSVOA_U

ClientSampleId :

VU0406WBL01

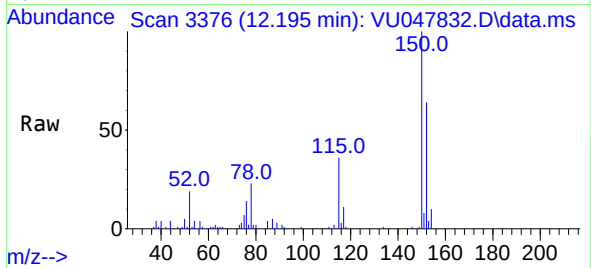

Tgt Ion:152 Resp: 18230

Ion Ratio Lower Upper

152 100

115 59.8 0.0 255.8

150 159.8 0.0 659.8

