

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040622\
 Data File : VU047833.D
 Acq On : 06 Apr 2022 17:03
 Operator : SY/MD
 Sample : VU0406WBL02
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0406WBL02

Quant Time: Apr 07 06:40:14 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U040622DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Thu Apr 07 06:19:08 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Fluorobenzene	6.118	96	47808	1.000	ug/l	# 0.00
System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.636	95	14140	0.818	ug/l	0.00
Spiked Amount 1.000			Recovery	=	82.000%	
68) 1,2-Dichlorobenzene-d4	12.198	152	17831	0.855	ug/l	0.00
Spiked Amount 1.000			Recovery	=	85.000%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040622\
Data File : VU047833.D
Acq On : 06 Apr 2022 17:03
Operator : SY/MD
Sample : VU0406WBL02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0406WBL02

Quant Time: Apr 07 06:40:14 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U040622DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Thu Apr 07 06:19:08 2022
Response via : Initial Calibration




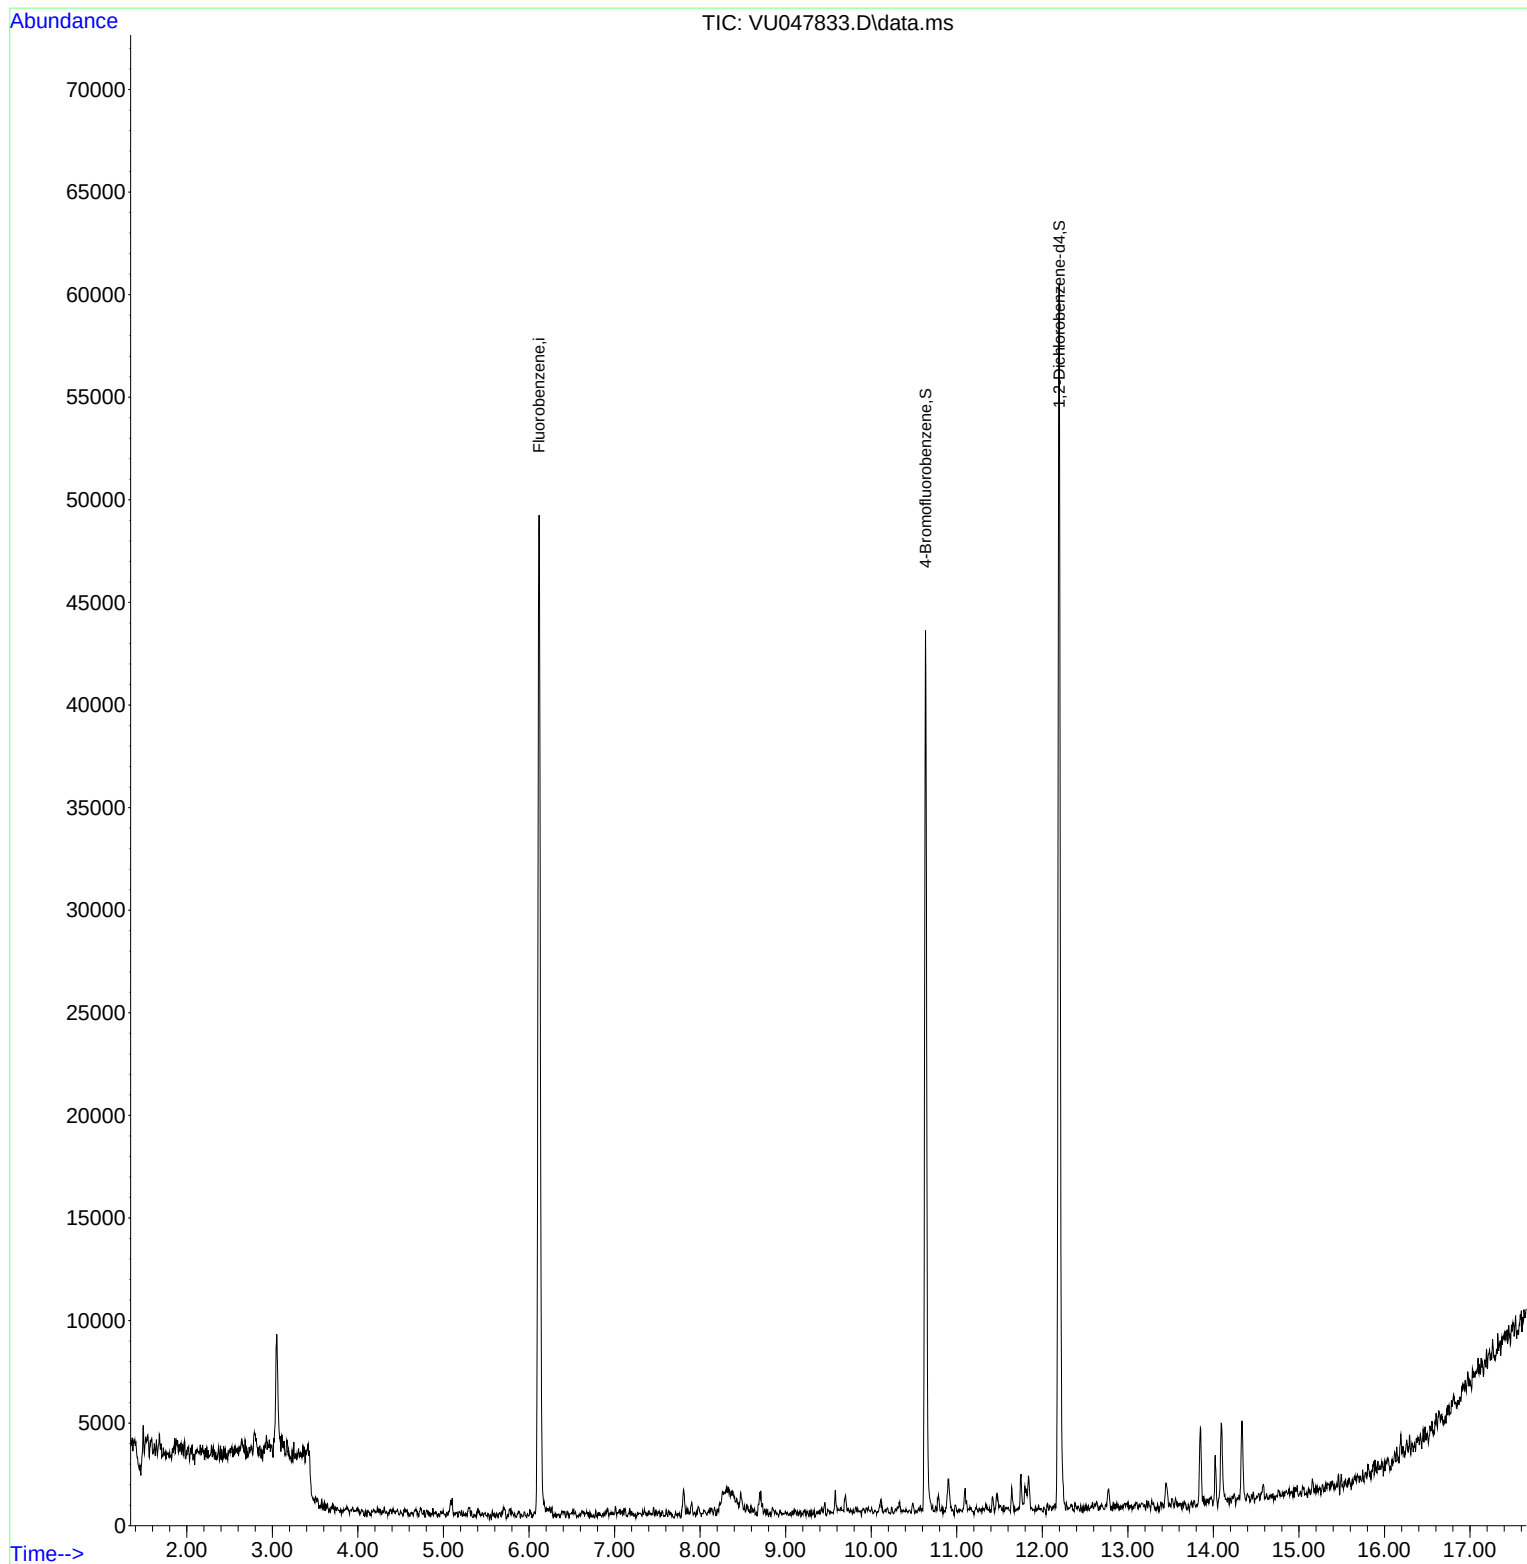


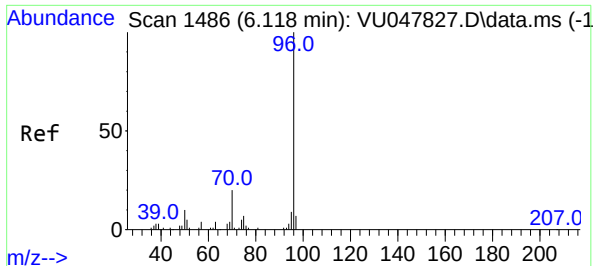

#1
Fluorobenzene
Concen: 1.000 ug/l
RT: 6.118 min Scan# 1486
Delta R.T. 0.000 min
Lab File: VU047833.D
Acq: 06 Apr 2022 17:03




Instrument :
MSVOA_U
ClientSampleId :
VU0406WBL02


Tgt Ion: 96	Resp: 47808
Ion Ratio	Lower Upper
96 100	
70 19.3	15.4 23.0
95 9.4	7.6 11.4
97 6.4	0.0 0.0#

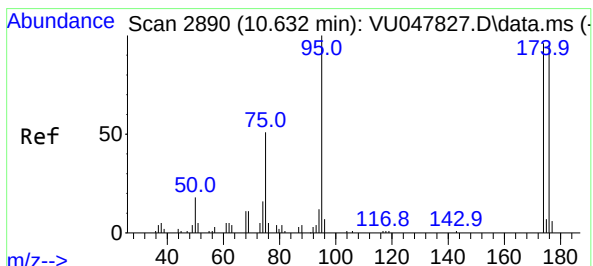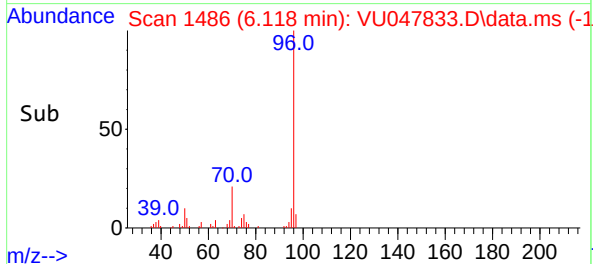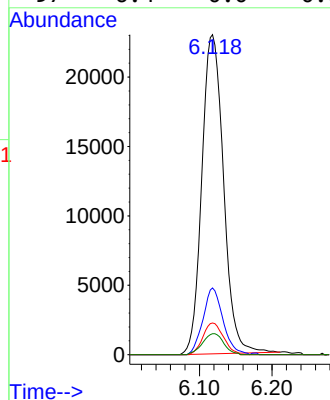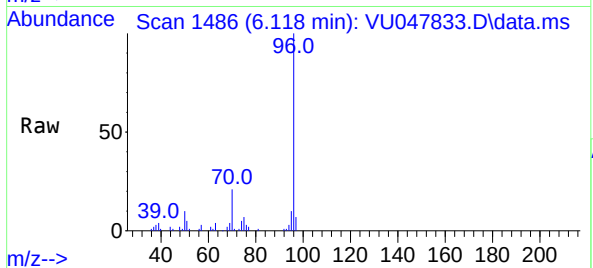

#57
4-Bromofluorobenzene
Concen: 0.818 ug/l
RT: 10.636 min Scan# 2891
Delta R.T. 0.003 min
Lab File: VU047833.D
Acq: 06 Apr 2022 17:03

Tgt Ion: 95	Resp: 14140
Ion Ratio	Lower Upper
95 100	
174 102.8	76.9 115.3
176 98.3	76.4 114.6

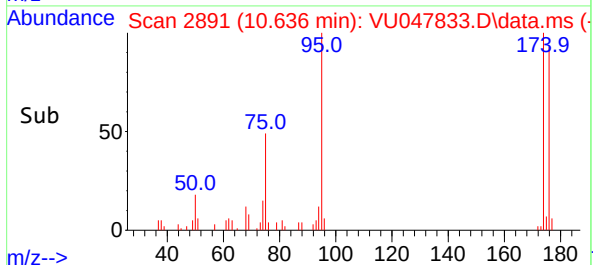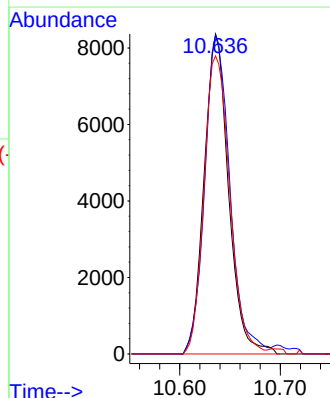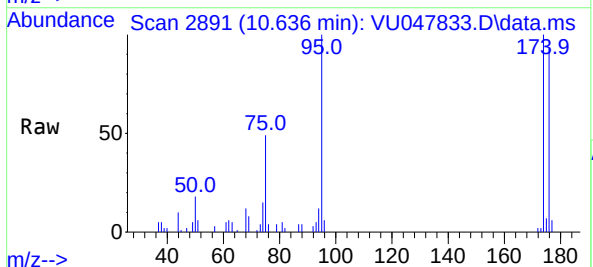

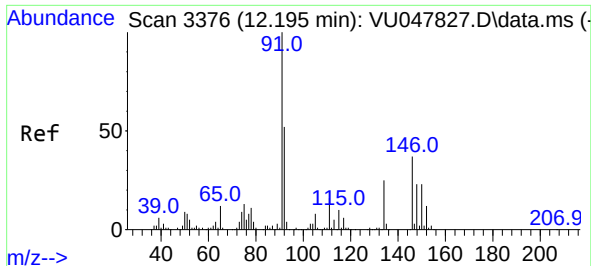

#68

1,2-Dichlorobenzene-d4

Concen: 0.855 ug/l

RT: 12.198 min Scan# 31

Delta R.T. 0.003 min

Lab File: VU047833.D


Acq: 06 Apr 2022 17:03

Instrument :

MSVOA_U

ClientSampleId :

VU0406WBL02

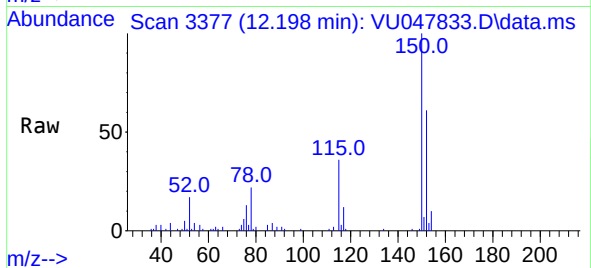

Tgt Ion:152 Resp: 17831

Ion Ratio Lower Upper

152 100

115 61.3 0.0 255.8

150 162.0 0.0 659.8

