

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040622\
 Data File : VU047832.D
 Acq On : 06 Apr 2022 16:35
 Operator : SY/MD
 Sample : VU0406WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0406WBL01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U040622DW.M

Title : METHOD 524.2 VOLATILES DRINKING WATER

Signal : TIC: VU047832.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.787	135	139	140	rBV3	1764	1154	1.02%	0.305%
2	2.575	378	384	389	rBV4	976	1208	1.07%	0.319%
3	2.842	464	467	471	rVB4	1518	1168	1.04%	0.309%
4	3.051	523	532	543	rVB3	6220	11703	10.38%	3.095%
5	5.083	1155	1164	1168	rBV3	1146	1529	1.36%	0.404%
6	6.118	1473	1486	1511	rBV	49261	97901	86.82%	25.892%
7	7.806	2001	2011	2017	rBV4	2115	3278	2.91%	0.867%
8	8.693	2282	2287	2297	rVB2	1709	2170	1.92%	0.574%
9	9.574	2554	2561	2569	rVB3	861	1230	1.09%	0.325%
10	9.697	2592	2599	2610	rVB4	1397	2391	2.12%	0.632%
11	10.636	2881	2891	2905	rBV	44313	71379	63.30%	18.877%
12	10.783	2931	2937	2944	rBV6	1285	2009	1.78%	0.531%
13	10.906	2964	2975	2987	rBV5	2156	3741	3.32%	0.989%
14	10.989	2994	3001	3006	rBV2	1007	1270	1.13%	0.336%
15	11.095	3027	3034	3044	rVB5	1943	3328	2.95%	0.880%
16	11.423	3129	3136	3144	rVB5	1445	2288	2.03%	0.605%
17	11.471	3144	3151	3157	rBV4	1808	2492	2.21%	0.659%
18	11.642	3199	3204	3211	rBV2	2201	2413	2.14%	0.638%
19	11.751	3230	3238	3246	rBV6	2103	3167	2.81%	0.838%
20	11.799	3246	3253	3254	rBV4	1835	1839	1.63%	0.486%
21	11.841	3260	3266	3272	rVB4	2608	3552	3.15%	0.939%
22	12.198	3366	3377	3399	rBV	62821	112768	100.00%	29.823%
23	13.452	3758	3767	3776	rVB2	2652	3686	3.27%	0.975%
24	13.844	3880	3889	3899	rBV4	6327	9681	8.58%	2.560%
25	14.024	3938	3945	3952	rVB4	4278	5179	4.59%	1.370%
26	14.092	3957	3966	3976	rBV	9489	14248	12.63%	3.768%
27	14.333	4032	4041	4050	rBV3	7430	11346	10.06%	3.001%




Sum of corrected areas: 378118

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040622\
Data File : VU047832.D
Acq On : 06 Apr 2022 16:35
Operator : SY/MD
Sample : VU0406WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0406WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U040622DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

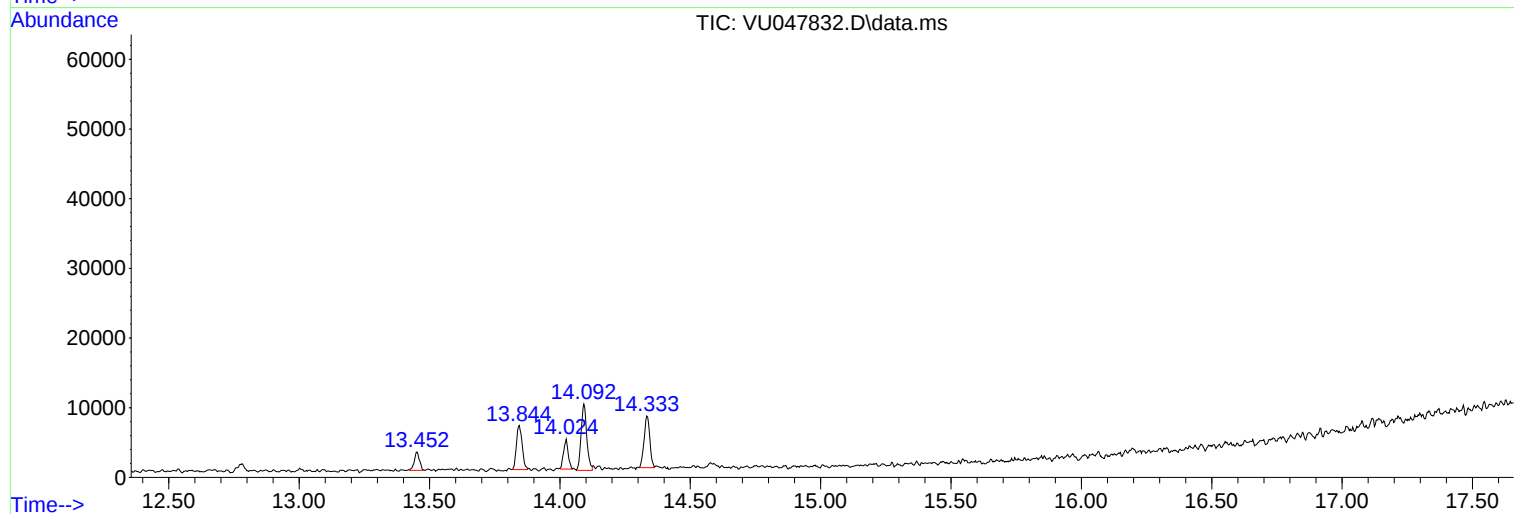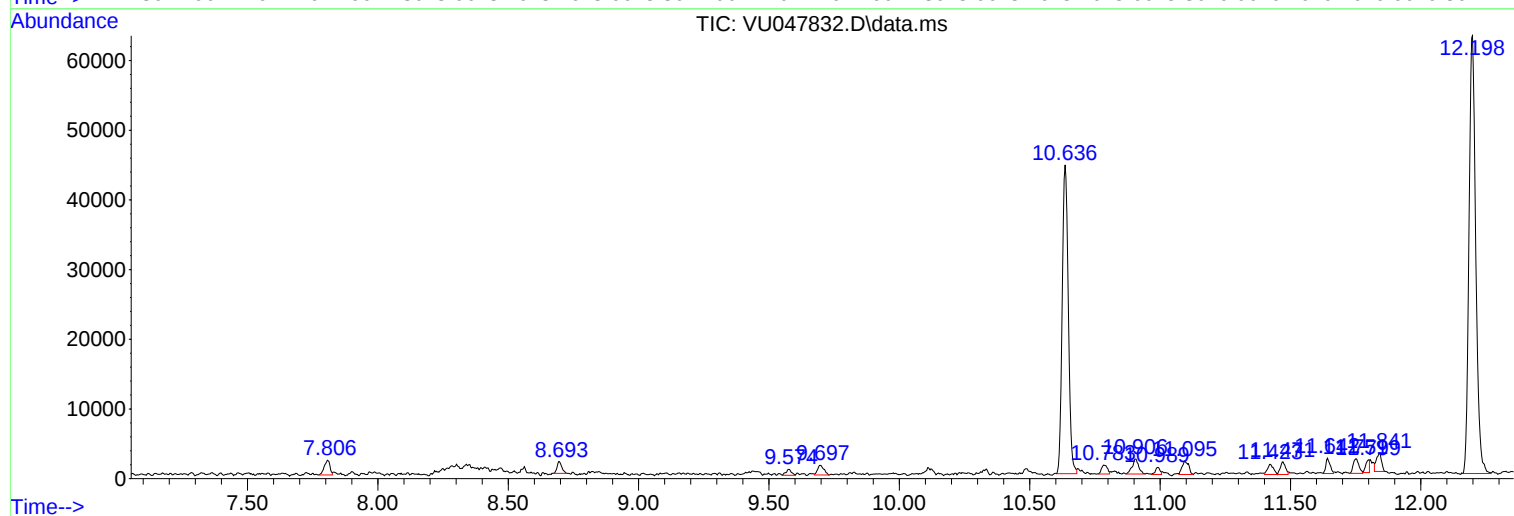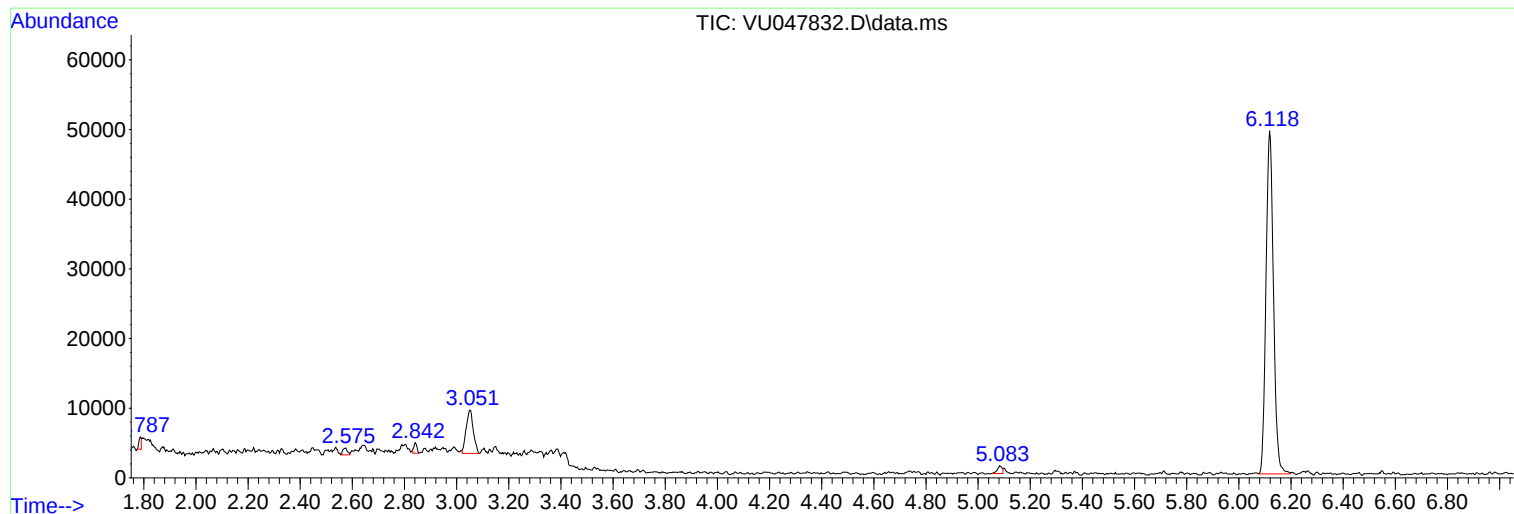

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040622\
Data File : VU047832.D
Acq On : 06 Apr 2022 16:35
Operator : SY/MD
Sample : VU0406WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0406WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U040622DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040622\
Data File : VU047832.D
Acq On : 06 Apr 2022 16:35
Operator : SY/MD
Sample : VU0406WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0406WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U040622DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------