

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040622\
 Data File : VU047833.D
 Acq On : 06 Apr 2022 17:03
 Operator : SY/MD
 Sample : VU0406WBL02
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0406WBL02

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U040622DW.M

Title : METHOD 524.2 VOLATILES DRINKING WATER

Signal : TIC: VU047833.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.051	526	532	544	rVB5	5100	8139	7.66%	2.493%
2	6.118	1472	1486	1504	rBV	48676	96615	90.97%	29.597%
3	7.806	2001	2011	2020	rBV4	1417	2541	2.39%	0.778%
4	8.475	2212	2219	2230	rVB5	843	1351	1.27%	0.414%
5	9.581	2556	2563	2570	rBV2	1122	1285	1.21%	0.394%
6	9.700	2594	2600	2605	rBV5	803	1077	1.01%	0.330%
7	10.636	2881	2891	2913	rBV2	42911	71397	67.23%	21.871%
8	10.906	2966	2975	2986	rVB5	1527	2909	2.74%	0.891%
9	11.099	3024	3035	3038	rBV4	1170	1424	1.34%	0.436%
10	11.468	3142	3150	3157	rBV4	909	1543	1.45%	0.473%
11	11.642	3200	3204	3213	rVB2	1223	1421	1.34%	0.435%
12	11.751	3232	3238	3243	rBV4	1696	1941	1.83%	0.595%
13	11.838	3261	3265	3273	rVB4	1565	2133	2.01%	0.653%
14	12.198	3364	3377	3396	rBV	59686	106200	100.00%	32.533%
15	12.774	3550	3556	3563	rVB3	1014	1613	1.52%	0.494%
16	13.446	3757	3765	3775	rBV4	1205	2265	2.13%	0.694%
17	13.848	3881	3890	3898	rBV4	3729	5654	5.32%	1.732%
18	14.021	3935	3944	3953	rVB6	2561	3256	3.07%	0.997%
19	14.092	3953	3966	3977	rBV2	4108	7863	7.40%	2.409%
20	14.333	4033	4041	4054	rBV4	3829	5812	5.47%	1.780%


Sum of corrected areas: 326439

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040622\
Data File : VU047833.D
Acq On : 06 Apr 2022 17:03
Operator : SY/MD
Sample : VU0406WBL02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0406WBL02

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U040622DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

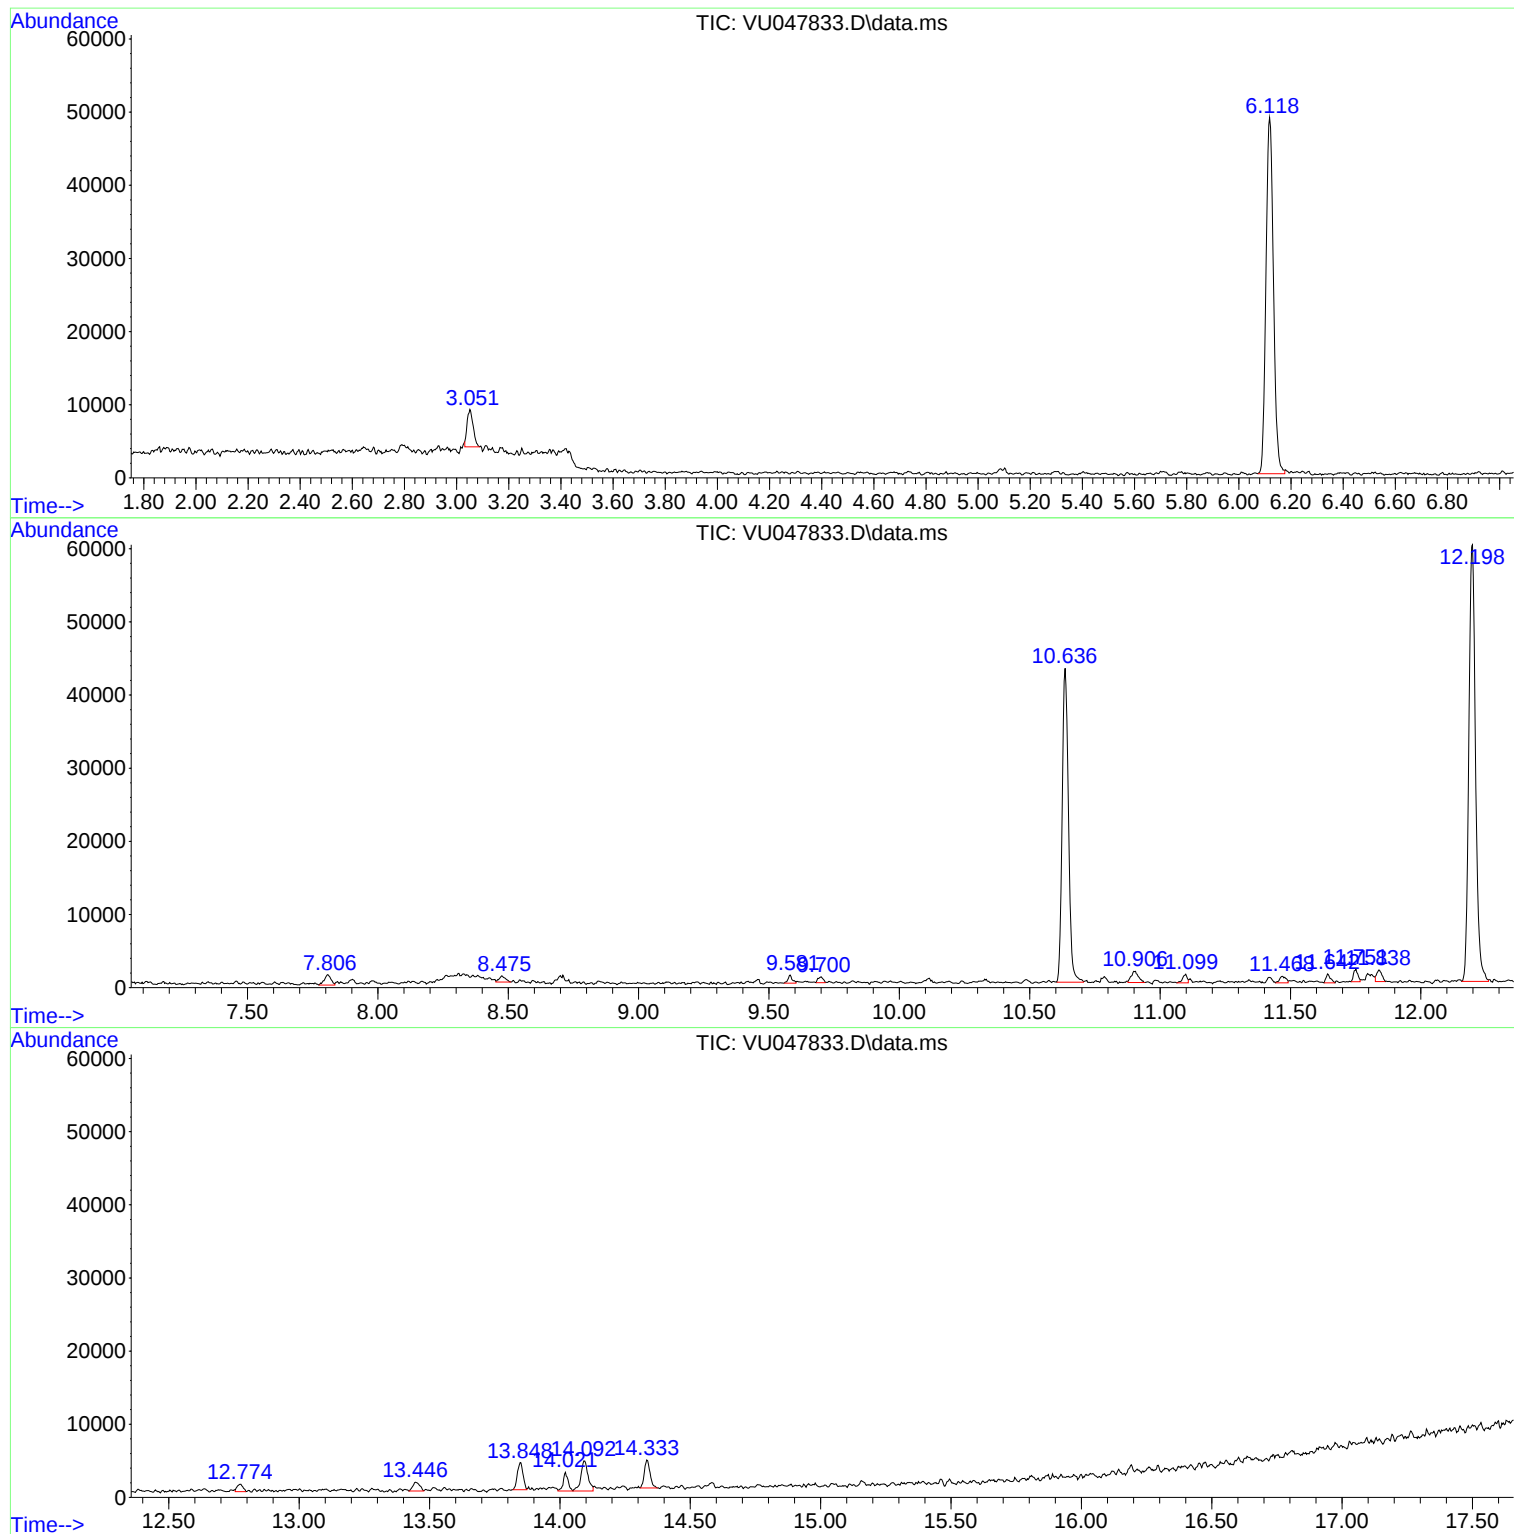

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040622\
Data File : VU047833.D
Acq On : 06 Apr 2022 17:03
Operator : SY/MD
Sample : VU0406WBL02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0406WBL02

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U040622DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040622\
Data File : VU047833.D
Acq On : 06 Apr 2022 17:03
Operator : SY/MD
Sample : VU0406WBL02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0406WBL02

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U040622DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------