

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040623\
 Data File : VU053586.D
 Acq On : 06 Apr 2023 11:37
 Operator : JC/MD
 Sample : VU0406MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK071

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

Signal : TIC: VU053586.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	100	rVB	143728	164147	17.53%	2.218%
2	1.909	169	177	193	rBV	107255	150310	16.06%	2.031%
3	2.565	369	381	397	rBV	207056	339891	36.31%	4.593%
4	2.758	438	441	443	rBV2	251	160	0.02%	0.002%
5	2.793	445	452	460	rVB	2054	3142	0.34%	0.042%
6	2.848	466	469	472	rBV2	294	265	0.03%	0.004%
7	2.903	484	486	491	rVB	356	298	0.03%	0.004%
8	2.948	496	500	504	rVB2	322	246	0.03%	0.003%
9	2.973	504	508	510	rBV2	263	177	0.02%	0.002%
10	3.044	521	530	542	rVB5	3514	6283	0.67%	0.085%
11	3.137	555	559	564	rBV2	234	250	0.03%	0.003%
12	3.160	564	566	575	rVB3	551	475	0.05%	0.006%
13	3.211	576	582	585	rVV2	272	284	0.03%	0.004%
14	3.243	589	592	595	rVB2	263	176	0.02%	0.002%
15	3.279	600	603	606	rVB	324	202	0.02%	0.003%
16	3.343	616	623	625	rBV3	973	863	0.09%	0.012%
17	3.568	691	693	697	rVB	339	177	0.02%	0.002%
18	3.719	735	740	745	rVB	287	260	0.03%	0.004%
19	3.813	765	769	772	rBV	233	187	0.02%	0.003%
20	3.829	772	774	781	rVB2	295	262	0.03%	0.004%
21	3.899	792	796	800	rBV	173	158	0.02%	0.002%
22	3.941	807	809	812	rVB	322	165	0.02%	0.002%
23	3.964	812	816	820	rBV	170	167	0.02%	0.002%
24	4.028	831	836	840	rBV2	287	262	0.03%	0.004%
25	4.054	841	844	847	rVB	351	206	0.02%	0.003%
26	4.076	847	851	853	rBV2	237	185	0.02%	0.002%
27	4.131	865	868	872	rVB2	198	151	0.02%	0.002%
28	4.259	904	908	911	rBV	287	197	0.02%	0.003%
29	4.456	965	969	979	rVB	183	239	0.03%	0.003%
30	4.497	979	982	986	rBV2	266	245	0.03%	0.003%
31	4.613	1006	1018	1050	rBV	74742	182796	19.53%	2.470%
32	4.944	1118	1121	1125	rVB	288	187	0.02%	0.003%
33	4.999	1133	1138	1140	rBV2	234	189	0.02%	0.003%
34	5.057	1140	1156	1180	rVV	174028	381679	40.77%	5.157%
35	5.333	1239	1242	1244	rBV	173	143	0.02%	0.002%
36	5.375	1251	1255	1256	rBV	231	159	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040623\
 Data File : VU053586.D
 Acq On : 06 Apr 2023 11:37
 Operator : JC/MD
 Sample : VU0406MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK071

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

37	5.620	1327	1331	1335	rBV2	284	195	0.02%	0.003%
38	5.719	1341	1362	1388	rBV2	344789	936186	100.00%	12.650%
39	6.124	1484	1488	1490	rVB	391	262	0.03%	0.004%
40	6.182	1503	1506	1511	rBV2	283	212	0.02%	0.003%
41	6.243	1511	1525	1549	rBV	297000	565891	60.45%	7.646%
42	6.452	1586	1590	1596	rBV3	427	468	0.05%	0.006%
43	6.529	1602	1614	1625	rVB6	5935	11625	1.24%	0.157%
44	6.684	1649	1662	1684	rBV	213714	417527	44.60%	5.642%
45	6.854	1711	1715	1716	rBV	253	157	0.02%	0.002%
46	6.976	1750	1753	1758	rBV	129	146	0.02%	0.002%
47	7.192	1812	1820	1823	rBV3	910	1146	0.12%	0.015%
48	7.240	1832	1835	1838	rBV2	212	155	0.02%	0.002%
49	7.407	1883	1887	1889	rBV	274	154	0.02%	0.002%
50	7.562	1923	1935	1963	rVV	121599	216638	23.14%	2.927%
51	7.677	1969	1971	1973	rBV2	382	228	0.02%	0.003%
52	7.780	1996	2003	2004	rBV3	514	514	0.05%	0.007%
53	7.790	2004	2006	2008	rVB	423	179	0.02%	0.002%
54	7.893	2022	2038	2069	rBV	449010	786071	83.97%	10.621%
55	8.115	2102	2107	2110	rBV	203	218	0.02%	0.003%
56	8.176	2114	2126	2143	rBV	82487	145810	15.57%	1.970%
57	8.275	2154	2157	2160	rBV3	342	291	0.03%	0.004%
58	8.327	2171	2173	2182	rVB2	306	239	0.03%	0.003%
59	8.407	2195	2198	2201	rVB	369	245	0.03%	0.003%
60	8.439	2201	2208	2212	rBV2	288	342	0.04%	0.005%
61	8.552	2237	2243	2249	rVB3	2225	2801	0.30%	0.038%
62	8.626	2254	2266	2302	rBV	218068	413254	44.14%	5.584%
63	8.835	2328	2331	2334	rBV2	263	174	0.02%	0.002%
64	8.922	2354	2358	2362	rBV	392	334	0.04%	0.005%
65	8.967	2369	2372	2375	rVB	320	153	0.02%	0.002%
66	9.057	2398	2400	2403	rBV	276	162	0.02%	0.002%
67	9.108	2410	2416	2420	rBV2	206	226	0.02%	0.003%
68	9.217	2446	2450	2452	rBV2	219	163	0.02%	0.002%
69	9.359	2491	2494	2496	rBV2	266	177	0.02%	0.002%
70	9.414	2498	2511	2532	rBV	400998	678702	72.50%	9.171%
71	9.571	2552	2560	2567	rVV3	1475	2371	0.25%	0.032%
72	9.600	2567	2569	2575	rVB2	393	314	0.03%	0.004%
73	9.693	2588	2598	2609	rBV6	1457	2472	0.26%	0.033%
74	9.774	2620	2623	2627	rVB2	205	177	0.02%	0.002%
75	10.053	2706	2710	2714	rBV2	354	359	0.04%	0.005%
76	10.118	2719	2730	2737	rBV6	2381	4132	0.44%	0.056%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040623\
 Data File : VU053586.D
 Acq On : 06 Apr 2023 11:37
 Operator : JC/MD
 Sample : VU0406MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK071

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

77	10.439	2825	2830	2833	rBV	230	197	0.02%	0.003%
78	10.478	2836	2842	2852	rVV3	1016	1577	0.17%	0.021%
79	10.639	2890	2892	2895	rVB2	332	186	0.02%	0.003%
80	10.690	2906	2908	2913	rBV	195	172	0.02%	0.002%
81	10.751	2915	2927	2945	rBV	297840	481566	51.44%	6.507%
82	11.089	3025	3032	3038	rBV3	1124	1617	0.17%	0.022%
83	11.288	3091	3094	3102	rVB2	253	271	0.03%	0.004%
84	11.417	3129	3134	3137	rBV2	327	271	0.03%	0.004%
85	11.468	3145	3150	3161	rVB2	2064	2775	0.30%	0.037%
86	11.651	3204	3207	3214	rVB2	276	237	0.03%	0.003%
87	11.745	3229	3236	3244	rBV3	3600	5302	0.57%	0.072%
88	11.809	3244	3256	3280	rVV	433033	693625	74.09%	9.372%
89	12.188	3361	3374	3392	rBV	449743	727265	77.68%	9.827%
90	12.385	3433	3435	3438	rBV2	274	168	0.02%	0.002%
91	12.713	3535	3537	3539	rBV	240	143	0.02%	0.002%
92	12.790	3559	3561	3566	rBV	217	147	0.02%	0.002%
93	13.008	3626	3629	3633	rBV2	334	198	0.02%	0.003%
94	13.114	3659	3662	3664	rBV	248	170	0.02%	0.002%
95	13.217	3689	3694	3710	rVB5	3973	6651	0.71%	0.090%
96	13.391	3745	3748	3755	rBV	511	473	0.05%	0.006%
97	13.516	3783	3787	3789	rBV2	456	404	0.04%	0.005%
98	13.841	3879	3888	3897	rBV3	9904	15306	1.63%	0.207%
99	14.089	3956	3965	3986	rBV2	12361	22892	2.45%	0.309%
100	14.327	4031	4039	4051	rBV3	8070	13097	1.40%	0.177%




Sum of corrected areas: 7400763

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040623\
Data File : VU053586.D
Acq On : 06 Apr 2023 11:37
Operator : JC/MD
Sample : VU0406MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK071

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

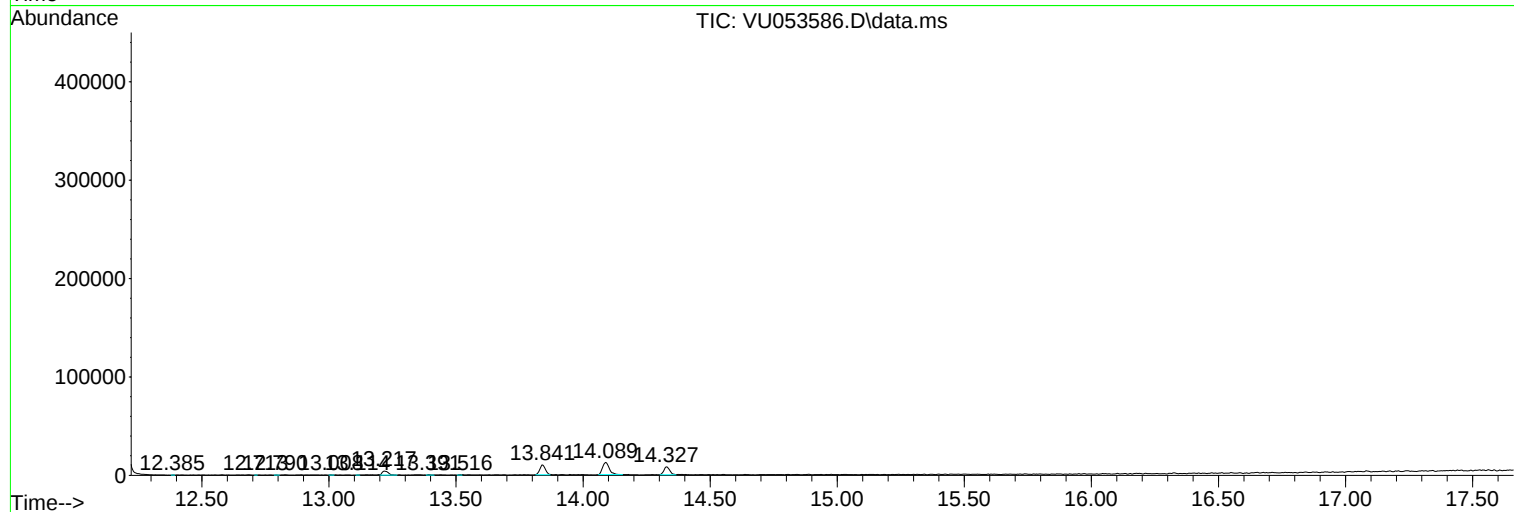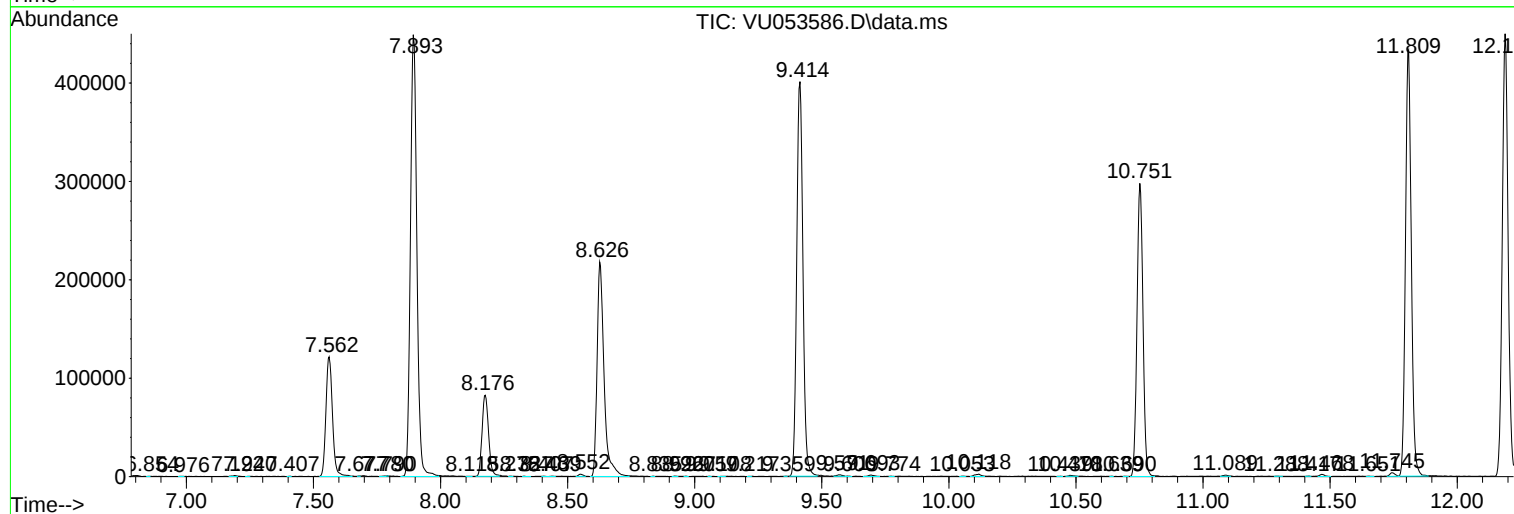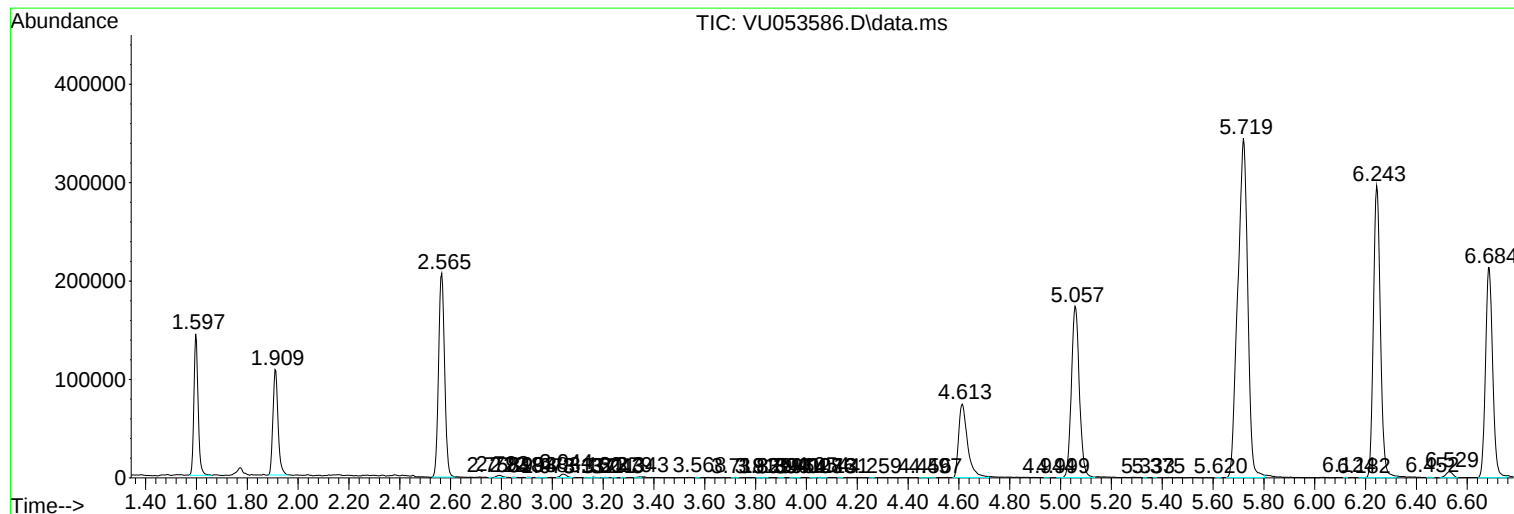

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040623\
Data File : VU053586.D
Acq On : 06 Apr 2023 11:37
Operator : JC/MD
Sample : VU0406MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK071

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040623\
Data File : VU053586.D
Acq On : 06 Apr 2023 11:37
Operator : JC/MD
Sample : VU0406MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK071

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------