

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040623\
 Data File : VU053587.D
 Acq On : 06 Apr 2023 12:03
 Operator : JC/MD
 Sample : VU0406WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK072

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

Signal : TIC: VU053587.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	95	rVB	139511	158000	16.95%	2.161%
2	1.909	169	177	195	rVB	103600	144835	15.54%	1.981%
3	2.565	369	381	401	rBV	207605	331086	35.52%	4.528%
4	3.044	521	530	543	rVB4	4016	7295	0.78%	0.100%
5	3.176	569	571	572	rBV4	234	109	0.01%	0.001%
6	3.340	617	622	623	rBV4	359	297	0.03%	0.004%
7	3.424	646	648	652	rVB	239	125	0.01%	0.002%
8	3.549	684	687	690	rBV	249	204	0.02%	0.003%
9	3.832	772	775	776	rBV	203	101	0.01%	0.001%
10	3.842	776	778	781	rVV	301	162	0.02%	0.002%
11	3.867	784	786	789	rVB2	265	153	0.02%	0.002%
12	3.906	795	798	804	rVB	307	307	0.03%	0.004%
13	3.999	824	827	830	rBV	228	143	0.02%	0.002%
14	4.244	899	903	906	rBV	272	237	0.03%	0.003%
15	4.362	938	940	942	rBV	166	89	0.01%	0.001%
16	4.433	959	962	969	rBV2	266	319	0.03%	0.004%
17	4.613	1006	1018	1045	rBV	75360	183719	19.71%	2.513%
18	4.993	1133	1136	1140	rBV	259	184	0.02%	0.003%
19	5.060	1140	1157	1177	rBV	171082	372433	39.95%	5.094%
20	5.282	1223	1226	1232	rVB2	456	373	0.04%	0.005%
21	5.436	1269	1274	1278	rBV2	385	471	0.05%	0.006%
22	5.719	1339	1362	1395	rBV2	335808	932197	100.00%	12.749%
23	6.243	1512	1525	1553	rBV	293628	562178	60.31%	7.689%
24	6.469	1591	1595	1597	rBV	271	223	0.02%	0.003%
25	6.526	1603	1613	1625	rBV7	5612	11045	1.18%	0.151%
26	6.581	1628	1630	1633	rBV	135	89	0.01%	0.001%
27	6.629	1642	1645	1648	rBV	221	128	0.01%	0.002%
28	6.687	1648	1663	1681	rBV	210406	412115	44.21%	5.636%
29	6.890	1723	1726	1728	rVV	213	112	0.01%	0.002%
30	6.909	1728	1732	1735	rVB2	306	212	0.02%	0.003%
31	6.928	1735	1738	1743	rBV2	269	245	0.03%	0.003%
32	7.022	1764	1767	1768	rBV	198	112	0.01%	0.002%
33	7.456	1900	1902	1904	rBV	160	76	0.01%	0.001%
34	7.562	1922	1935	1959	rBV	124365	218744	23.47%	2.992%
35	7.694	1970	1976	1980	rBV2	724	973	0.10%	0.013%
36	7.748	1990	1993	1995	rBV	216	104	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040623\
 Data File : VU053587.D
 Acq On : 06 Apr 2023 12:03
 Operator : JC/MD
 Sample : VU0406WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK072

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

37	7.793	2003	2007	2015	rBV3	591	808	0.09%	0.011%
38	7.893	2025	2038	2061	rBV	455625	779153	83.58%	10.656%
39	8.079	2094	2096	2099	rBV2	415	232	0.02%	0.003%
40	8.176	2114	2126	2151	rBV	87540	147196	15.79%	2.013%
41	8.295	2160	2163	2167	rBV	267	238	0.03%	0.003%
42	8.327	2170	2173	2176	rBV	281	218	0.02%	0.003%
43	8.439	2206	2208	2210	rVB	187	55	0.01%	0.001%
44	8.542	2236	2240	2241	rBV2	735	439	0.05%	0.006%
45	8.626	2255	2266	2302	rBV2	220798	416365	44.66%	5.695%
46	9.121	2418	2420	2423	rVB	301	138	0.01%	0.002%
47	9.144	2424	2427	2429	rVB2	241	142	0.02%	0.002%
48	9.198	2441	2444	2448	rBV2	226	200	0.02%	0.003%
49	9.414	2498	2511	2537	rBV	406100	678165	72.75%	9.275%
50	9.620	2573	2575	2577	rBV	376	134	0.01%	0.002%
51	9.864	2648	2651	2655	rBV	226	144	0.02%	0.002%
52	9.922	2667	2669	2675	rBV2	193	201	0.02%	0.003%
53	9.999	2690	2693	2694	rBV	244	125	0.01%	0.002%
54	10.095	2720	2723	2724	rBV	539	298	0.03%	0.004%
55	10.105	2724	2726	2728	rVV3	730	428	0.05%	0.006%
56	10.343	2797	2800	2801	rBV	219	104	0.01%	0.001%
57	10.751	2915	2927	2946	rBV	302836	483064	51.82%	6.607%
58	11.472	3145	3151	3160	rVB4	980	1564	0.17%	0.021%
59	11.745	3228	3236	3244	rBV3	2156	3150	0.34%	0.043%
60	11.809	3244	3256	3276	rBV	448836	713190	76.51%	9.754%
61	12.189	3362	3374	3392	rBV	455298	737020	79.06%	10.080%
62	12.378	3430	3433	3438	rBV3	422	405	0.04%	0.006%
63	13.217	3690	3694	3696	rBV3	1702	1304	0.14%	0.018%
64	13.841	3882	3888	3897	rVB5	6065	8018	0.86%	0.110%


Sum of corrected areas: 7311693

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040623\
Data File : VU053587.D
Acq On : 06 Apr 2023 12:03
Operator : JC/MD
Sample : VU0406WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK072

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

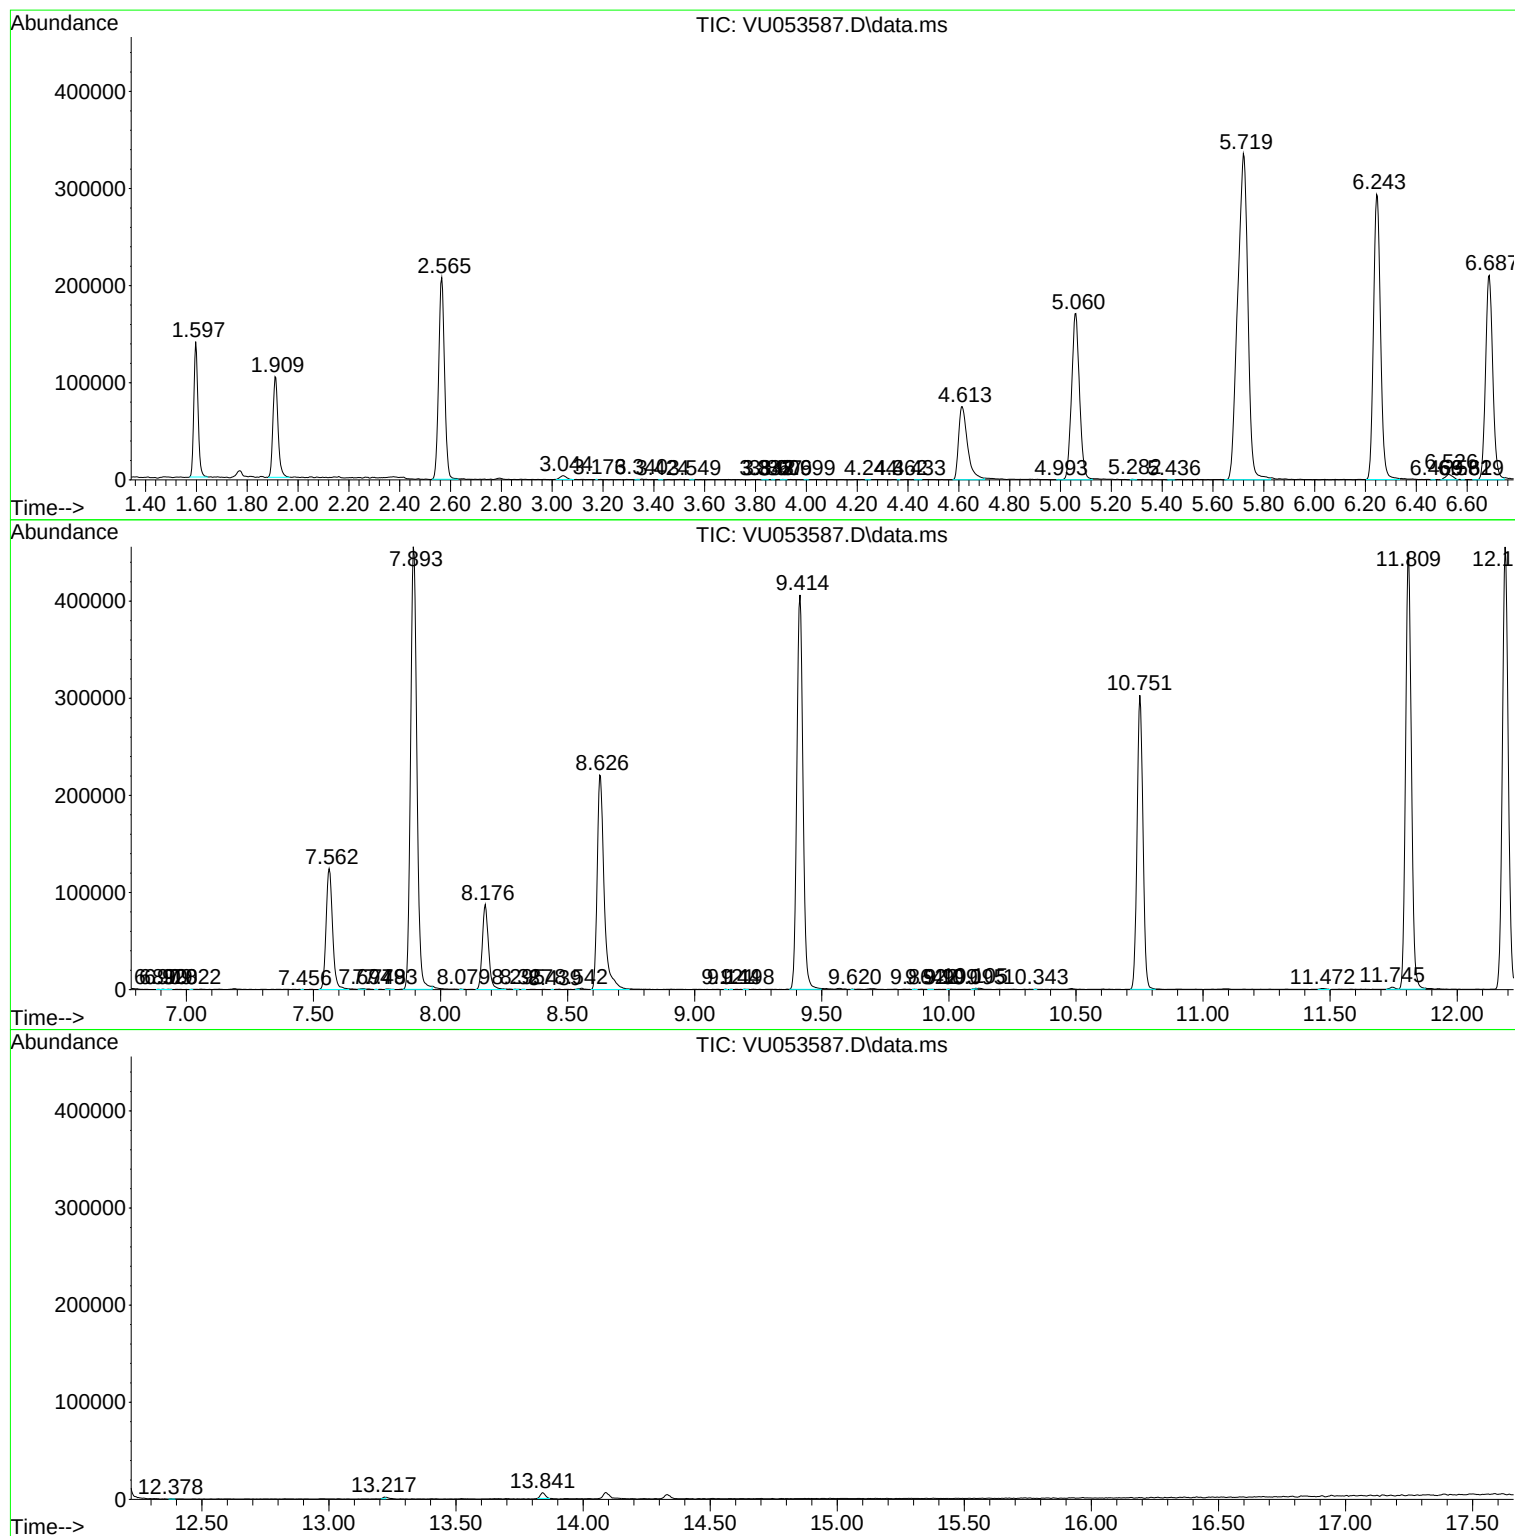

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040623\
Data File : VU053587.D
Acq On : 06 Apr 2023 12:03
Operator : JC/MD
Sample : VU0406WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK072

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040623\
Data File : VU053587.D
Acq On : 06 Apr 2023 12:03
Operator : JC/MD
Sample : VU0406WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK072

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------