
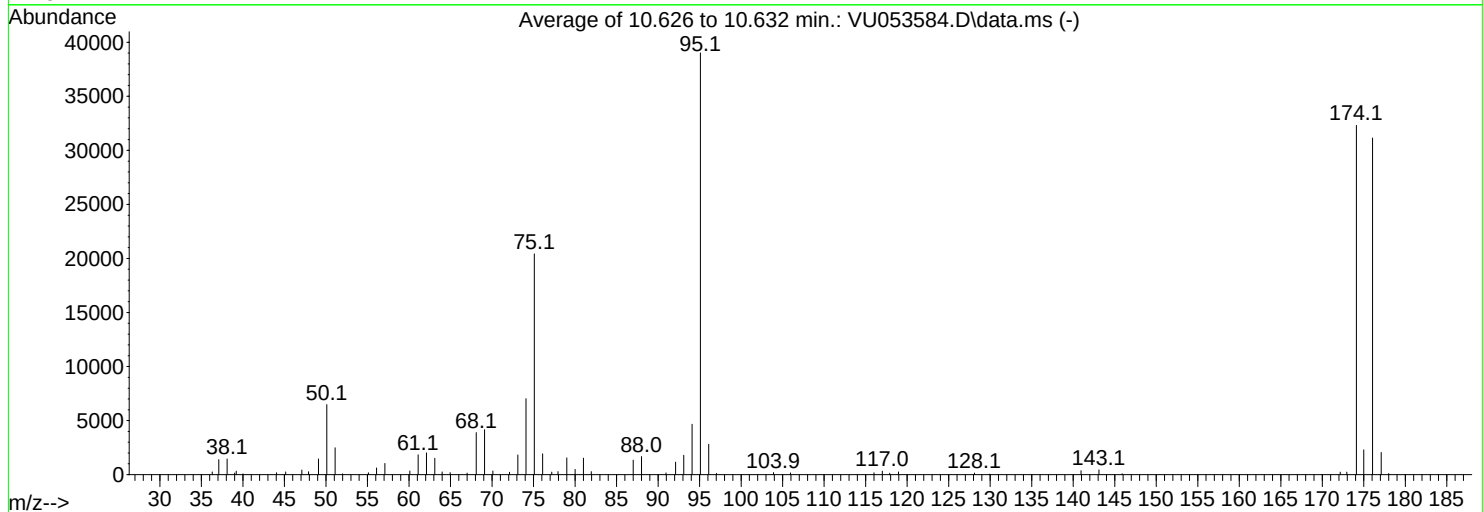


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040623\
 Data File : VU053584.D
 Acq On : 06 Apr 2023 09:00
 Operator : JC/MD
 Sample : BFB175
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB175

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis
 Last Update : Sat Apr 01 04:51:17 2023

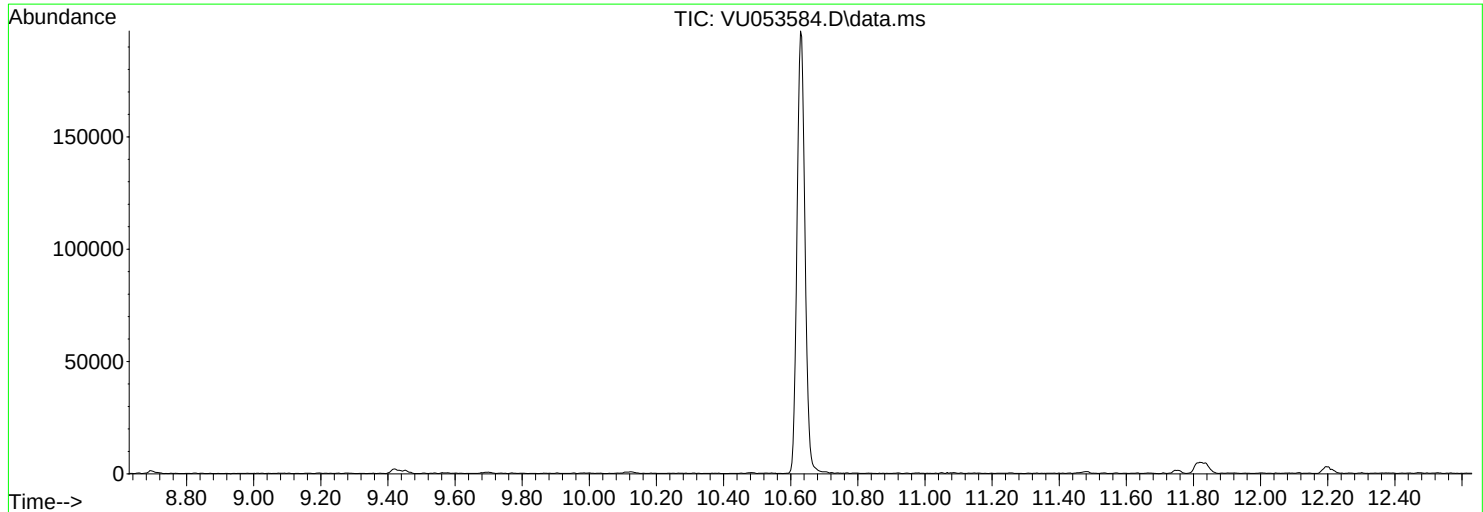

AutoFind: Scans 2888, 2889, 2890; Background Corrected with Scan 2877

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.6	6486	PASS
75	95	30	80	52.3	20424	PASS
95	95	100	100	100.0	39019	PASS
96	95	5	9	7.2	2818	PASS
173	174	0.00	2	0.7	231	PASS
174	95	50	120	82.8	32315	PASS
175	174	5	9	7.1	2302	PASS
176	174	95	101	96.4	31139	PASS
177	176	5	9	6.6	2052	PASS

m/z	Abundance
44.10	292.0

Instrument :
MSVOA_U
ClientSampleId :
BFB175

m/z	Abundance
36.10	241.0
37.10	1429.0
38.10	1429.0
39.00	450.0
44.10	474.0
45.10	246.0
47.10	409.0
47.90	258.0
49.10	1478.0
50.10	6270.0
51.10	2418.0
55.10	126.0
56.10	630.0
57.10	1012.0
60.10	267.0
61.10	1646.0
62.10	1874.0
63.10	1470.0
64.00	243.0
64.90	199.0
67.00	149.0
68.10	3933.0
69.10	3901.0
70.10	290.0
72.10	225.0
73.10	1770.0
74.10	6595.0
75.10	19560.0
76.10	1932.0
77.20	201.0
77.90	310.0
79.00	1537.0
80.00	499.0
81.00	1413.0
81.90	295.0
87.00	1298.0
88.00	1666.0
91.00	192.0
92.10	1167.0
93.10	1651.0
94.10	4525.0
95.10	37384.0
96.10	2553.0
97.10	125.0
103.90	186.0
106.00	187.0
116.00	152.0
117.00	313.0
117.90	115.0
119.00	257.0
128.10	118.0
141.00	359.0
143.10	493.0
145.90	120.0
172.10	283.0
173.00	224.0
174.10	30344.0
175.00	2126.0
176.10	29456.0
177.10	1964.0

Instrument :
MSVOA_U
ClientSampleId :
BFB175

m/z	Abundance
36.30	269.0
37.10	1385.0
38.10	1471.0
39.20	442.0
40.00	103.0
44.00	475.0
45.20	271.0
47.10	441.0
47.90	277.0
49.10	1463.0
50.10	6576.0
51.10	2604.0
52.00	111.0
55.10	182.0
56.10	610.0
57.10	1043.0
60.10	356.0
61.10	1848.0
62.10	2111.0
63.10	1596.0
64.00	255.0
65.00	202.0
67.00	165.0
68.10	3962.0
69.10	4272.0
70.10	354.0
72.10	229.0
73.10	1934.0
74.10	7271.0
75.10	21072.0
76.10	1982.0
77.30	264.0
78.00	298.0
79.00	1602.0
80.00	488.0
81.00	1595.0
81.90	275.0
87.00	1327.0
88.00	1732.0
91.00	162.0
92.10	1147.0
93.10	1872.0
94.10	4829.0
95.10	40192.0
96.10	2908.0
97.00	117.0
103.90	188.0
106.00	169.0
116.00	171.0
117.00	345.0
117.90	143.0
118.90	278.0
128.10	152.0
141.00	382.0
143.10	438.0
145.90	139.0
172.20	236.0
172.90	225.0
174.10	33152.0
175.00	2346.0
176.10	32288.0
177.10	2124.0
178.00	146.0

Instrument :
MSVOA_U
ClientSampleId :
BFB175

m/z	Abundance
36.30	262.0
37.10	1355.0
38.10	1447.0
39.20	534.0
40.00	137.0
44.10	445.0
45.20	232.0
47.10	441.0
47.90	271.0
49.10	1390.0
50.10	6611.0
51.10	2464.0
52.00	119.0
55.10	227.0
56.10	613.0
57.10	1072.0
60.10	391.0
61.10	1995.0
62.10	2068.0
63.10	1474.0
64.00	245.0
65.00	167.0
67.00	133.0
68.10	3768.0
69.10	4304.0
70.10	382.0
72.10	208.0
73.10	1769.0
74.10	7225.0
75.10	20640.0
76.10	1841.0
77.10	249.0
78.00	260.0
79.00	1507.0
80.00	491.0
81.00	1563.0
82.00	275.0
87.00	1395.0
88.00	1599.0
90.90	125.0
92.10	1150.0
93.10	1873.0
94.10	4649.0
95.10	39480.0
96.10	2992.0
97.10	109.0
103.90	187.0
105.90	137.0
116.00	201.0
117.00	328.0
117.90	151.0
118.90	238.0
128.10	182.0
129.90	124.0
140.90	380.0
143.10	403.0
172.20	175.0
172.90	244.0
174.10	33448.0
175.00	2435.0
176.00	31672.0
177.10	2067.0
178.00	173.0

Instrument :
MSVOA_U
ClientSampleId :
BFB175